

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031623\
 Data File : PP056503.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2023 13:52
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/17/2023
 Supervised By :Ankita Jodhani 03/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 04:37:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 17 04:34:46 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.437	3.671	36278425	34558176	17.757	17.567
2) SA Decachlor...	10.275	8.777	25356458	29094659	17.502m	19.128

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031623\
Data File : PP056503.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2023 13:52
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2023
Supervised By :Ankita Jodhani 03/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 04:37:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031623.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 17 04:34:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

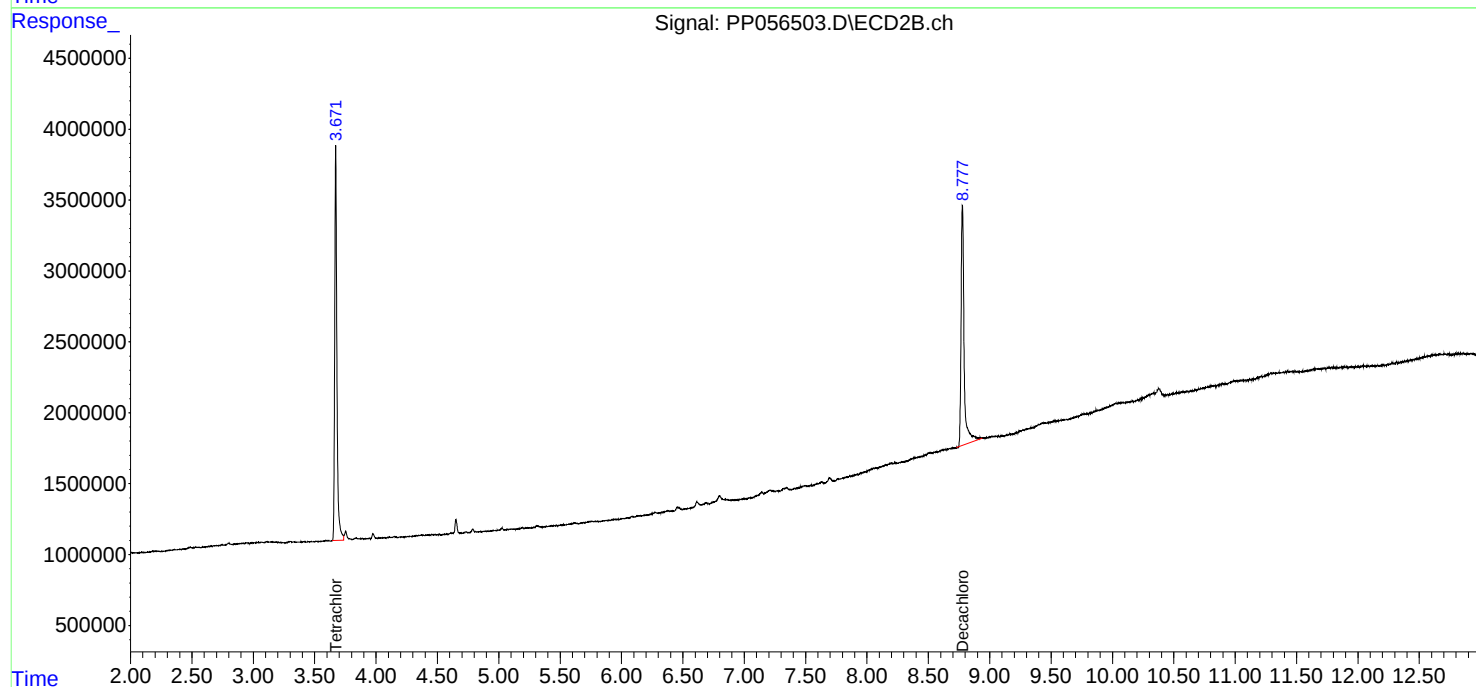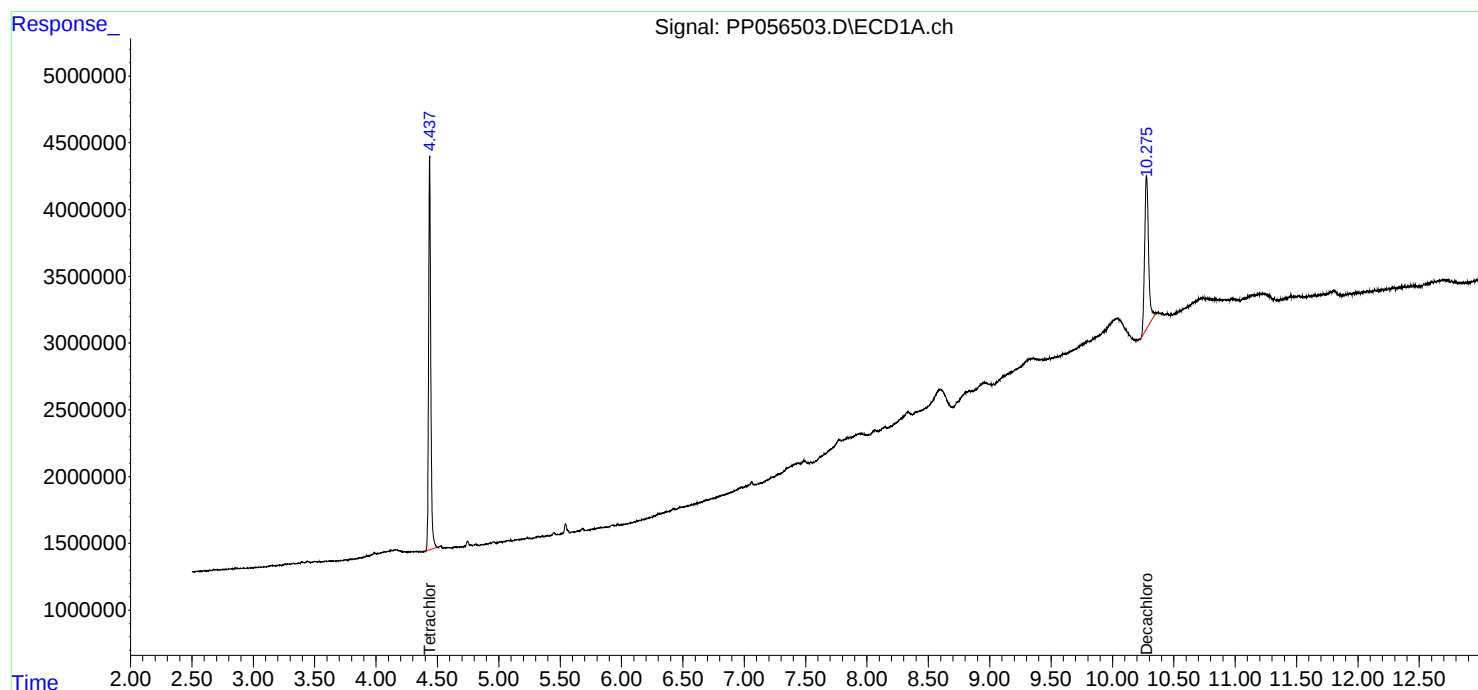

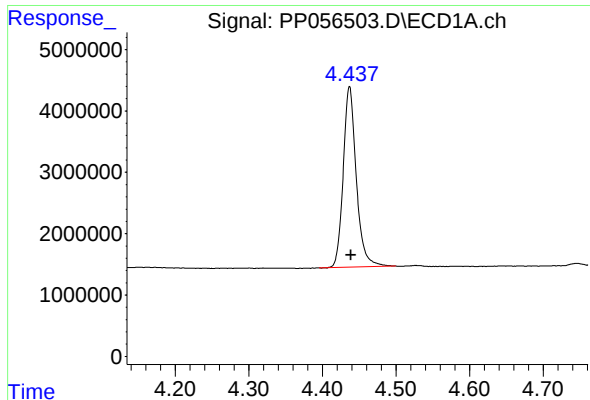


#1 Tetrachloro-m-xylene

R.T.: 4.437 min
Delta R.T.: -0.002 min
Response: 36278425
Conc: 17.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2023
Supervised By :Ankita Jodhani 03/17/2023

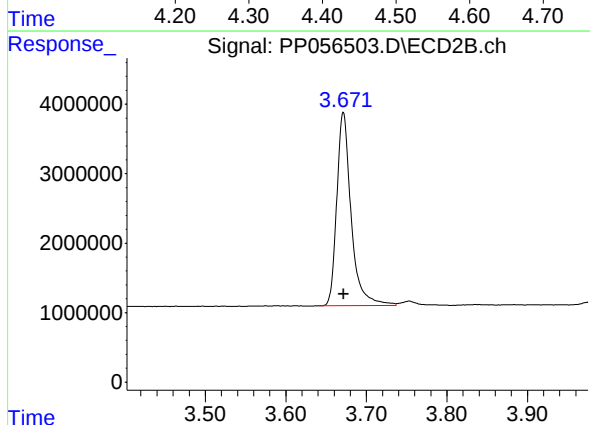


#1 Tetrachloro-m-xylene

R.T.: 3.671 min
Delta R.T.: 0.000 min
Response: 34558176
Conc: 17.57 ng/ml

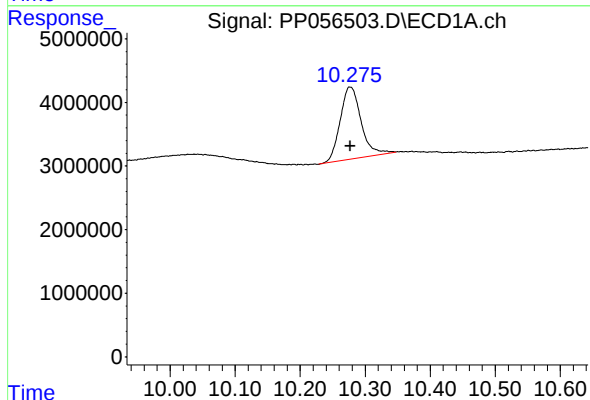

#2 Decachlorobiphenyl

R.T.: 10.275 min
Delta R.T.: -0.002 min
Response: 25356458
Conc: 17.50 ng/ml m

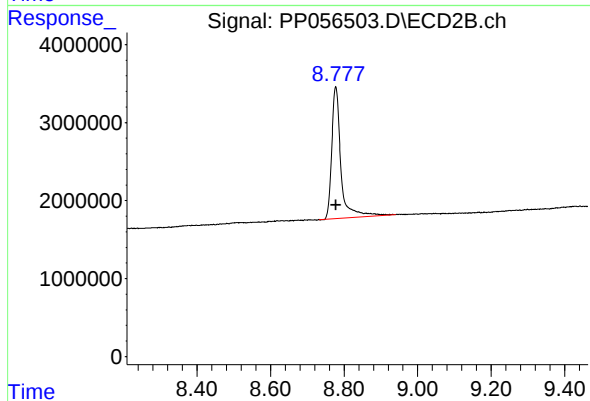

#2 Decachlorobiphenyl

R.T.: 8.777 min
Delta R.T.: 0.000 min
Response: 29094659
Conc: 19.13 ng/ml