

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031623\
 Data File : PP056525.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2023 19:56
 Operator : YP\AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/17/2023
 Supervised By :Ankita Jodhani 03/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 03:15:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 17 03:03:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.438	3.671	9559862	8585336	4.662	4.465
2) SA Decachlor...	10.278	8.774	5272632	6960275	3.829m	4.691m
Target Compounds						
26) L6 AR-1254-1	6.475	5.590	3675808	5458807	50.261	51.260
27) L6 AR-1254-2	6.695	5.739	5272822	4621998	49.272	51.084
28) L6 AR-1254-3	7.063	6.148	5055749	7050064	47.373	50.052
29) L6 AR-1254-4	7.351	6.379	3227884	3800831	48.177	51.298
30) L6 AR-1254-5	7.772	6.803	3831806	6615032	50.511	55.682

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031623\
Data File : PP056525.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2023 19:56
Operator : YP\AJ
Sample : AR1254ICC050
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2023
Supervised By :Ankita Jodhani 03/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 03:15:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031623.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 17 03:03:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

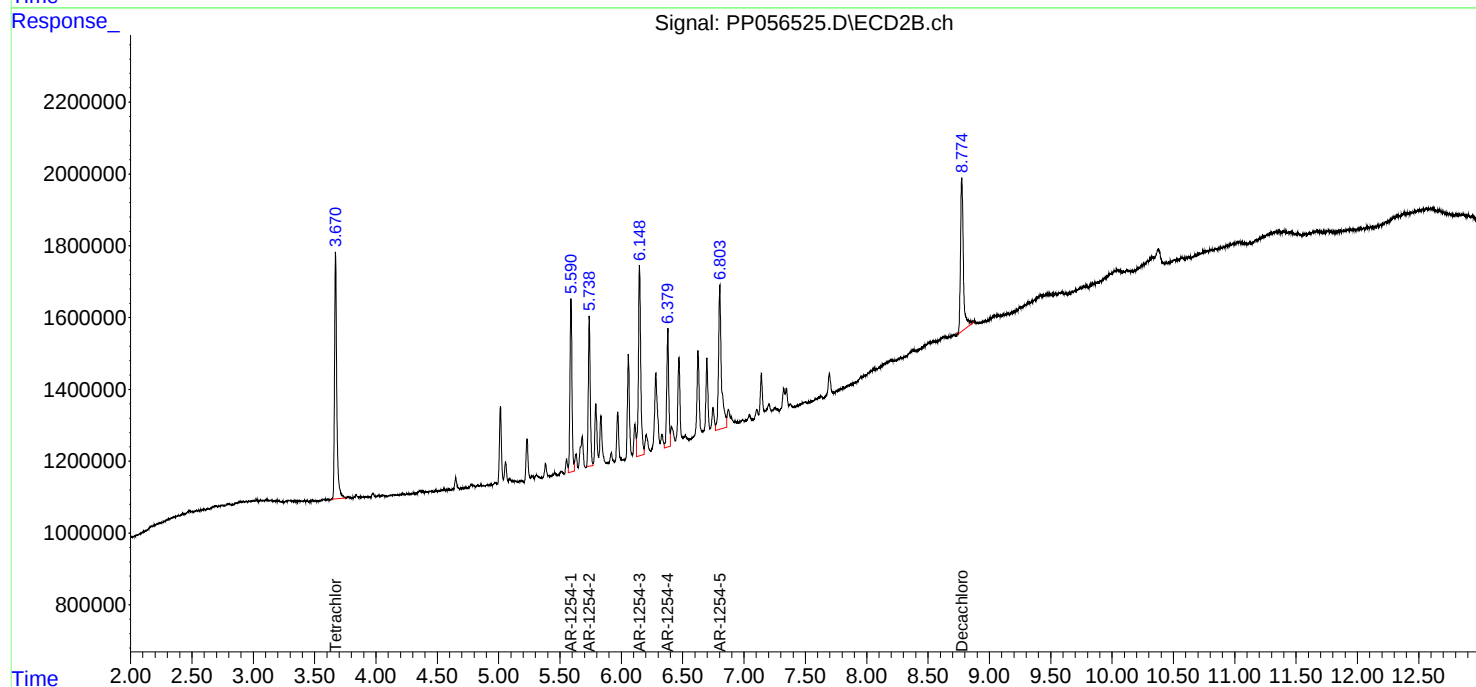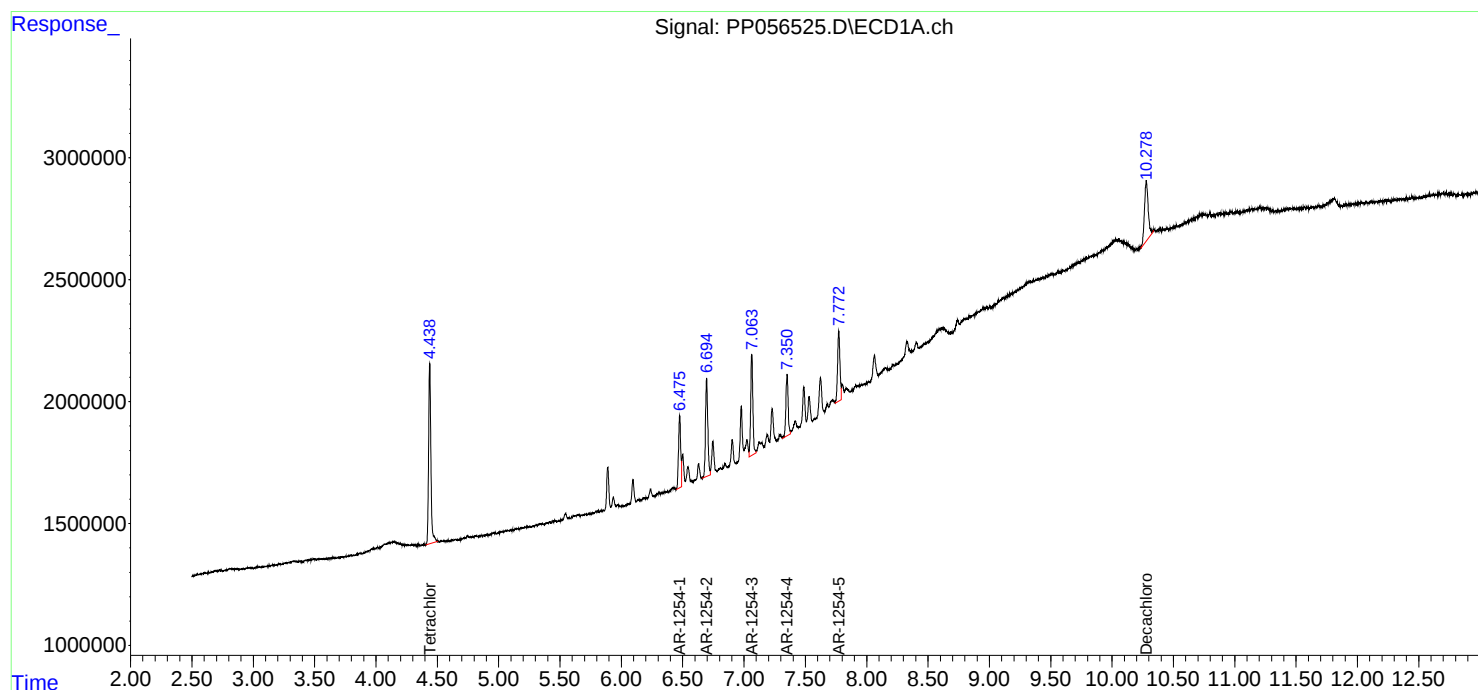

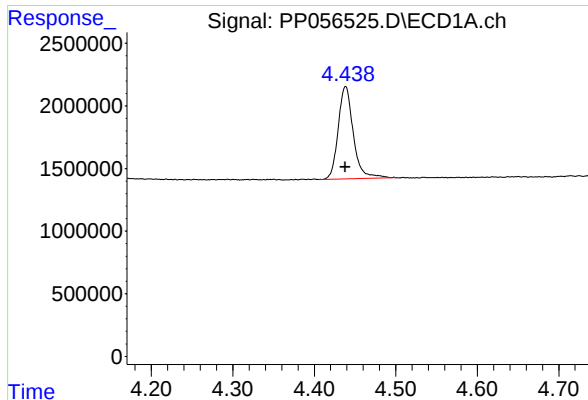


#1 Tetrachloro-m-xylene

R.T.: 4.438 min
Delta R.T.: 0.000 min
Response: 9559862
Conc: 4.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2023
Supervised By :Ankita Jodhani 03/17/2023

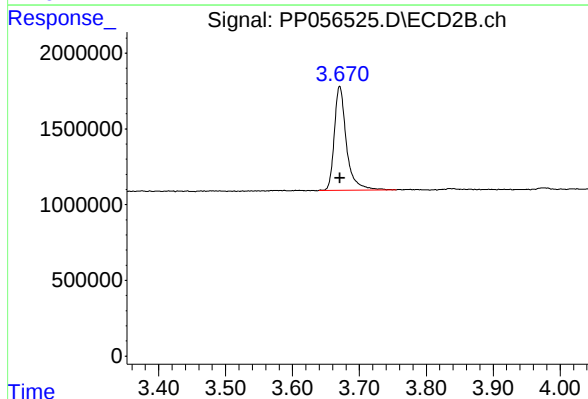


#1 Tetrachloro-m-xylene

R.T.: 3.671 min
Delta R.T.: 0.000 min
Response: 8585336
Conc: 4.46 ng/ml

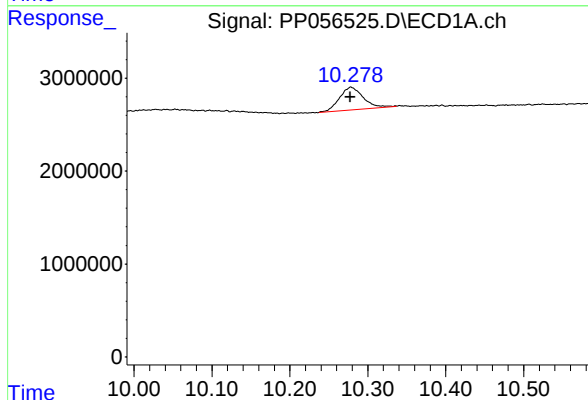


#2 Decachlorobiphenyl

R.T.: 10.278 min
Delta R.T.: 0.000 min
Response: 5272632
Conc: 3.83 ng/ml m

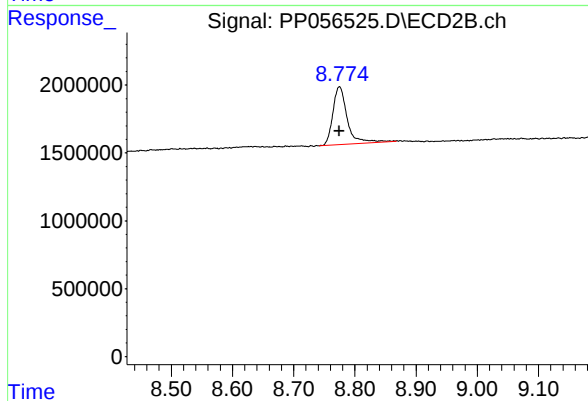

#2 Decachlorobiphenyl

R.T.: 8.774 min
Delta R.T.: 0.000 min
Response: 6960275
Conc: 4.69 ng/ml m

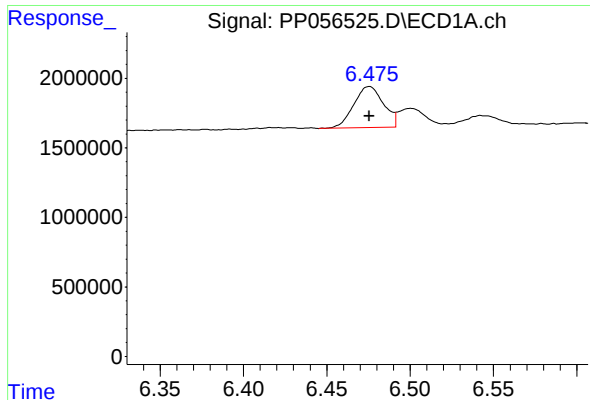


#26 AR-1254-1

R.T.: 6.475 min
Delta R.T.: 0.000 min
Response: 3675808
Conc: 50.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2023
Supervised By :Ankita Jodhani 03/17/2023

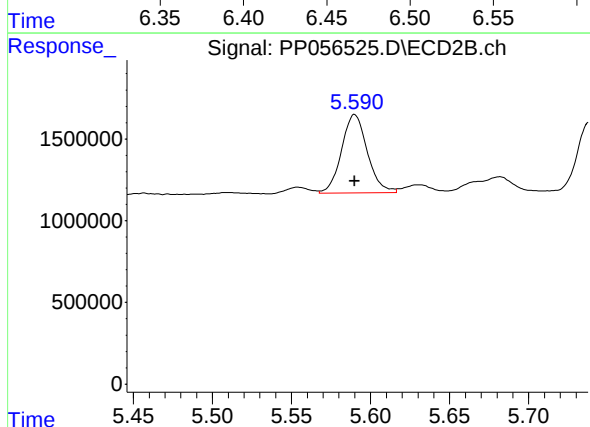


#26 AR-1254-1

R.T.: 5.590 min
Delta R.T.: 0.000 min
Response: 5458807
Conc: 51.26 ng/ml

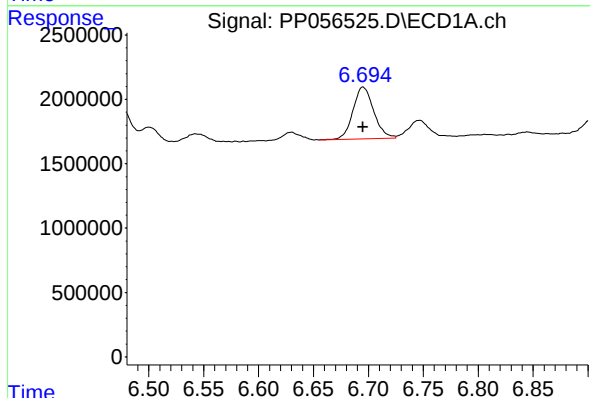


#27 AR-1254-2

R.T.: 6.695 min
Delta R.T.: 0.000 min
Response: 5272822
Conc: 49.27 ng/ml

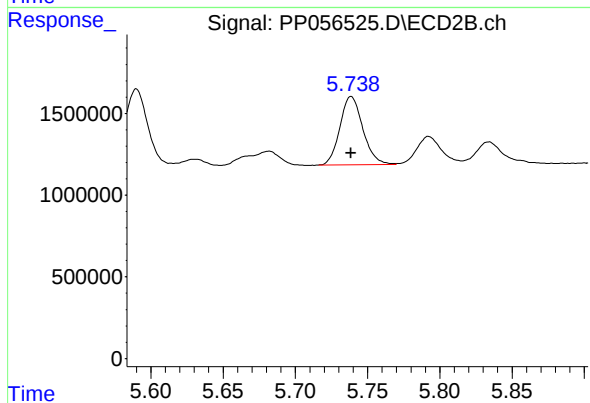

#27 AR-1254-2

R.T.: 5.739 min
Delta R.T.: 0.000 min
Response: 4621998
Conc: 51.08 ng/ml

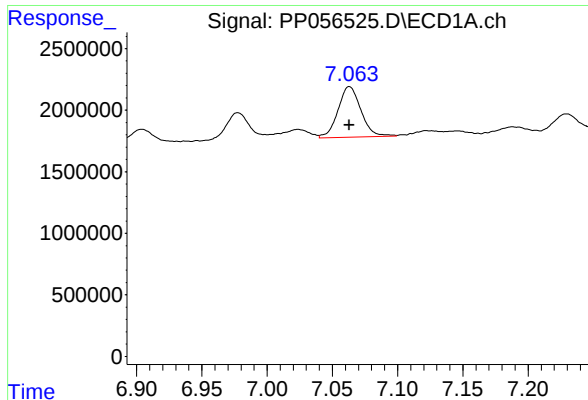


#28 AR-1254-3

R.T.: 7.063 min
Delta R.T.: 0.000 min
Response: 5055749
Conc: 47.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2023
Supervised By :Ankita Jodhani 03/17/2023

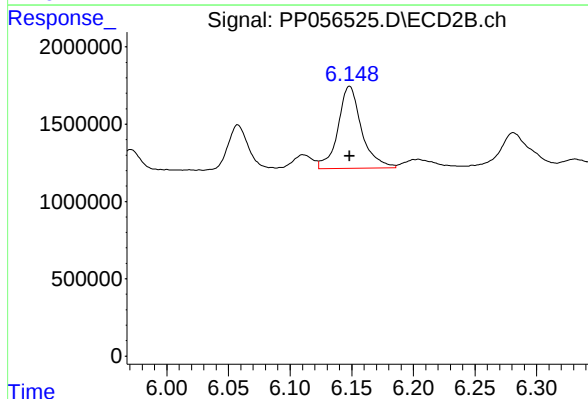


#28 AR-1254-3

R.T.: 6.148 min
Delta R.T.: 0.000 min
Response: 7050064
Conc: 50.05 ng/ml

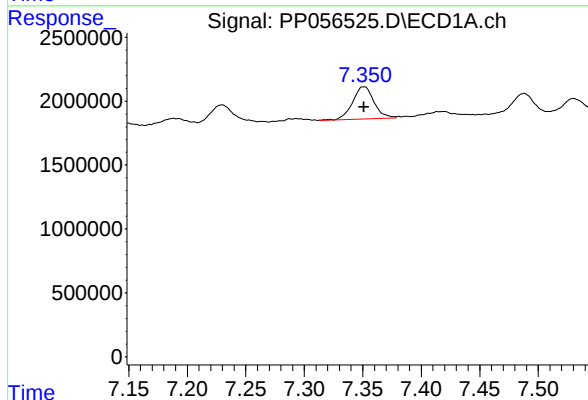


#29 AR-1254-4

R.T.: 7.351 min
Delta R.T.: 0.000 min
Response: 3227884
Conc: 48.18 ng/ml

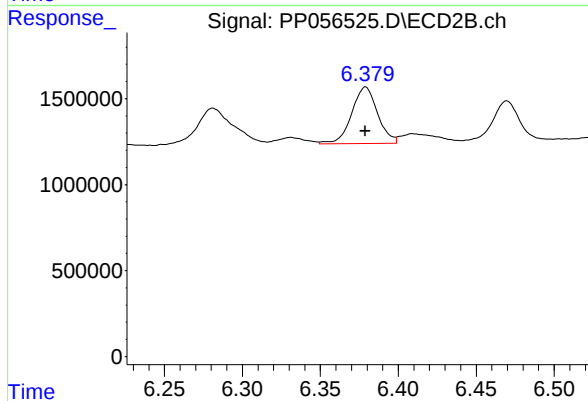

#29 AR-1254-4

R.T.: 6.379 min
Delta R.T.: 0.000 min
Response: 3800831
Conc: 51.30 ng/ml

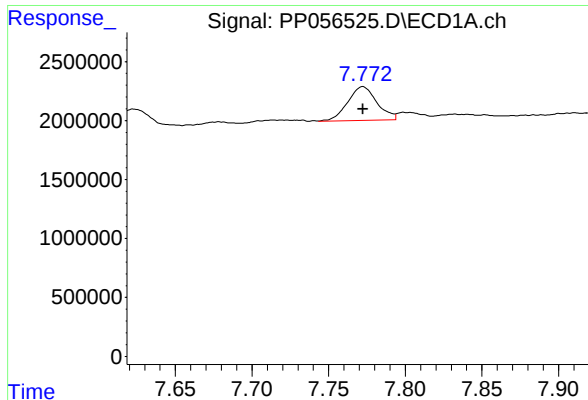


#30 AR-1254-5

R.T.: 7.772 min
Delta R.T.: 0.000 min
Response: 3831806
Conc: 50.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2023
Supervised By :Ankita Jodhani 03/17/2023

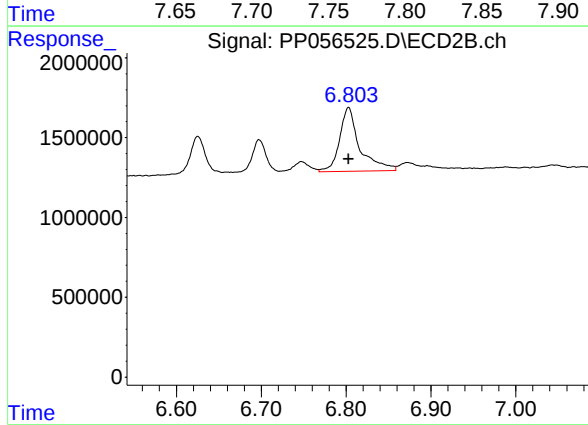

#30 AR-1254-5

R.T.: 6.803 min
Delta R.T.: 0.000 min
Response: 6615032
Conc: 55.68 ng/ml