

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031623\
 Data File : PP056531.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2023 21:35
 Operator : YP\AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1268ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/17/2023
 Supervised By :Ankita Jodhani 03/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 04:14:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 17 04:11:27 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.438	3.670	9902297	8942966	4.810	4.672
2) SA Decachlor...	10.278	8.773	9496914	13499672	3.855m	5.210 #
Target Compounds						
41) L9 AR-1268-1	8.721	7.633	9008388	10739273	44.824	51.123
42) L9 AR-1268-2	8.818	7.697	8312000	10034340	47.184	50.817
43) L9 AR-1268-3	9.054	7.909	7399649	8784953	44.767m	50.824
44) L9 AR-1268-4	9.492	8.198	2197004	2871034	42.347	51.362
45) L9 AR-1268-5	9.924	8.503	19847466	21166475	42.758	47.401m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031623\
Data File : PP056531.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2023 21:35
Operator : YP\AJ
Sample : AR1268ICC050
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2023
Supervised By :Ankita Jodhani 03/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 04:14:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031623.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 17 04:11:27 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

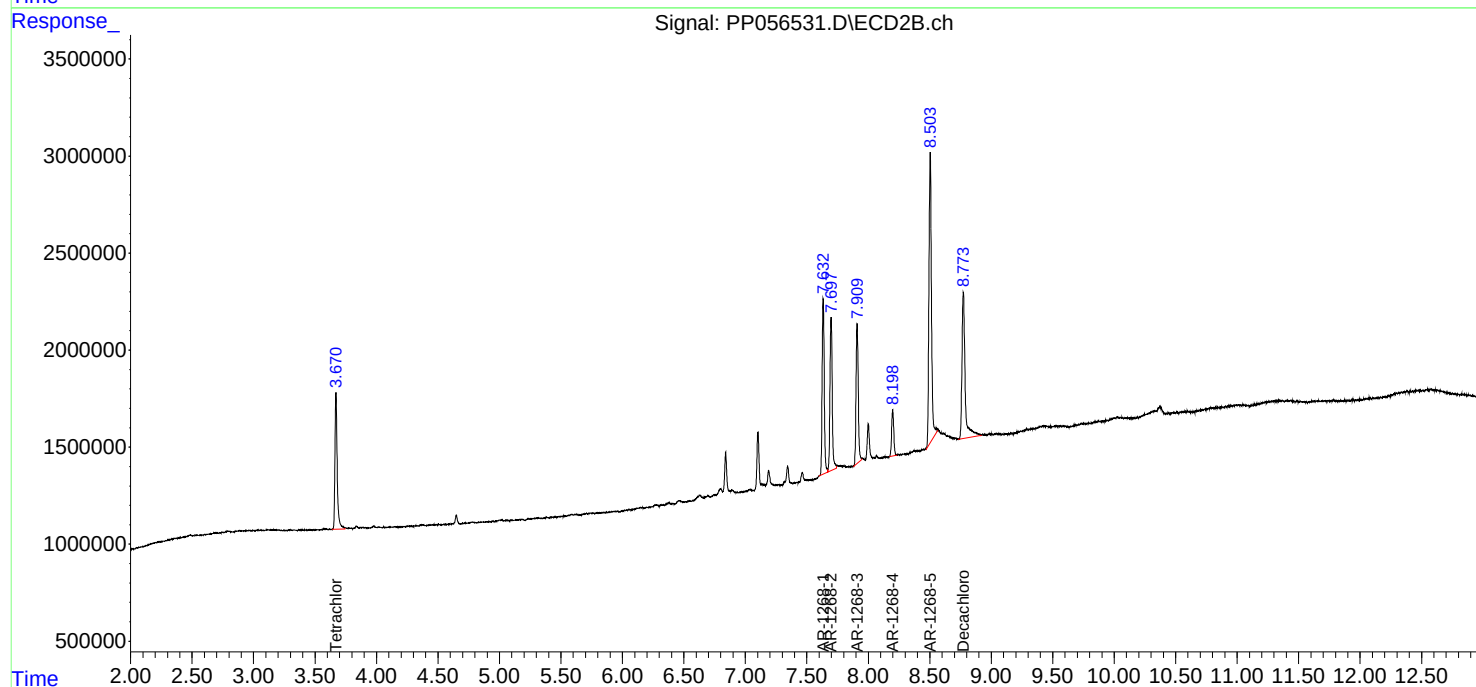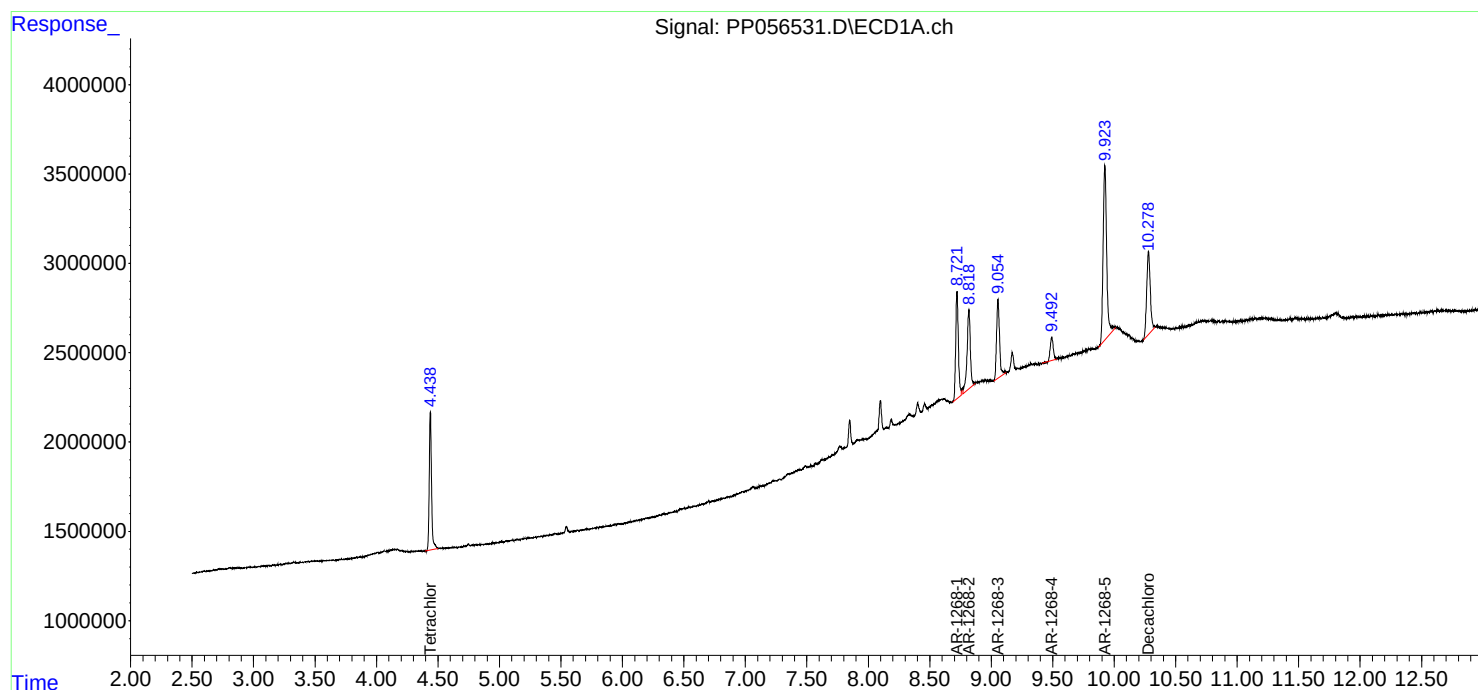

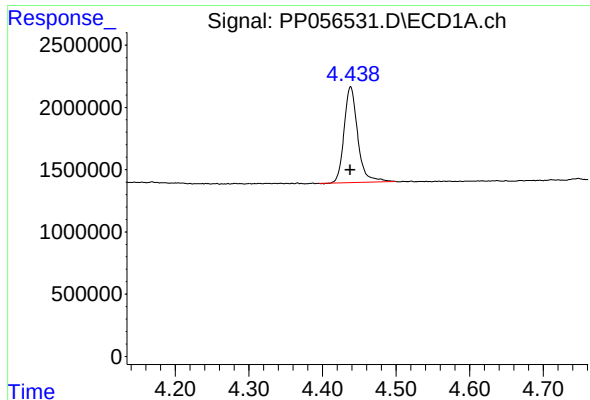


#1 Tetrachloro-m-xylene

R.T.: 4.438 min
Delta R.T.: 0.000 min
Response: 9902297
Conc: 4.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2023
Supervised By :Ankita Jodhani 03/17/2023

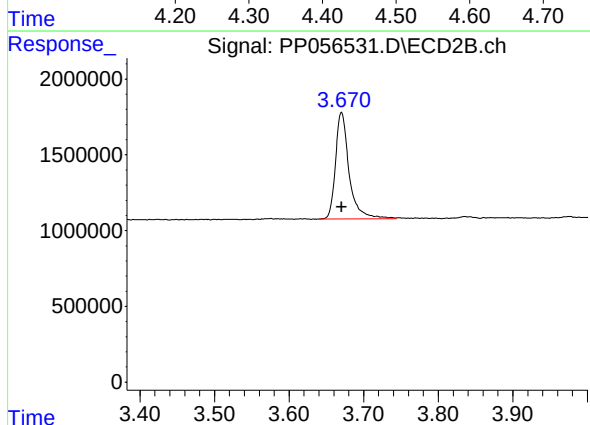


#1 Tetrachloro-m-xylene

R.T.: 3.670 min
Delta R.T.: 0.000 min
Response: 8942966
Conc: 4.67 ng/ml

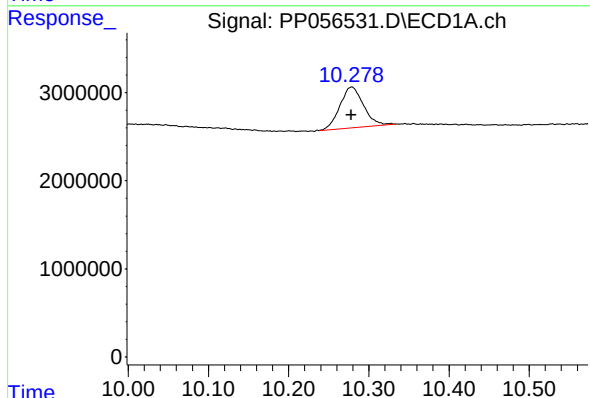


#2 Decachlorobiphenyl

R.T.: 10.278 min
Delta R.T.: 0.000 min
Response: 9496914
Conc: 3.86 ng/ml m

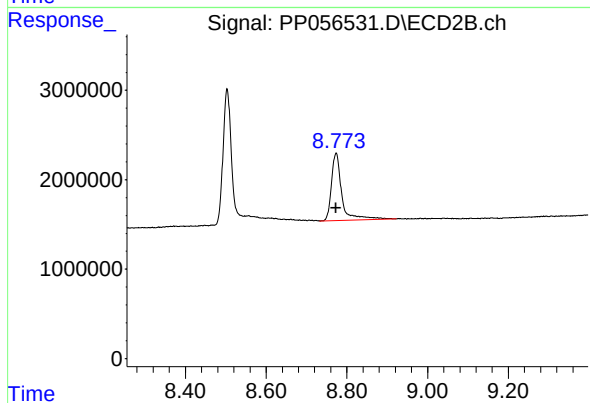

#2 Decachlorobiphenyl

R.T.: 8.773 min
Delta R.T.: 0.000 min
Response: 13499672
Conc: 5.21 ng/ml

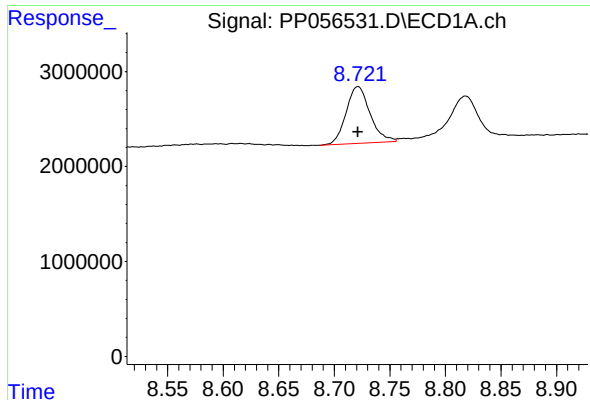


#41 AR-1268-1

R.T.: 8.721 min
Delta R.T.: 0.000 min
Response: 9008388
Conc: 44.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2023
Supervised By :Ankita Jodhani 03/17/2023

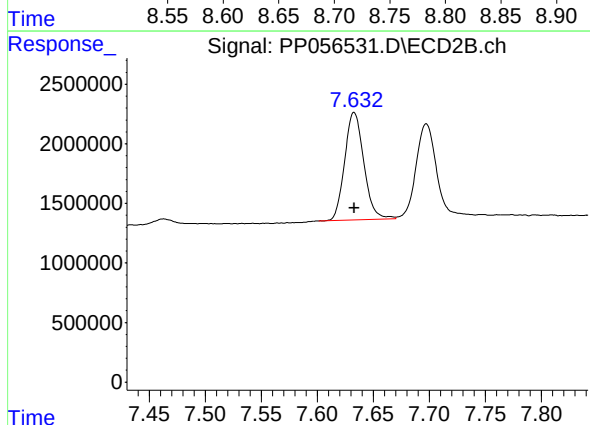


#41 AR-1268-1

R.T.: 7.633 min
Delta R.T.: 0.000 min
Response: 10739273
Conc: 51.12 ng/ml

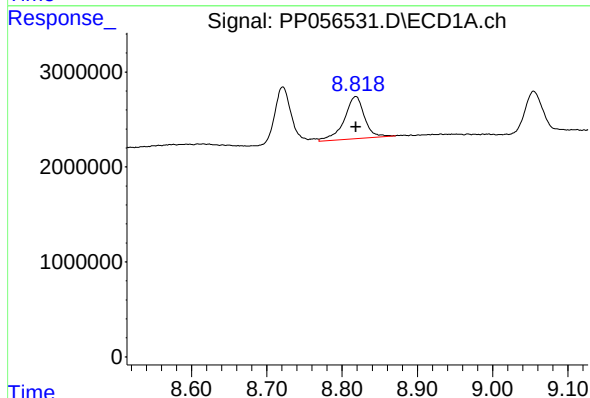


#42 AR-1268-2

R.T.: 8.818 min
Delta R.T.: 0.000 min
Response: 8312000
Conc: 47.18 ng/ml

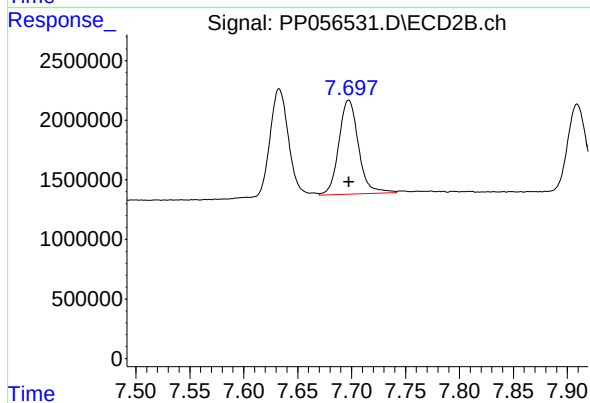

#42 AR-1268-2

R.T.: 7.697 min
Delta R.T.: 0.000 min
Response: 10034340
Conc: 50.82 ng/ml

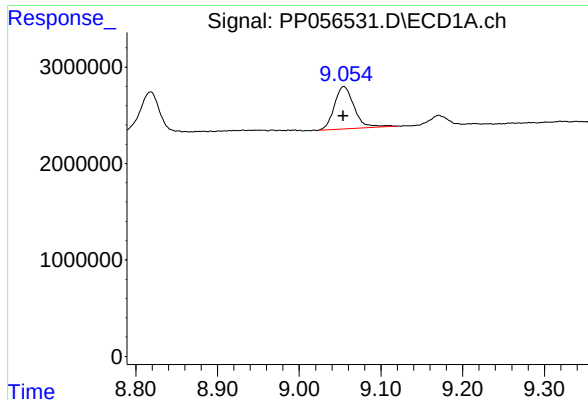


#43 AR-1268-3

R.T.: 9.054 min
Delta R.T.: 0.000 min
Response: 7399649
Conc: 44.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2023
Supervised By :Ankita Jodhani 03/17/2023

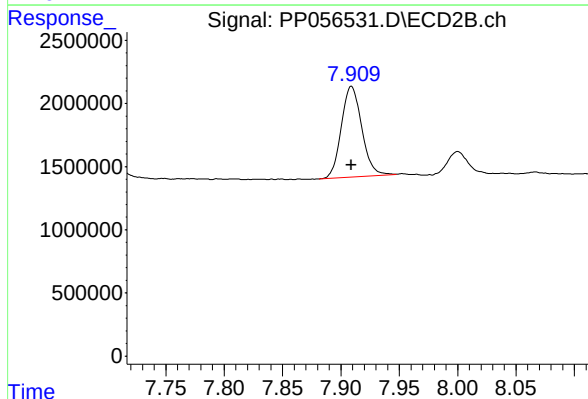


#43 AR-1268-3

R.T.: 7.909 min
Delta R.T.: 0.000 min
Response: 8784953
Conc: 50.82 ng/ml

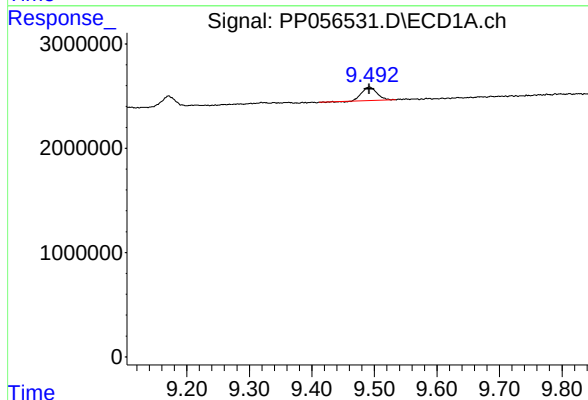


#44 AR-1268-4

R.T.: 9.492 min
Delta R.T.: 0.000 min
Response: 2197004
Conc: 42.35 ng/ml

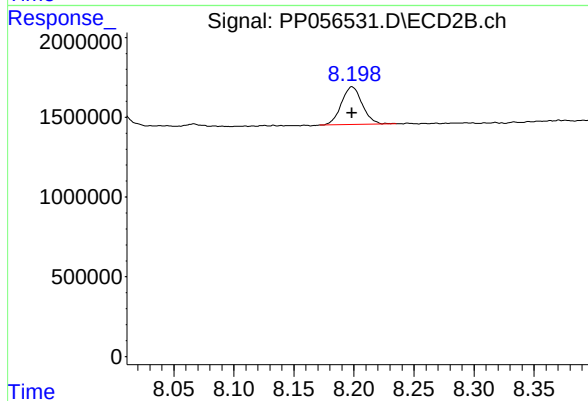

#44 AR-1268-4

R.T.: 8.198 min
Delta R.T.: 0.000 min
Response: 2871034
Conc: 51.36 ng/ml

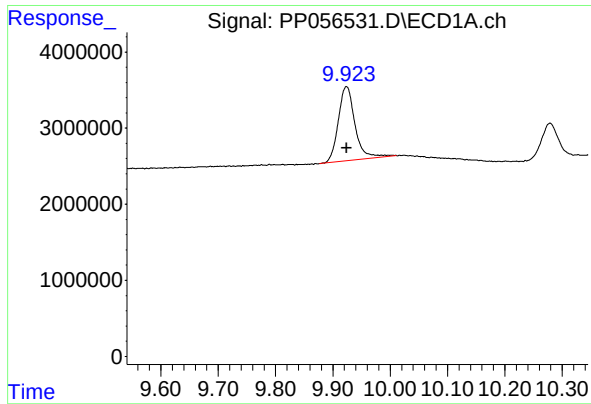


#45 AR-1268-5

R.T.: 9.924 min
Delta R.T.: 0.000 min
Response: 19847466
Conc: 42.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2023
Supervised By :Ankita Jodhani 03/17/2023

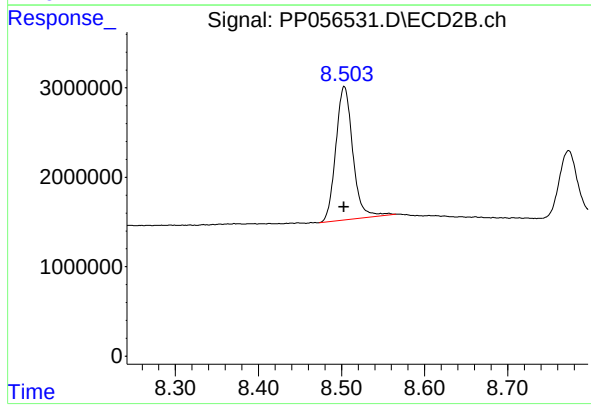

#45 AR-1268-5

R.T.: 8.503 min
Delta R.T.: 0.000 min
Response: 21166475
Conc: 47.40 ng/ml