

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031721\
 Data File : PP034098.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Mar 2021 17:02
 Operator : DD\AJ
 Sample : M1697-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-4A-(1-1.5)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 07:09:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.852	4.263	1965305	1033085	22.714	25.429
2) SA Decachlor...	10.780	9.582f	1386560	521382	16.418	19.538

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031721\
Data File : PP034098.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Mar 2021 17:02
Operator : DD\AJ
Sample : M1697-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SB-4A-(1-1.5)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 07:09:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

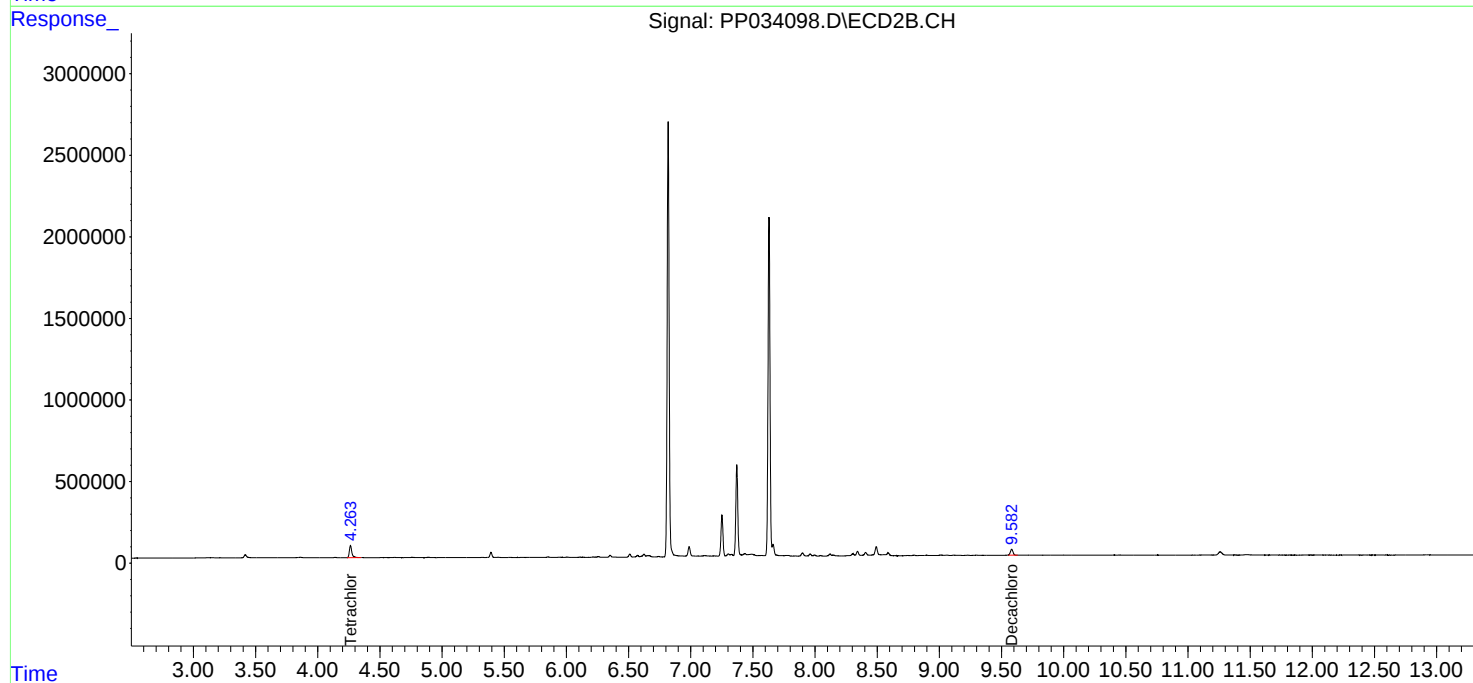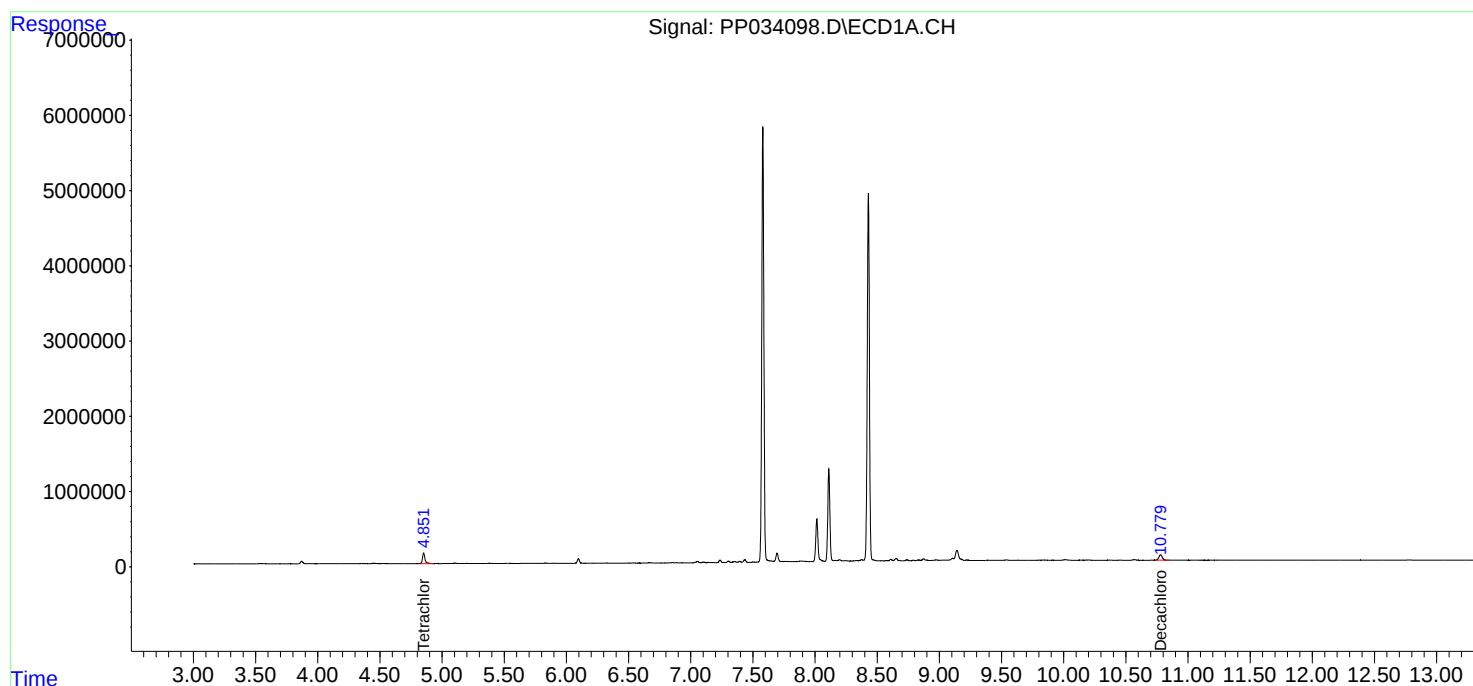


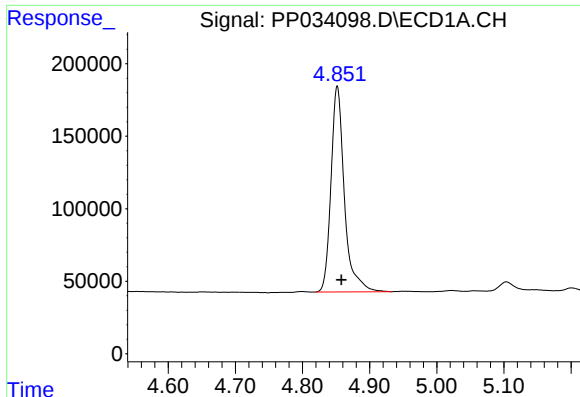

#1 Tetrachloro-m-xylene


R.T.: 4.852 min
Delta R.T.: -0.006 min
Response: 1965305
Conc: 22.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-4A-(1-1.5)

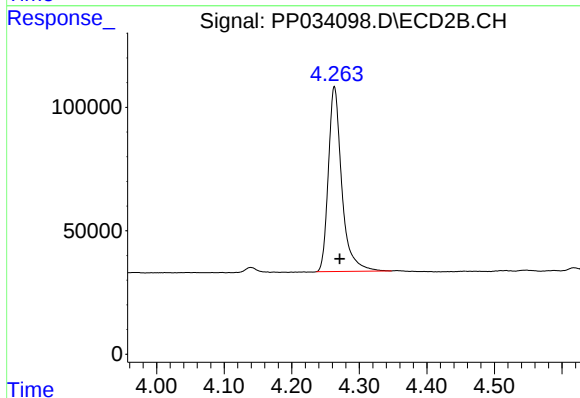


#1 Tetrachloro-m-xylene

R.T.: 4.263 min
Delta R.T.: -0.008 min
Response: 1033085
Conc: 25.43 ng/ml

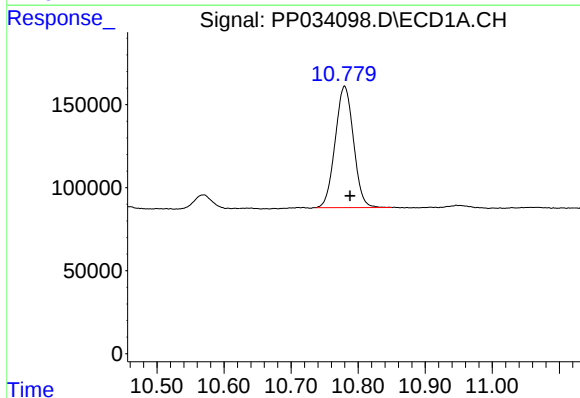

#2 Decachlorobiphenyl

R.T.: 10.780 min
Delta R.T.: -0.008 min
Response: 1386560
Conc: 16.42 ng/ml

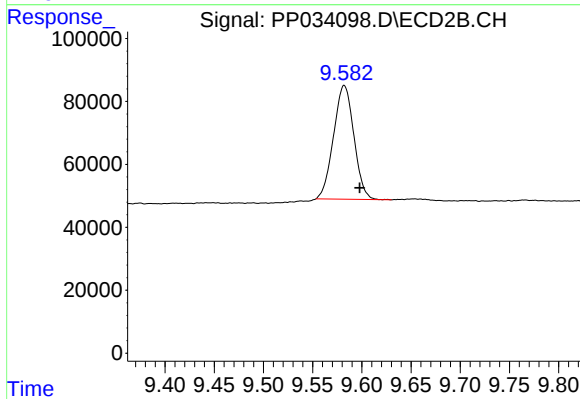

#2 Decachlorobiphenyl

R.T.: 9.582 min
Delta R.T.: -0.016 min
Response: 521382
Conc: 19.54 ng/ml