

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031721\
 Data File : PP034106.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Mar 2021 19:17
 Operator : DD\AJ
 Sample : M1697-08
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-3A-(1-1.5)

Manual Integrations
 APPROVED

Ankita
 3/18/2021 4:00:09 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 07:11:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.852	4.263	2158025	1219163	24.941	30.010
2) SA Decachlor...	10.779	9.582f	1617648	573751	19.154	21.501m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031721\
Data File : PP034106.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Mar 2021 19:17
Operator : DD\AJ
Sample : M1697-08
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SB-3A-(1-1.5)


Manual Integrations
APPROVED

Ankita
3/18/2021 4:00:09 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 07:11:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

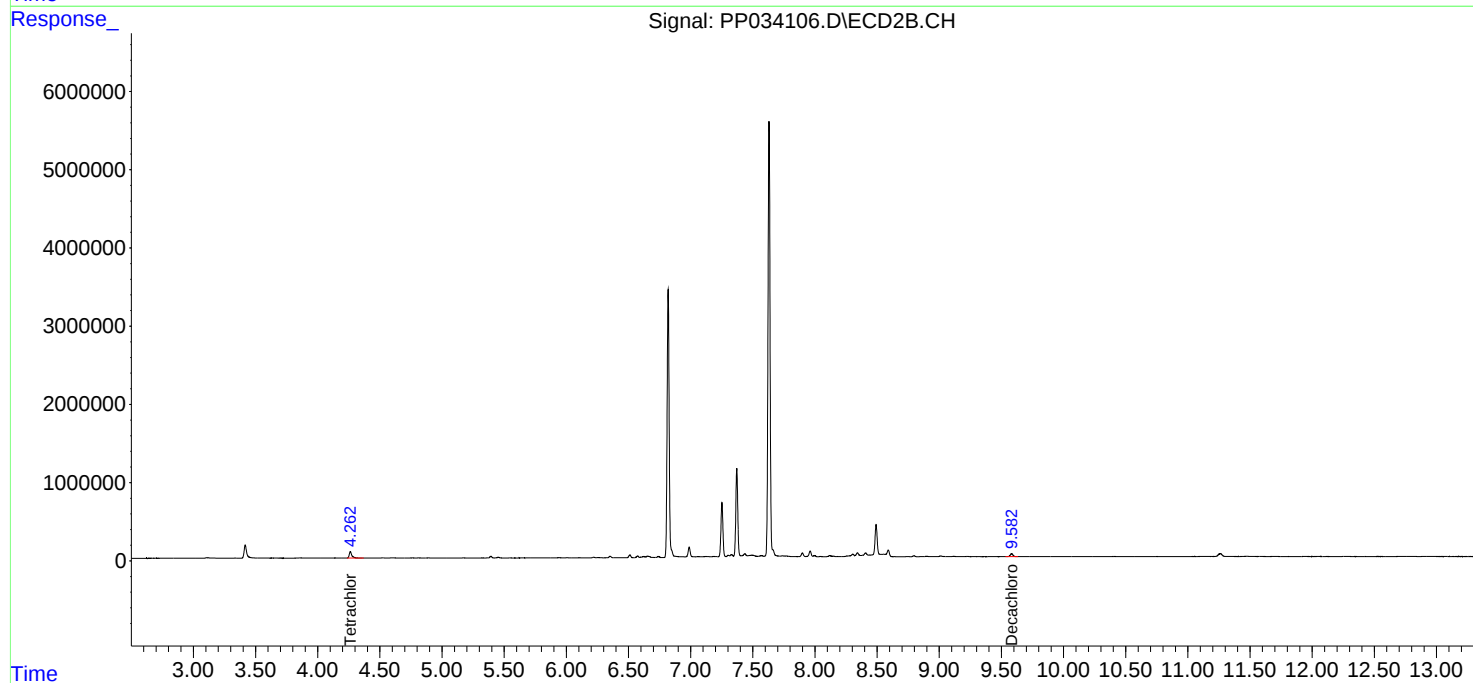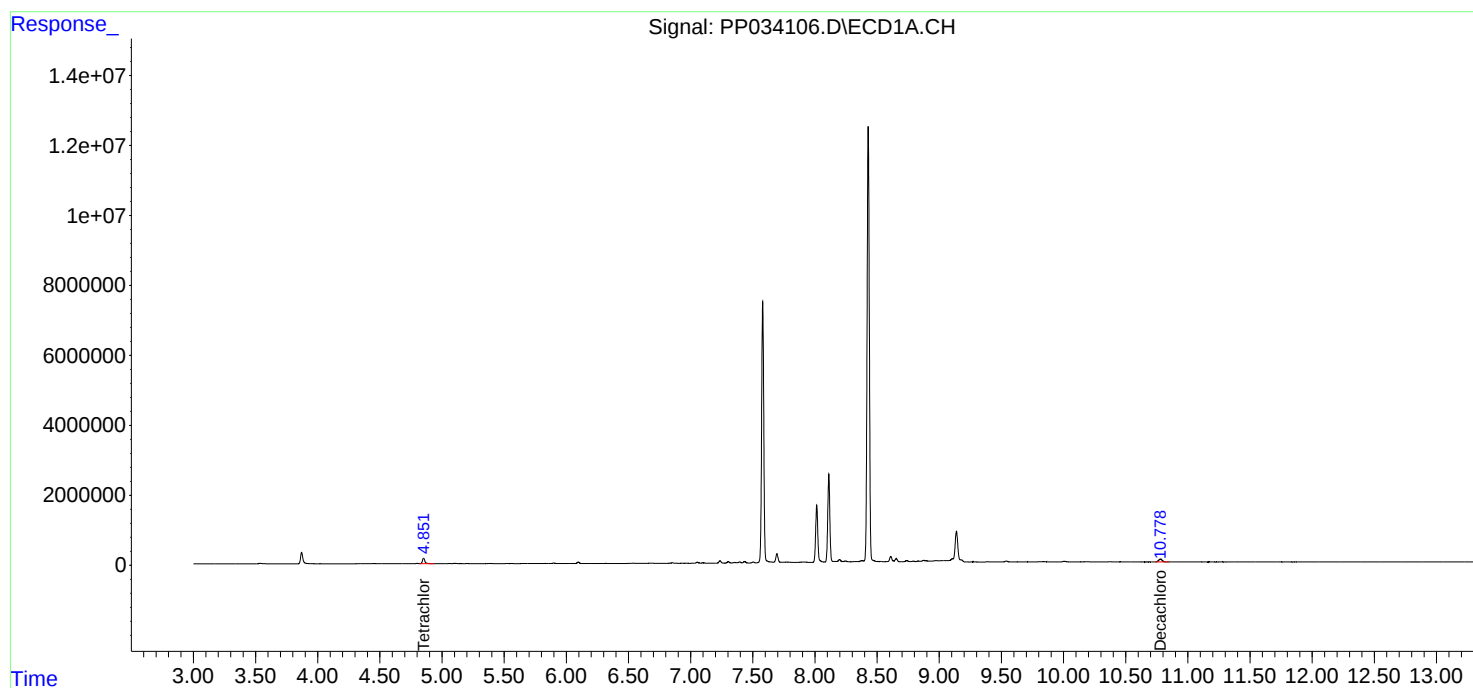

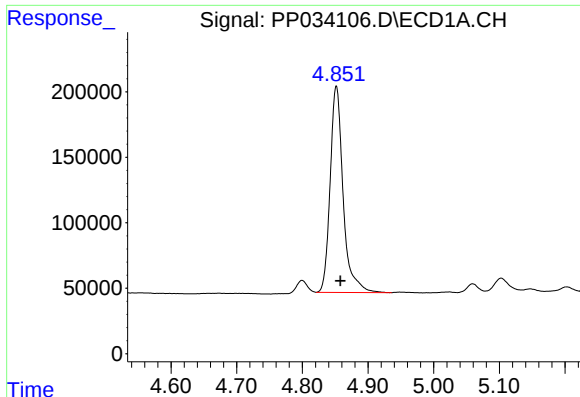


#1 Tetrachloro-m-xylene

R.T.: 4.852 min
Delta R.T.: -0.006 min
Response: 2158025
Conc: 24.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-3A-(1-1.5)


Manual Integrations
APPROVED

Ankita
3/18/2021 4:00:09 PM

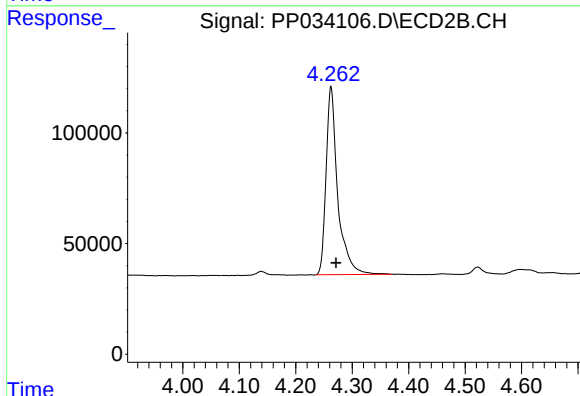


#1 Tetrachloro-m-xylene

R.T.: 4.263 min
Delta R.T.: -0.009 min
Response: 1219163
Conc: 30.01 ng/ml

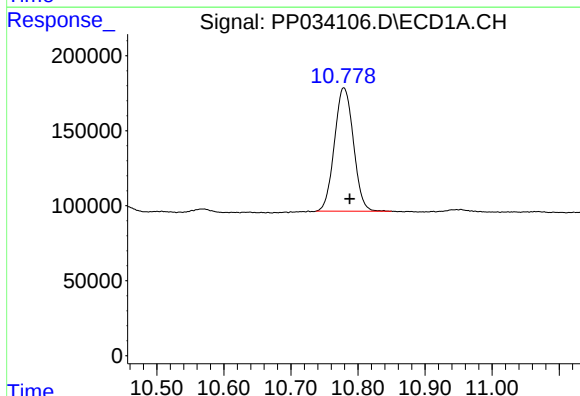

#2 Decachlorobiphenyl

R.T.: 10.779 min
Delta R.T.: -0.009 min
Response: 1617648
Conc: 19.15 ng/ml

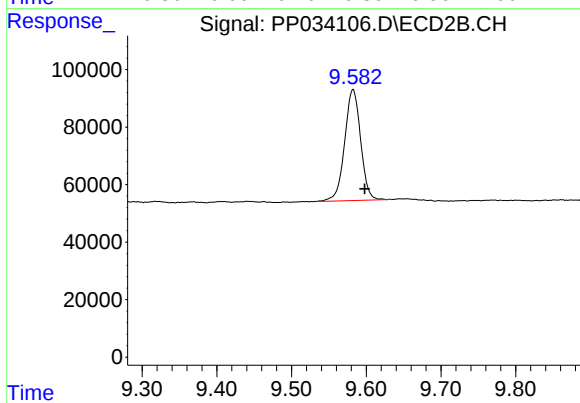

#2 Decachlorobiphenyl

R.T.: 9.582 min
Delta R.T.: -0.016 min
Response: 573751
Conc: 21.50 ng/ml m