

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031722\
 Data File : PP044833.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2022 00:22
 Operator : YP\AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/17/2022
 Supervised By :Ankita Jodhani 03/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 03:49:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 17 03:20:00 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.897	3.155	8444960	6953563	4.319m	4.693
2) SA Decachlor...	10.023	8.514	6577810	7506471	4.841	5.253
Target Compounds						
26) L6 AR-1254-1	6.074	5.151	3432201	4741732	51.690	54.833
27) L6 AR-1254-2	6.313	5.311	5080519	4054679	50.850	54.488
28) L6 AR-1254-3	6.714	5.743	5104808	5898784	49.910	51.339
29) L6 AR-1254-4	7.027	5.993	3674266	3825086	50.516	51.305
30) L6 AR-1254-5	7.489	6.443	3747155	5121328	48.448	49.735

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031722\
Data File : PP044833.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2022 00:22
Operator : YP\AJ
Sample : AR1254ICC050
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 03:49:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 17 03:20:00 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

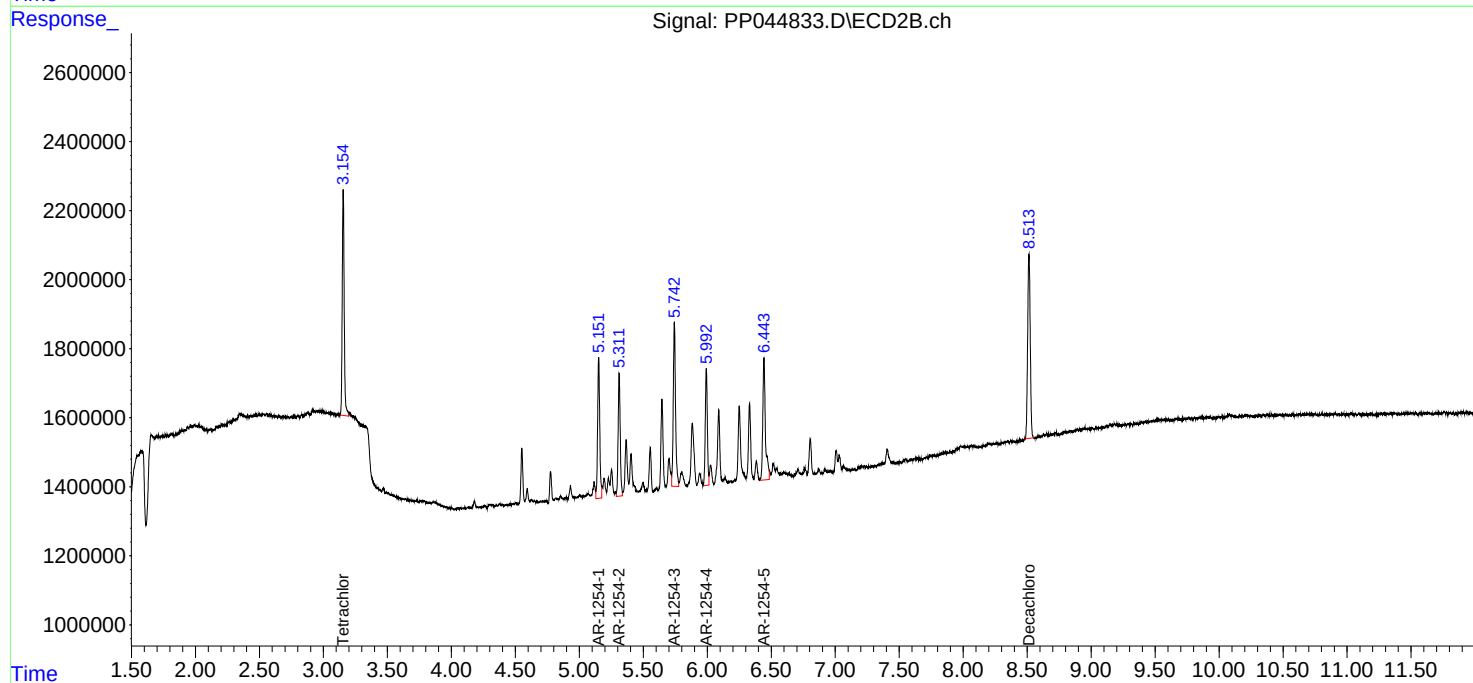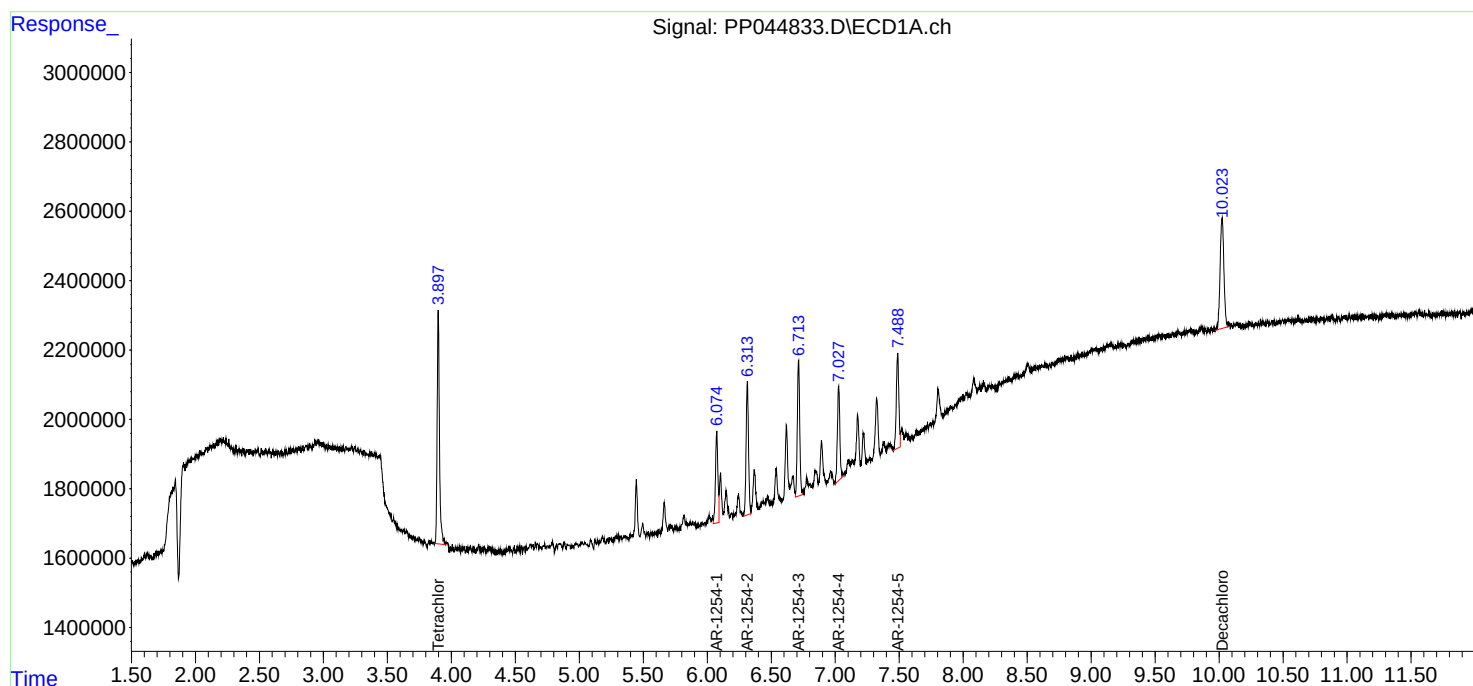

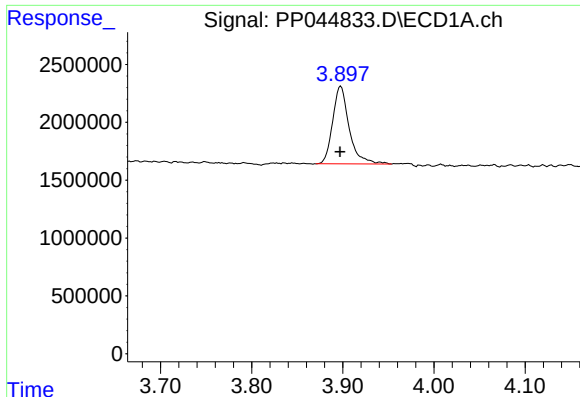


#1 Tetrachloro-m-xylene

R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 8444960
Conc: 4.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254IC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

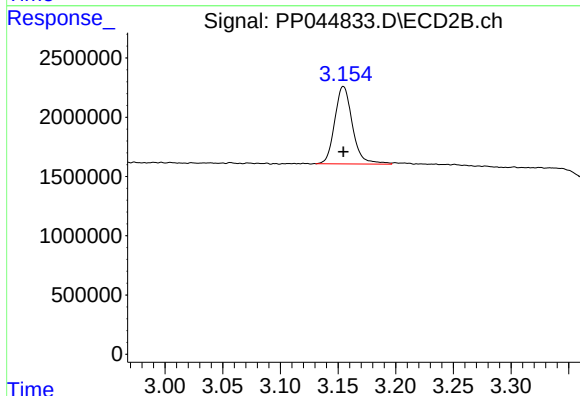


#1 Tetrachloro-m-xylene

R.T.: 3.155 min
Delta R.T.: 0.000 min
Response: 6953563
Conc: 4.69 ng/ml

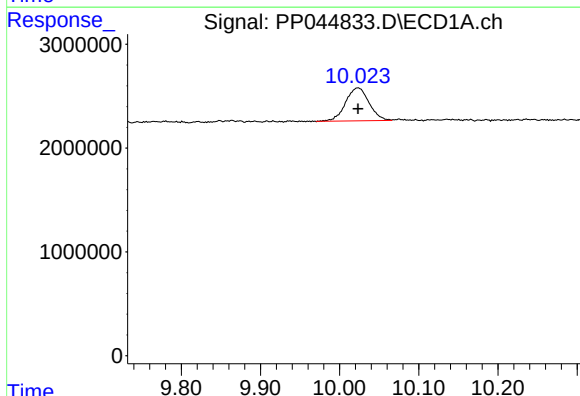


#2 Decachlorobiphenyl

R.T.: 10.023 min
Delta R.T.: 0.000 min
Response: 6577810
Conc: 4.84 ng/ml

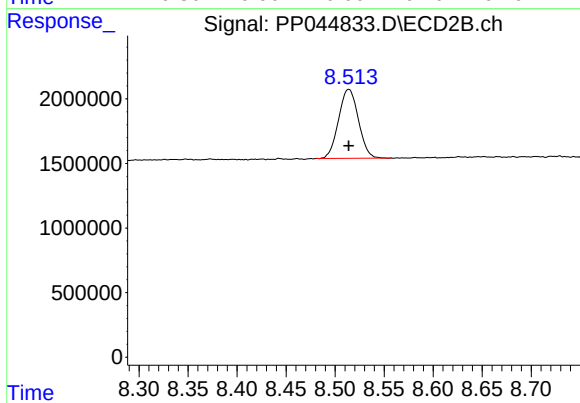

#2 Decachlorobiphenyl

R.T.: 8.514 min
Delta R.T.: 0.000 min
Response: 7506471
Conc: 5.25 ng/ml

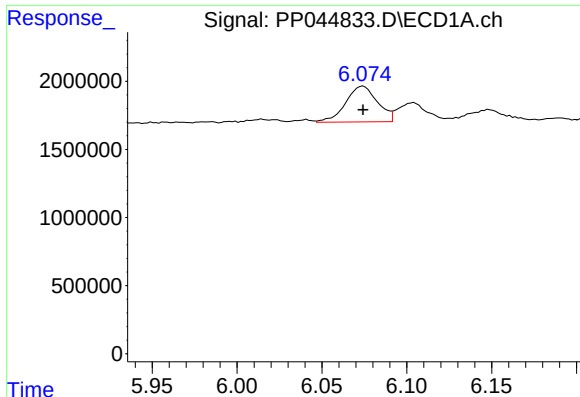


#26 AR-1254-1

R.T.: 6.074 min
Delta R.T.: 0.000 min
Response: 3432201
Conc: 51.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

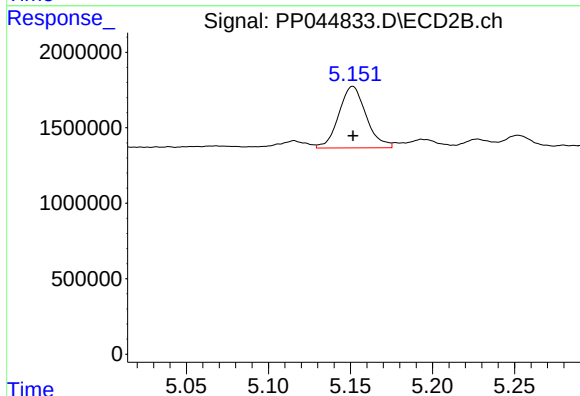


#26 AR-1254-1

R.T.: 5.151 min
Delta R.T.: 0.000 min
Response: 4741732
Conc: 54.83 ng/ml

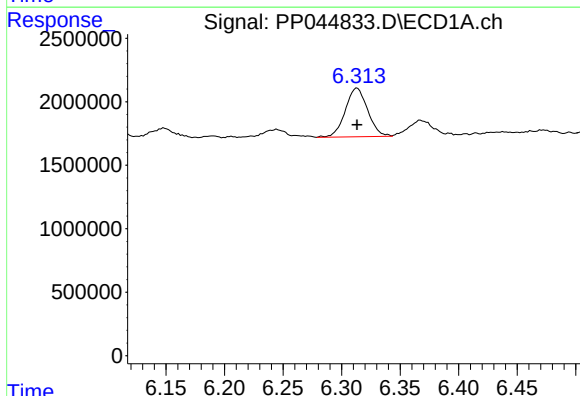


#27 AR-1254-2

R.T.: 6.313 min
Delta R.T.: 0.000 min
Response: 5080519
Conc: 50.85 ng/ml

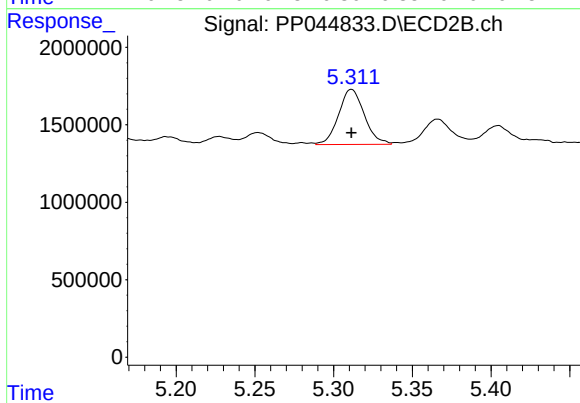

#27 AR-1254-2

R.T.: 5.311 min
Delta R.T.: 0.000 min
Response: 4054679
Conc: 54.49 ng/ml

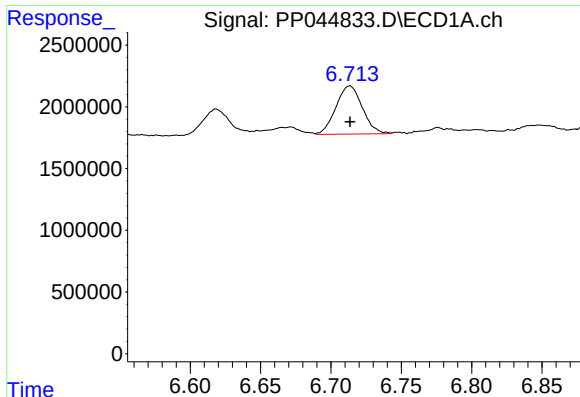


#28 AR-1254-3

R.T.: 6.714 min
Delta R.T.: 0.000 min
Response: 5104808
Conc: 49.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

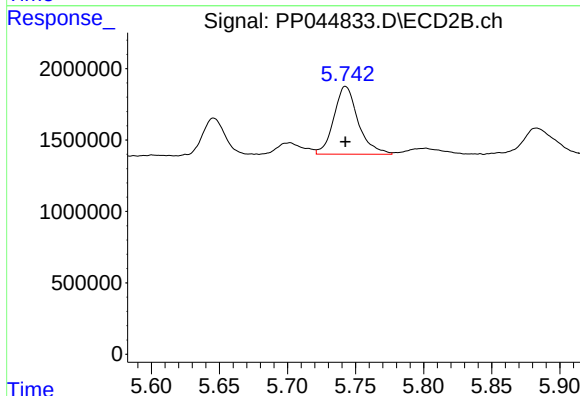


#28 AR-1254-3

R.T.: 5.743 min
Delta R.T.: 0.000 min
Response: 5898784
Conc: 51.34 ng/ml

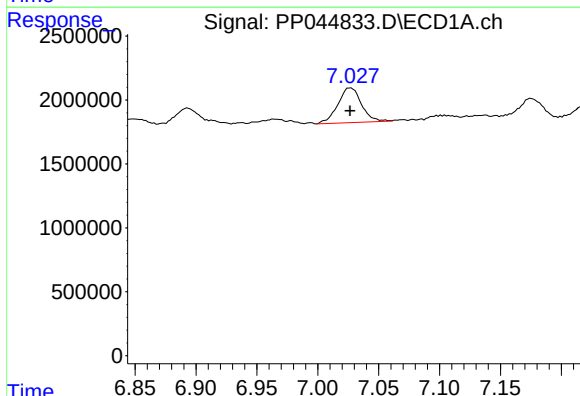


#29 AR-1254-4

R.T.: 7.027 min
Delta R.T.: 0.000 min
Response: 3674266
Conc: 50.52 ng/ml

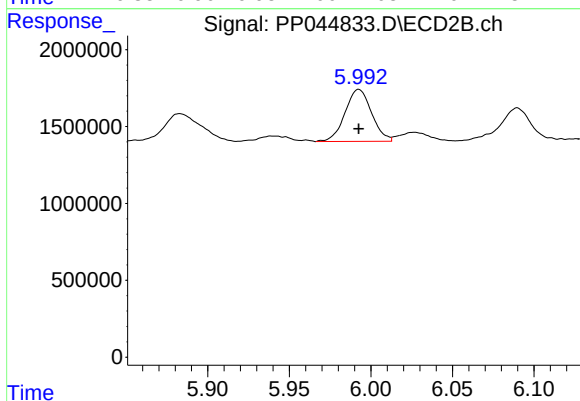

#29 AR-1254-4

R.T.: 5.993 min
Delta R.T.: 0.000 min
Response: 3825086
Conc: 51.31 ng/ml

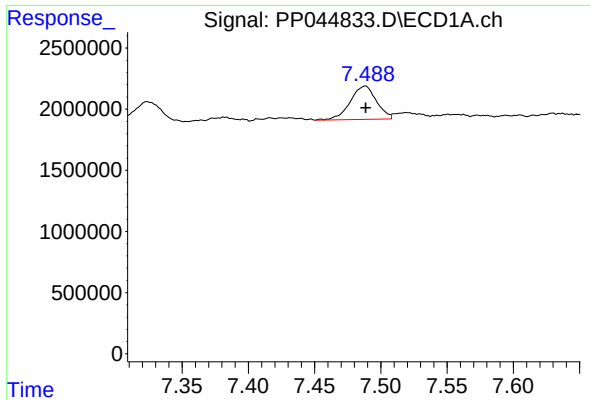


#30 AR-1254-5

R.T.: 7.489 min
Delta R.T.: 0.000 min
Response: 3747155
Conc: 48.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

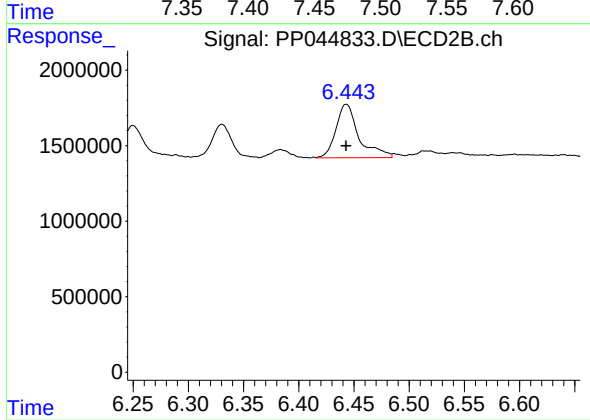

#30 AR-1254-5

R.T.: 6.443 min
Delta R.T.: 0.000 min
Response: 5121328
Conc: 49.74 ng/ml