

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031819\
 Data File : PP029364.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Mar 2019 15:09
 Operator : EI\MA
 Sample : I.BLK
 Misc : hexane
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 01:49:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 22 02:24:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.931	12.126	14022688	16825925	466.546	443.342
Target Compounds							
5) T	DICAMBA	0.000	12.405	0	435609	N.D.	3.403 #
13) T	2,4-DB	16.230	0.000	90618	0	4.744	N.D. #
15) T	Picloram	17.462	0.000	113311	0	0.408	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031819\
Data File : PP029364.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Mar 2019 15:09
Operator : EI\MA
Sample : I.BLK
Misc : hexane
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 01:49:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
Quant Title : 8080.M
QLast Update : Fri Feb 22 02:24:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

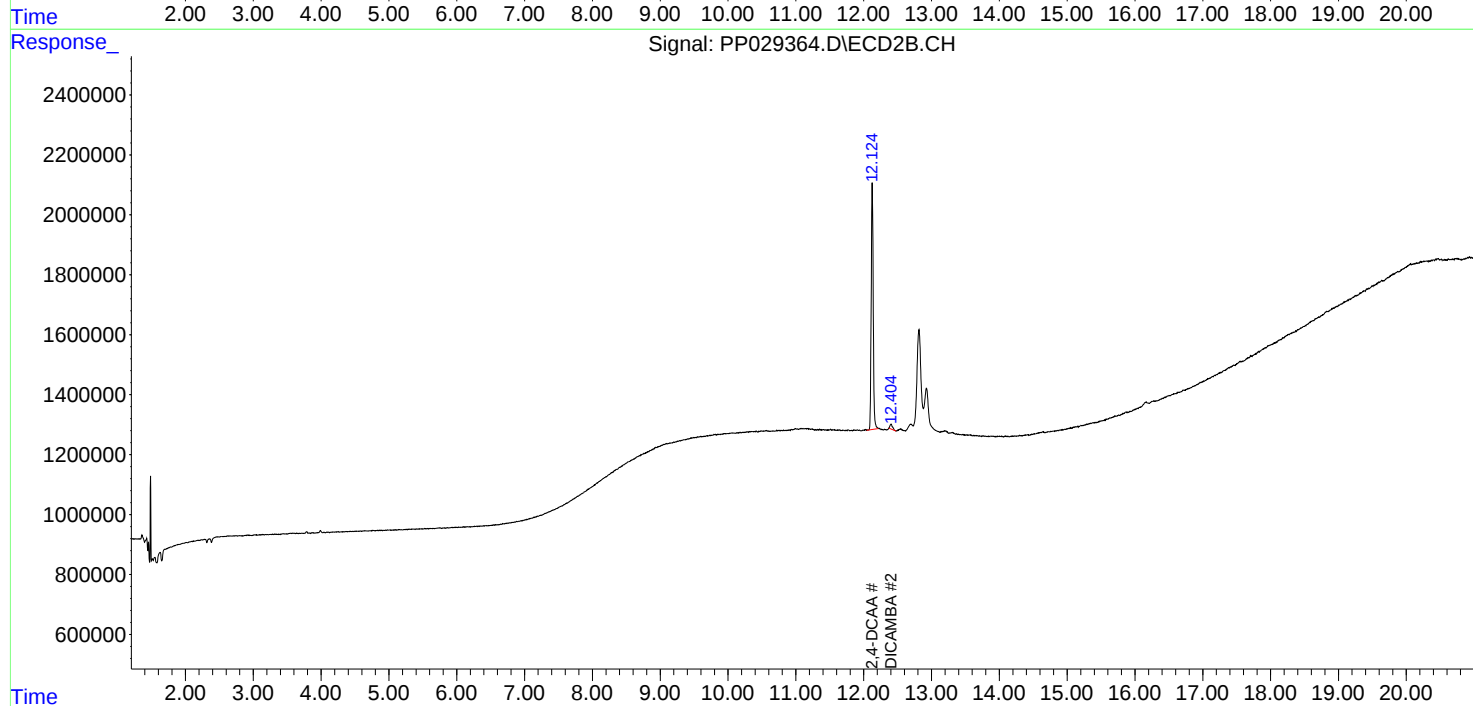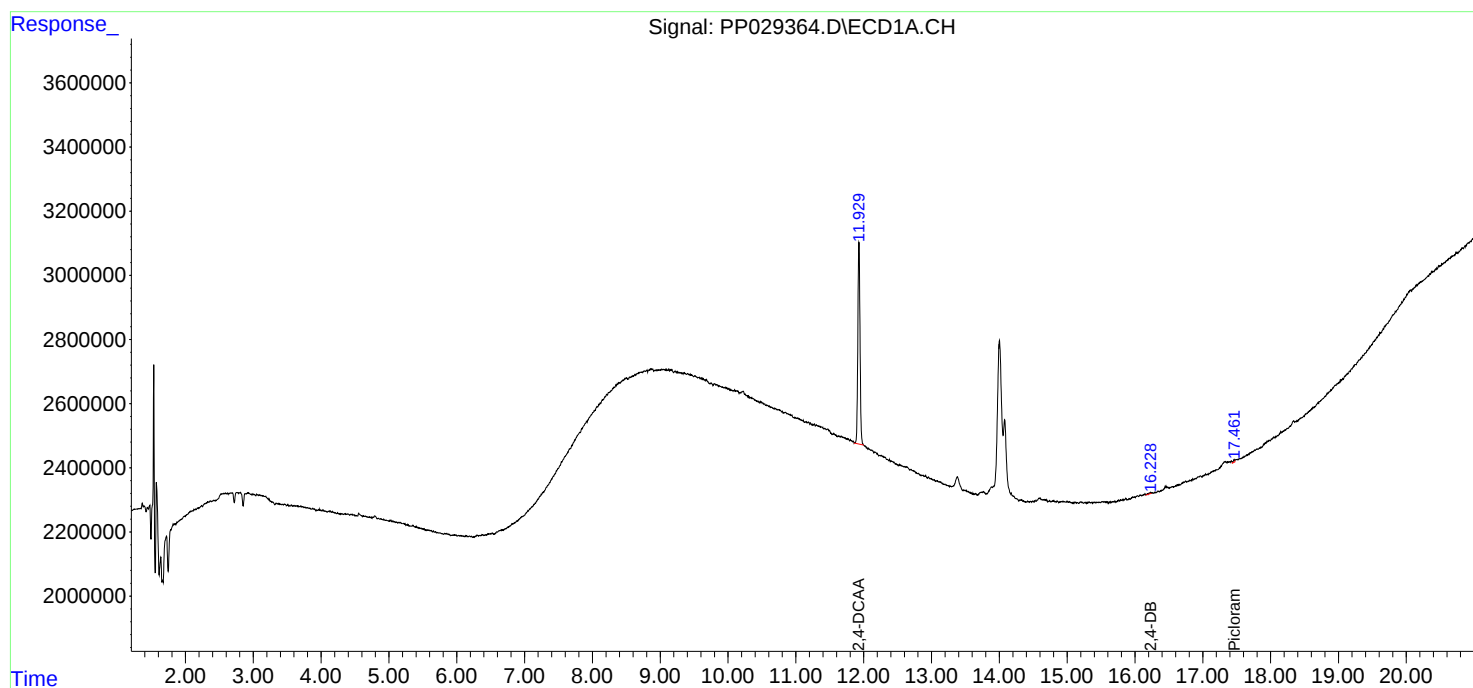


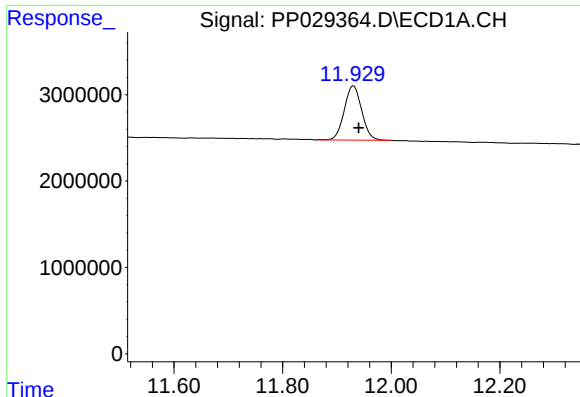

#4 2,4-DCAA


R.T.: 11.931 min
Delta R.T.: -0.010 min
Response: 14022688
Conc: 466.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

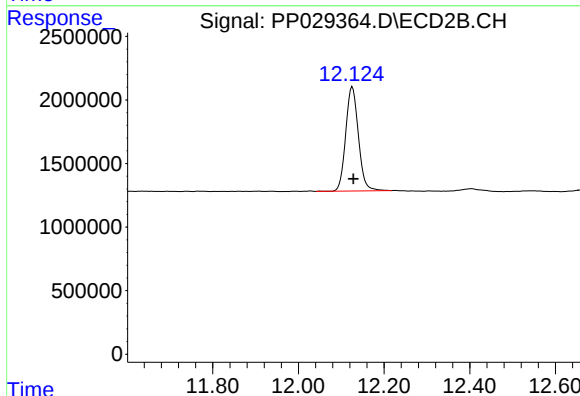


#4 2,4-DCAA

R.T.: 12.126 min
Delta R.T.: -0.003 min
Response: 16825925
Conc: 443.34 ng/ml

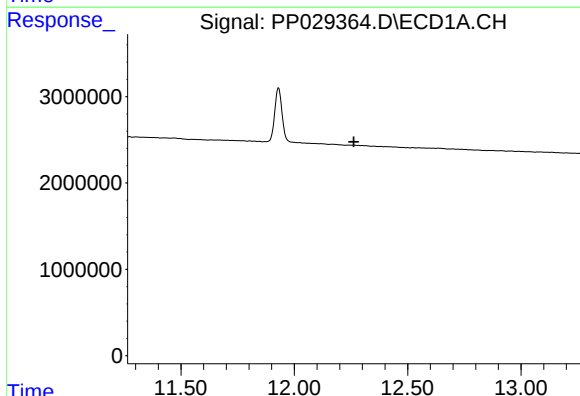


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 12.262 min
Response: 0
Conc: N.D.

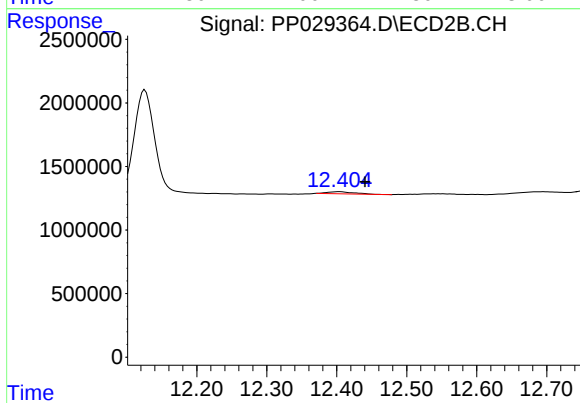

#5 DICAMBA


R.T.: 12.405 min
Delta R.T.: -0.036 min
Response: 435609
Conc: 3.40 ng/ml

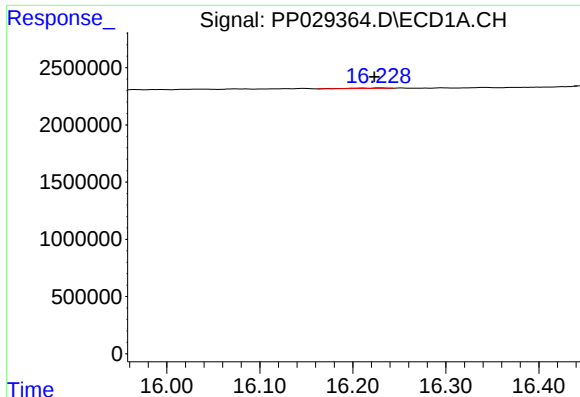

#13 2,4-DB


R.T.: 16.230 min
Delta R.T.: 0.007 min
Response: 90618
Conc: 4.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

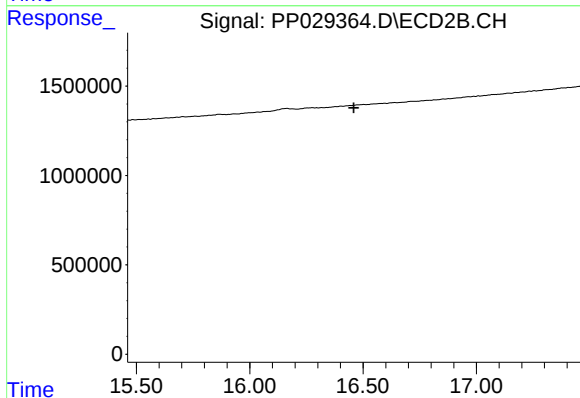


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 16.460 min
Response: 0
Conc: N.D.

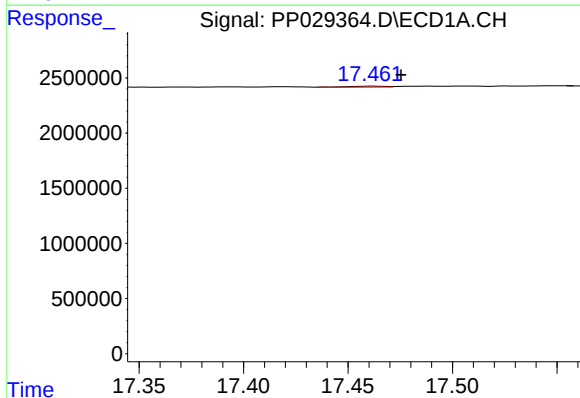

#15 Picloram

R.T.: 17.462 min
Delta R.T.: -0.014 min
Response: 113311
Conc: 0.41 ng/ml

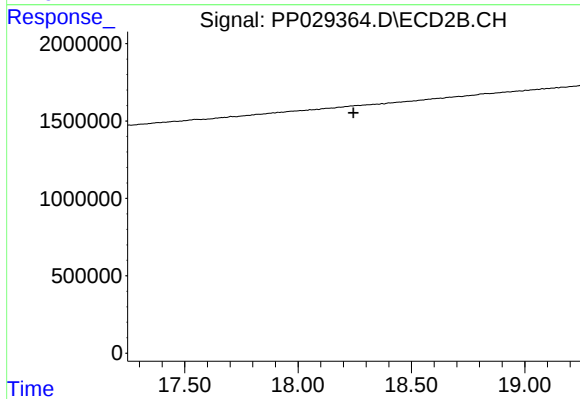

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 18.245 min
Response: 0
Conc: N.D.