

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031819\
 Data File : PP029367.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Mar 2019 16:26
 Operator : EI\MA
 Sample : K1691-12
 Misc : hexane
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CL-01-031519-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 01:49:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 22 02:24:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.930	12.125	13720834	18010723	456.503	474.559
Target Compounds							
1) T	Dalapon	0.000	2.982	0	41406	N.D.	0.800 #
8) T	DICHLORPROP	0.000	13.559	0	849694	N.D.	25.132 #
11) T	2,4,5-TP ...	0.000	15.194	0	2278923	N.D.	11.204 #
12) T	2,4,5-T	0.000	15.858	0	1673362	N.D.	10.107 #
13) T	2,4-DB	16.207	0.000	577886	0	30.252	N.D. #
14) T	DINOSEB	17.694	16.787	87575	242038	0.601	1.847 #
15) T	Picloram	17.476	18.289	187381	2780841	0.674	12.358 #
16) T	DCPA	0.000	18.079	0	2517830	N.D.	10.834 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031819\
Data File : PP029367.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Mar 2019 16:26
Operator : EI\MA
Sample : K1691-12
Misc : hexane
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
CL-01-031519-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 01:49:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
Quant Title : 8080.M
QLast Update : Fri Feb 22 02:24:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

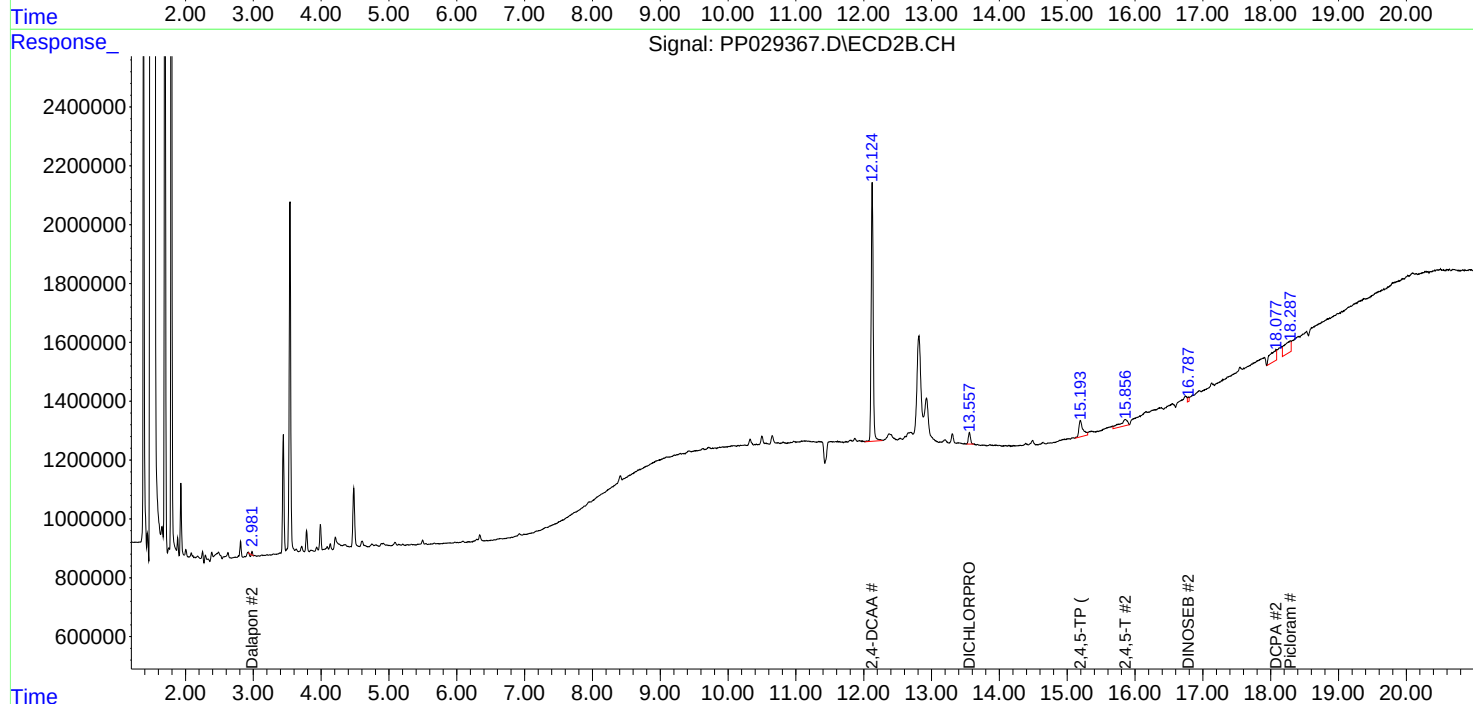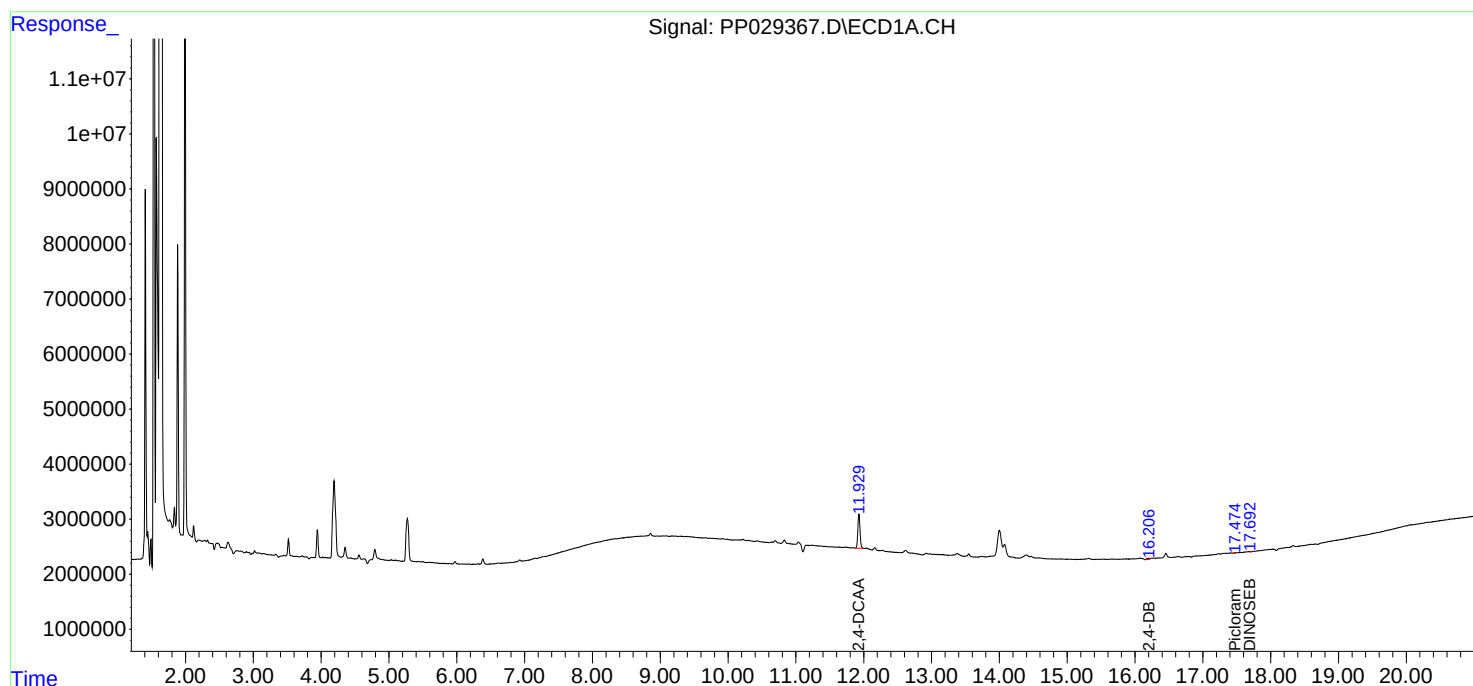


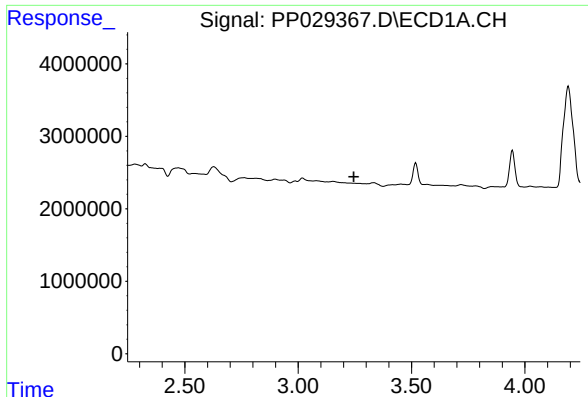

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.246 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CL-01-031519-B

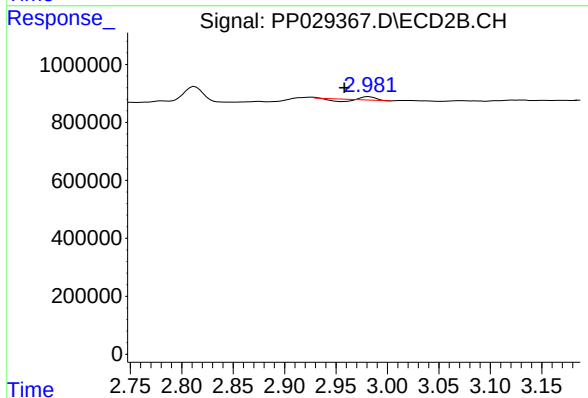


#1 Dalapon

R.T.: 2.982 min
Delta R.T.: 0.024 min
Response: 41406
Conc: 0.80 ng/ml

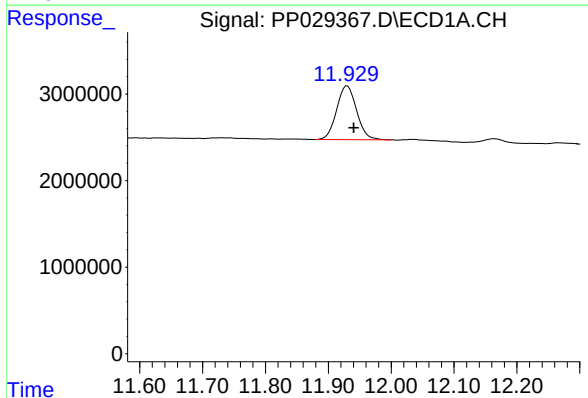


#4 2,4-DCAA

R.T.: 11.930 min
Delta R.T.: -0.010 min
Response: 13720834
Conc: 456.50 ng/ml

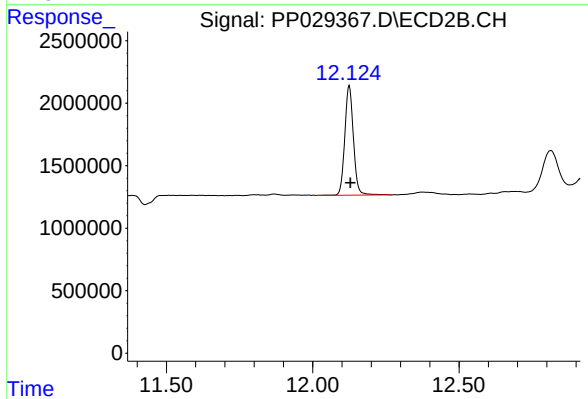

#4 2,4-DCAA


R.T.: 12.125 min
Delta R.T.: -0.004 min
Response: 18010723
Conc: 474.56 ng/ml

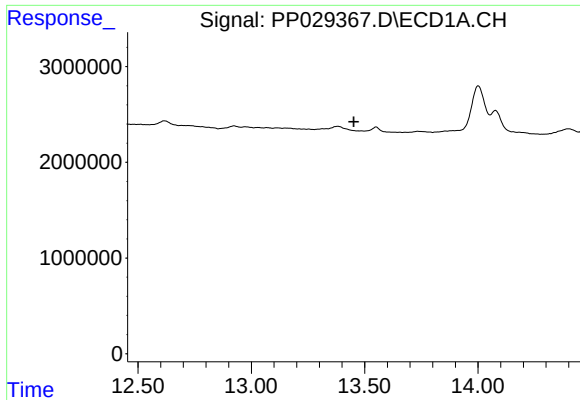

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.452 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CL-01-031519-B

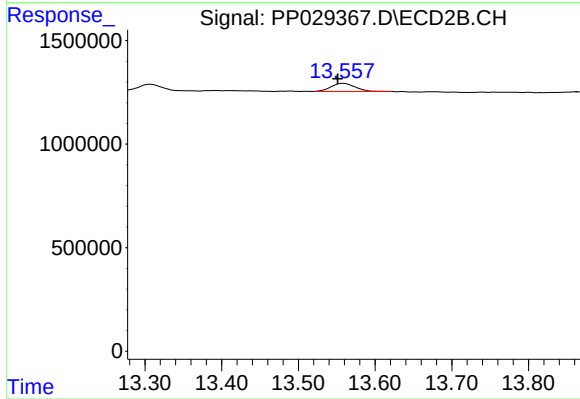


#8 DICHLORPROP

R.T.: 13.559 min
Delta R.T.: 0.007 min
Response: 849694
Conc: 25.13 ng/ml

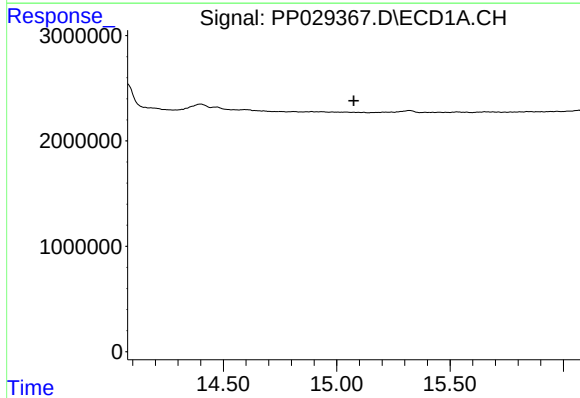


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 15.075 min
Response: 0
Conc: N.D.

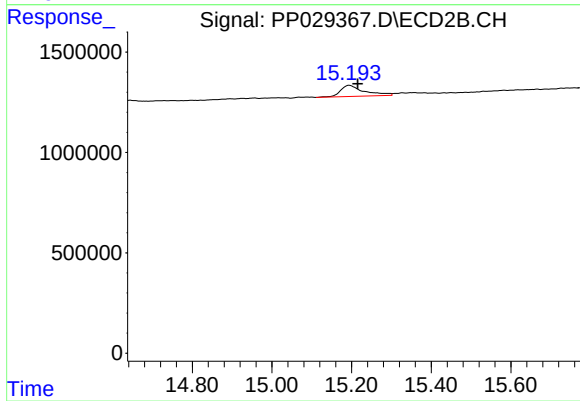

#11 2,4,5-TP (SILVEX)


R.T.: 15.194 min
Delta R.T.: -0.021 min
Response: 2278923
Conc: 11.20 ng/ml

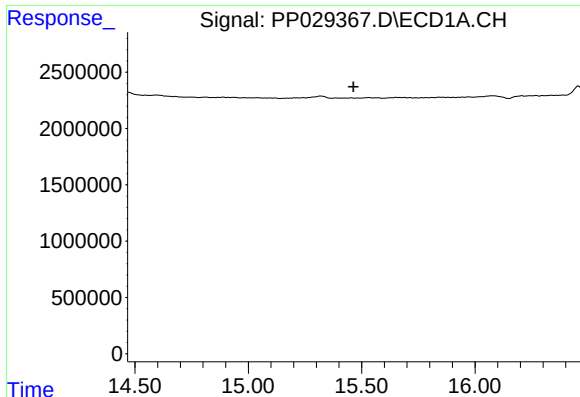

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.464 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CL-01-031519-B

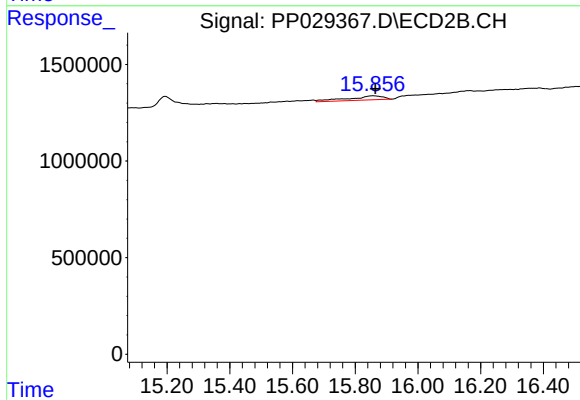


#12 2,4,5-T

R.T.: 15.858 min
Delta R.T.: -0.007 min
Response: 1673362
Conc: 10.11 ng/ml

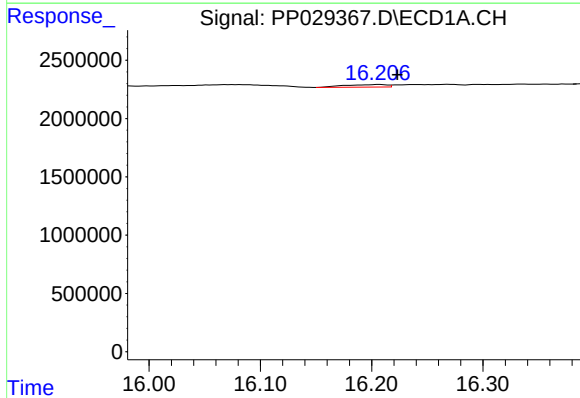


#13 2,4-DB

R.T.: 16.207 min
Delta R.T.: -0.016 min
Response: 577886
Conc: 30.25 ng/ml

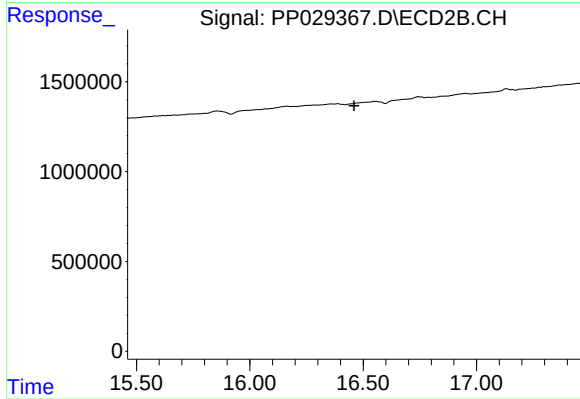

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 16.460 min
Response: 0
Conc: N.D.

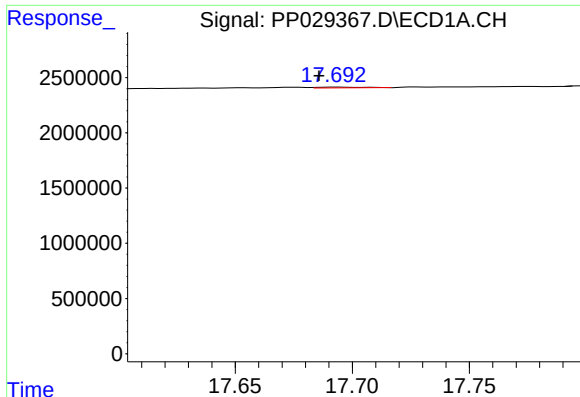

#14 DINOSEB


R.T.: 17.694 min
Delta R.T.: 0.008 min
Response: 87575
Conc: 0.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
CL-01-031519-B

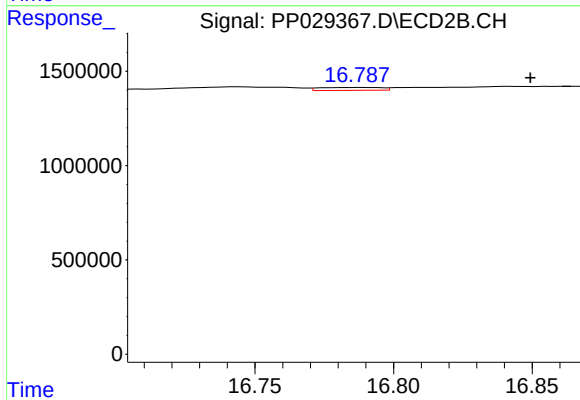


#14 DINOSEB

R.T.: 16.787 min
Delta R.T.: -0.062 min
Response: 242038
Conc: 1.85 ng/ml

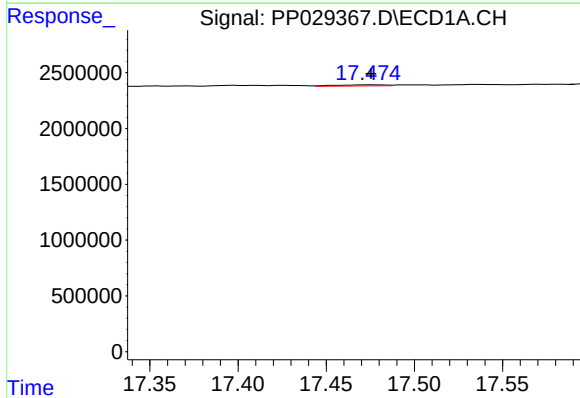


#15 Picloram

R.T.: 17.476 min
Delta R.T.: 0.000 min
Response: 187381
Conc: 0.67 ng/ml

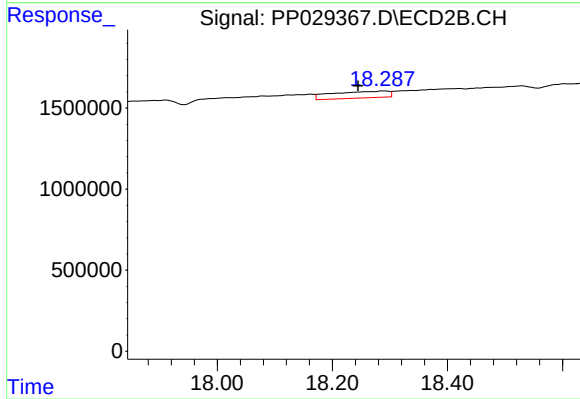

#15 Picloram


R.T.: 18.289 min
Delta R.T.: 0.045 min
Response: 2780841
Conc: 12.36 ng/ml

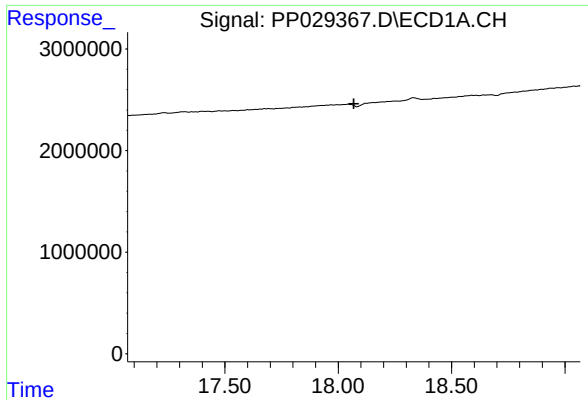

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 18.069 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CL-01-031519-B

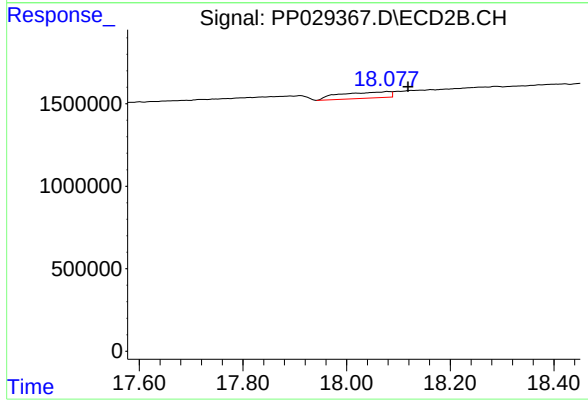

#16 DCPA

R.T.: 18.079 min
Delta R.T.: -0.039 min
Response: 2517830
Conc: 10.83 ng/ml