

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031819\
 Data File : PP029382.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Mar 2019 22:47
 Operator : EI\MA
 Sample : K1958-04
 Misc : hexane
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 01:51:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 22 02:24:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.929	12.125	15468870	19893327	514.662	524.164
Target Compounds							
8) T	DICHLORPROP	0.000	13.560	0	454171	N.D.	13.434 #
12) T	2,4,5-T	0.000	15.849	0	1266423	N.D.	7.649 #
15) T	Picloram	17.480	18.209	505156	4905795	1.817	21.801 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031819\
Data File : PP029382.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Mar 2019 22:47
Operator : EI\MA
Sample : K1958-04
Misc : hexane
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
TP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 01:51:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
Quant Title : 8080.M
QLast Update : Fri Feb 22 02:24:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

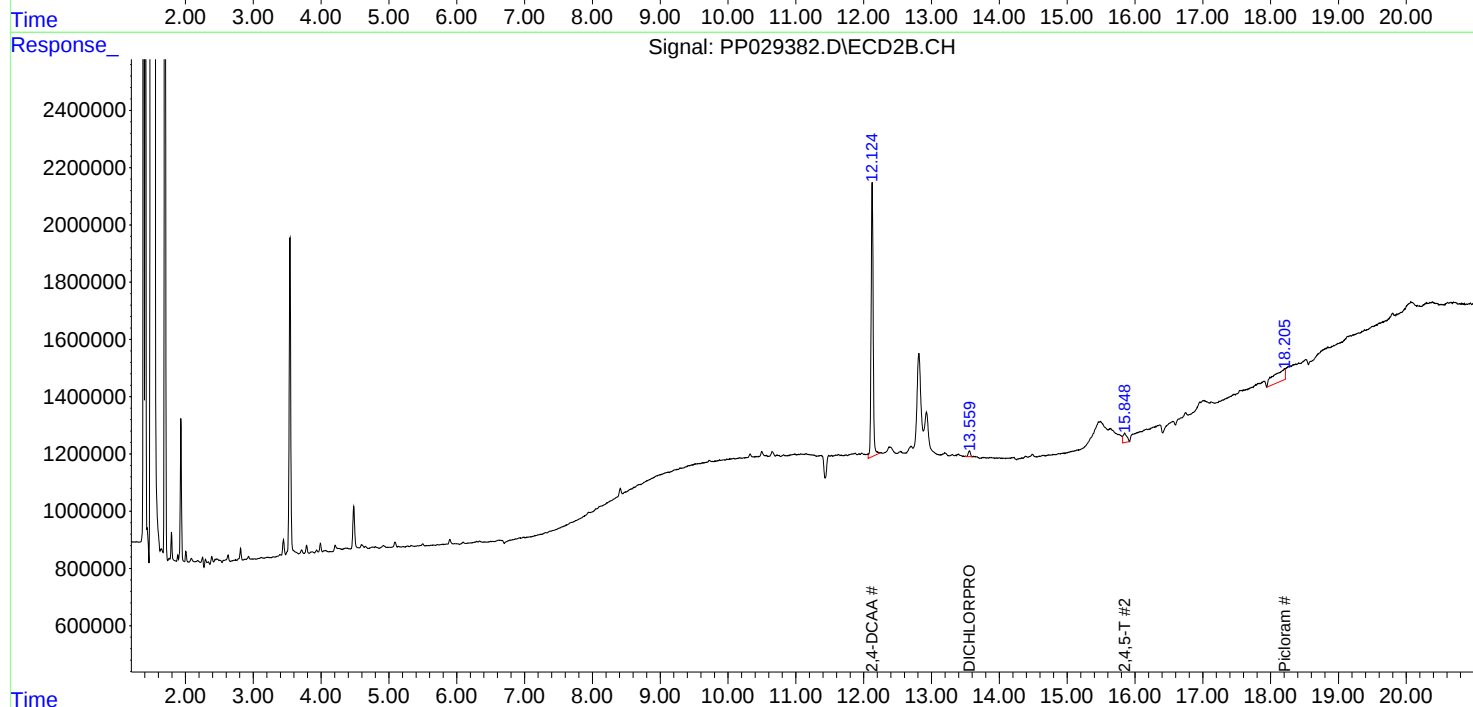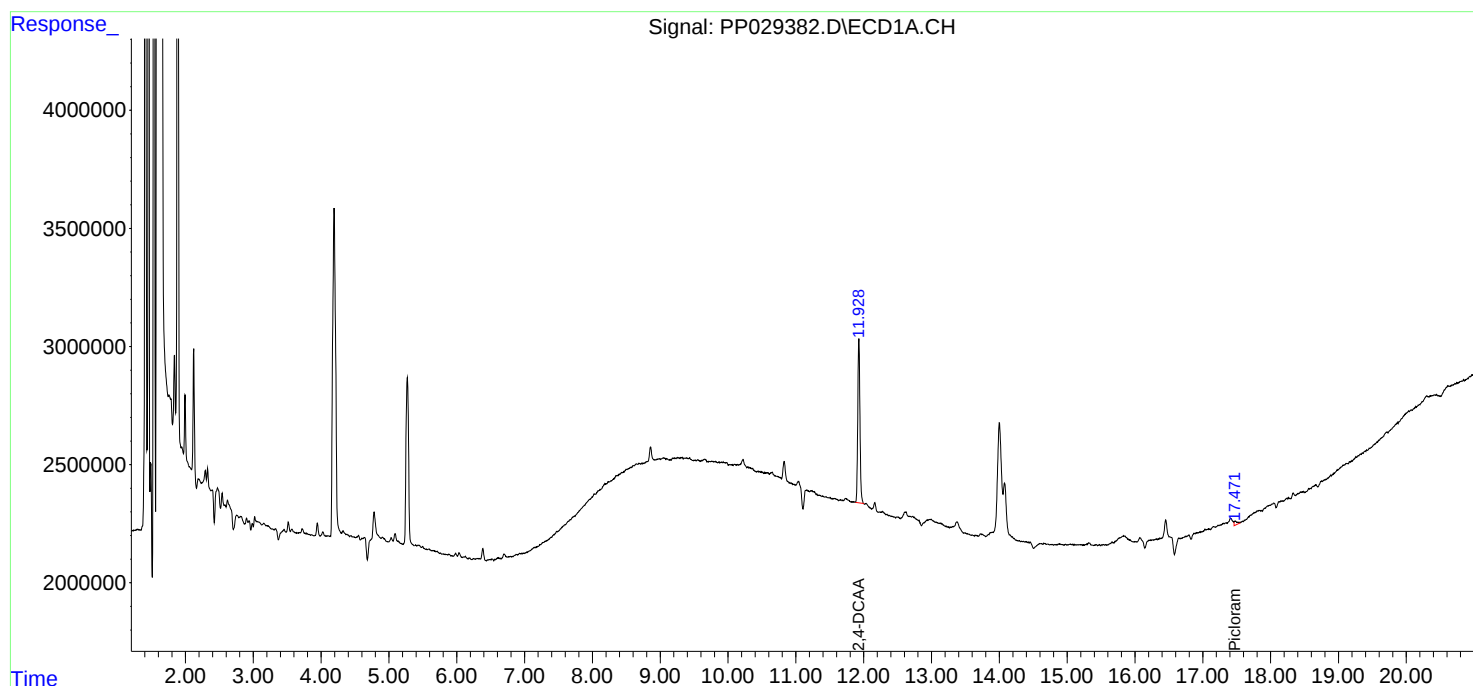


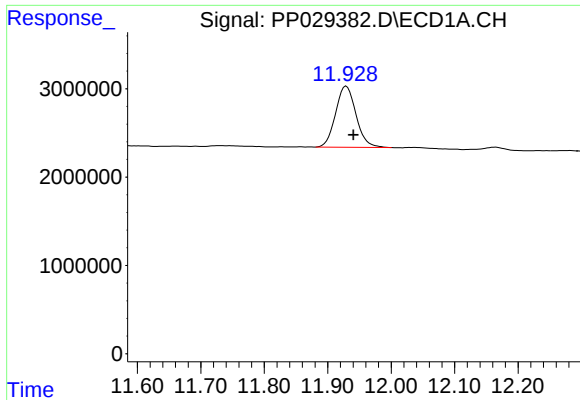

#4 2,4-DCAA


R.T.: 11.929 min
Delta R.T.: -0.011 min
Response: 15468870
Conc: 514.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-2

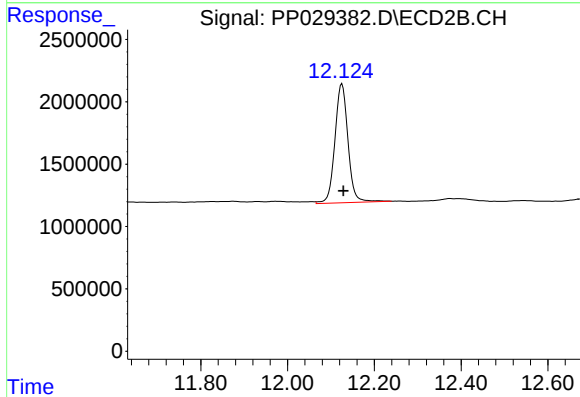


#4 2,4-DCAA

R.T.: 12.125 min
Delta R.T.: -0.003 min
Response: 19893327
Conc: 524.16 ng/ml

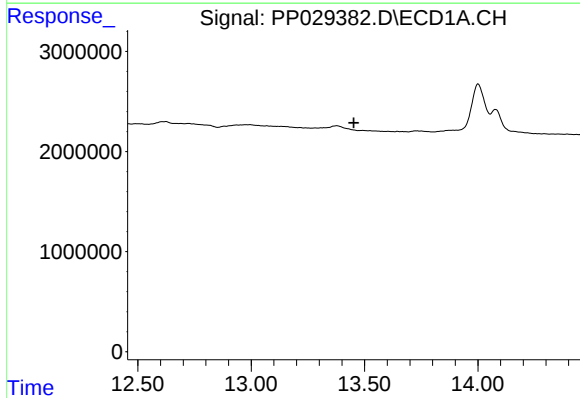


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.452 min
Response: 0
Conc: N.D.

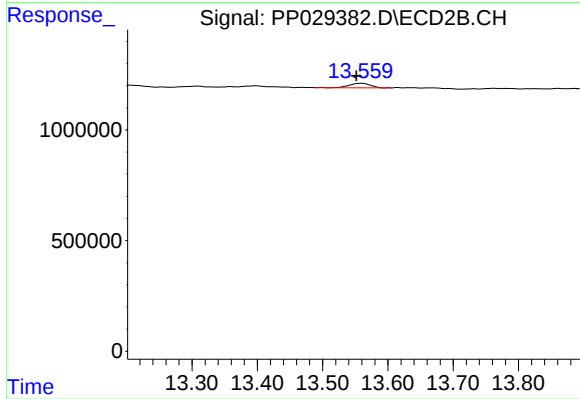

#8 DICHLORPROP


R.T.: 13.560 min
Delta R.T.: 0.009 min
Response: 454171
Conc: 13.43 ng/ml

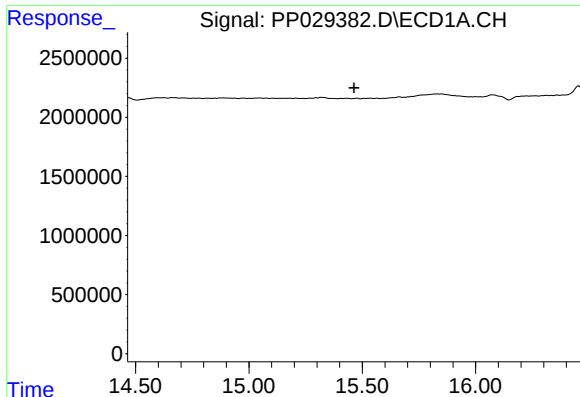

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.464 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TP-2

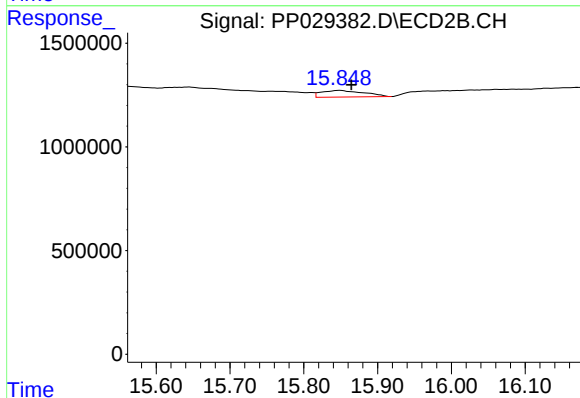


#12 2,4,5-T

R.T.: 15.849 min
Delta R.T.: -0.015 min
Response: 1266423
Conc: 7.65 ng/ml

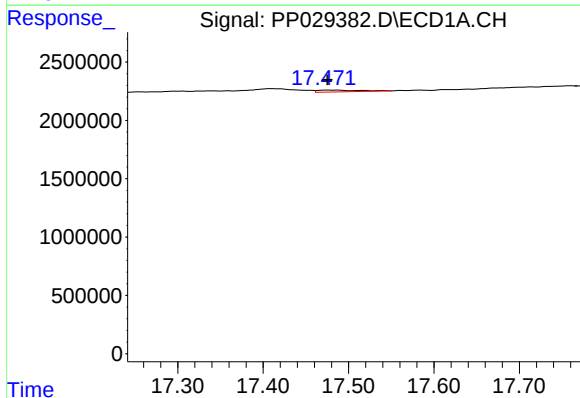

#15 Picloram

R.T.: 17.480 min
Delta R.T.: 0.004 min
Response: 505156
Conc: 1.82 ng/ml

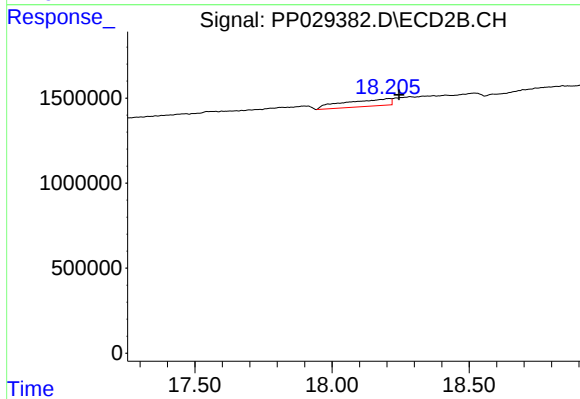

#15 Picloram

R.T.: 18.209 min
Delta R.T.: -0.036 min
Response: 4905795
Conc: 21.80 ng/ml