

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031821\
 Data File : PP034145.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Mar 2021 23:26
 Operator : DD\AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1268ICC050

Manual Integrations
 APPROVED

Ankita
 3/22/2021 2:39:22 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 05:17:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 19 05:08:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.851	4.262	431489	234058	5.189	5.377
2) SA Decachlor...	10.783	9.582	673632	234949	5.257	5.478
Target Compounds						
41) L9 AR-1268-1	9.328	8.461	519007	217439	52.344m	54.685m
42) L9 AR-1268-2	9.422	8.525	476384	196875	51.057	53.051m
43) L9 AR-1268-3	9.638	8.734	444312	187044	50.607m	54.987m
44) L9 AR-1268-4	10.065	9.022	147252	64378	46.628m	54.671m
45) L9 AR-1268-5	10.462	9.321	1320139	474004	47.631m	50.840

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031821\
Data File : PP034145.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Mar 2021 23:26
Operator : DD\AJ
Sample : AR1268ICC050
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Ankita
3/22/2021 2:39:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 05:17:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 19 05:08:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

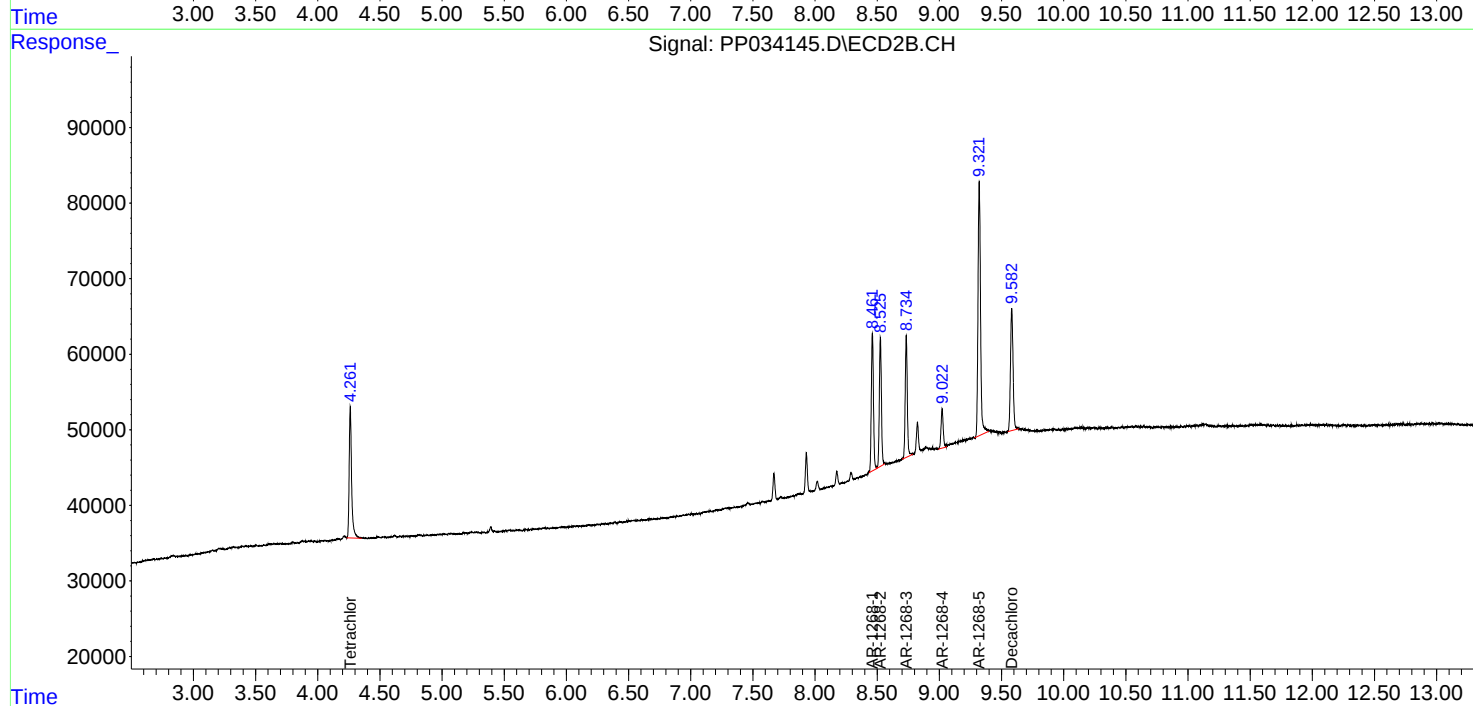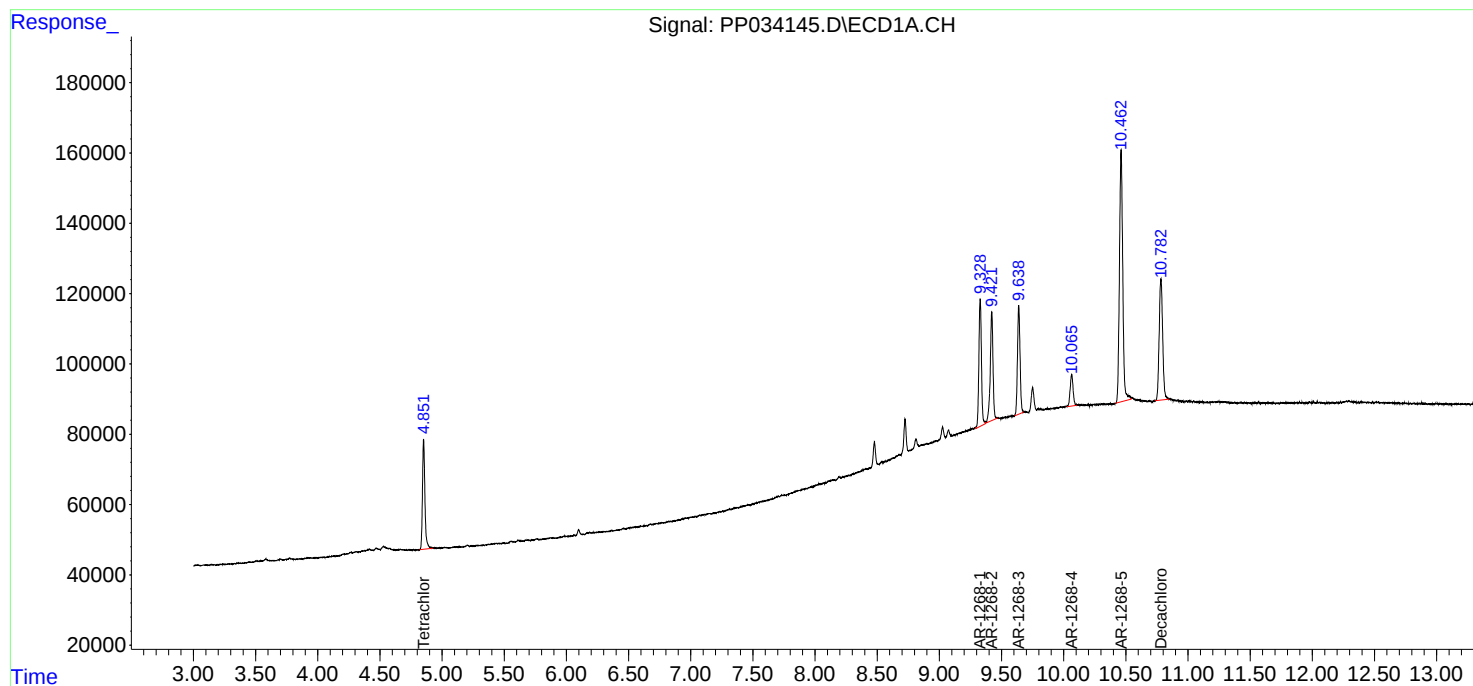

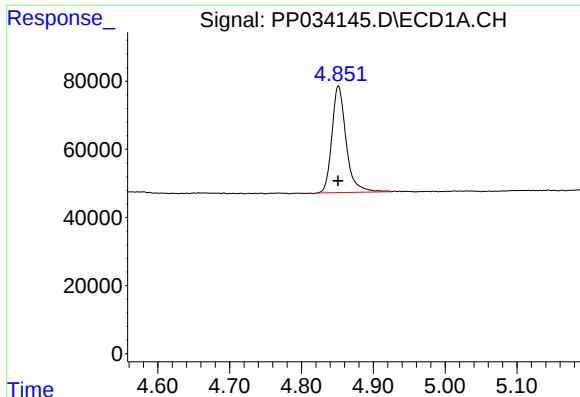


#1 Tetrachloro-m-xylene

R.T.: 4.851 min
Delta R.T.: 0.000 min
Response: 431489
Conc: 5.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Ankita
3/22/2021 2:39:22 PM

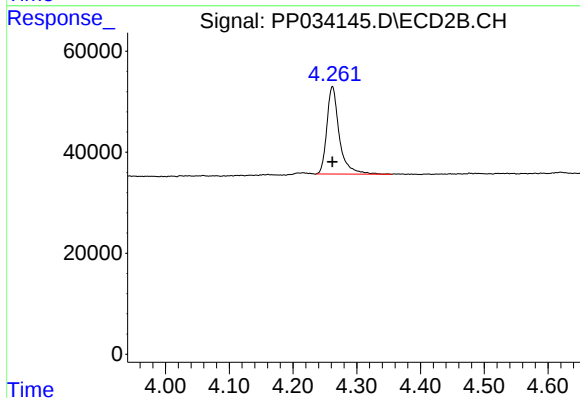


#1 Tetrachloro-m-xylene

R.T.: 4.262 min
Delta R.T.: 0.000 min
Response: 234058
Conc: 5.38 ng/ml

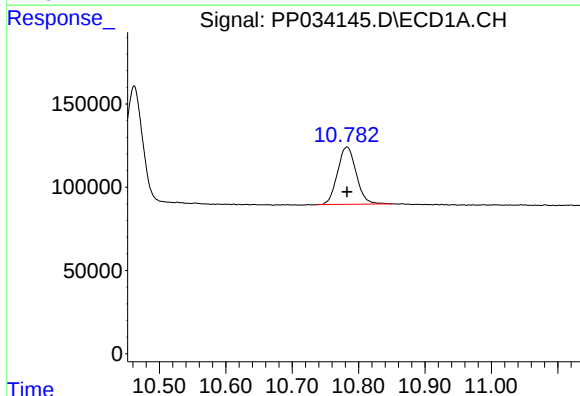


#2 Decachlorobiphenyl

R.T.: 10.783 min
Delta R.T.: 0.000 min
Response: 673632
Conc: 5.26 ng/ml

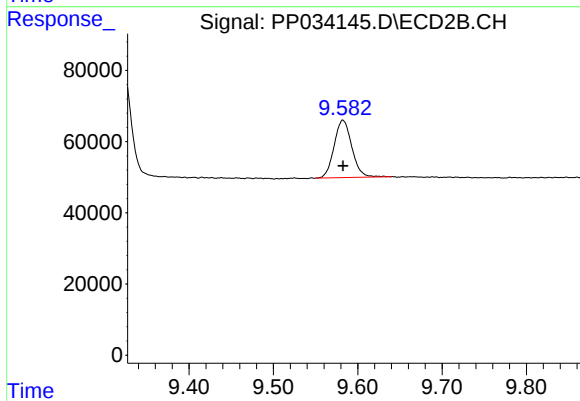

#2 Decachlorobiphenyl

R.T.: 9.582 min
Delta R.T.: 0.000 min
Response: 234949
Conc: 5.48 ng/ml

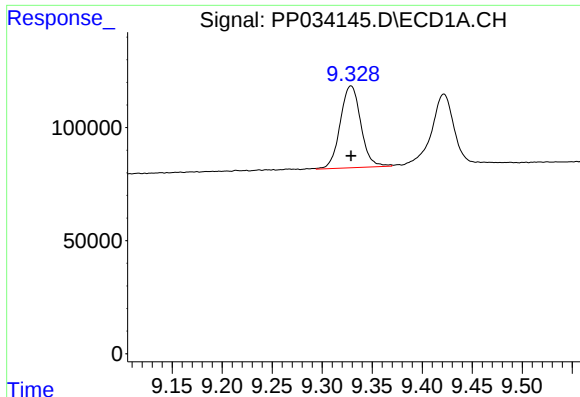


#41 AR-1268-1

R.T.: 9.328 min
Delta R.T.: 0.000 min
Response: 519007
Conc: 52.34 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Ankita
3/22/2021 2:39:22 PM

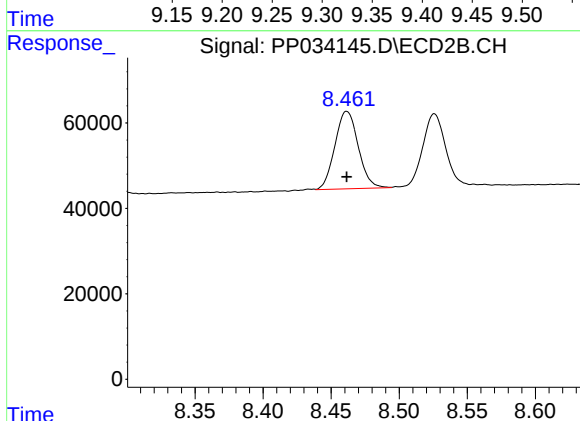


#41 AR-1268-1

R.T.: 8.461 min
Delta R.T.: 0.000 min
Response: 217439
Conc: 54.68 ng/ml m

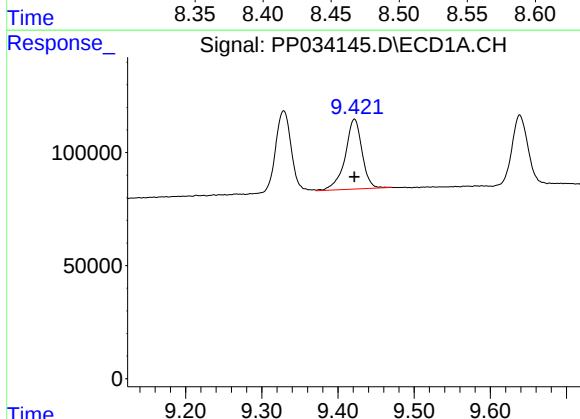


#42 AR-1268-2

R.T.: 9.422 min
Delta R.T.: 0.000 min
Response: 476384
Conc: 51.06 ng/ml

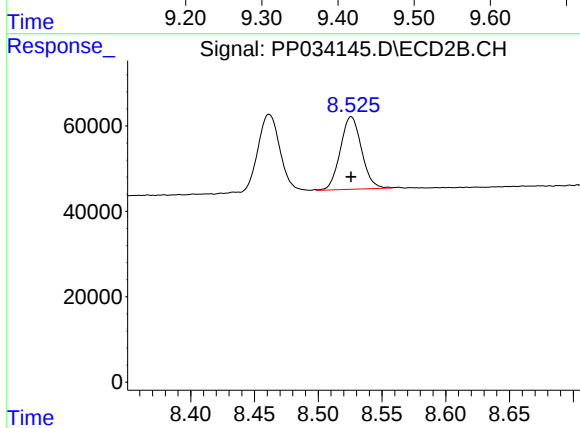

#42 AR-1268-2

R.T.: 8.525 min
Delta R.T.: 0.000 min
Response: 196875
Conc: 53.05 ng/ml m

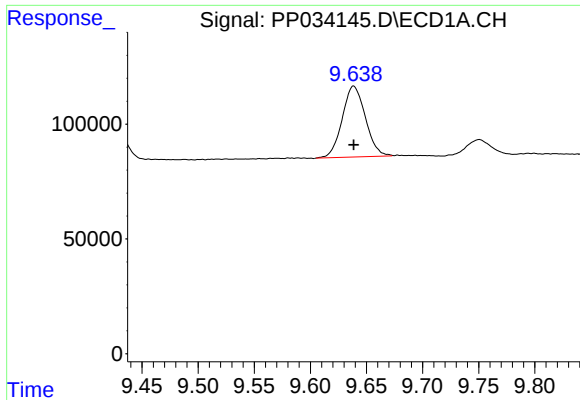


#43 AR-1268-3

R.T.: 9.638 min
Delta R.T.: 0.000 min
Response: 444312
Conc: 50.61 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Ankita
3/22/2021 2:39:22 PM

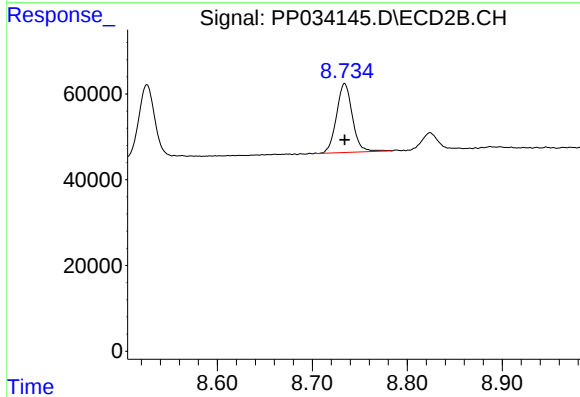


#43 AR-1268-3

R.T.: 8.734 min
Delta R.T.: 0.000 min
Response: 187044
Conc: 54.99 ng/ml m

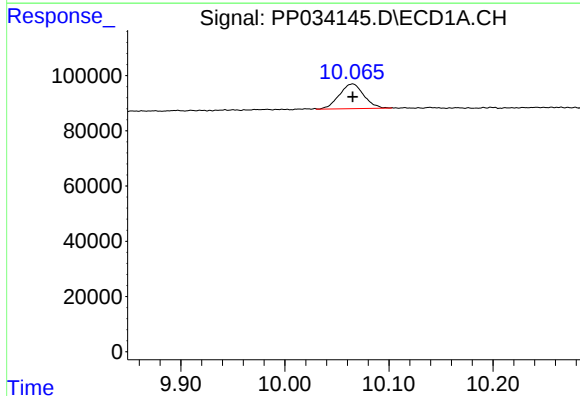


#44 AR-1268-4

R.T.: 10.065 min
Delta R.T.: 0.000 min
Response: 147252
Conc: 46.63 ng/ml m

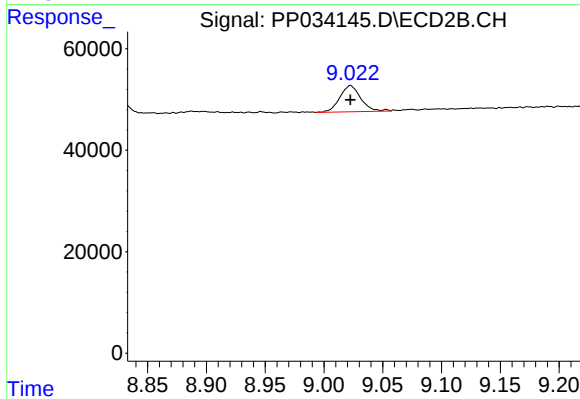

#44 AR-1268-4

R.T.: 9.022 min
Delta R.T.: 0.000 min
Response: 64378
Conc: 54.67 ng/ml m

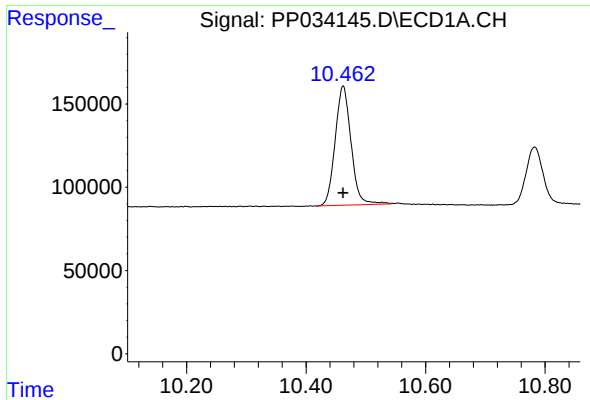


#45 AR-1268-5

R.T.: 10.462 min
Delta R.T.: 0.000 min
Response: 1320139
Conc: 47.63 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050

Manual Integrations
APPROVED

Ankita
3/22/2021 2:39:22 PM

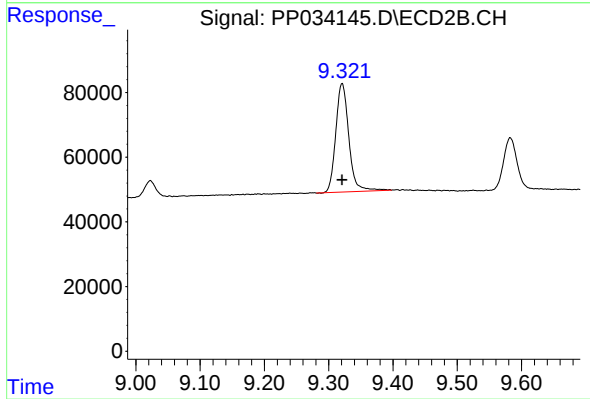

#45 AR-1268-5

R.T.: 9.321 min
Delta R.T.: 0.000 min
Response: 474004
Conc: 50.84 ng/ml