

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031825\
 Data File : PP070670.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 20:27
 Operator : YP\AJ
 Sample : Q1591-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 GAS-TRE-25-0026

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 01:25:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 12 02:42:43 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.521	3.823	33582322	21662834	21.591	21.614
2) SA Decachlor...	10.242	8.869	17482780	15262285	16.457	15.600

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031825\
Data File : PP070670.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 20:27
Operator : YP\AJ
Sample : Q1591-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
GAS-TRE-25-0026

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 01:25:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 12 02:42:43 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

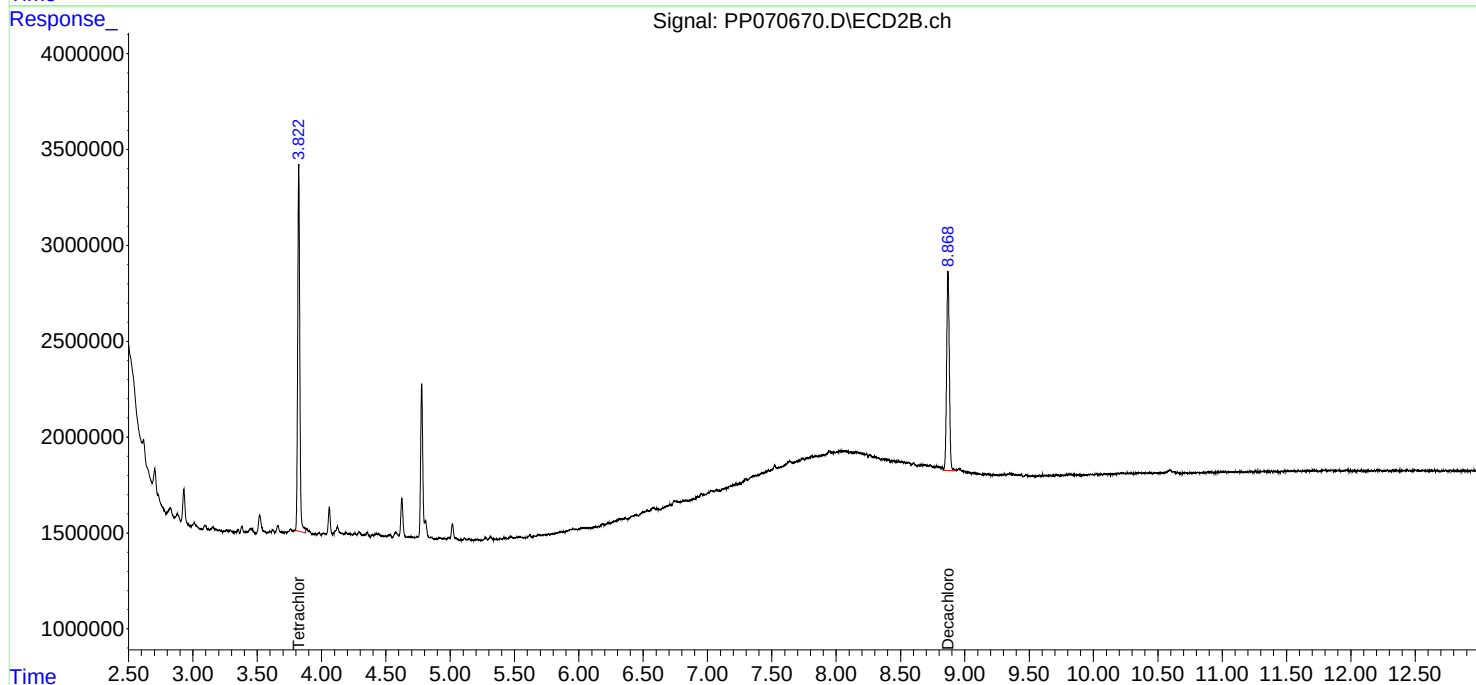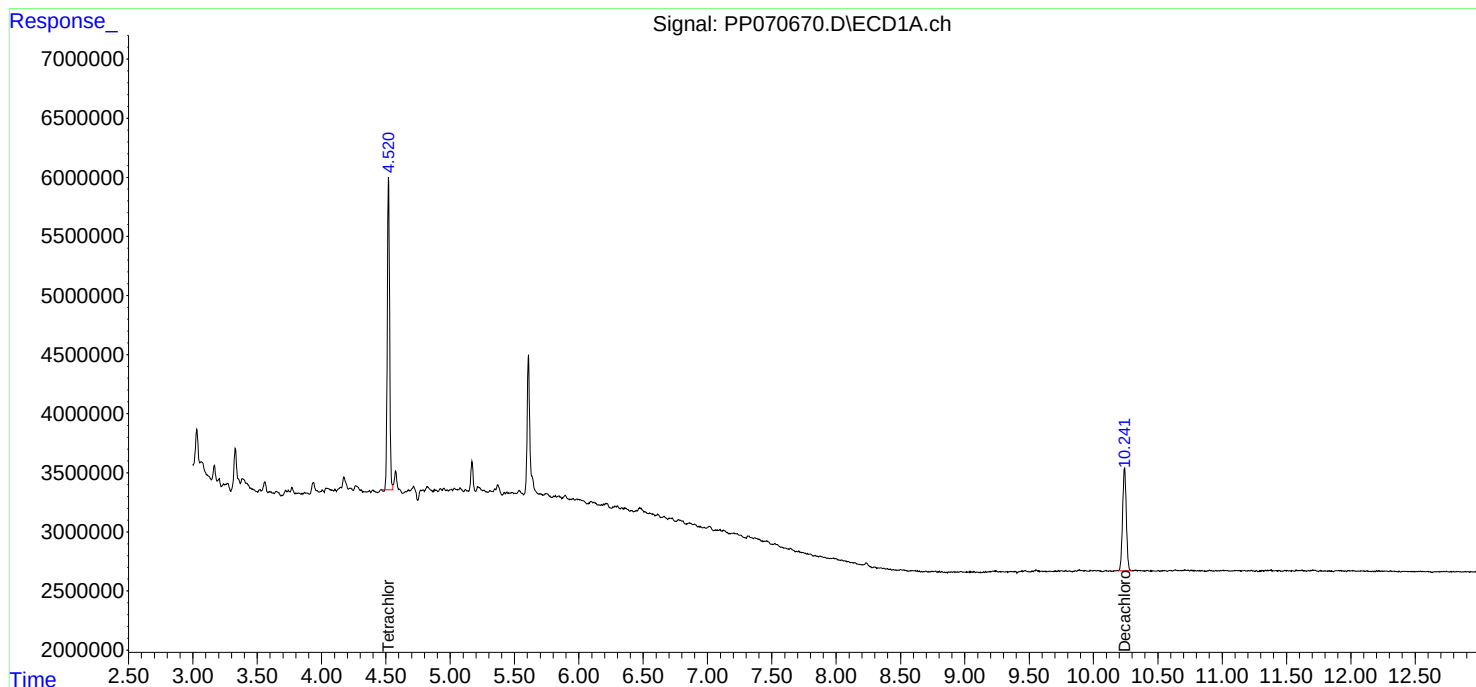


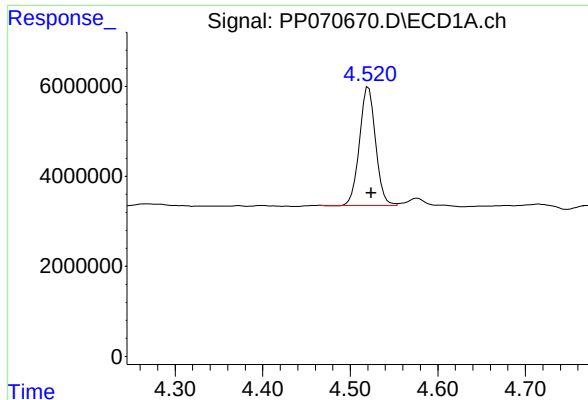

#1 Tetrachloro-m-xylene


R.T.: 4.521 min
Delta R.T.: -0.003 min
Response: 33582322
Conc: 21.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
GAS-TRE-25-0026

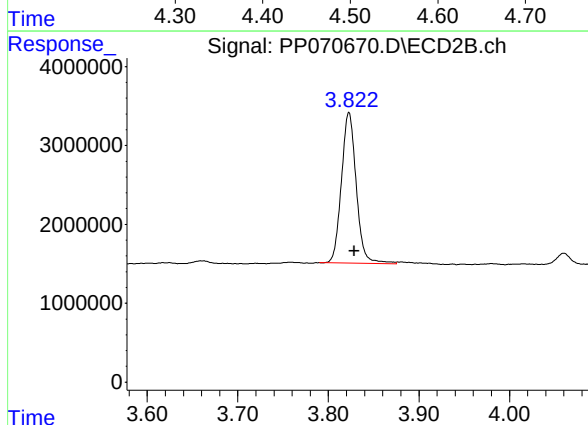


#1 Tetrachloro-m-xylene

R.T.: 3.823 min
Delta R.T.: -0.006 min
Response: 21662834
Conc: 21.61 ng/ml

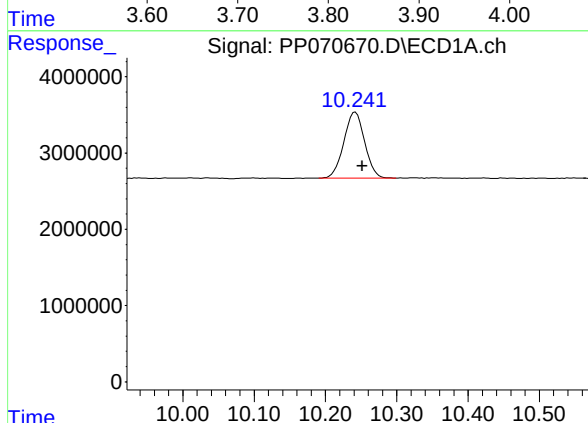

#2 Decachlorobiphenyl

R.T.: 10.242 min
Delta R.T.: -0.010 min
Response: 17482780
Conc: 16.46 ng/ml

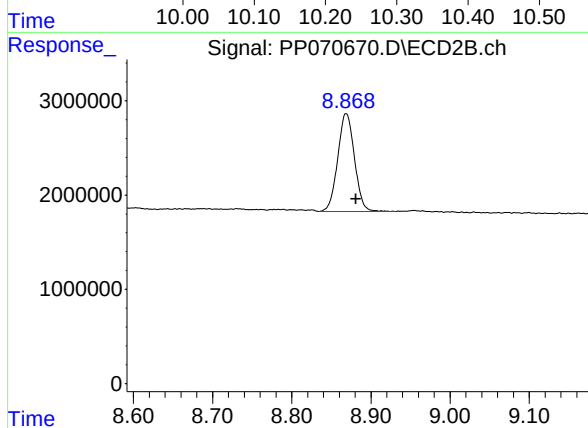

#2 Decachlorobiphenyl

R.T.: 8.869 min
Delta R.T.: -0.012 min
Response: 15262285
Conc: 15.60 ng/ml