

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031825\
 Data File : PP070671.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 20:44
 Operator : YP\AJ
 Sample : Q1591-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 GAS-TRE-25-0027

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/19/2025
 Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 01:25:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 12 02:42:43 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.519	3.825	33143109	22316494	21.309m	22.266
2) SA Decachlor...	10.239	8.869	19830830	16680556	18.667	17.049

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031825\
Data File : PP070671.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 20:44
Operator : YP\AJ
Sample : Q1591-05
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
GAS-TRE-25-0027


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/19/2025
Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 01:25:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 12 02:42:43 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

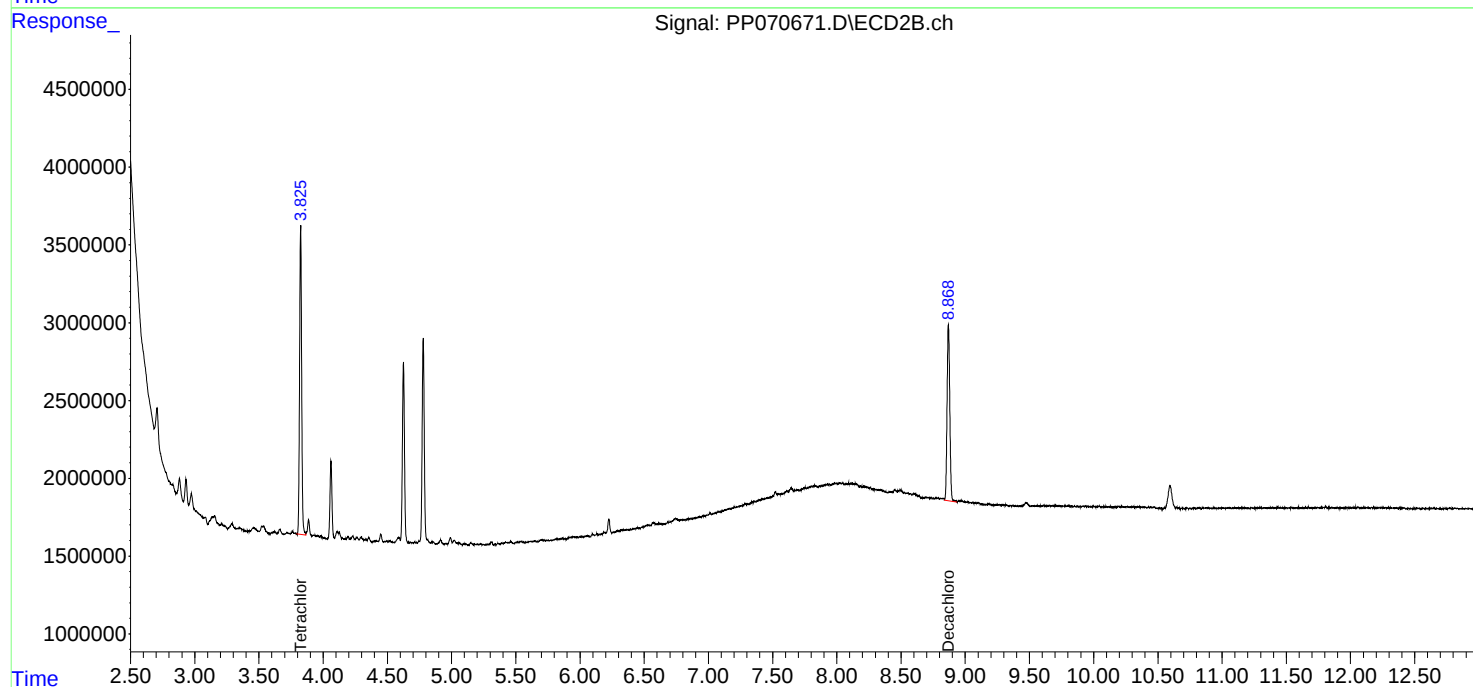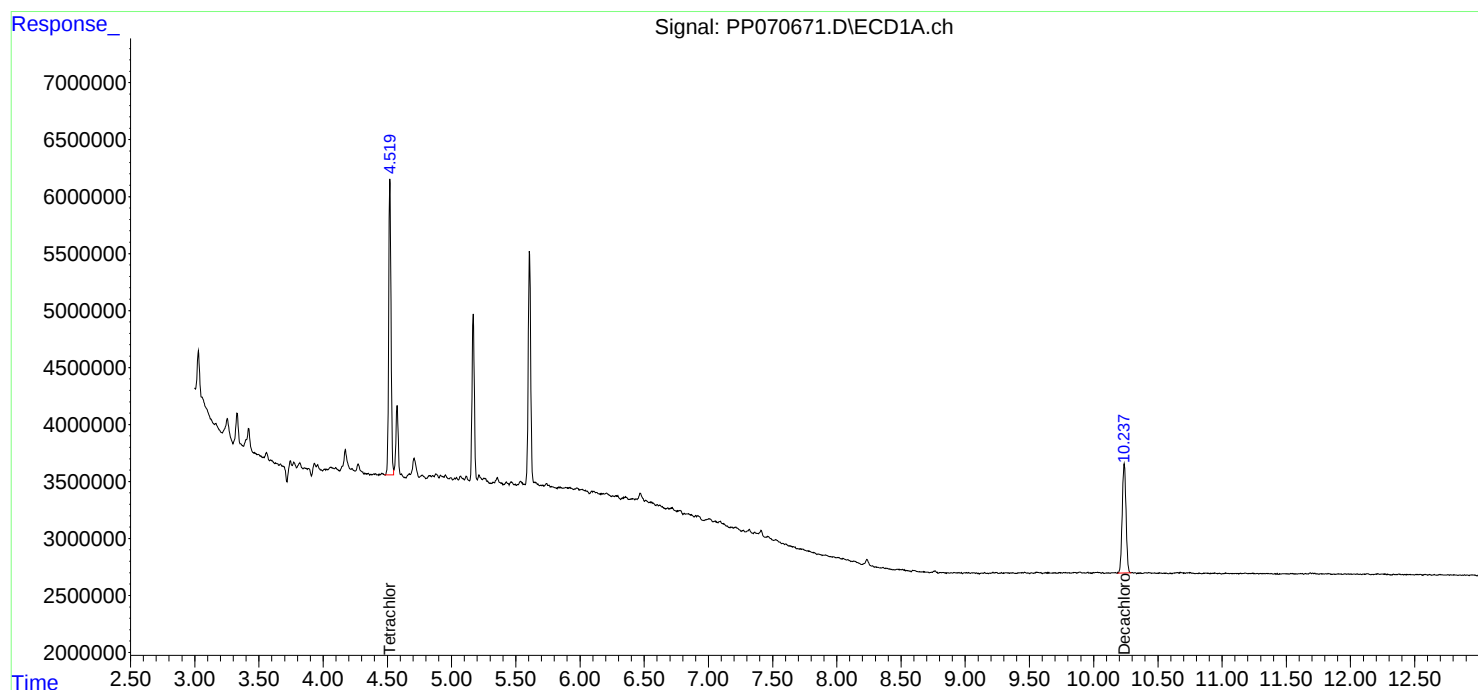

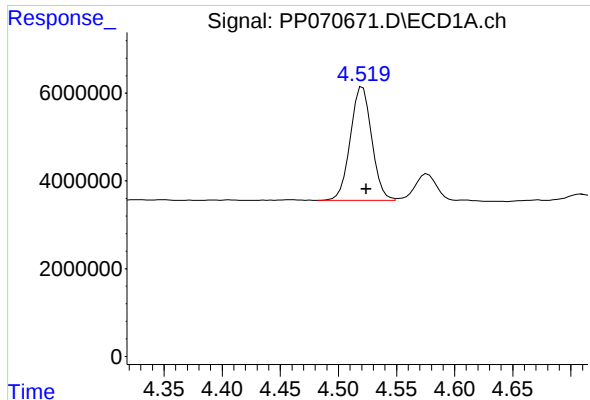


#1 Tetrachloro-m-xylene

R.T.: 4.519 min
Delta R.T.: -0.005 min
Response: 33143109
Conc: 21.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
GAS-TRE-25-0027


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/19/2025
Supervised By :mohammad ahmed 03/24/2025

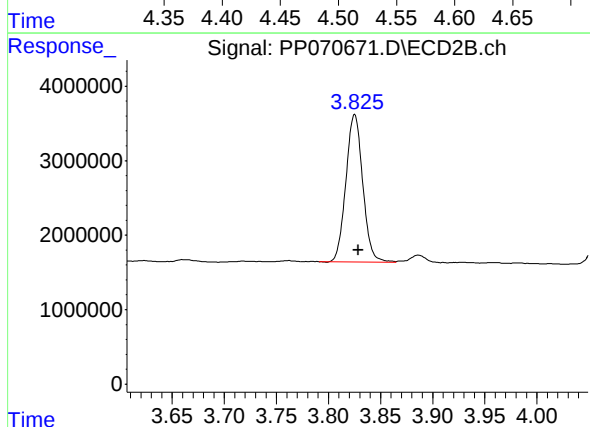


#1 Tetrachloro-m-xylene

R.T.: 3.825 min
Delta R.T.: -0.004 min
Response: 22316494
Conc: 22.27 ng/ml

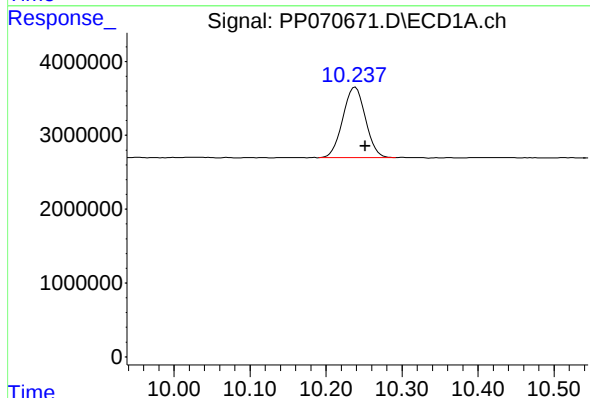

#2 Decachlorobiphenyl

R.T.: 10.239 min
Delta R.T.: -0.013 min
Response: 19830830
Conc: 18.67 ng/ml

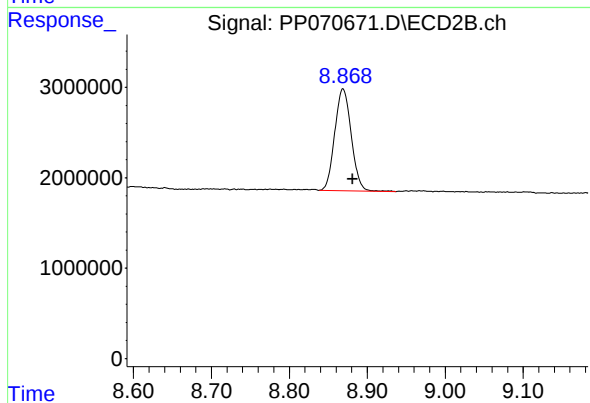

#2 Decachlorobiphenyl

R.T.: 8.869 min
Delta R.T.: -0.012 min
Response: 16680556
Conc: 17.05 ng/ml