

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031919\
 Data File : PP029397.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Mar 2019 13:14
 Operator : EI\MA
 Sample : K1807-46
 Misc : hexane
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-23

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 15:13:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 22 02:24:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.926	12.123	17282503	21382451	575.003	563.400
Target Compounds							
1) T	Dalapon	3.297	2.979	742951	-645845	12.683	N.D. #
8) T	DICHLORPROP	0.000	13.556	0	1119349	N.D.	33.108 #
10) T	Pentachlo...	0.000	14.642	0	1726477	N.D.	3.355 #
11) T	2,4,5-TP ...	0.000	15.212	0	2752217	N.D.	13.531 #
12) T	2,4,5-T	15.441	15.851	7749449	10957185	36.707	66.177 #
13) T	2,4-DB	16.221	0.000	21778749	0	1140.110	N.D. #
14) T	DINOSEB	17.703	16.912	2583916	18444539	17.743	140.720 #
15) T	Picloram	17.485	0.000	4667846	0	16.788	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031919\
Data File : PP029397.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Mar 2019 13:14
Operator : EI\MA
Sample : K1807-46
Misc : hexane
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
TP-23

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 15:13:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
Quant Title : 8080.M
QLast Update : Fri Feb 22 02:24:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

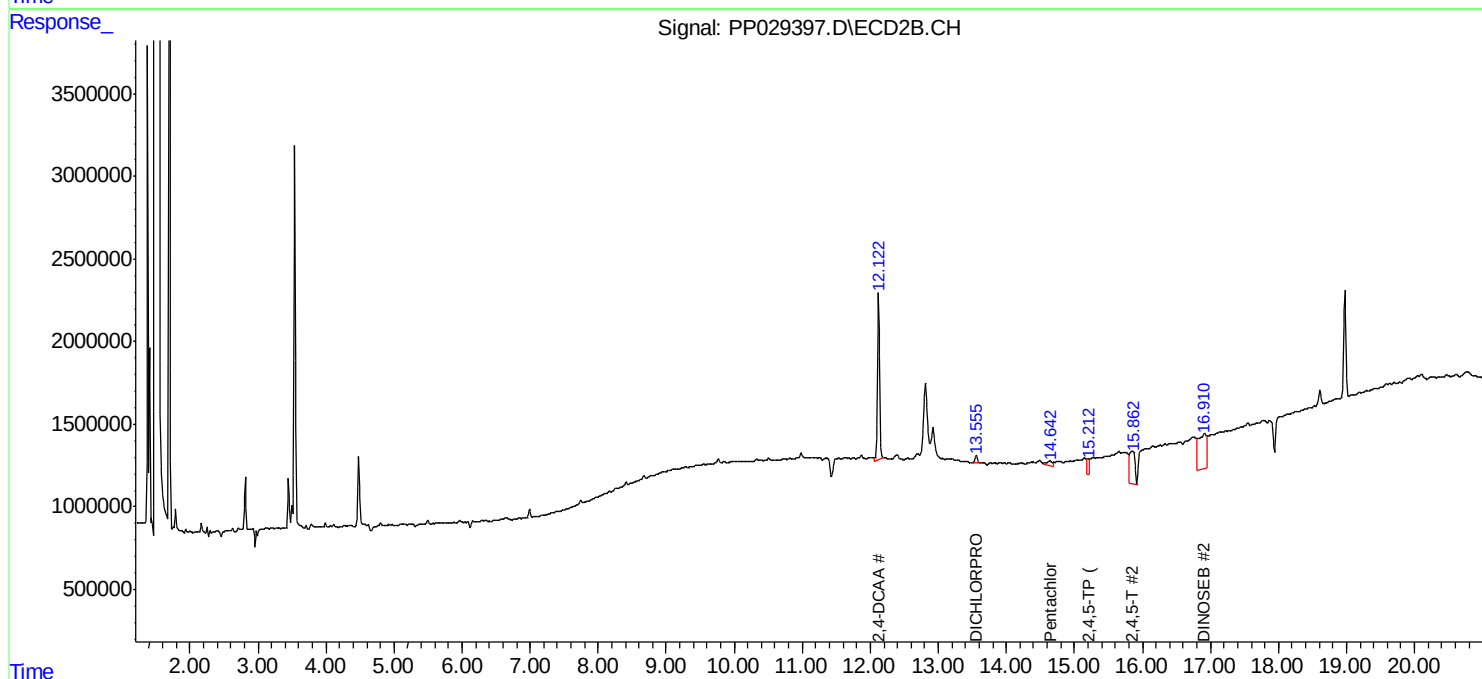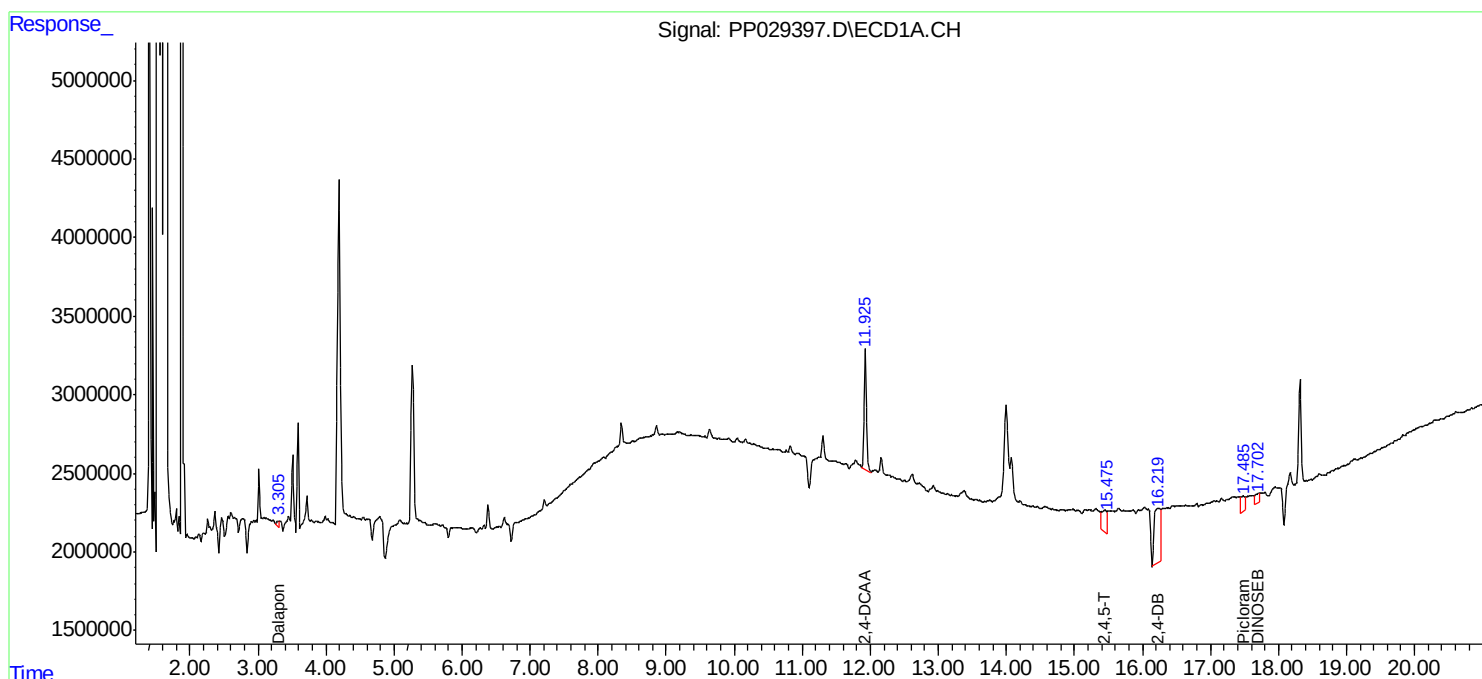


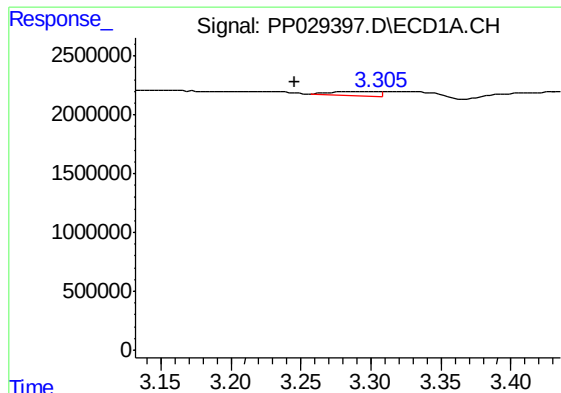

#1 Dalapon


R.T.: 3.297 min
Delta R.T.: 0.051 min
Response: 742951
Conc: 12.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-23

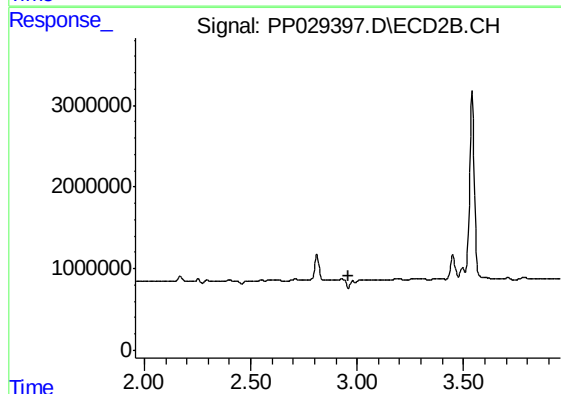


#1 Dalapon

R.T.: 2.979 min
Delta R.T.: 0.021 min
Response: -645845
Conc: N.D.

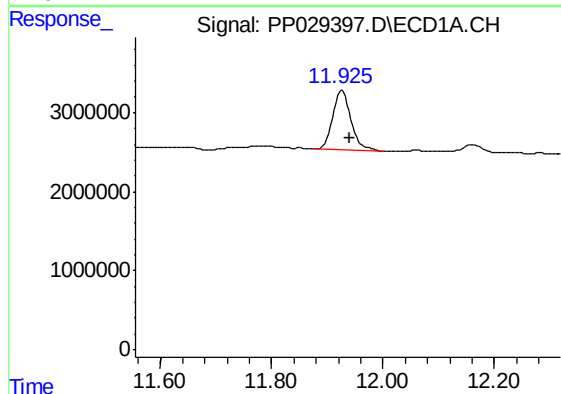


#4 2,4-DCAA

R.T.: 11.926 min
Delta R.T.: -0.014 min
Response: 17282503
Conc: 575.00 ng/ml

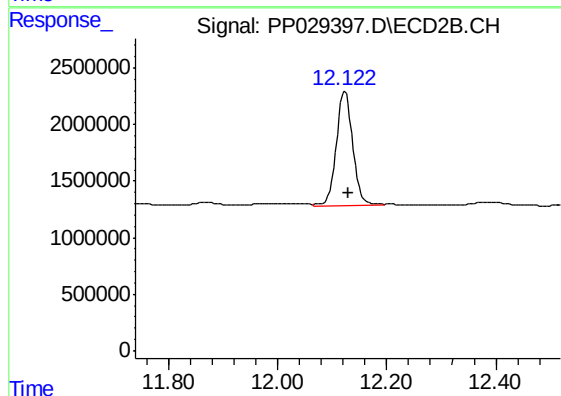

#4 2,4-DCAA


R.T.: 12.123 min
Delta R.T.: -0.005 min
Response: 21382451
Conc: 563.40 ng/ml

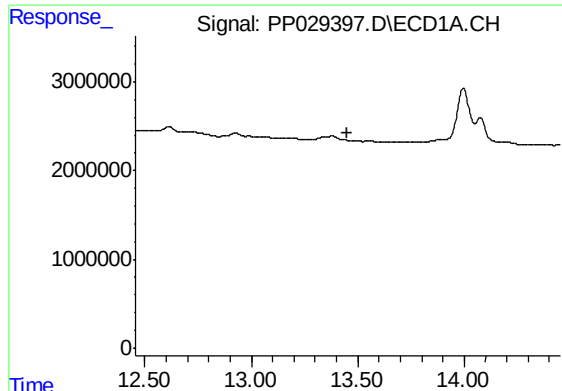

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 13.452 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TP-23

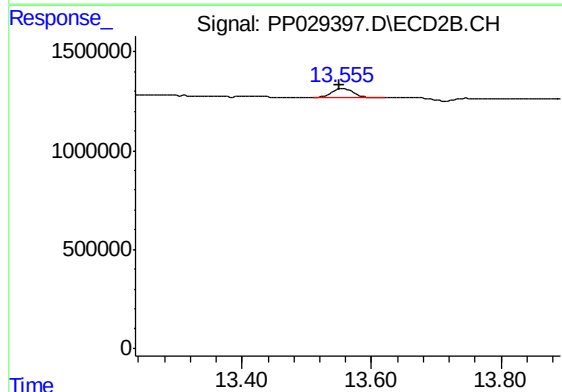


#8 DICHLORPROP

R.T.: 13.556 min
Delta R.T.: 0.004 min
Response: 1119349
Conc: 33.11 ng/ml

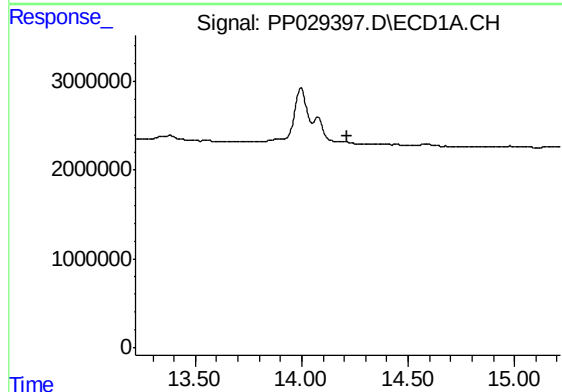


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 14.216 min
Response: 0
Conc: N.D.

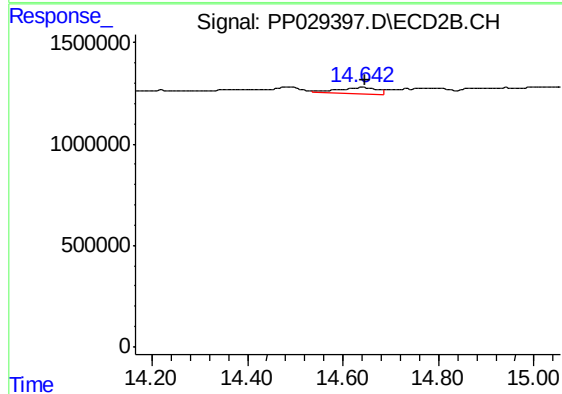

#10 Pentachlorophenol


R.T.: 14.642 min
Delta R.T.: -0.003 min
Response: 1726477
Conc: 3.35 ng/ml

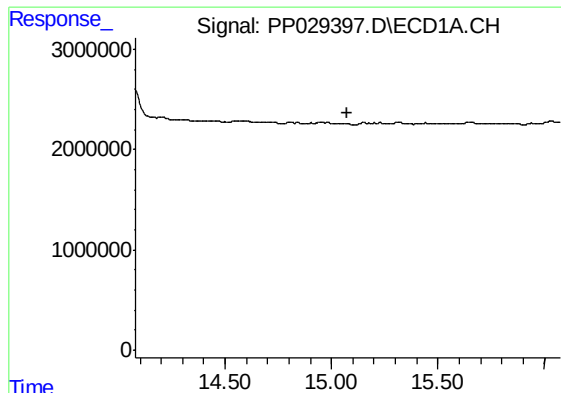

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 15.075 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TP-23

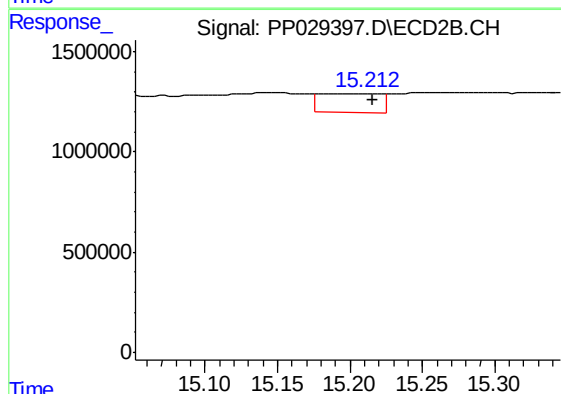


#11 2,4,5-TP (SILVEX)

R.T.: 15.212 min
Delta R.T.: -0.003 min
Response: 2752217
Conc: 13.53 ng/ml

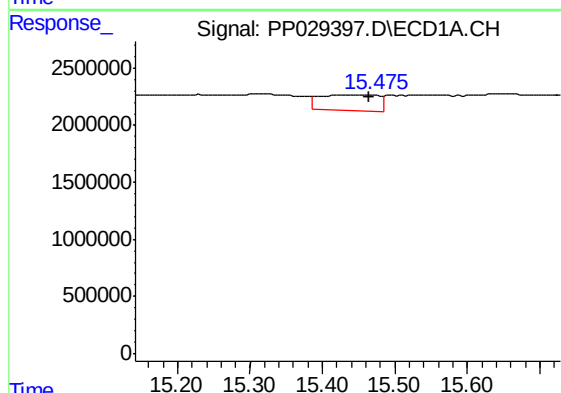


#12 2,4,5-T

R.T.: 15.441 min
Delta R.T.: -0.023 min
Response: 7749449
Conc: 36.71 ng/ml

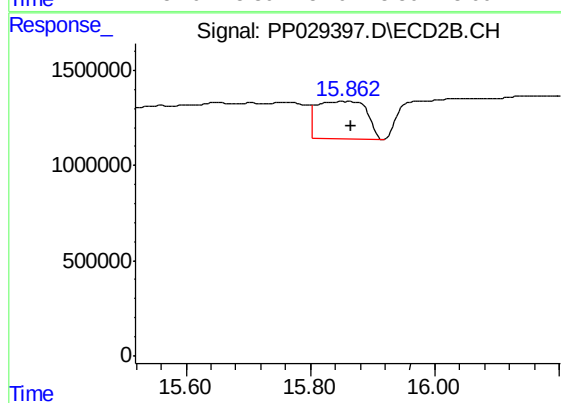

#12 2,4,5-T


R.T.: 15.851 min
Delta R.T.: -0.013 min
Response: 10957185
Conc: 66.18 ng/ml

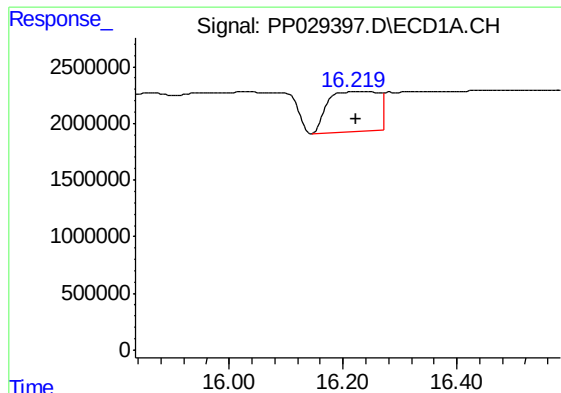

#13 2,4-DB


R.T.: 16.221 min
Delta R.T.: -0.003 min
Response: 21778749
Conc: 1140.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-23

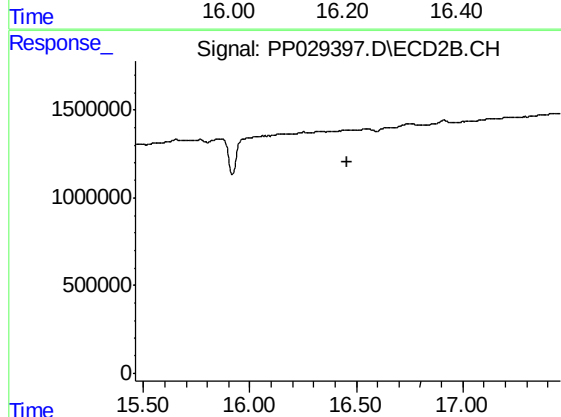


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 16.460 min
Response: 0
Conc: N.D.

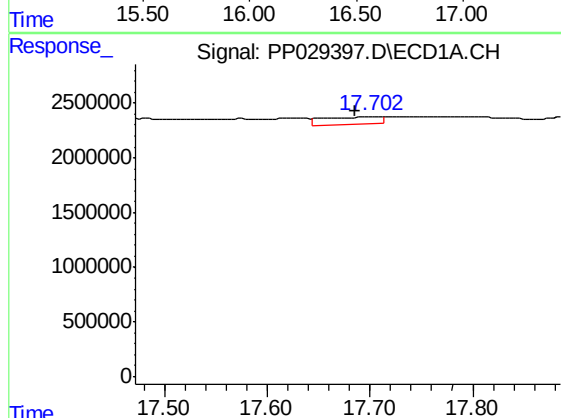


#14 DINOSEB

R.T.: 17.703 min
Delta R.T.: 0.018 min
Response: 2583916
Conc: 17.74 ng/ml

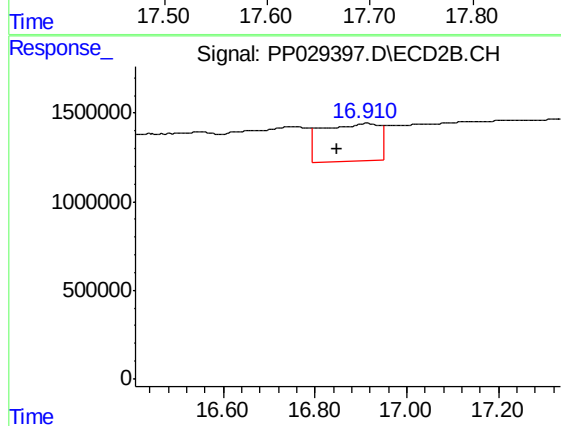

#14 DINOSEB


R.T.: 16.912 min
Delta R.T.: 0.063 min
Response: 18444539
Conc: 140.72 ng/ml

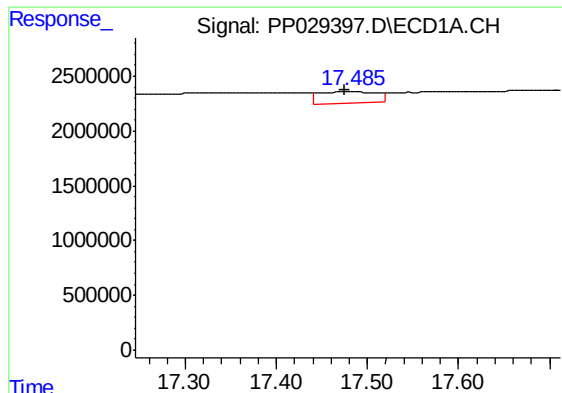

#15 Picloram

R.T.: 17.485 min
Delta R.T.: 0.010 min
Response: 4667846
Conc: 16.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-23

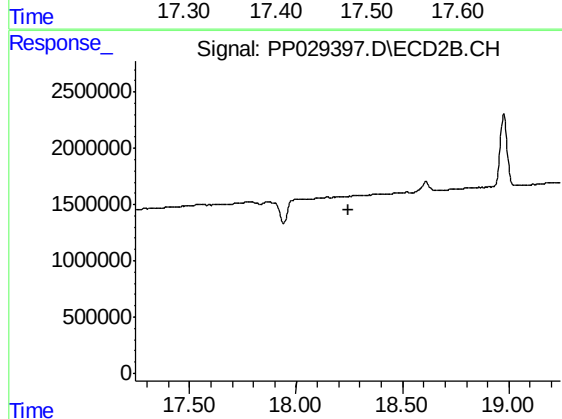

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 18.245 min
Response: 0
Conc: N.D.