

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031919\
 Data File : PP029403.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Mar 2019 15:47
 Operator : EI\MA
 Sample : K1901-04
 Misc : hexane
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-3(7-8)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 16:57:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 22 02:24:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.927	12.123	9649432	11332661	321.045	298.601
Target Compounds							
8) T	DICHLORPROP	0.000	13.561	0	1255134	N.D.	37.124 #
10) T	Pentachlo...	0.000	14.639	0	512377	N.D.	0.996 #
11) T	2,4,5-TP ...	0.000	15.147	0	575849	N.D.	2.831 #
12) T	2,4,5-T	15.484	15.853	3800216	5008119	18.001	30.247 #
13) T	2,4-DB	16.204	16.437	6689057	5326617	350.170	236.459 #
14) T	DINOSEB	17.710	16.817	1392594	2706281	9.563	20.647 #
15) T	Picloram	17.479	18.233	1394947	11469579	5.017	50.971 #
16) T	DCPA	0.000	18.097	0	5428541	N.D.	23.359 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031919\
Data File : PP029403.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Mar 2019 15:47
Operator : EI\MA
Sample : K1901-04
Misc : hexane
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
SB-3(7-8)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 16:57:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
Quant Title : 8080.M
QLast Update : Fri Feb 22 02:24:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

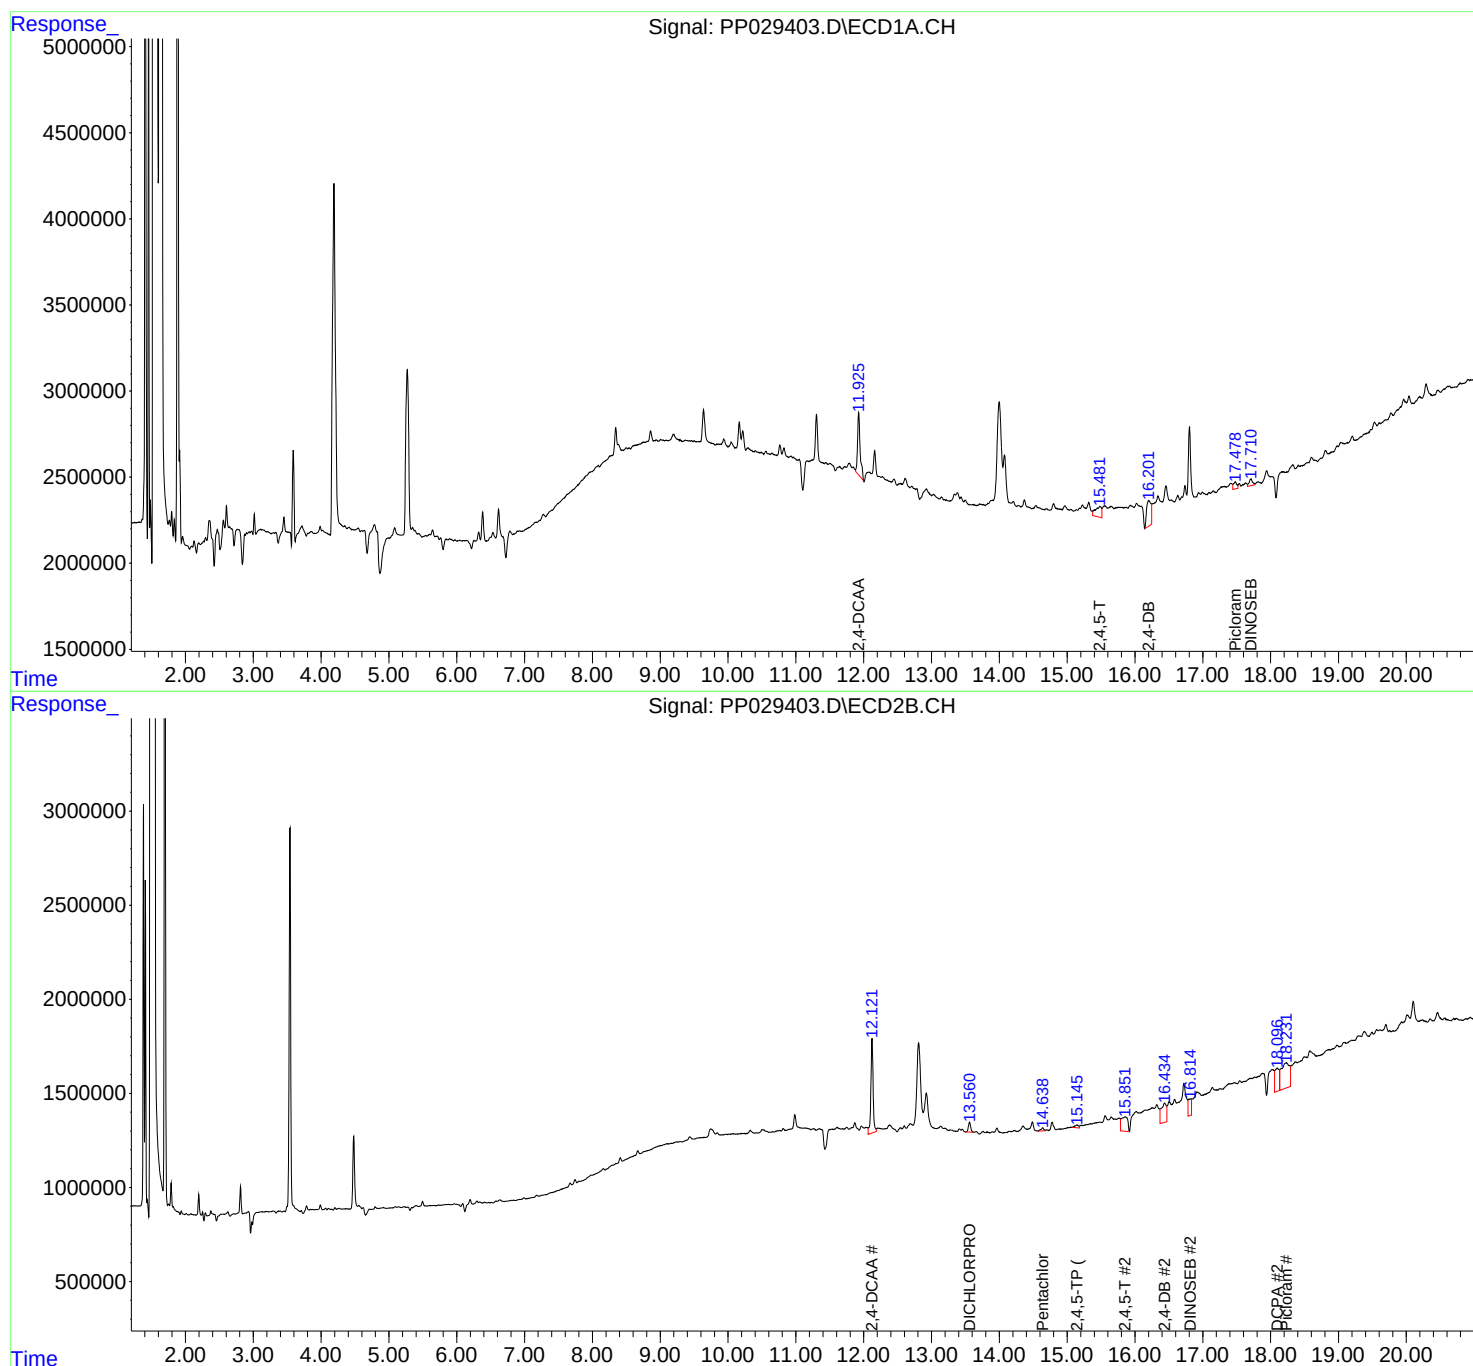


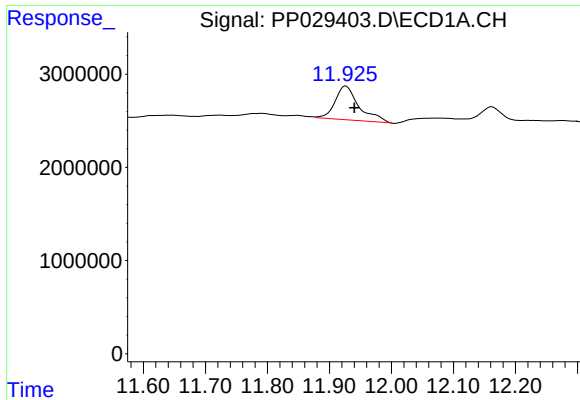

#4 2,4-DCAA


R.T.: 11.927 min
Delta R.T.: -0.014 min
Response: 9649432
Conc: 321.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-3(7-8)

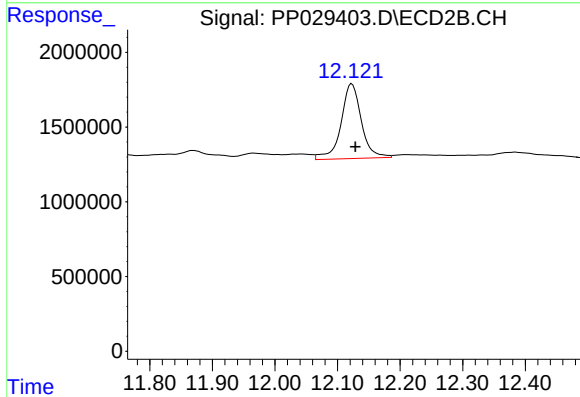


#4 2,4-DCAA

R.T.: 12.123 min
Delta R.T.: -0.006 min
Response: 11332661
Conc: 298.60 ng/ml

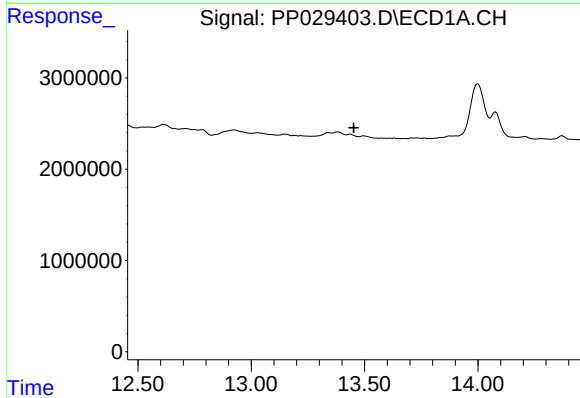


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.452 min
Response: 0
Conc: N.D.

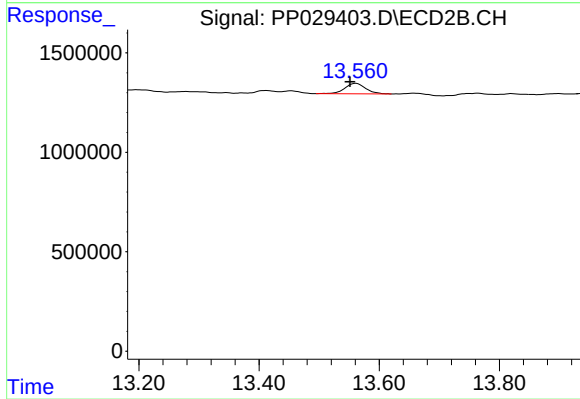

#8 DICHLORPROP


R.T.: 13.561 min
Delta R.T.: 0.010 min
Response: 1255134
Conc: 37.12 ng/ml

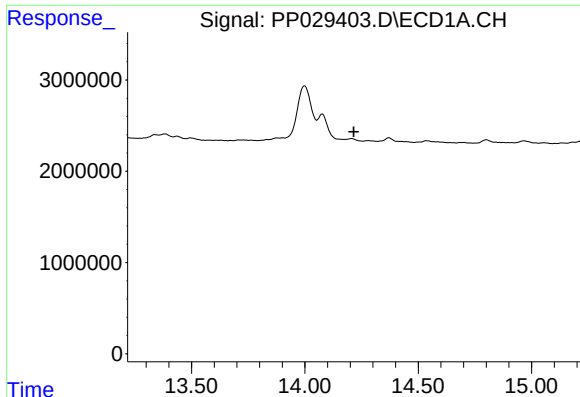

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 14.216 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SB-3(7-8)

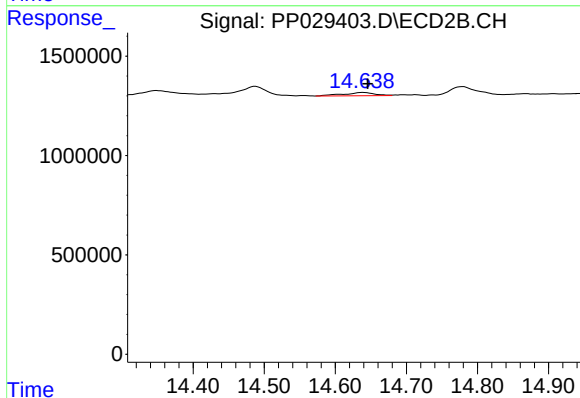


#10 Pentachlorophenol

R.T.: 14.639 min
Delta R.T.: -0.006 min
Response: 512377
Conc: 1.00 ng/ml

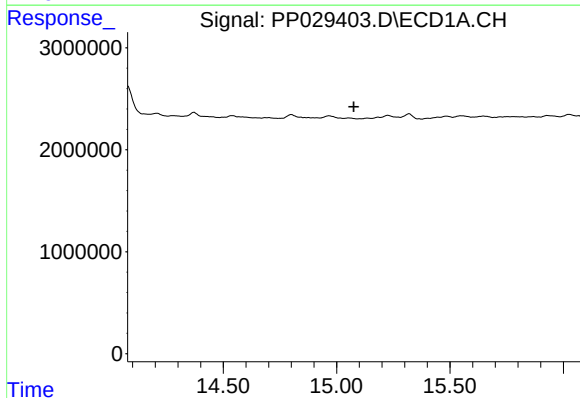


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 15.075 min
Response: 0
Conc: N.D.

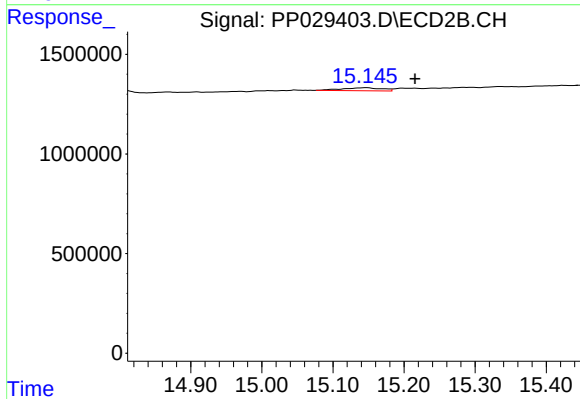

#11 2,4,5-TP (SILVEX)


R.T.: 15.147 min
Delta R.T.: -0.068 min
Response: 575849
Conc: 2.83 ng/ml

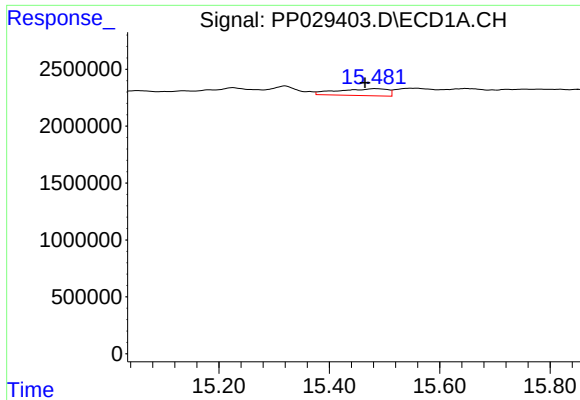

#12 2,4,5-T


R.T.: 15.484 min
Delta R.T.: 0.020 min
Response: 3800216
Conc: 18.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-3(7-8)

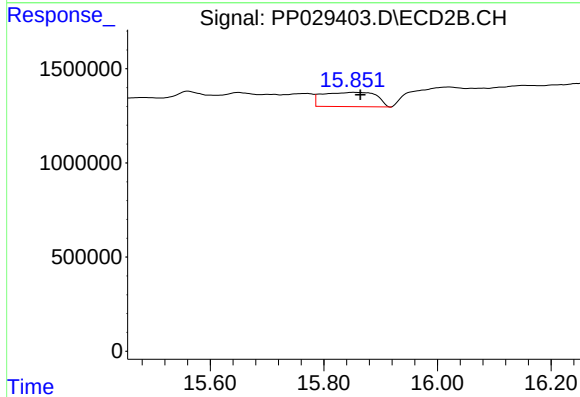


#12 2,4,5-T

R.T.: 15.853 min
Delta R.T.: -0.011 min
Response: 5008119
Conc: 30.25 ng/ml

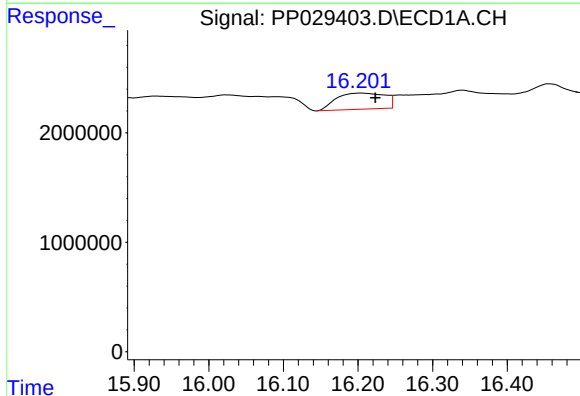


#13 2,4-DB

R.T.: 16.204 min
Delta R.T.: -0.019 min
Response: 6689057
Conc: 350.17 ng/ml

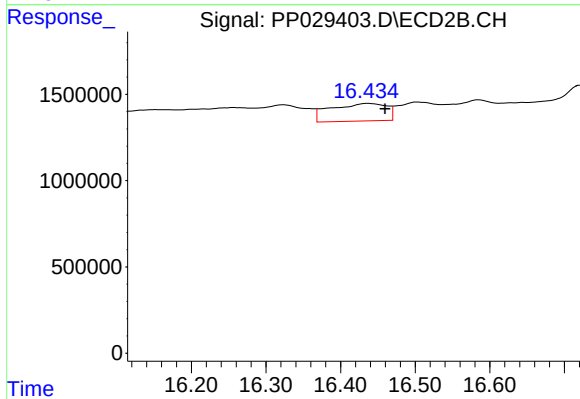

#13 2,4-DB


R.T.: 16.437 min
Delta R.T.: -0.023 min
Response: 5326617
Conc: 236.46 ng/ml

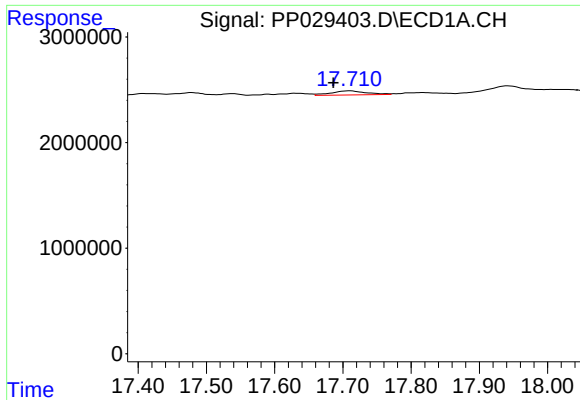

#14 DINOSEB


R.T.: 17.710 min
Delta R.T.: 0.024 min
Response: 1392594
Conc: 9.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-3(7-8)

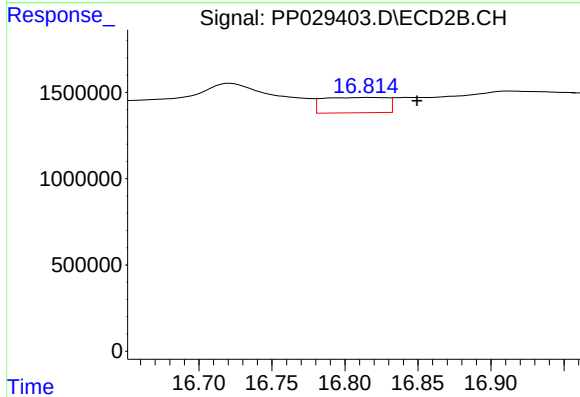


#14 DINOSEB

R.T.: 16.817 min
Delta R.T.: -0.032 min
Response: 2706281
Conc: 20.65 ng/ml

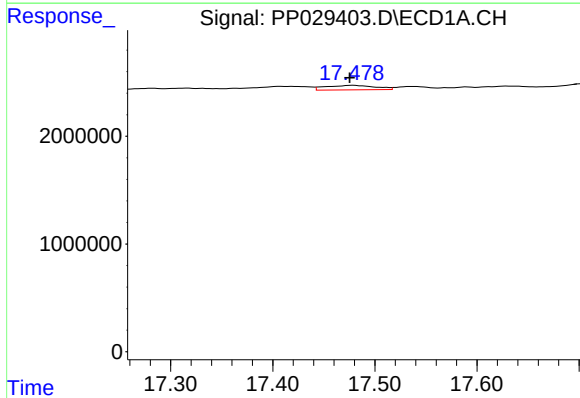


#15 Picloram

R.T.: 17.479 min
Delta R.T.: 0.003 min
Response: 1394947
Conc: 5.02 ng/ml

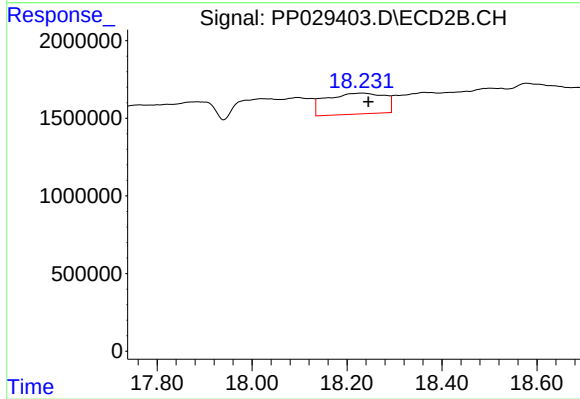

#15 Picloram


R.T.: 18.233 min
Delta R.T.: -0.012 min
Response: 11469579
Conc: 50.97 ng/ml

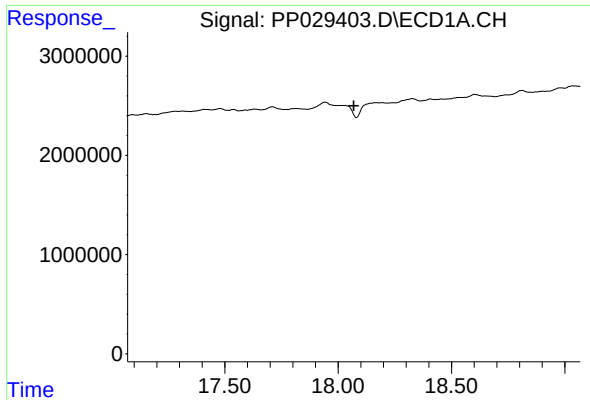

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 18.069 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SB-3(7-8)

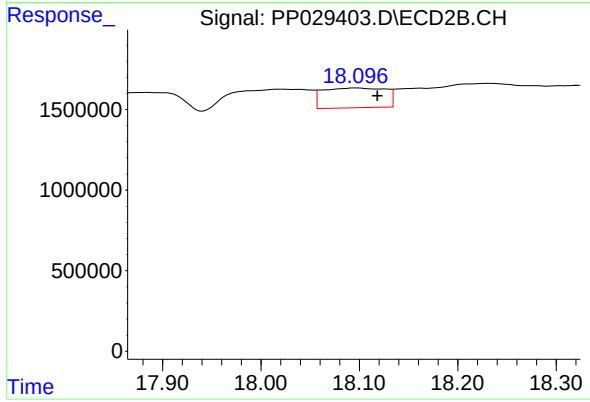

#16 DCPA

R.T.: 18.097 min
Delta R.T.: -0.022 min
Response: 5428541
Conc: 23.36 ng/ml