

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031919\
 Data File : PP029408.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Mar 2019 18:21
 Operator : EI\MA
 Sample : K1901-10
 Misc : hexane
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-16(7-8)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 03:35:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 22 02:24:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.928	12.125	4143566	4600490	137.860	121.217
Target Compounds							
5) T	DICAMBA	12.276	0.000	481892	0	3.624	N.D. #
8) T	DICHLORPROP	0.000	13.558	0	1167462	N.D.	34.531 #
11) T	2,4,5-TP ...	0.000	15.217	0	2080234	N.D.	10.227 #
12) T	2,4,5-T	15.496	15.873	4172667	2985210	19.765	18.030
13) T	2,4-DB	16.206	16.513	6877956	5212776	360.059	231.405 #
14) T	DINOSEB	17.721	0.000	2685720	0	18.442	N.D. #
15) T	Picloram	17.495	18.256	1527412	1265597	5.493	5.624
16) T	DCPA	0.000	18.099	0	12979713	N.D.	55.852 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031919\
Data File : PP029408.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Mar 2019 18:21
Operator : EI\MA
Sample : K1901-10
Misc : hexane
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
SB-16(7-8)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 03:35:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
Quant Title : 8080.M
QLast Update : Fri Feb 22 02:24:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

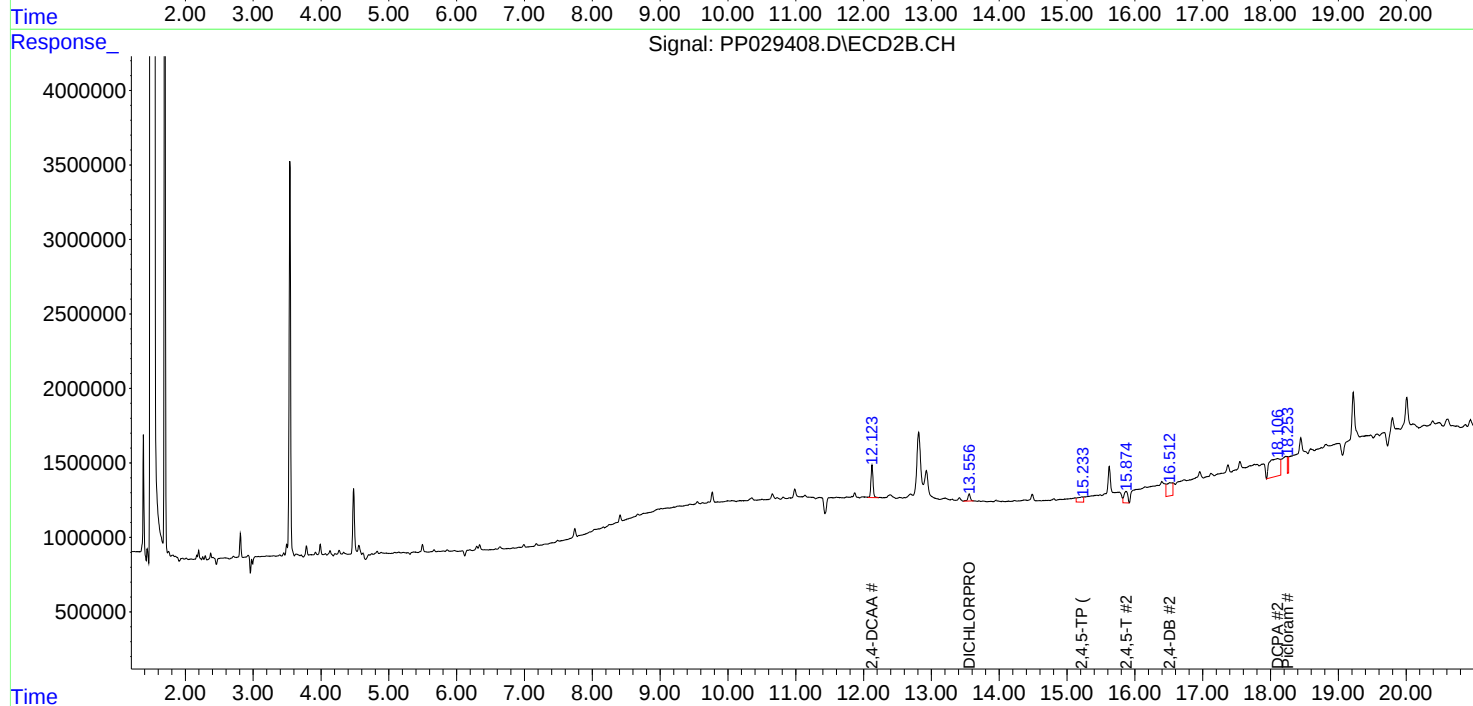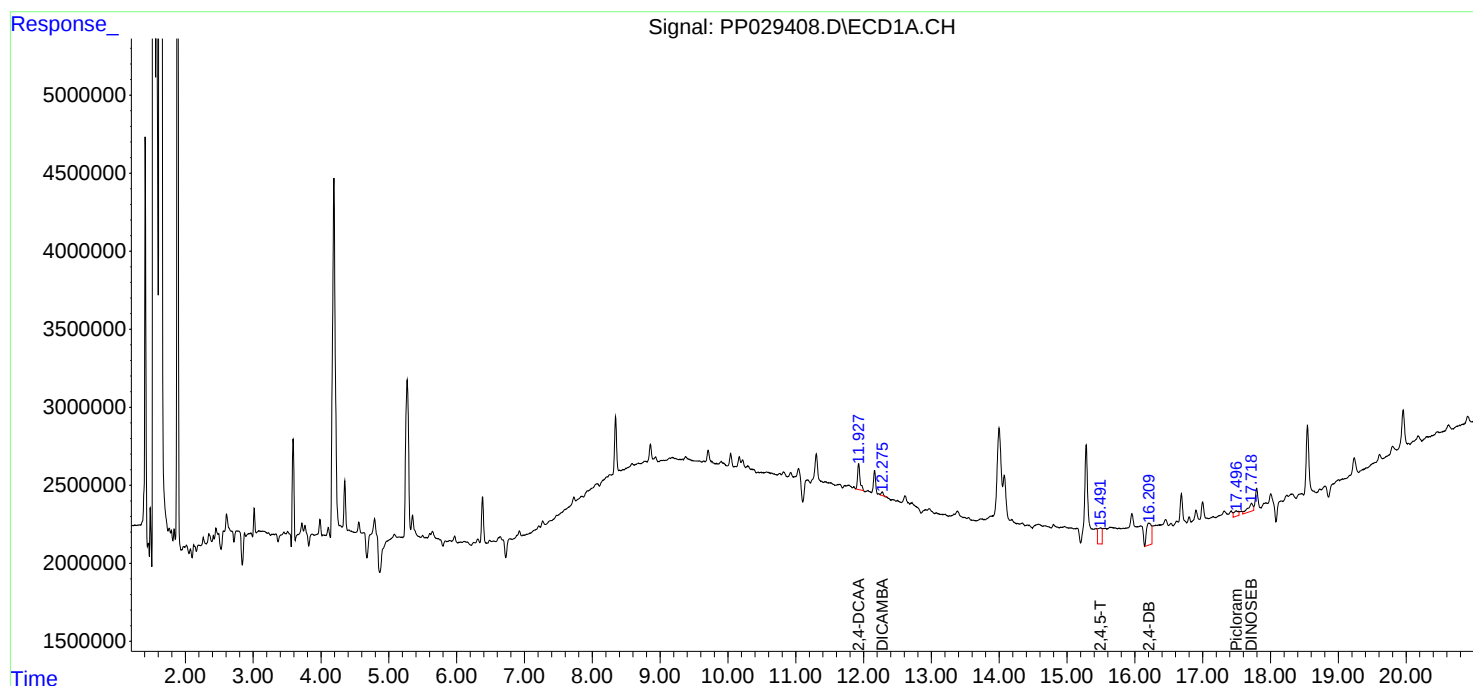


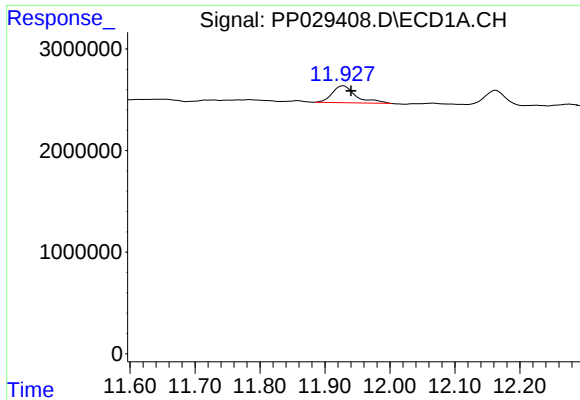

#4 2,4-DCAA


R.T.: 11.928 min
Delta R.T.: -0.012 min
Response: 4143566
Conc: 137.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-16(7-8)

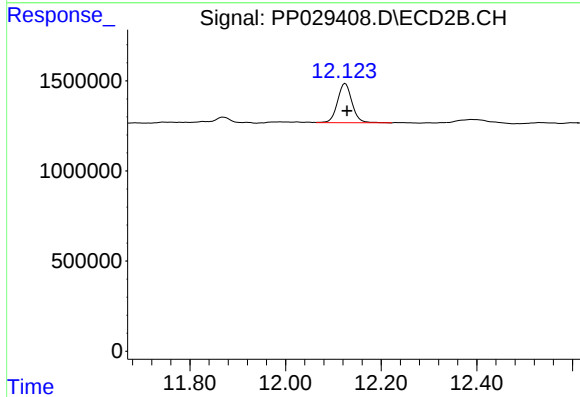


#4 2,4-DCAA

R.T.: 12.125 min
Delta R.T.: -0.004 min
Response: 4600490
Conc: 121.22 ng/ml

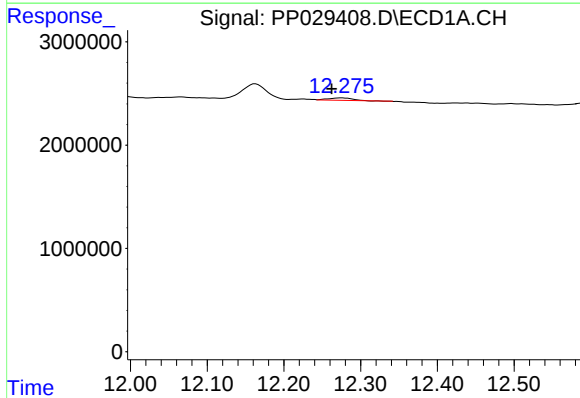


#5 DICAMBA

R.T.: 12.276 min
Delta R.T.: 0.014 min
Response: 481892
Conc: 3.62 ng/ml

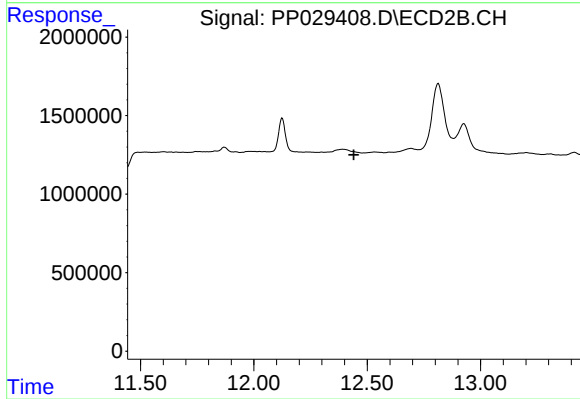

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 12.441 min
Response: 0
Conc: N.D.

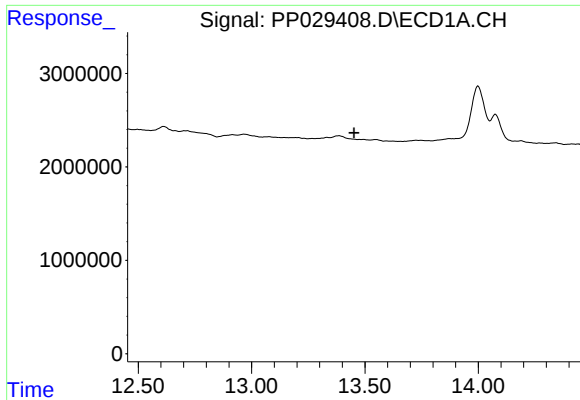

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 13.452 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SB-16(7-8)

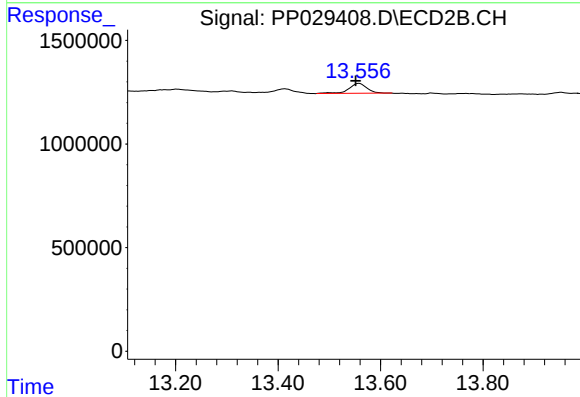


#8 DICHLORPROP

R.T.: 13.558 min
Delta R.T.: 0.006 min
Response: 1167462
Conc: 34.53 ng/ml

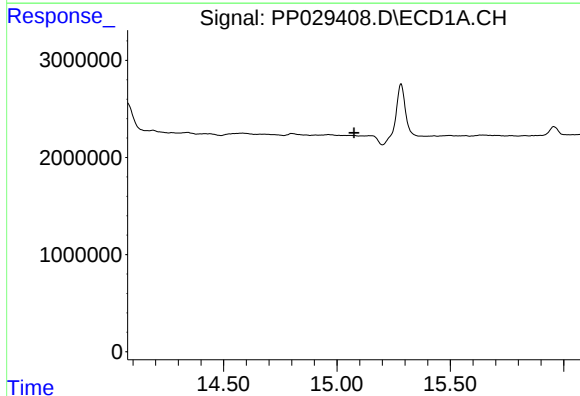


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 15.075 min
Response: 0
Conc: N.D.

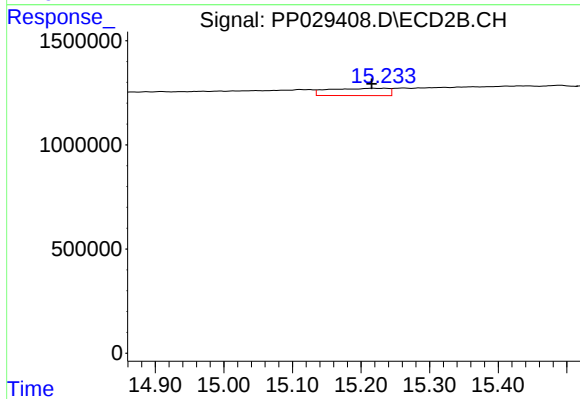

#11 2,4,5-TP (SILVEX)


R.T.: 15.217 min
Delta R.T.: 0.001 min
Response: 2080234
Conc: 10.23 ng/ml

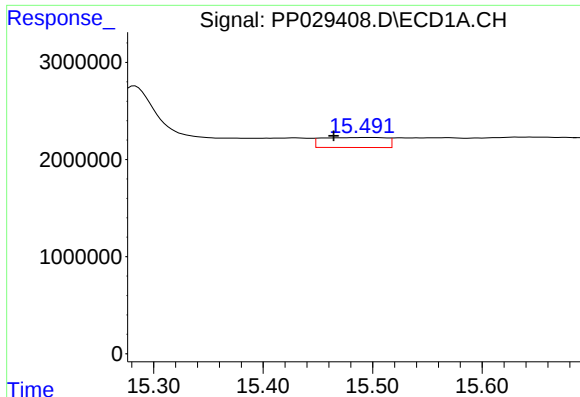

#12 2,4,5-T


R.T.: 15.496 min
Delta R.T.: 0.032 min
Response: 4172667
Conc: 19.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-16(7-8)

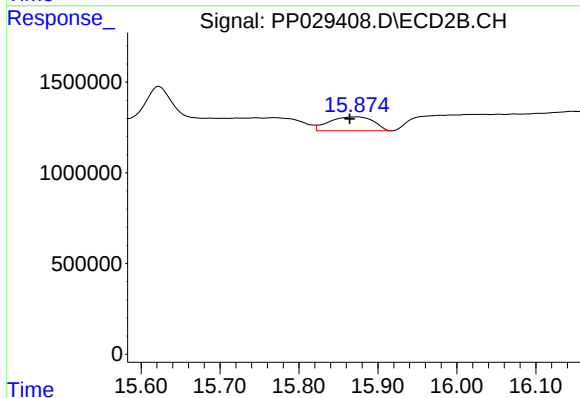


#12 2,4,5-T

R.T.: 15.873 min
Delta R.T.: 0.009 min
Response: 2985210
Conc: 18.03 ng/ml

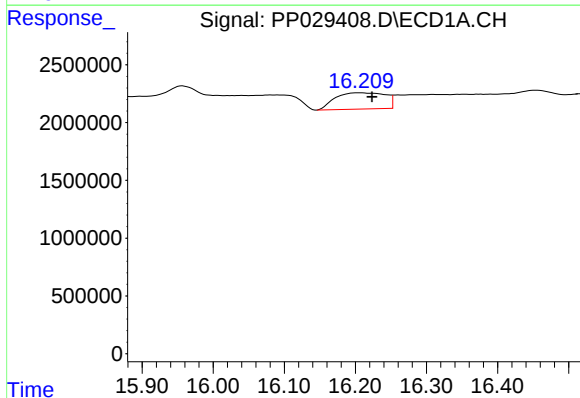


#13 2,4-DB

R.T.: 16.206 min
Delta R.T.: -0.017 min
Response: 6877956
Conc: 360.06 ng/ml

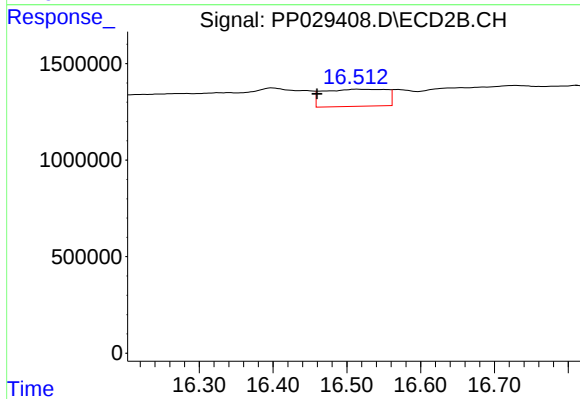

#13 2,4-DB


R.T.: 16.513 min
Delta R.T.: 0.054 min
Response: 5212776
Conc: 231.41 ng/ml

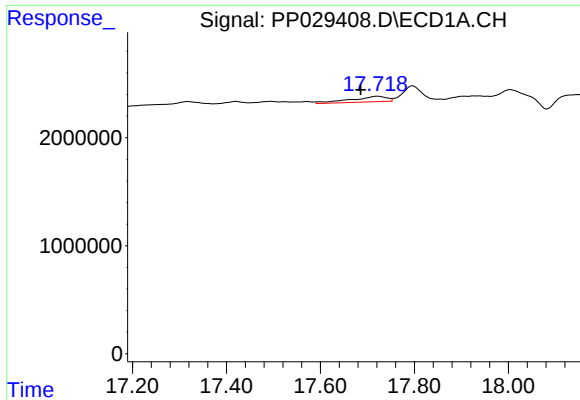

#14 DINOSEB


R.T.: 17.721 min
Delta R.T.: 0.035 min
Response: 2685720
Conc: 18.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-16(7-8)

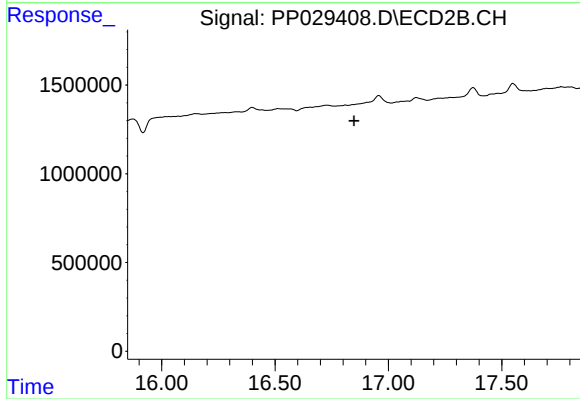


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 16.849 min
Response: 0
Conc: N.D.

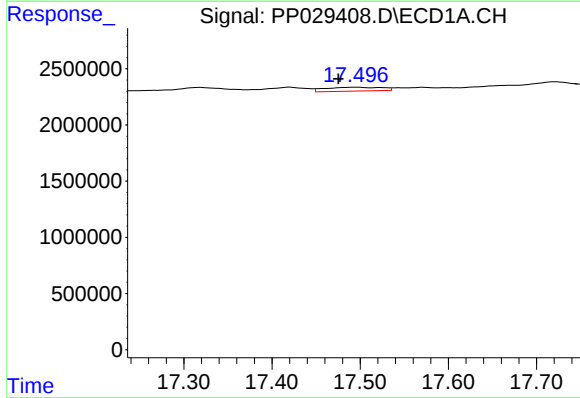


#15 Picloram

R.T.: 17.495 min
Delta R.T.: 0.020 min
Response: 1527412
Conc: 5.49 ng/ml

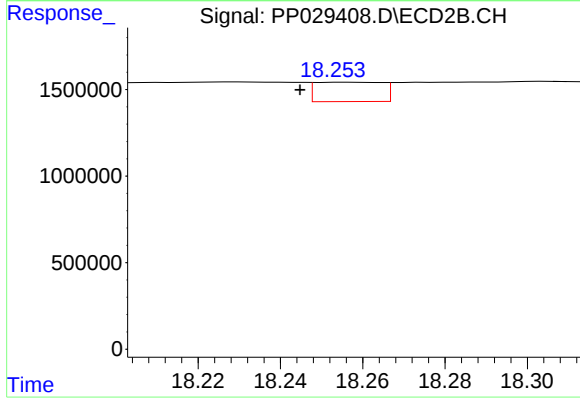

#15 Picloram


R.T.: 18.256 min
Delta R.T.: 0.011 min
Response: 1265597
Conc: 5.62 ng/ml

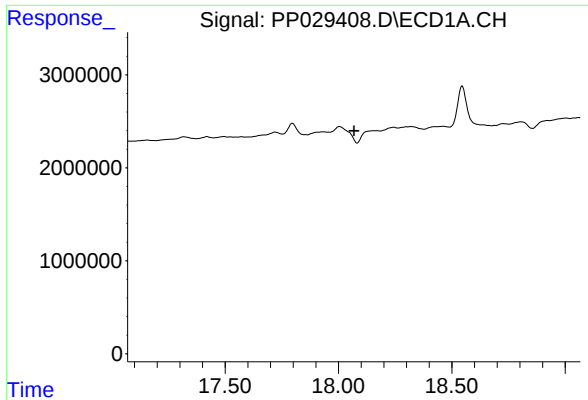

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 18.069 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SB-16(7-8)

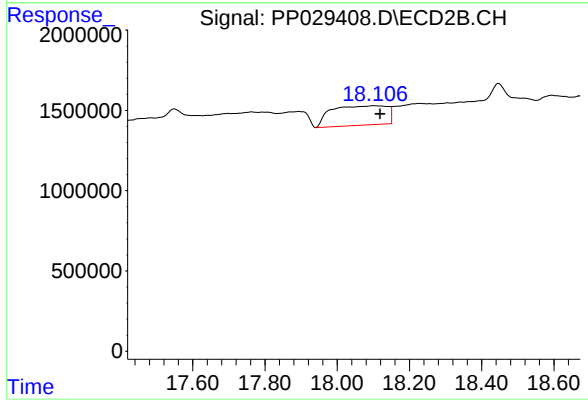

#16 DCPA

R.T.: 18.099 min
Delta R.T.: -0.019 min
Response: 12979713
Conc: 55.85 ng/ml