

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031919\
 Data File : PP029411.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Mar 2019 19:38
 Operator : EI\MA
 Sample : K1901-07
 Misc : hexane
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-6(0.5-1.5)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 03:35:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 22 02:24:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.927	12.123	15376049	19601842	511.574	516.483
Target Compounds							
3) T	4-Nitroph...	0.000	11.341	0	6726488	N.D.	280.881 #
8) T	DICHLORPROP	0.000	13.557	0	550314	N.D.	16.277 #
11) T	2,4,5-TP ...	0.000	15.284	0	5641457	N.D.	27.735 #
12) T	2,4,5-T	15.445	15.873	3801453	7518570	18.007	45.409 #
13) T	2,4-DB	16.204	16.433	15977460	9235956	836.414	410.002 #
14) T	DINOSEB	17.708	16.907	2833326	17085736	19.456	130.354 #
15) T	Picloram	17.489	0.000	3844219	0	13.826	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031919\
Data File : PP029411.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Mar 2019 19:38
Operator : EI\MA
Sample : K1901-07
Misc : hexane
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
SB-6(0.5-1.5)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 03:35:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
Quant Title : 8080.M
QLast Update : Fri Feb 22 02:24:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

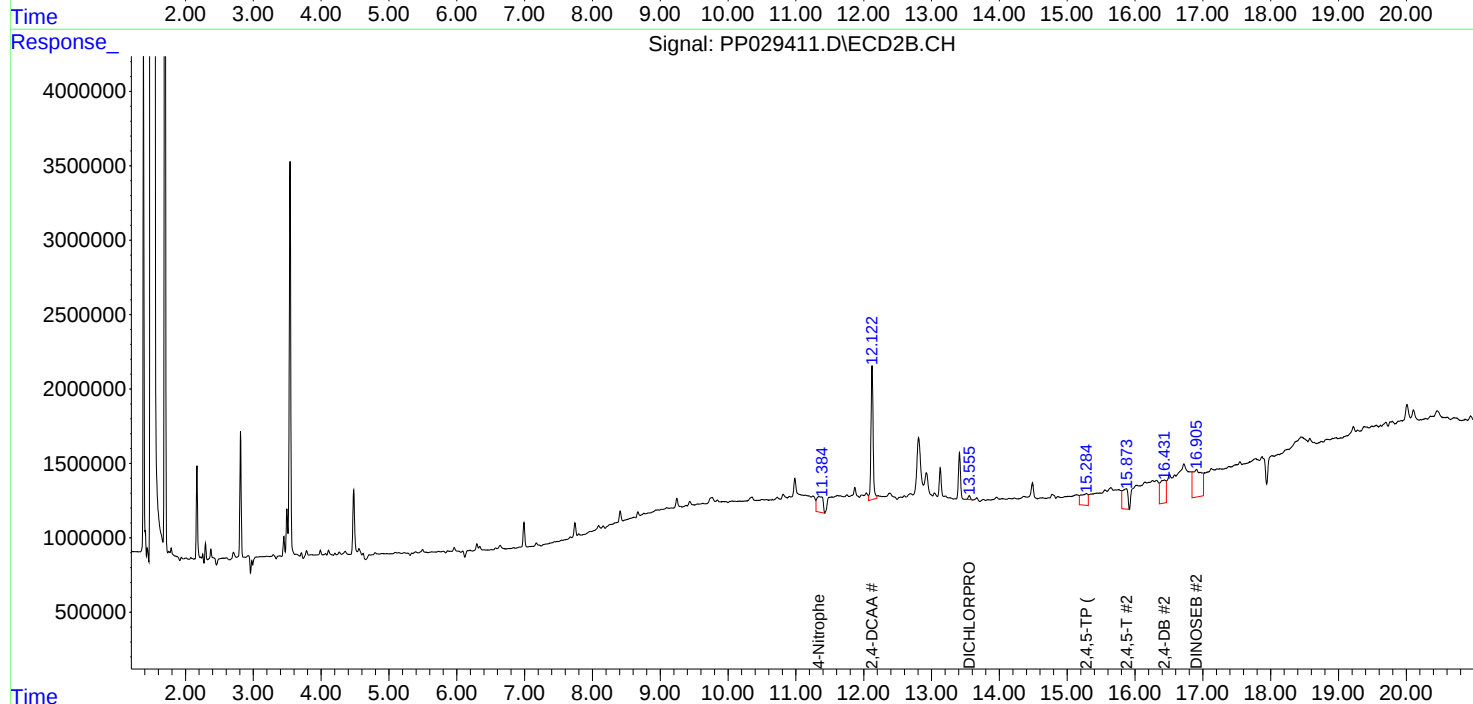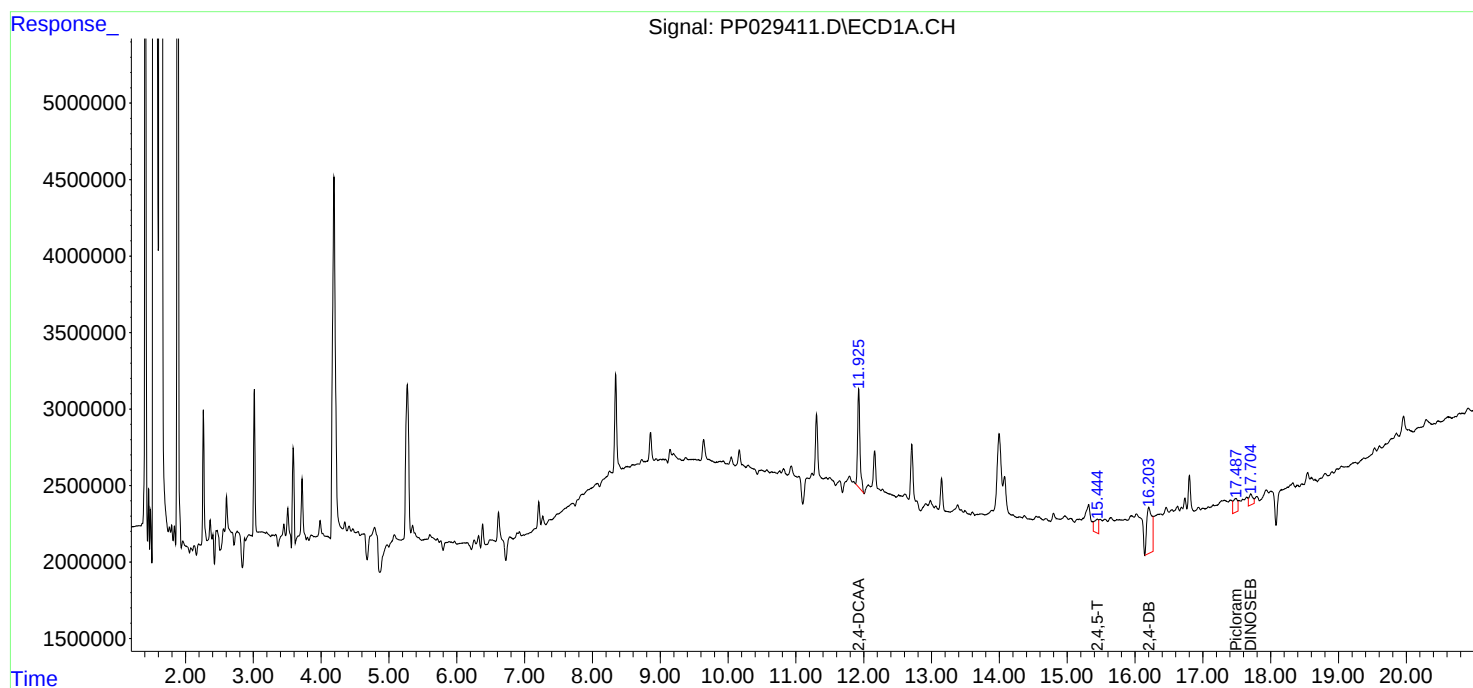


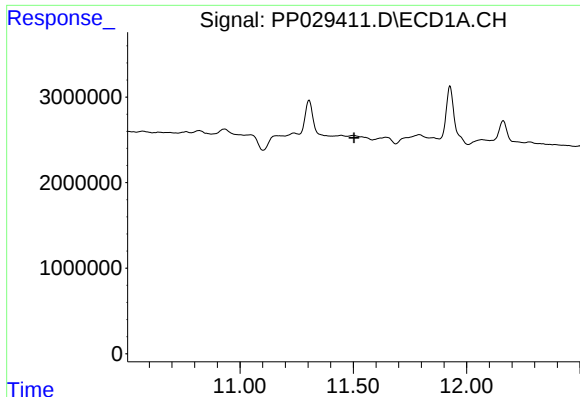

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.504 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SB-6(0.5-1.5)

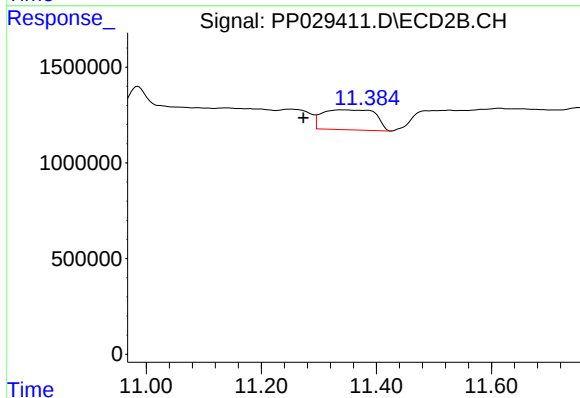


#3 4-Nitrophenol

R.T.: 11.341 min
Delta R.T.: 0.068 min
Response: 6726488
Conc: 280.88 ng/ml

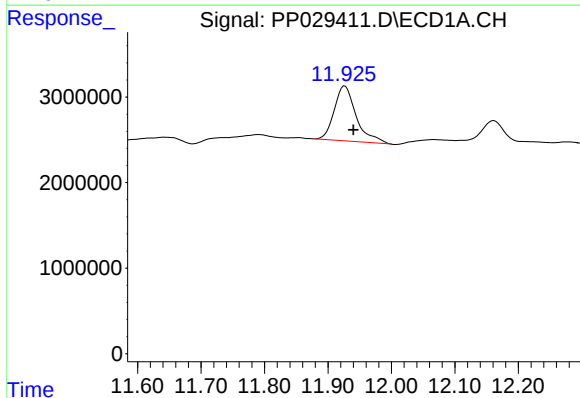


#4 2,4-DCAA

R.T.: 11.927 min
Delta R.T.: -0.014 min
Response: 15376049
Conc: 511.57 ng/ml

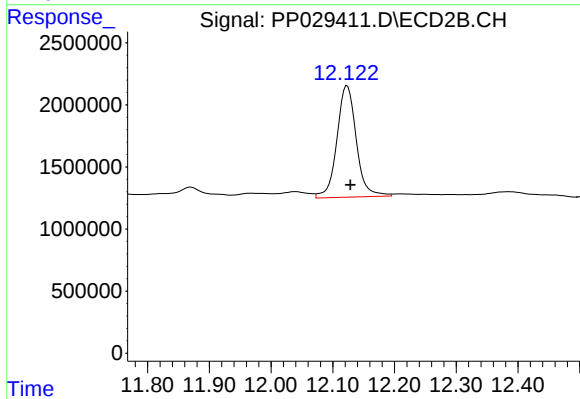

#4 2,4-DCAA


R.T.: 12.123 min
Delta R.T.: -0.005 min
Response: 19601842
Conc: 516.48 ng/ml

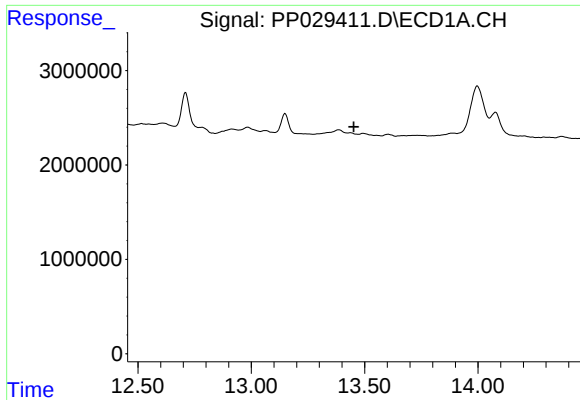

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.452 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SB-6(0.5-1.5)

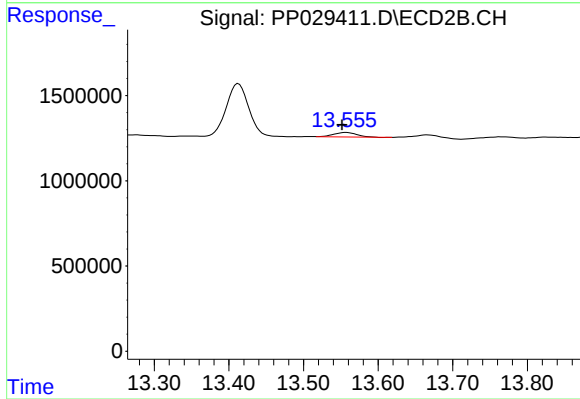


#8 DICHLORPROP

R.T.: 13.557 min
Delta R.T.: 0.006 min
Response: 550314
Conc: 16.28 ng/ml

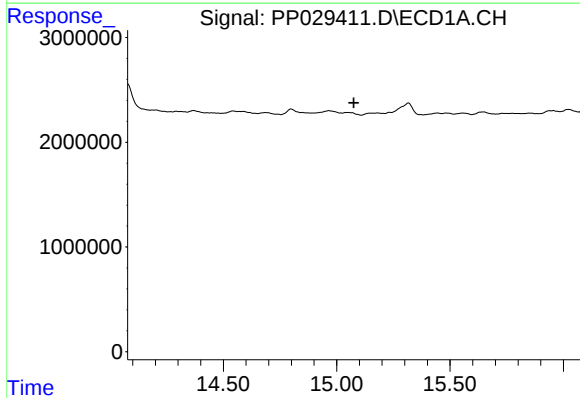


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 15.075 min
Response: 0
Conc: N.D.

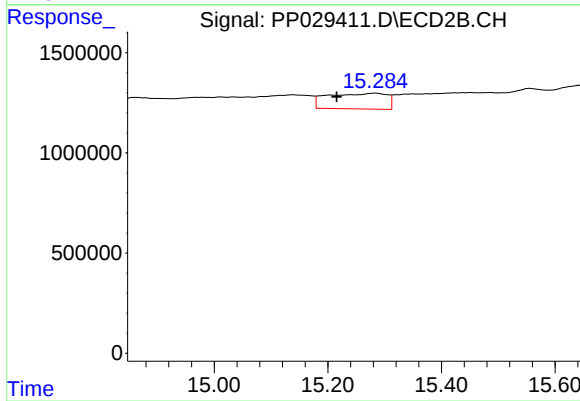

#11 2,4,5-TP (SILVEX)


R.T.: 15.284 min
Delta R.T.: 0.068 min
Response: 5641457
Conc: 27.73 ng/ml

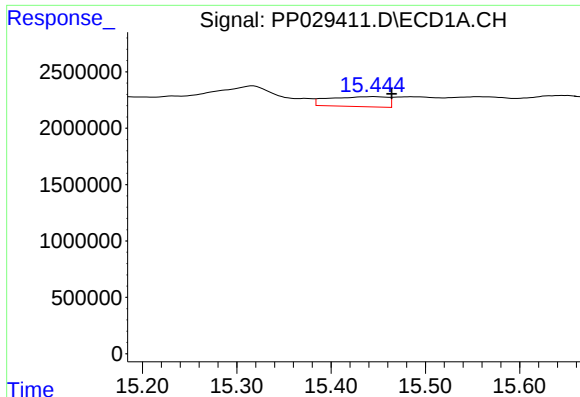

#12 2,4,5-T


R.T.: 15.445 min
Delta R.T.: -0.019 min
Response: 3801453
Conc: 18.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-6(0.5-1.5)

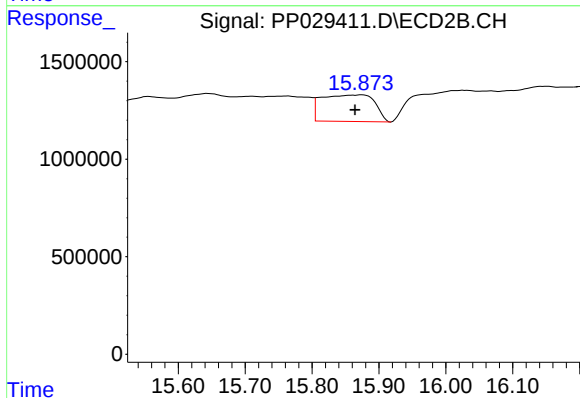


#12 2,4,5-T

R.T.: 15.873 min
Delta R.T.: 0.009 min
Response: 7518570
Conc: 45.41 ng/ml

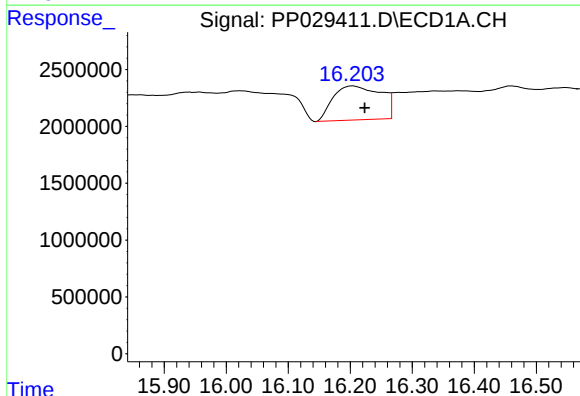


#13 2,4-DB

R.T.: 16.204 min
Delta R.T.: -0.020 min
Response: 15977460
Conc: 836.41 ng/ml

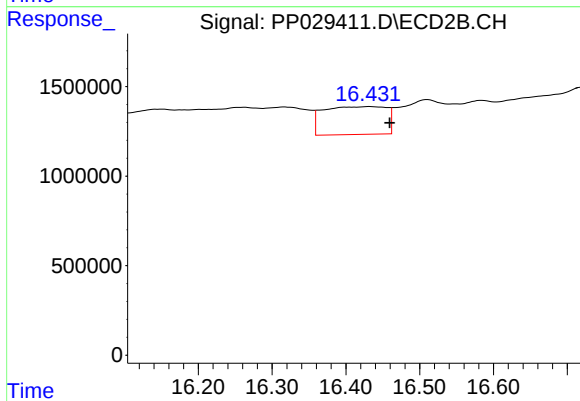

#13 2,4-DB


R.T.: 16.433 min
Delta R.T.: -0.027 min
Response: 9235956
Conc: 410.00 ng/ml

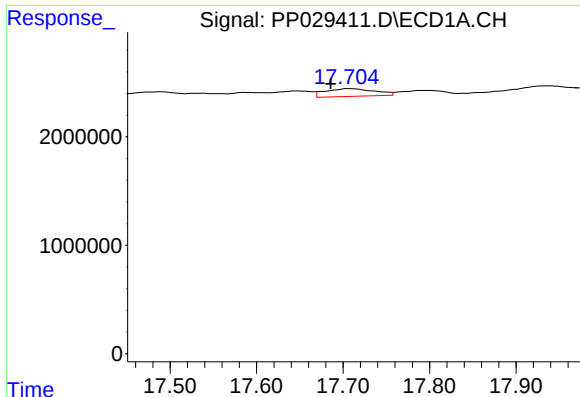

#14 DINOSEB


R.T.: 17.708 min
Delta R.T.: 0.023 min
Response: 2833326
Conc: 19.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-6(0.5-1.5)

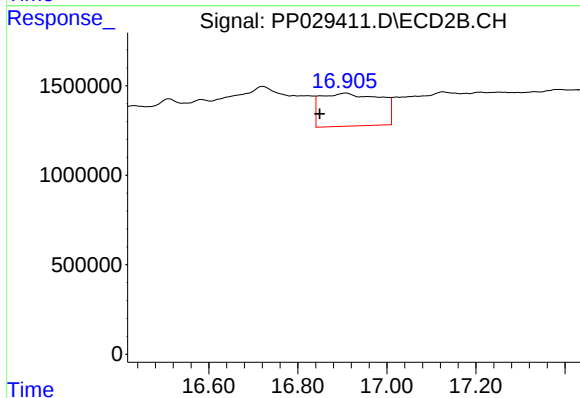


#14 DINOSEB

R.T.: 16.907 min
Delta R.T.: 0.058 min
Response: 17085736
Conc: 130.35 ng/ml

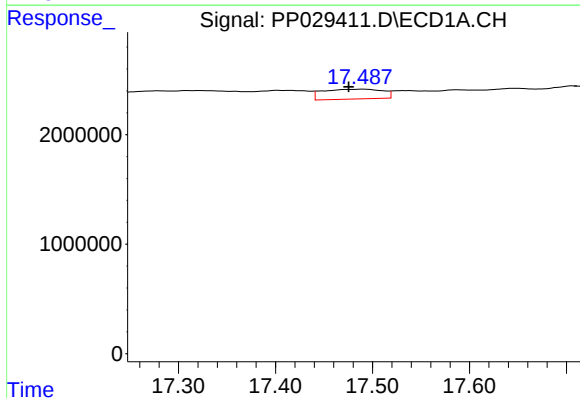

#15 Picloram

R.T.: 17.489 min
Delta R.T.: 0.014 min
Response: 3844219
Conc: 13.83 ng/ml

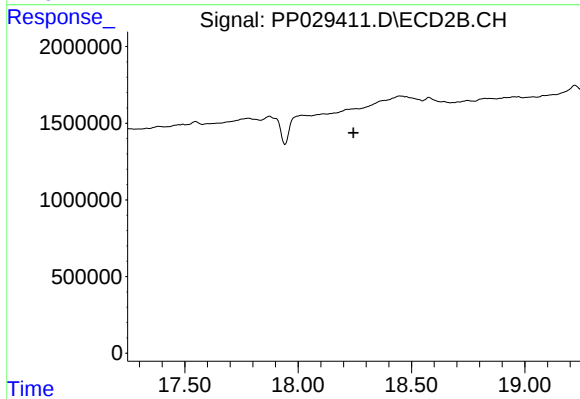

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 18.245 min
Response: 0
Conc: N.D.