

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031919\
 Data File : PP029414.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Mar 2019 20:54
 Operator : EI\MA
 Sample : PB118003BL
 Misc : hexane
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB118003BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 03:36:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 22 02:24:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.926	12.123	23018275	28164975	765.837	742.111
Target Compounds							
8) T	DICHLORPROP	0.000	13.557	0	600572	N.D.	17.764 #
12) T	2,4,5-T	0.000	15.860	0	4802045	N.D.	29.003 #
15) T	Picloram	17.470	0.000	8046139	0	28.938	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031919\
Data File : PP029414.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Mar 2019 20:54
Operator : EI\MA
Sample : PB118003BL
Misc : hexane
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB118003BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 03:36:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
Quant Title : 8080.M
QLast Update : Fri Feb 22 02:24:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

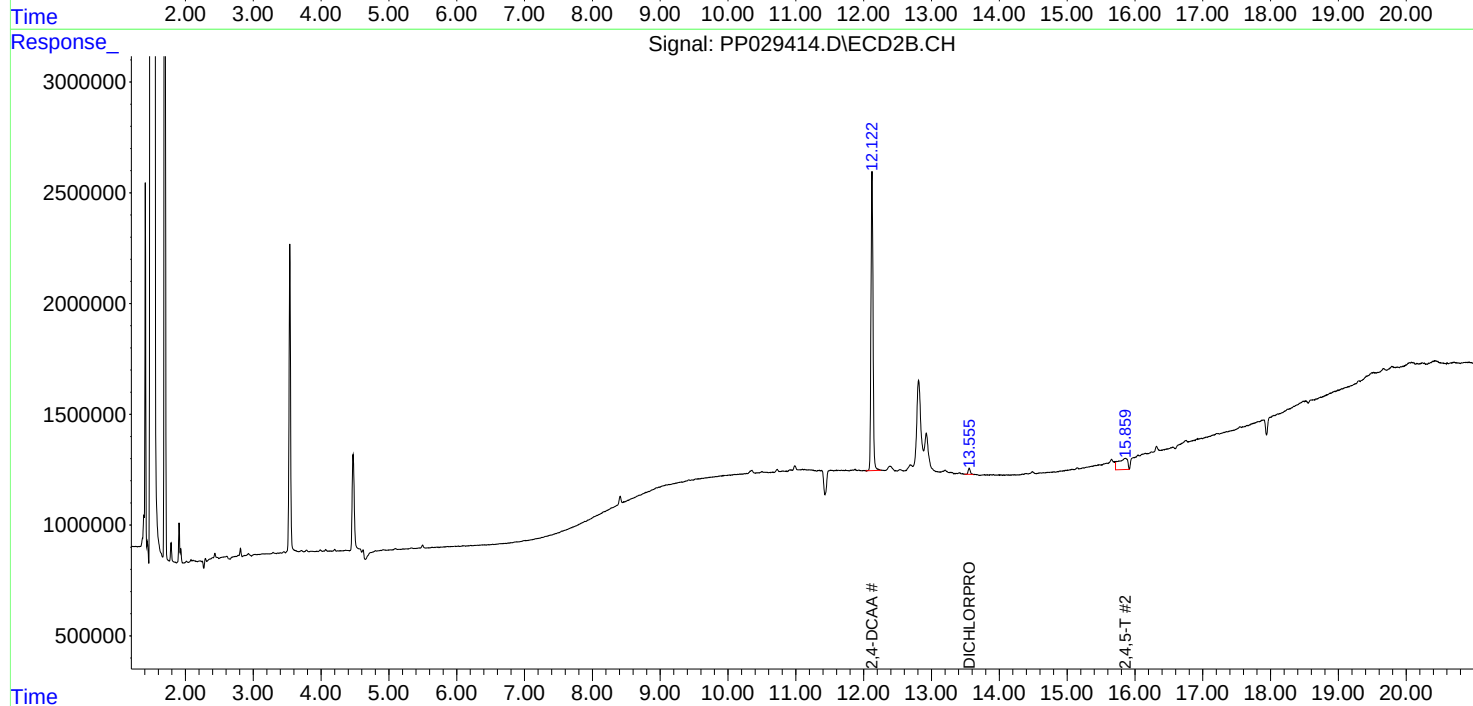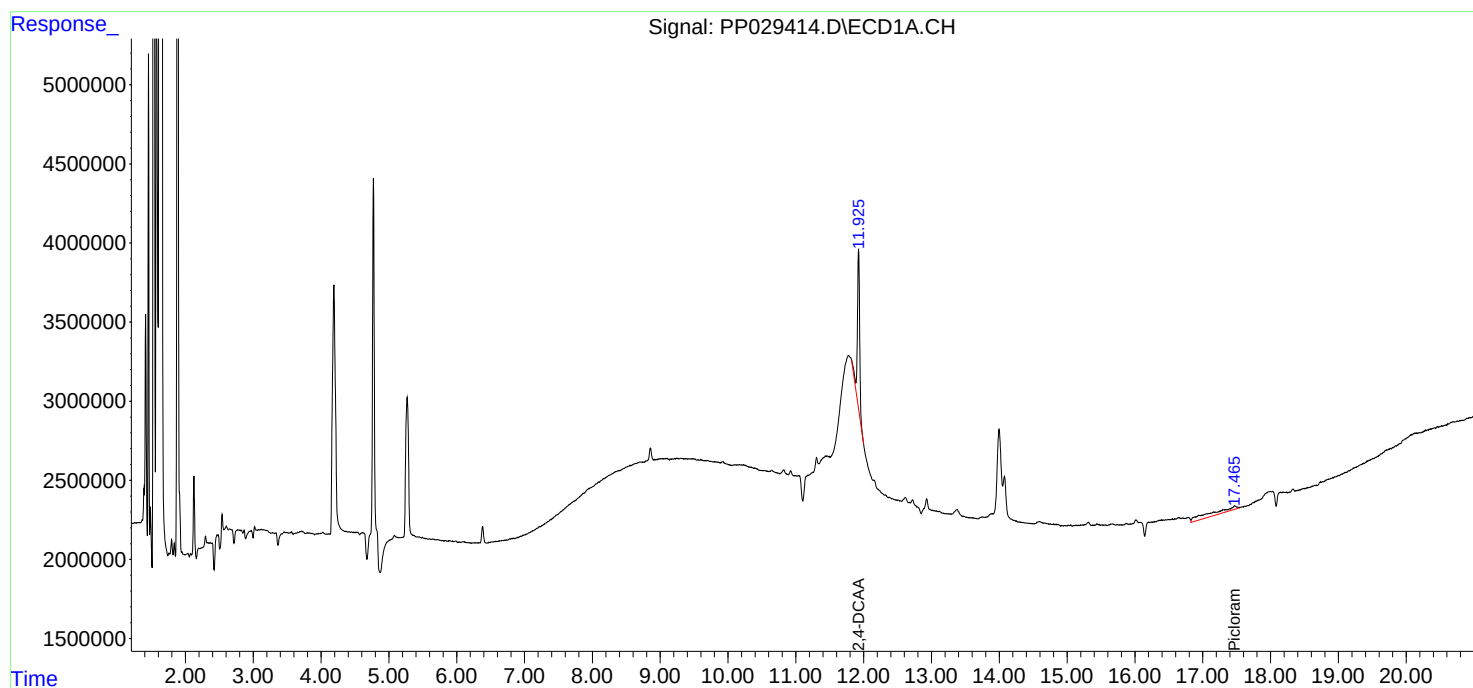


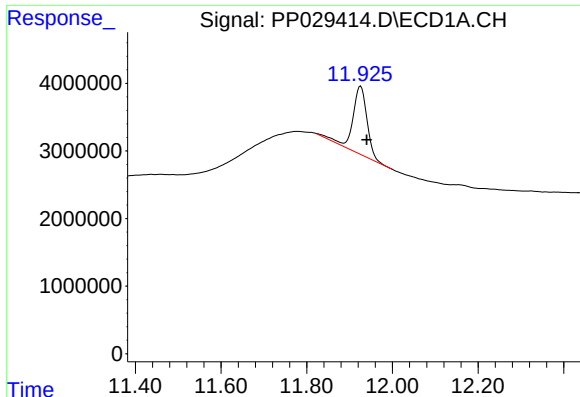

#4 2,4-DCAA


R.T.: 11.926 min
Delta R.T.: -0.015 min
Response: 23018275
Conc: 765.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB118003BL

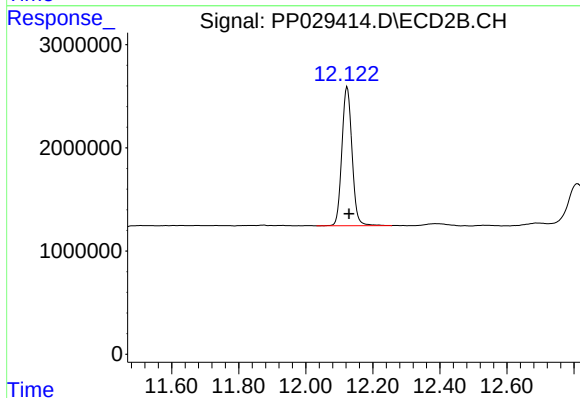


#4 2,4-DCAA

R.T.: 12.123 min
Delta R.T.: -0.005 min
Response: 28164975
Conc: 742.11 ng/ml

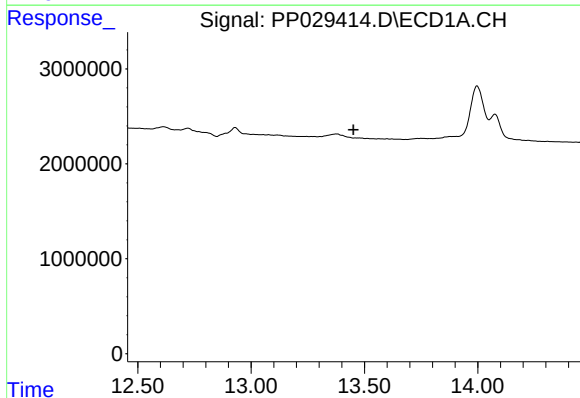


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.452 min
Response: 0
Conc: N.D.

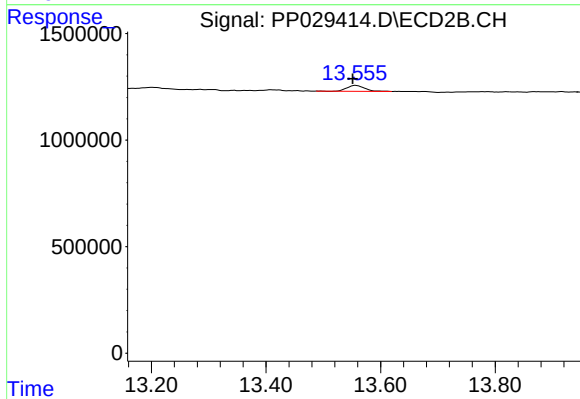

#8 DICHLORPROP


R.T.: 13.557 min
Delta R.T.: 0.005 min
Response: 600572
Conc: 17.76 ng/ml

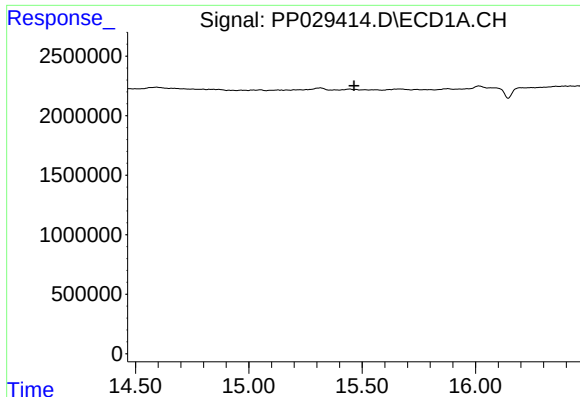

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.464 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PB118003BL

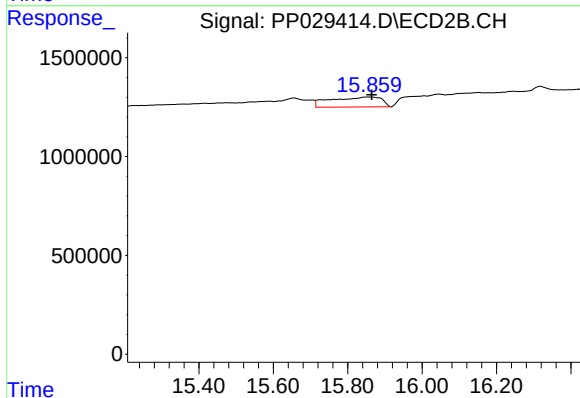


#12 2,4,5-T

R.T.: 15.860 min
Delta R.T.: -0.004 min
Response: 4802045
Conc: 29.00 ng/ml

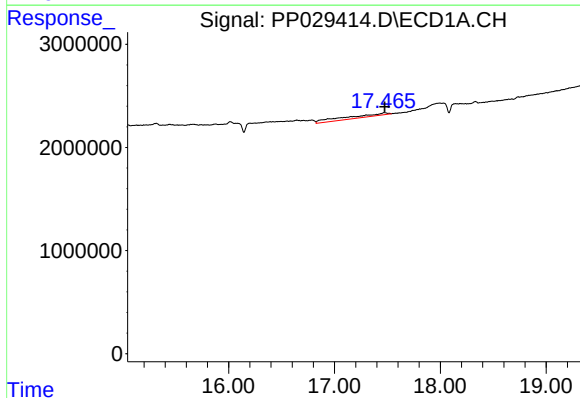

#15 Picloram

R.T.: 17.470 min
Delta R.T.: -0.006 min
Response: 8046139
Conc: 28.94 ng/ml

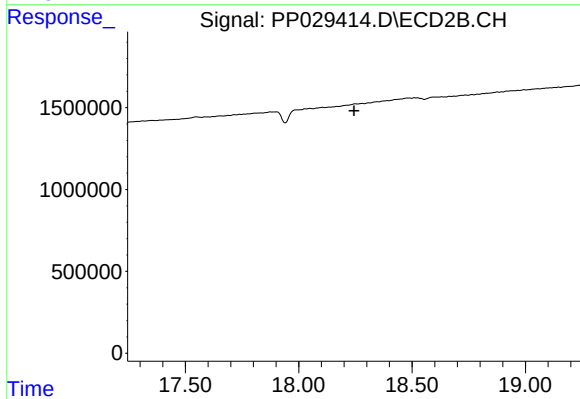

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 18.245 min
Response: 0
Conc: N.D.