

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031919\
 Data File : PP029427.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Mar 2019 2:25
 Operator : EI\MA
 Sample : K1935-11
 Misc : hexane
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-7(9-10)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 03:38:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 22 02:24:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.926	12.123	18884755	21900458	628.311	577.049
Target Compounds							
8) T	DICHLORPROP	13.439	13.556	392950	883403	12.735	26.129 #
10) T	Pentachlo...	0.000	14.605	0	91313	N.D.	0.177 #
11) T	2,4,5-TP ...	0.000	15.152	0	2434893	N.D.	11.971 #
12) T	2,4,5-T	15.438	15.851	691178	8453567	3.274	51.057 #
13) T	2,4-DB	16.227	16.444	16185324	9740699	847.296	432.409 #
14) T	DINOSEB	17.728	16.908	6023949	15453868	41.365	117.903 #
15) T	Picloram	17.487	0.000	15800731	0	56.827	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031919\
Data File : PP029427.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Mar 2019 2:25
Operator : EI\MA
Sample : K1935-11
Misc : hexane
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SB-7(9-10)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 03:38:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
Quant Title : 8080.M
QLast Update : Fri Feb 22 02:24:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

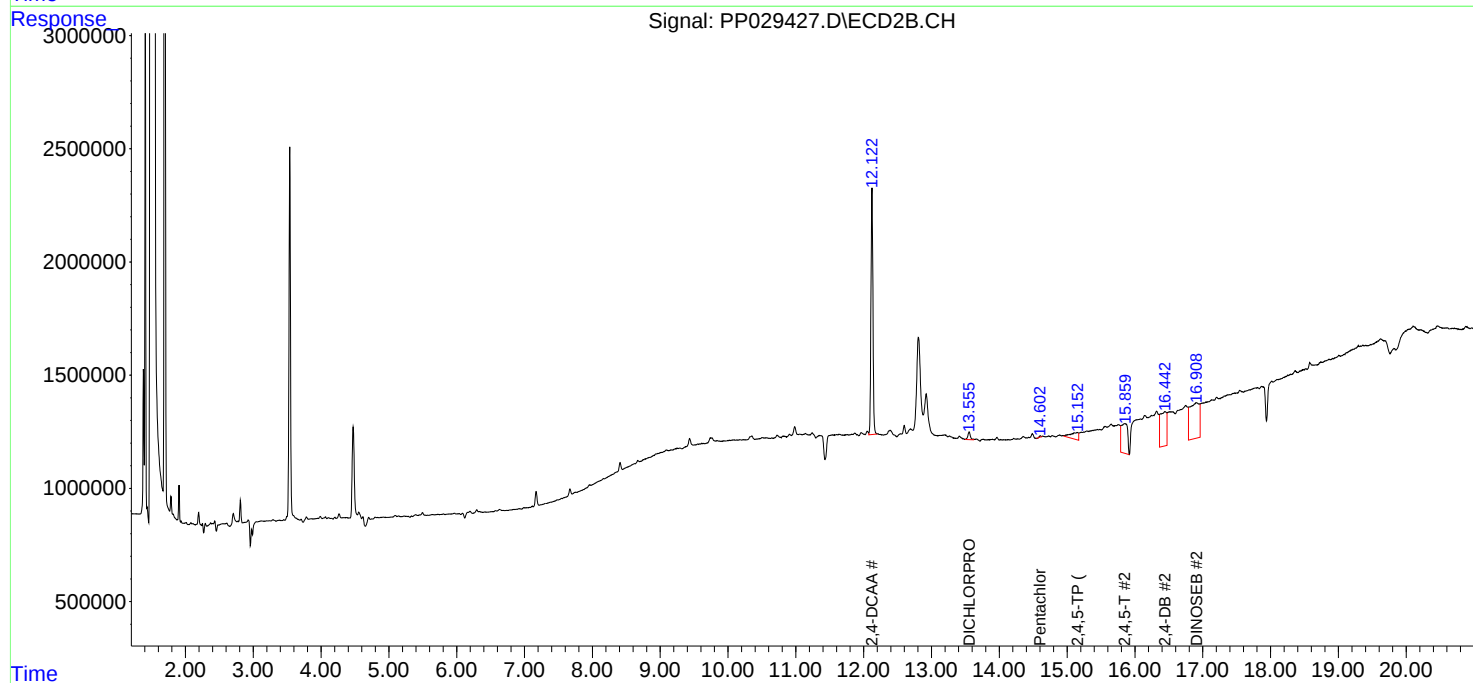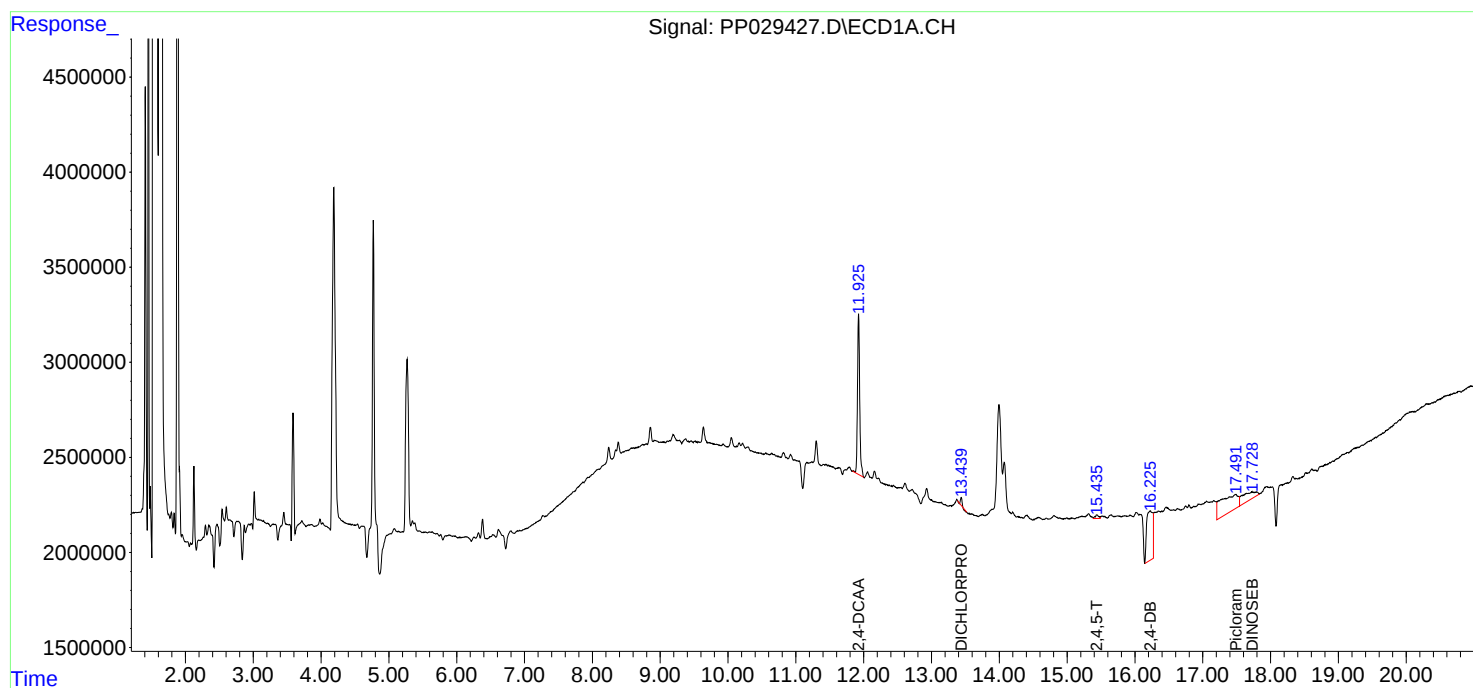


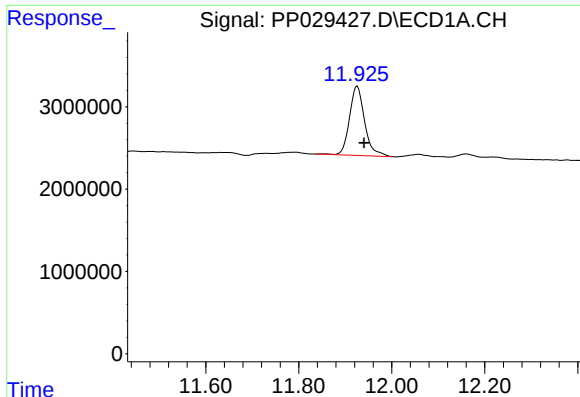

#4 2,4-DCAA


R.T.: 11.926 min
Delta R.T.: -0.015 min
Response: 18884755
Conc: 628.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-7(9-10)

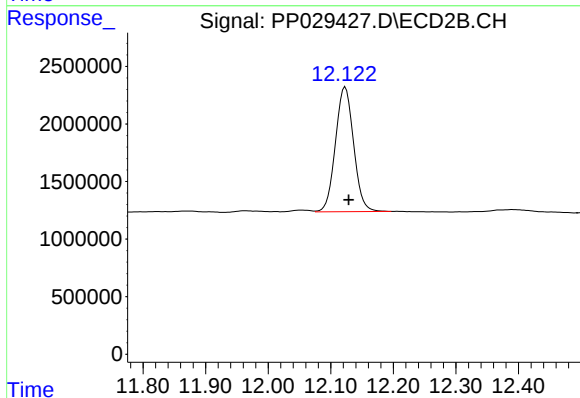


#4 2,4-DCAA

R.T.: 12.123 min
Delta R.T.: -0.005 min
Response: 21900458
Conc: 577.05 ng/ml

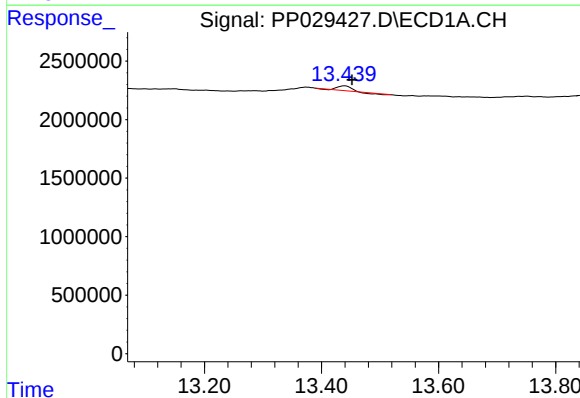


#8 DICHLORPROP

R.T.: 13.439 min
Delta R.T.: -0.013 min
Response: 392950
Conc: 12.74 ng/ml

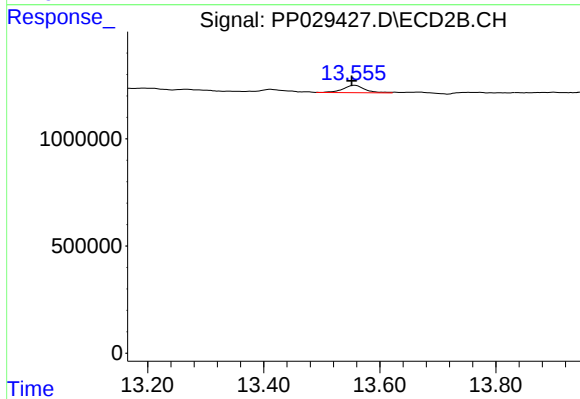

#8 DICHLORPROP


R.T.: 13.556 min
Delta R.T.: 0.005 min
Response: 883403
Conc: 26.13 ng/ml

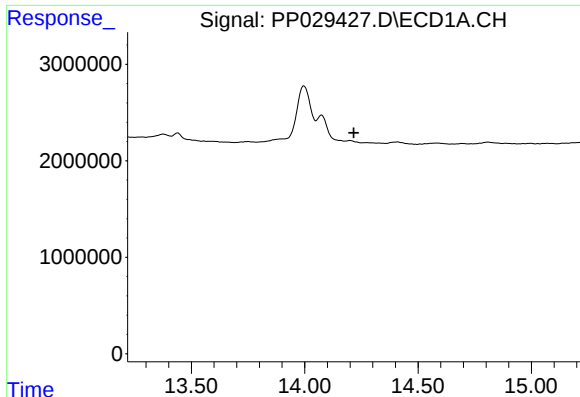

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 14.216 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SB-7(9-10)

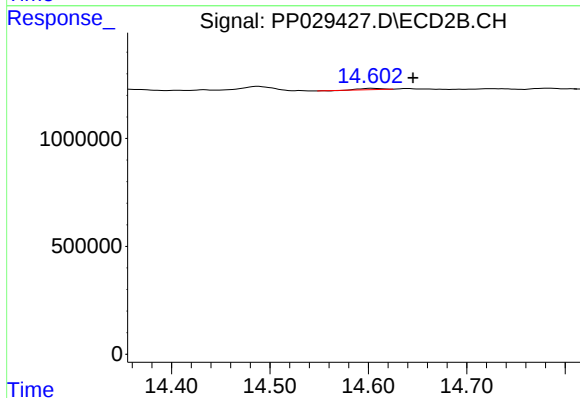


#10 Pentachlorophenol

R.T.: 14.605 min
Delta R.T.: -0.040 min
Response: 91313
Conc: 0.18 ng/ml

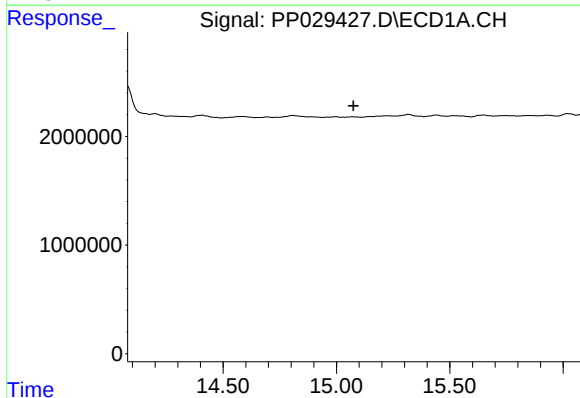


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 15.075 min
Response: 0
Conc: N.D.

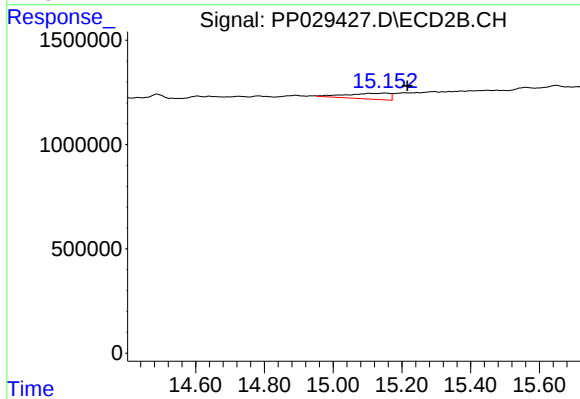

#11 2,4,5-TP (SILVEX)


R.T.: 15.152 min
Delta R.T.: -0.064 min
Response: 2434893
Conc: 11.97 ng/ml

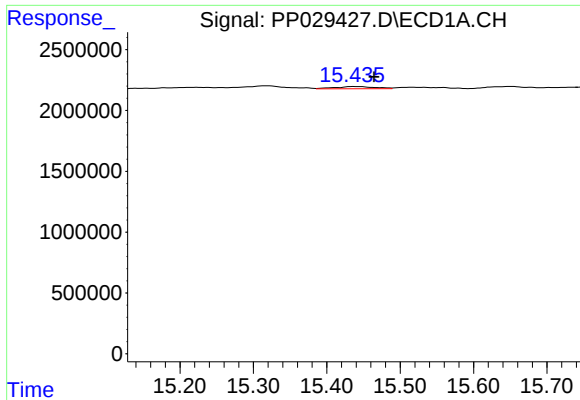

#12 2,4,5-T


R.T.: 15.438 min
Delta R.T.: -0.026 min
Response: 691178
Conc: 3.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-7(9-10)

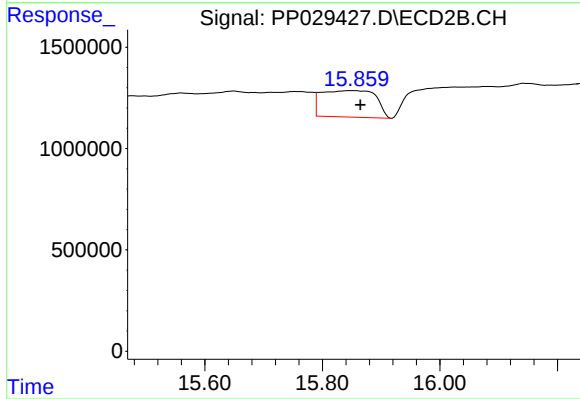


#12 2,4,5-T

R.T.: 15.851 min
Delta R.T.: -0.014 min
Response: 8453567
Conc: 51.06 ng/ml

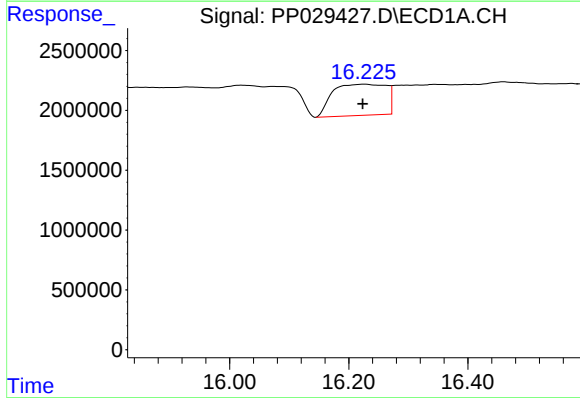


#13 2,4-DB

R.T.: 16.227 min
Delta R.T.: 0.003 min
Response: 16185324
Conc: 847.30 ng/ml

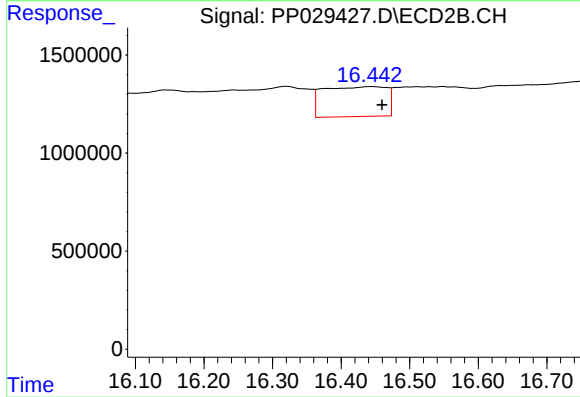

#13 2,4-DB


R.T.: 16.444 min
Delta R.T.: -0.016 min
Response: 9740699
Conc: 432.41 ng/ml

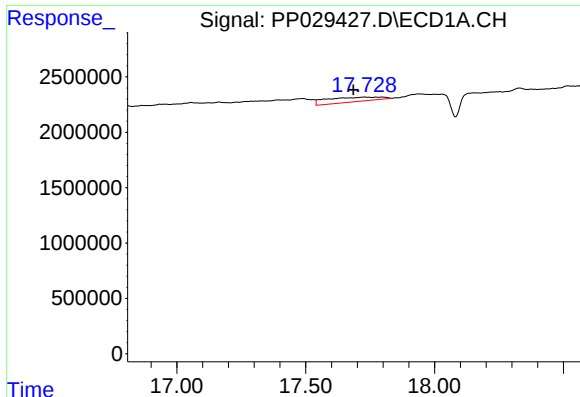

#14 DINOSEB


R.T.: 17.728 min
Delta R.T.: 0.042 min
Response: 6023949
Conc: 41.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-7(9-10)

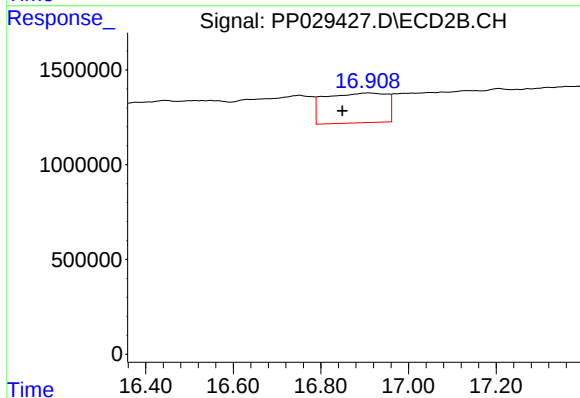


#14 DINOSEB

R.T.: 16.908 min
Delta R.T.: 0.059 min
Response: 15453868
Conc: 117.90 ng/ml

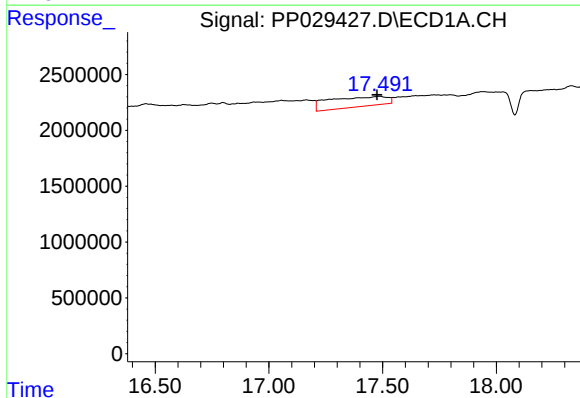

#15 Picloram

R.T.: 17.487 min
Delta R.T.: 0.011 min
Response: 15800731
Conc: 56.83 ng/ml

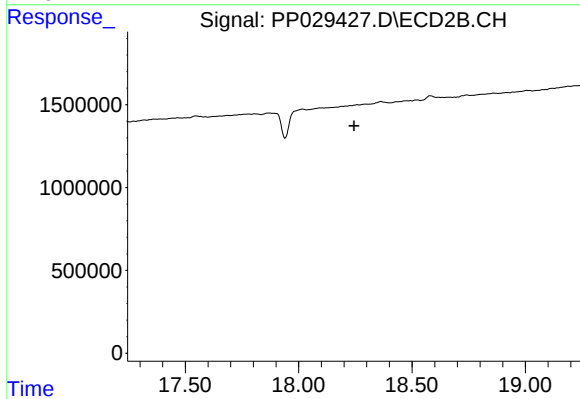

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 18.245 min
Response: 0
Conc: N.D.