

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031919\
 Data File : PP029428.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Mar 2019 2:51
 Operator : EI\MA
 Sample : K1951-01
 Misc : hexane
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FK-GF-03-006-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 03:38:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 22 02:24:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.926	12.123	10262142	14099307	341.430	371.499
Target Compounds							
8) T	DICHLORPROP	0.000	13.556	0	555414	N.D.	16.428 #
10) T	Pentachlo...	14.207	14.642	2633250	830062	4.041	1.613 #
11) T	2,4,5-TP ...	0.000	15.150	0	88384	N.D.	0.435 #
12) T	2,4,5-T	15.441	0.000	491222	0	2.327	N.D. #
13) T	2,4-DB	16.201	16.448	11841839	6597459	619.916	292.874 #
14) T	DINOSEB	17.649	16.859	5668411	5539576	38.923	42.264
15) T	Picloram	17.478	18.261	6046934	6695389	21.748	29.754 #
16) T	DCPA	0.000	18.113	0	3913816	N.D.	16.841 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031919\
Data File : PP029428.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Mar 2019 2:51
Operator : EI\MA
Sample : K1951-01
Misc : hexane
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
FK-GF-03-006-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 03:38:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
Quant Title : 8080.M
QLast Update : Fri Feb 22 02:24:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

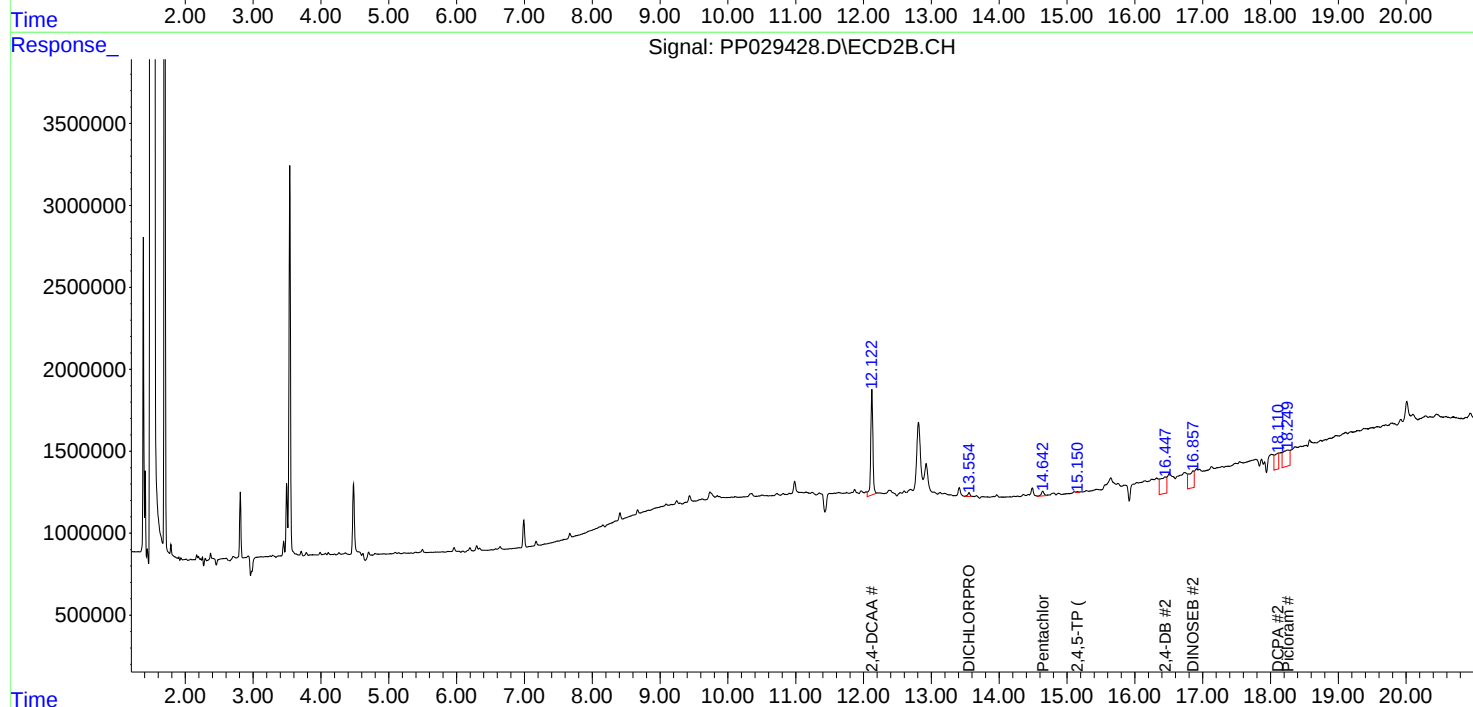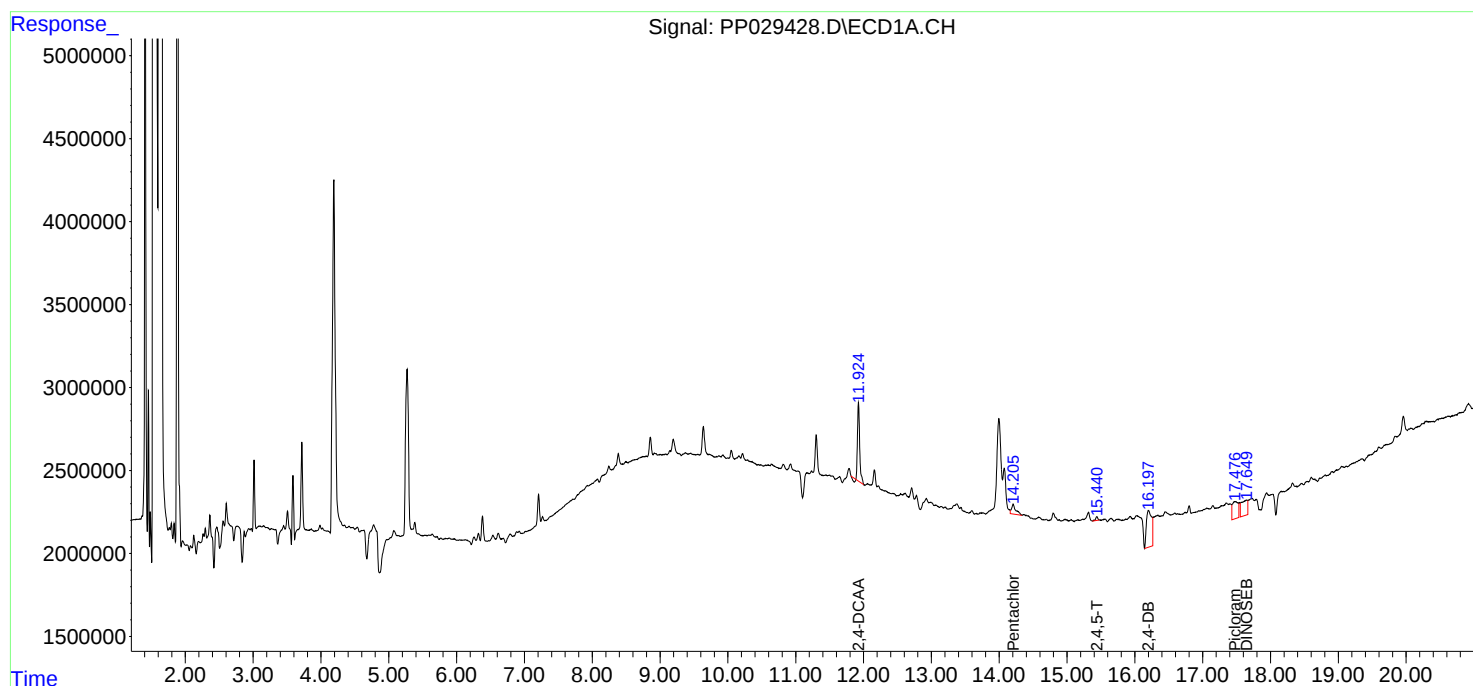


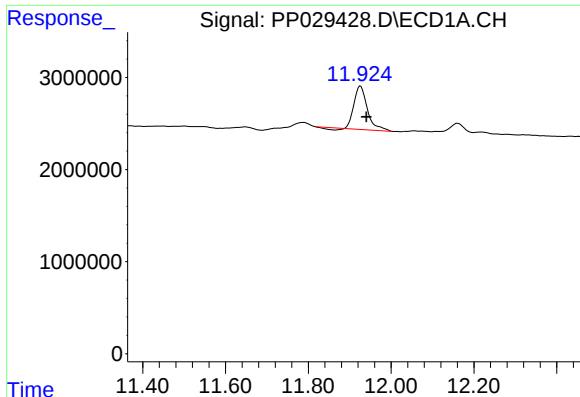

#4 2,4-DCAA


R.T.: 11.926 min
Delta R.T.: -0.015 min
Response: 10262142
Conc: 341.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-GF-03-006-A

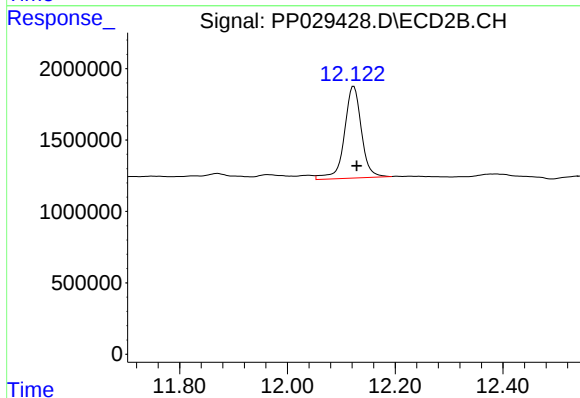


#4 2,4-DCAA

R.T.: 12.123 min
Delta R.T.: -0.005 min
Response: 14099307
Conc: 371.50 ng/ml

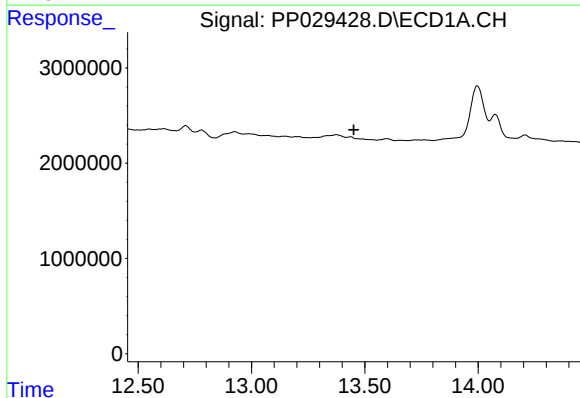


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.452 min
Response: 0
Conc: N.D.

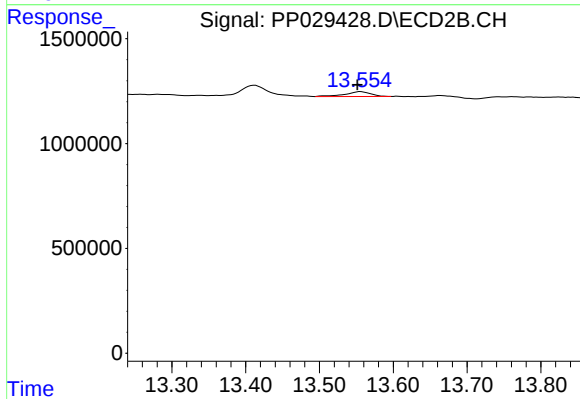

#8 DICHLORPROP


R.T.: 13.556 min
Delta R.T.: 0.004 min
Response: 555414
Conc: 16.43 ng/ml

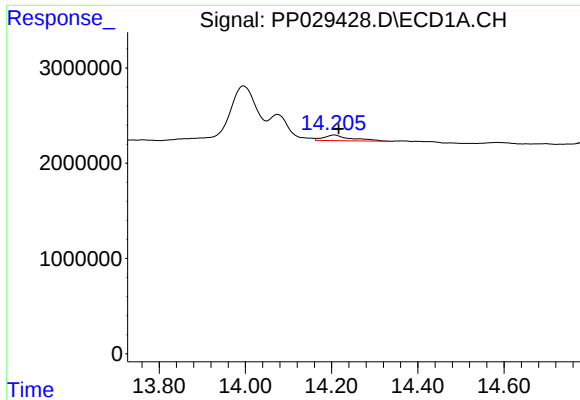

#10 Pentachlorophenol


R.T.: 14.207 min
Delta R.T.: -0.010 min
Response: 2633250
Conc: 4.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-GF-03-006-A

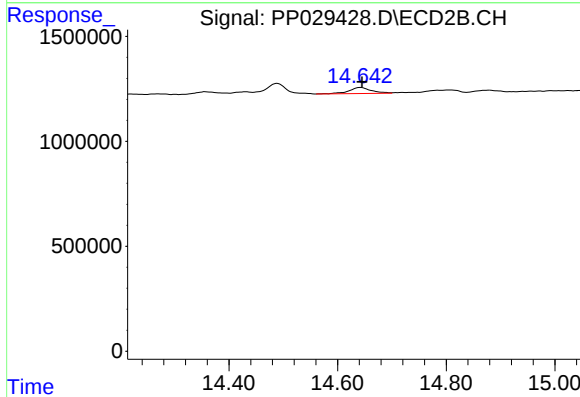


#10 Pentachlorophenol

R.T.: 14.642 min
Delta R.T.: -0.003 min
Response: 830062
Conc: 1.61 ng/ml

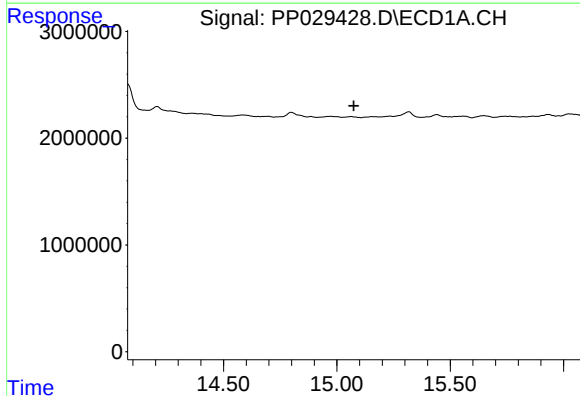


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 15.075 min
Response: 0
Conc: N.D.

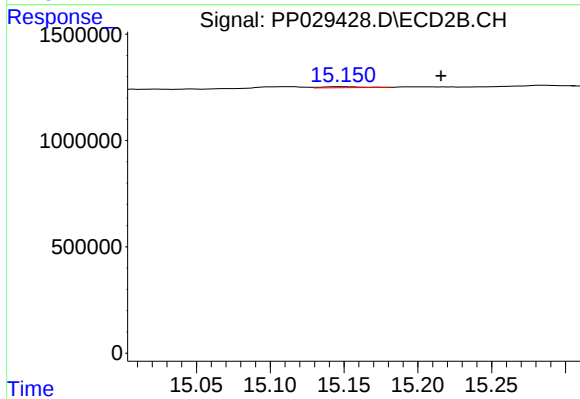

#11 2,4,5-TP (SILVEX)


R.T.: 15.150 min
Delta R.T.: -0.065 min
Response: 88384
Conc: 0.43 ng/ml

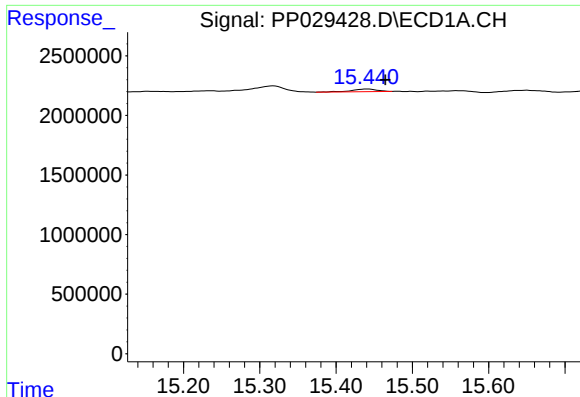

#12 2,4,5-T


R.T.: 15.441 min
Delta R.T.: -0.023 min
Response: 491222
Conc: 2.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-GF-03-006-A

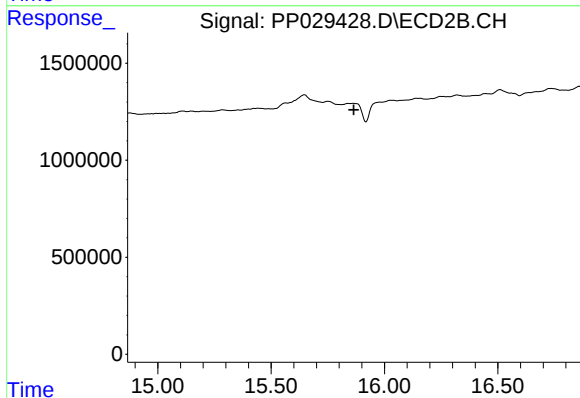


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 15.864 min
Response: 0
Conc: N.D.

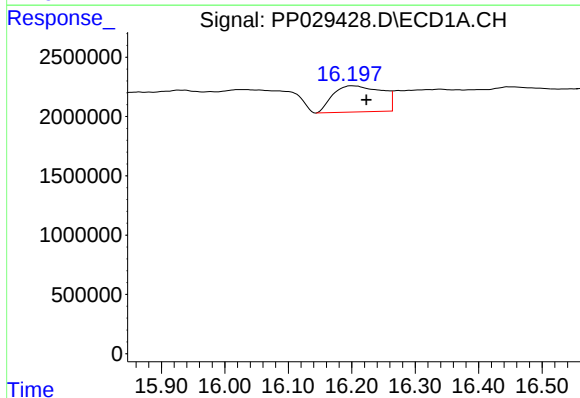


#13 2,4-DB

R.T.: 16.201 min
Delta R.T.: -0.023 min
Response: 11841839
Conc: 619.92 ng/ml

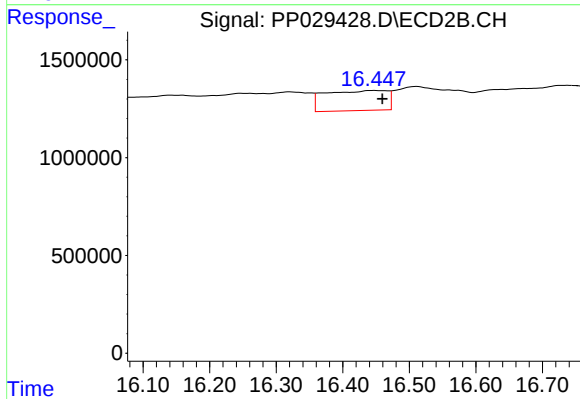

#13 2,4-DB


R.T.: 16.448 min
Delta R.T.: -0.012 min
Response: 6597459
Conc: 292.87 ng/ml

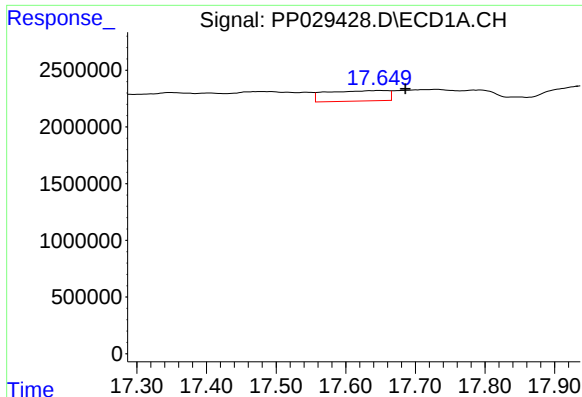

#14 DINOSEB


R.T.: 17.649 min
Delta R.T.: -0.037 min
Response: 5668411
Conc: 38.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-GF-03-006-A

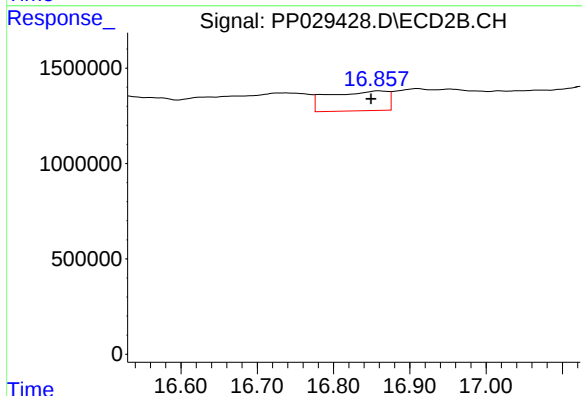


#14 DINOSEB

R.T.: 16.859 min
Delta R.T.: 0.010 min
Response: 5539576
Conc: 42.26 ng/ml

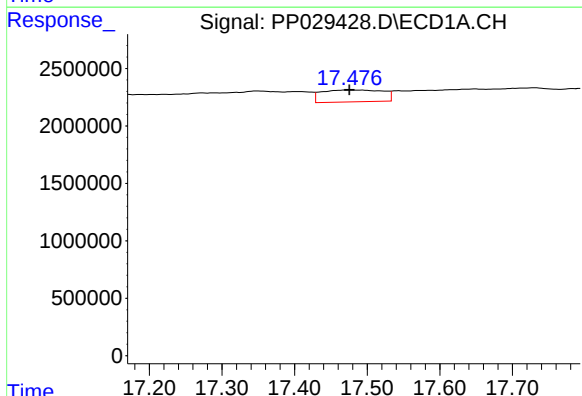


#15 Picloram

R.T.: 17.478 min
Delta R.T.: 0.003 min
Response: 6046934
Conc: 21.75 ng/ml

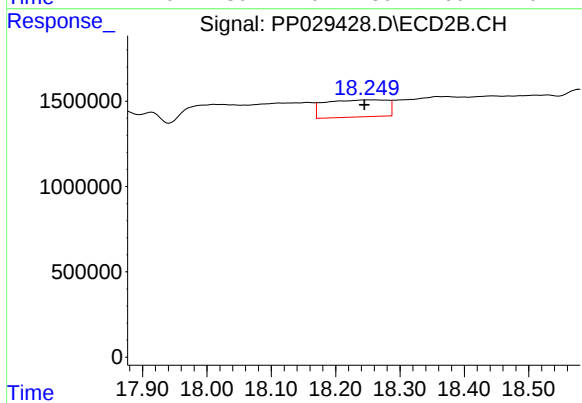

#15 Picloram


R.T.: 18.261 min
Delta R.T.: 0.017 min
Response: 6695389
Conc: 29.75 ng/ml

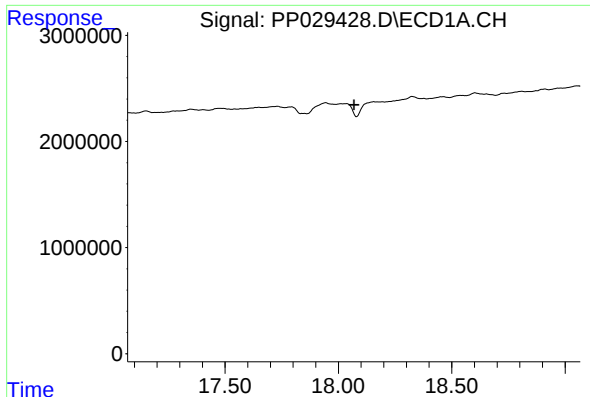

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 18.069 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
FK-GF-03-006-A

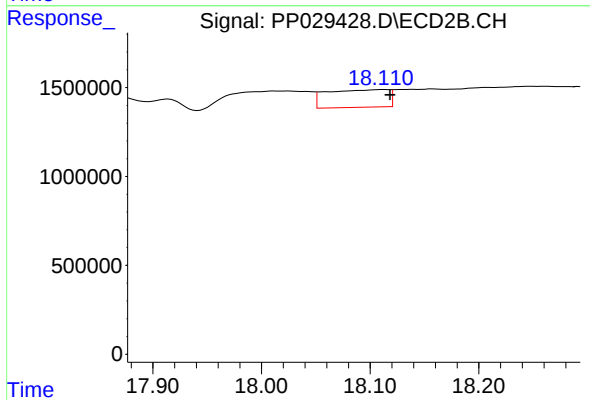

#16 DCPA

R.T.: 18.113 min
Delta R.T.: -0.005 min
Response: 3913816
Conc: 16.84 ng/ml