

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031919\
 Data File : PP029430.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Mar 2019 3:42
 Operator : EI\MA
 Sample : K1951-03MS
 Misc : hexane
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FK-GF-03-006-BMS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 04:54:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 22 02:24:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.928	12.126	1025171	1103593	34.108	29.078
Target Compounds							
8) T	DICHLORPROP	0.000	13.555	0	644928	N.D.	19.076 #
10) T	Pentachlo...	14.207	14.641	49587764	38932715	76.098	75.647
11) T	2,4,5-TP ...	15.064	15.213	1367621	1035304	5.765	5.090
12) T	2,4,5-T	15.452	15.863	712402	3603177	3.374	21.762 #
13) T	2,4-DB	16.213	16.457	10770981	19568415	563.857	868.681 #
14) T	DINOSEB	17.673	16.846	27834700	7388145	191.132	56.367 #
15) T	Picloram	17.465	18.245	19176918	10380789	68.969	46.132 #
16) T	DCPA	0.000	18.118	0	7479574	N.D.	32.185 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031919\
Data File : PP029430.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Mar 2019 3:42
Operator : EI\MA
Sample : K1951-03MS
Misc : hexane
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
FK-GF-03-006-BMS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 04:54:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
Quant Title : 8080.M
QLast Update : Fri Feb 22 02:24:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

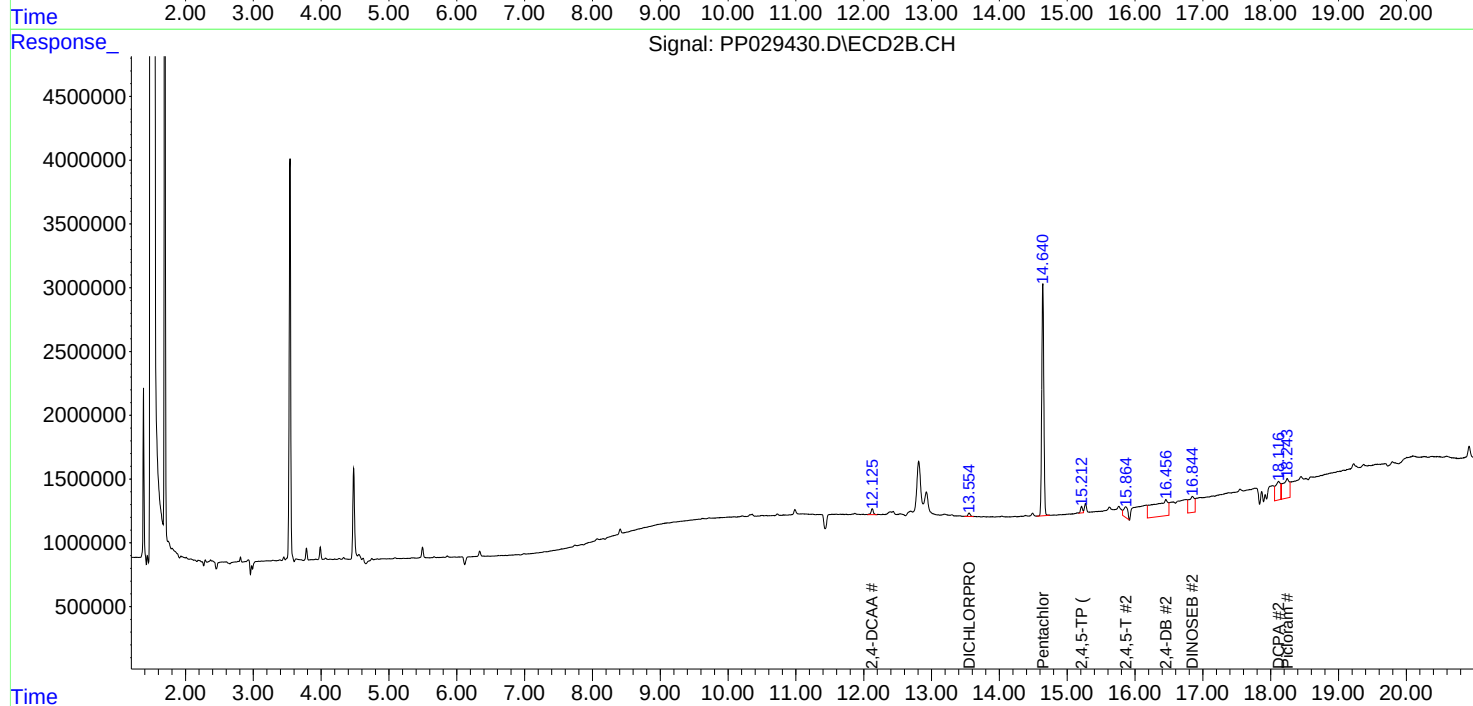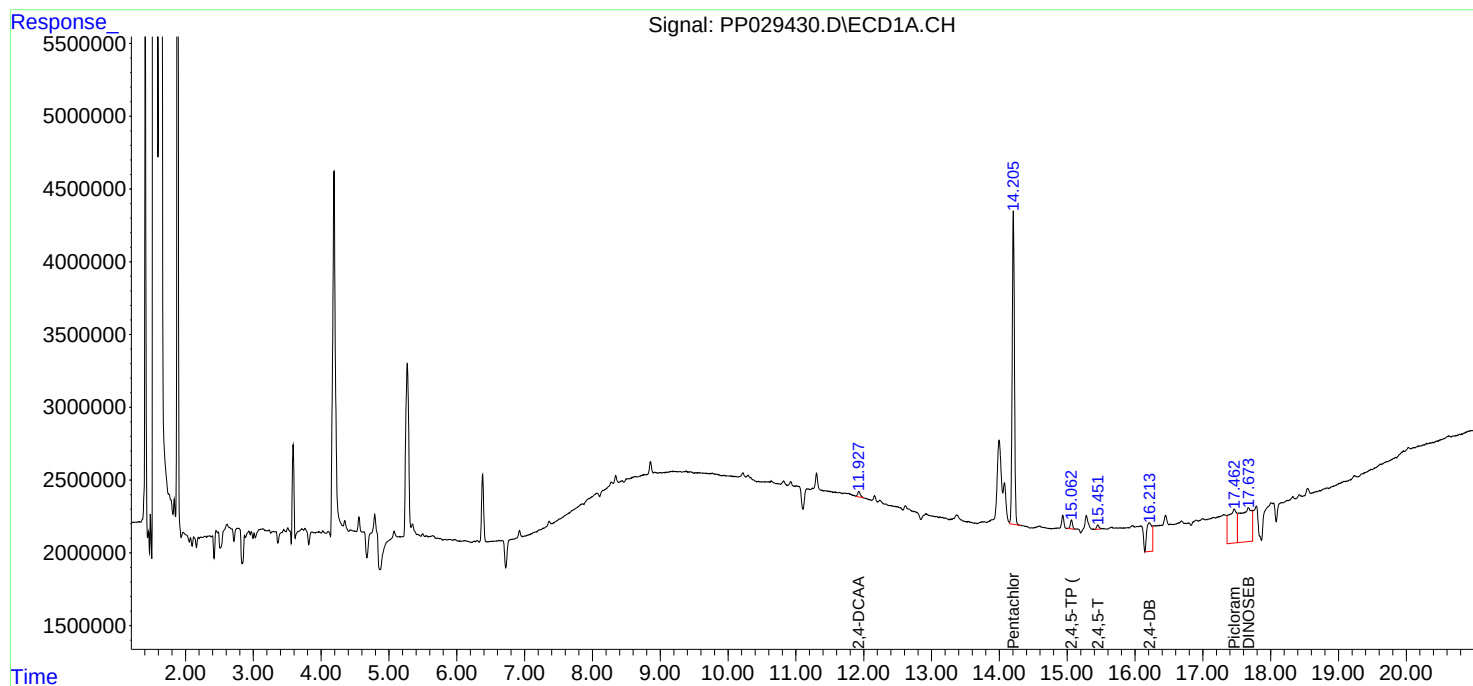


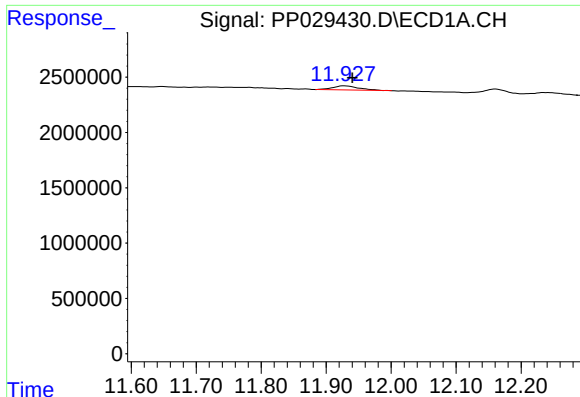

#4 2,4-DCAA


R.T.: 11.928 min
Delta R.T.: -0.013 min
Response: 1025171
Conc: 34.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-GF-03-006-BMS

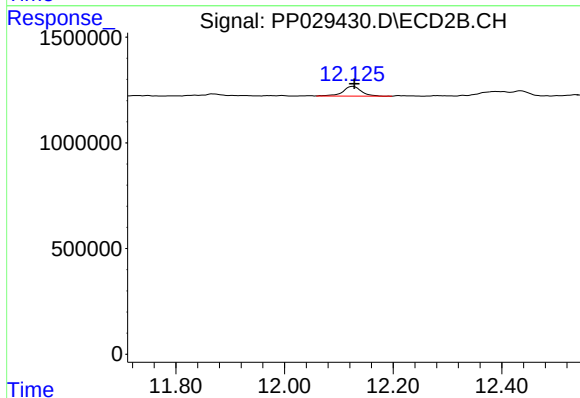


#4 2,4-DCAA

R.T.: 12.126 min
Delta R.T.: -0.003 min
Response: 1103593
Conc: 29.08 ng/ml

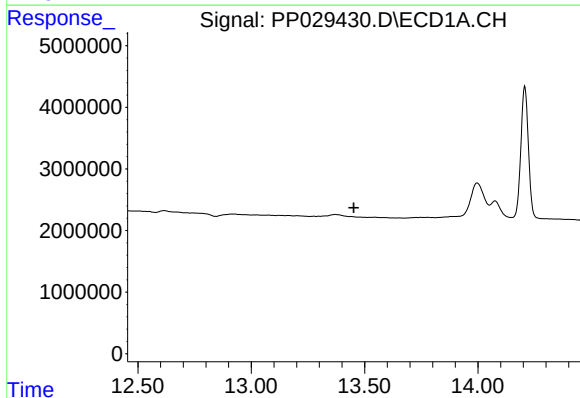


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.452 min
Response: 0
Conc: N.D.

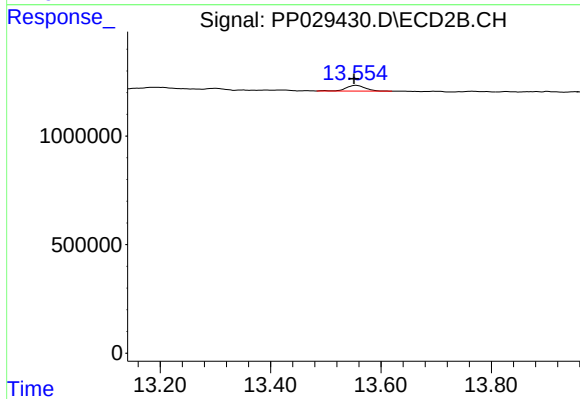

#8 DICHLORPROP


R.T.: 13.555 min
Delta R.T.: 0.003 min
Response: 644928
Conc: 19.08 ng/ml

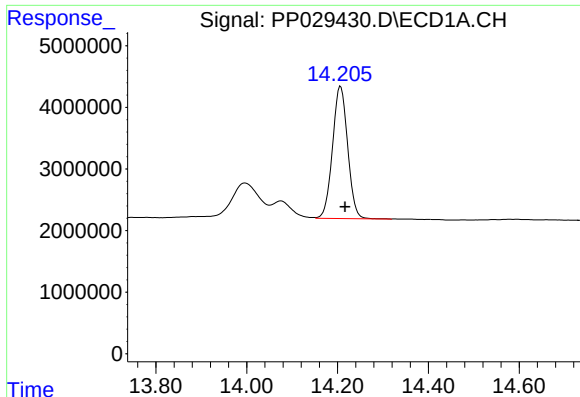

#10 Pentachlorophenol


R.T.: 14.207 min
Delta R.T.: -0.010 min
Response: 49587764
Conc: 76.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-GF-03-006-BMS

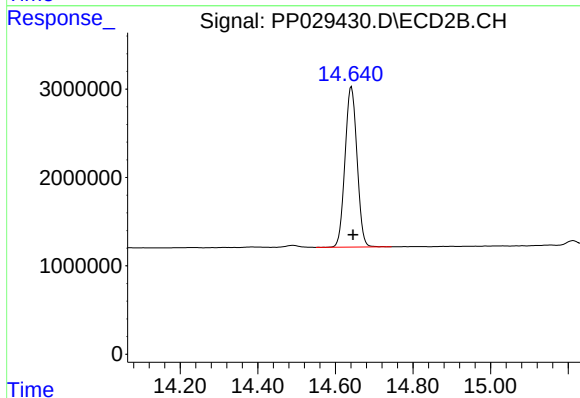


#10 Pentachlorophenol

R.T.: 14.641 min
Delta R.T.: -0.004 min
Response: 38932715
Conc: 75.65 ng/ml

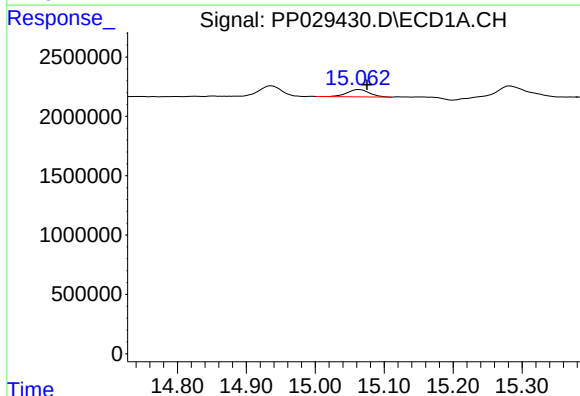


#11 2,4,5-TP (SILVEX)

R.T.: 15.064 min
Delta R.T.: -0.012 min
Response: 1367621
Conc: 5.76 ng/ml

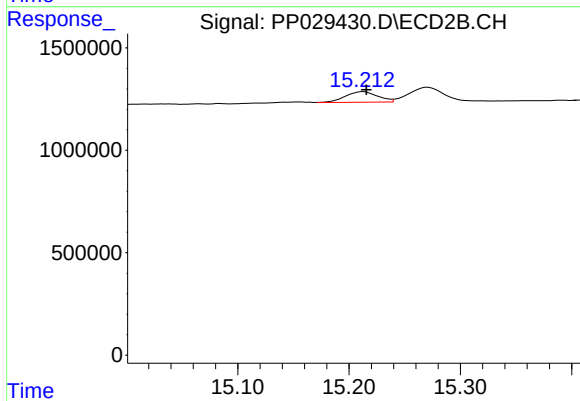

#11 2,4,5-TP (SILVEX)


R.T.: 15.213 min
Delta R.T.: -0.003 min
Response: 1035304
Conc: 5.09 ng/ml

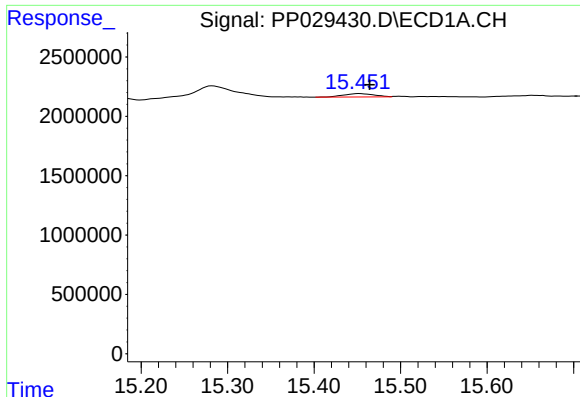

#12 2,4,5-T


R.T.: 15.452 min
Delta R.T.: -0.012 min
Response: 712402
Conc: 3.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-GF-03-006-BMS

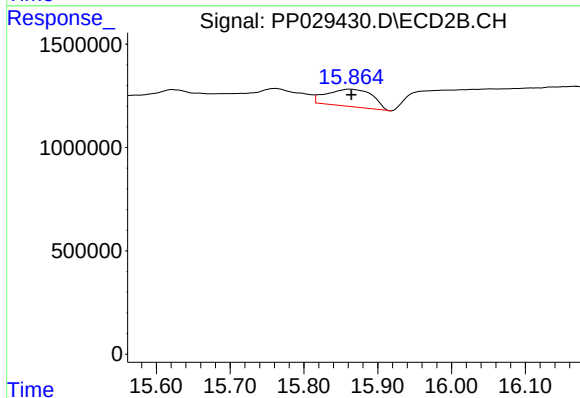


#12 2,4,5-T

R.T.: 15.863 min
Delta R.T.: -0.001 min
Response: 3603177
Conc: 21.76 ng/ml

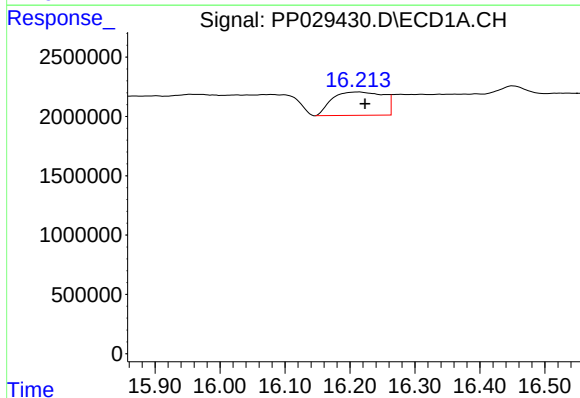


#13 2,4-DB

R.T.: 16.213 min
Delta R.T.: -0.010 min
Response: 10770981
Conc: 563.86 ng/ml

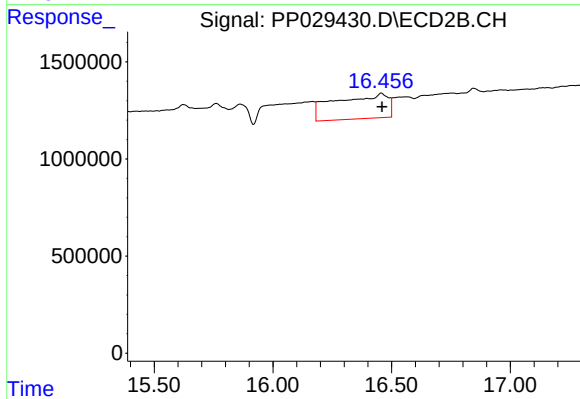

#13 2,4-DB


R.T.: 16.457 min
Delta R.T.: -0.003 min
Response: 19568415
Conc: 868.68 ng/ml

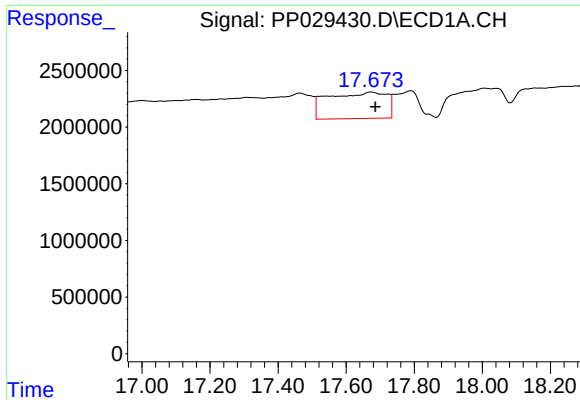

#14 DINOSEB


R.T.: 17.673 min
Delta R.T.: -0.013 min
Response: 27834700
Conc: 191.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-GF-03-006-BMS

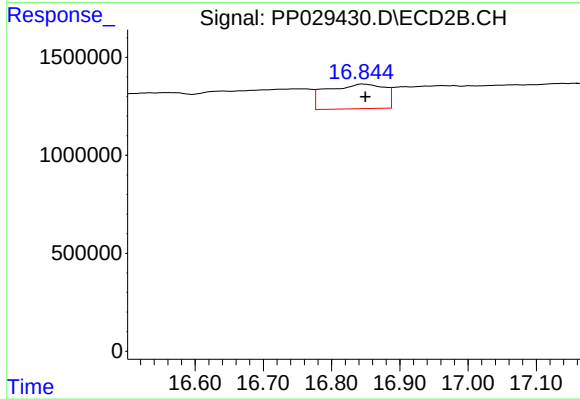


#14 DINOSEB

R.T.: 16.846 min
Delta R.T.: -0.003 min
Response: 7388145
Conc: 56.37 ng/ml

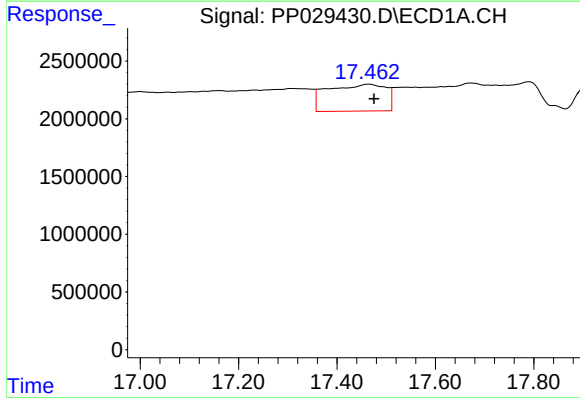


#15 Picloram

R.T.: 17.465 min
Delta R.T.: -0.011 min
Response: 19176918
Conc: 68.97 ng/ml

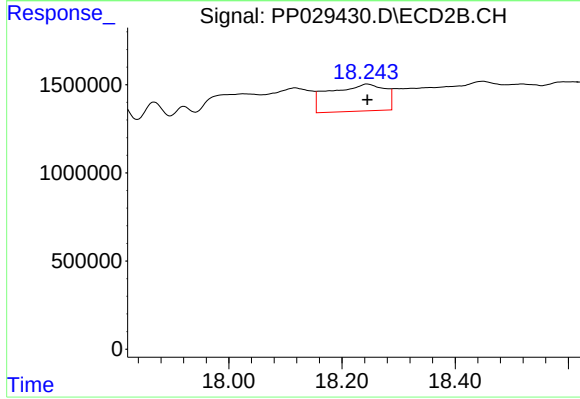

#15 Picloram


R.T.: 18.245 min
Delta R.T.: 0.000 min
Response: 10380789
Conc: 46.13 ng/ml

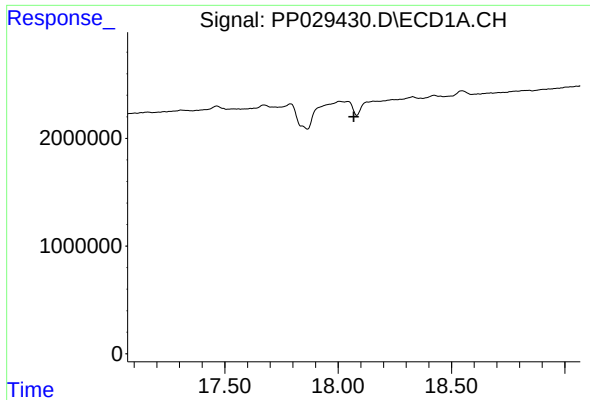

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 18.069 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
FK-GF-03-006-BMS

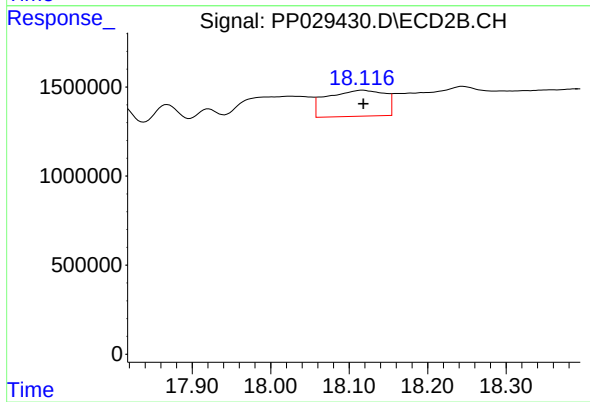

#16 DCPA

R.T.: 18.118 min
Delta R.T.: 0.000 min
Response: 7479574
Conc: 32.18 ng/ml