

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031921\
 Data File : PP034157.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Mar 2021 10:20
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 02:11:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.852	4.262	1771802	924188	21.091	20.884
2) SA Decachlor...	10.779	9.581	1675853	567359	21.355	21.500
Target Compounds						
9) L2 AR-1221-2	5.201	4.617	20620	11350	29.962	32.004



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031921\
Data File : PP034157.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Mar 2021 10:20
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 02:11:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

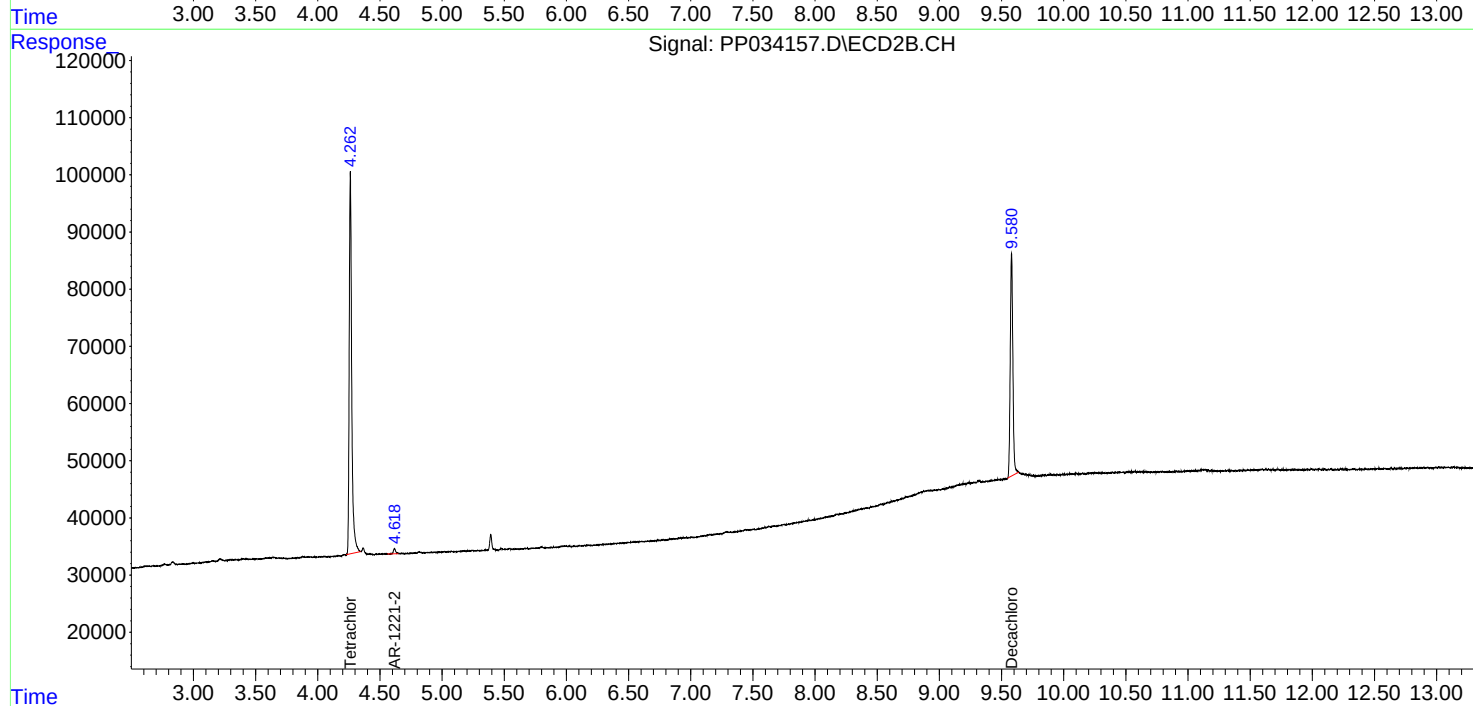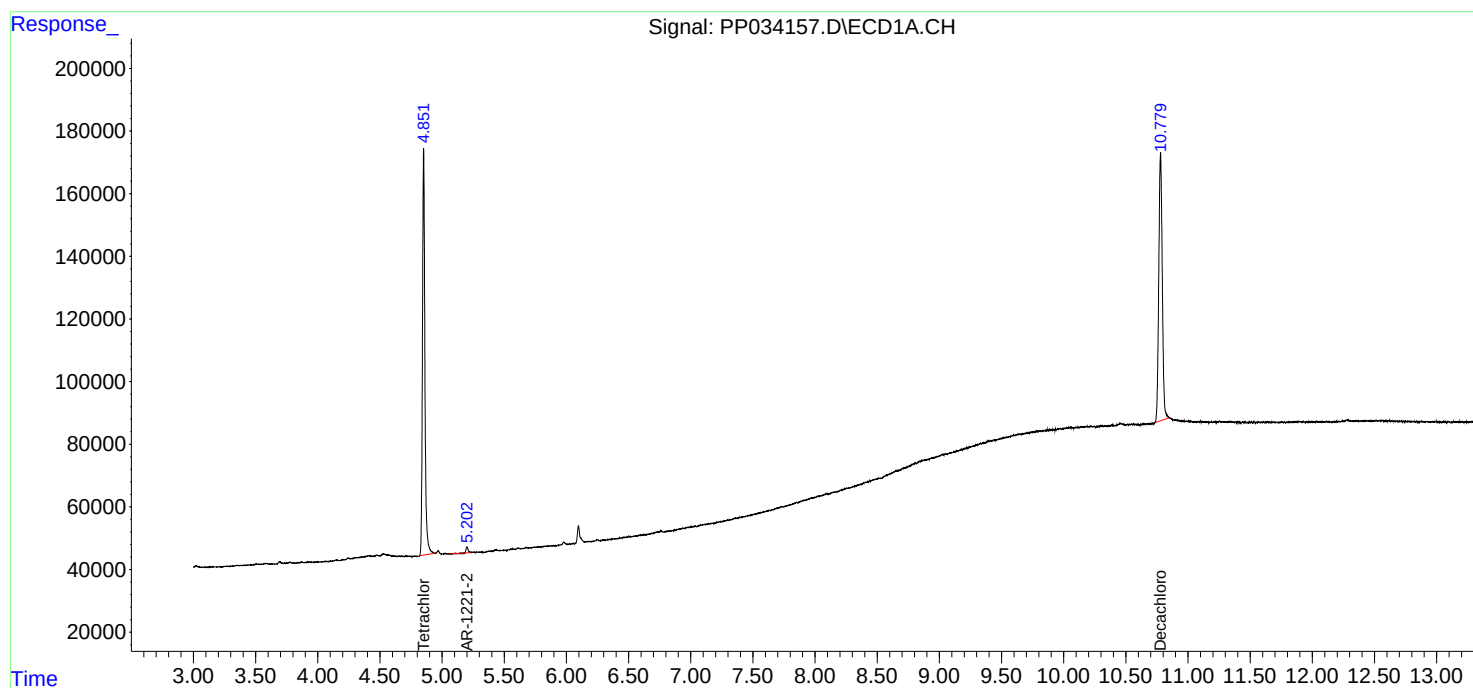


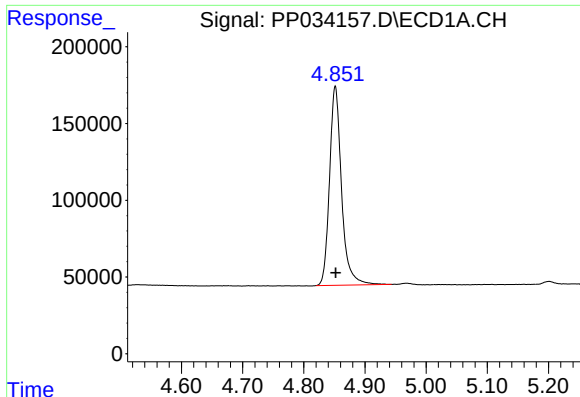

#1 Tetrachloro-m-xylene


R.T.: 4.852 min
Delta R.T.: 0.000 min
Response: 1771802
Conc: 21.09 ng/ml

Instrument :
ECD_P
ClientSampleId :

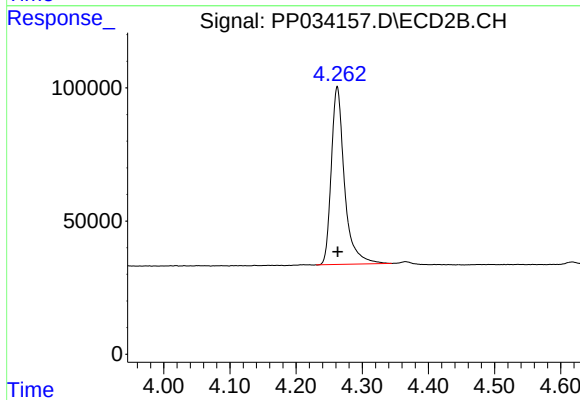


#1 Tetrachloro-m-xylene

R.T.: 4.262 min
Delta R.T.: 0.000 min
Response: 924188
Conc: 20.88 ng/ml

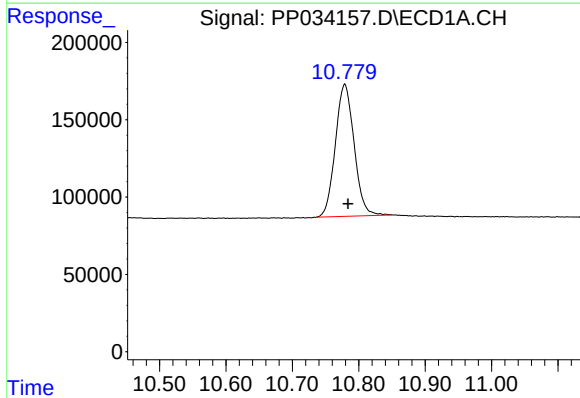


#2 Decachlorobiphenyl

R.T.: 10.779 min
Delta R.T.: -0.005 min
Response: 1675853
Conc: 21.35 ng/ml

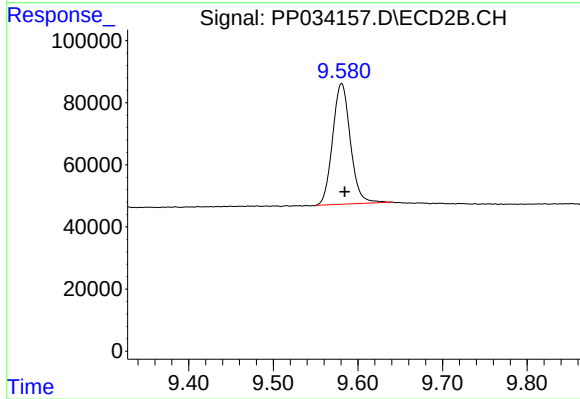

#2 Decachlorobiphenyl


R.T.: 9.581 min
Delta R.T.: -0.004 min
Response: 567359
Conc: 21.50 ng/ml

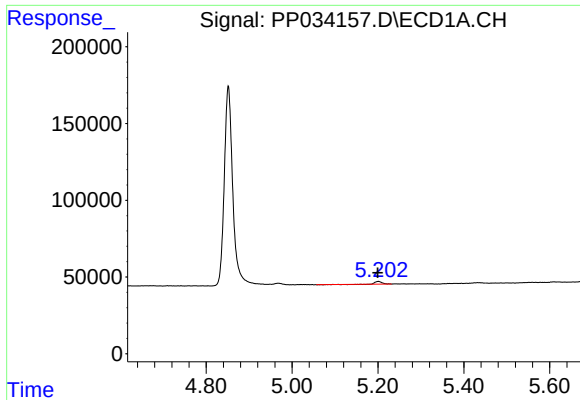

#9 AR-1221-2

R.T.: 5.201 min
Delta R.T.: 0.001 min
Response: 20620
Conc: 29.96 ng/ml

Instrument :
ECD_P
ClientSampleId :

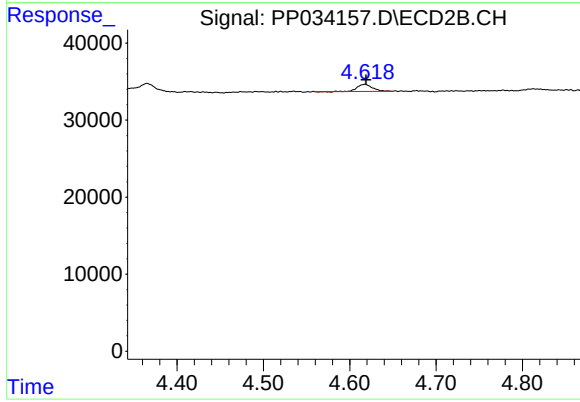

#9 AR-1221-2

R.T.: 4.617 min
Delta R.T.: -0.002 min
Response: 11350
Conc: 32.00 ng/ml