

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031921\
 Data File : PP034160.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Mar 2021 11:11
 Operator : DD\AJ
 Sample : M1702-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CT-3

Manual Integrations
 APPROVED

Ankita
 3/22/2021 2:40:59 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 02:35:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.851	4.262	1621396	856611	19.301	19.357
2)	SA Decachlor...	10.779	9.581	1643438	579480	20.942	21.959
Target Compounds							
21)	L5 AR-1248-1	6.166	5.518	135896	59692	90.892	86.775
22)	L5 AR-1248-2	6.459	5.780	123281	51299	58.749	51.371
23)	L5 AR-1248-3	6.675	5.827	190068	72064	74.634	68.335
24)	L5 AR-1248-4	7.101	6.013	209150	57276	80.949m	46.673m#
25)	L5 AR-1248-5	7.140	6.431	217629	74713	83.862m	73.999

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031921\
Data File : PP034160.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Mar 2021 11:11
Operator : DD\AJ
Sample : M1702-03
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CT-3


Manual Integrations
APPROVED

Ankita
3/22/2021 2:40:59 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 02:35:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

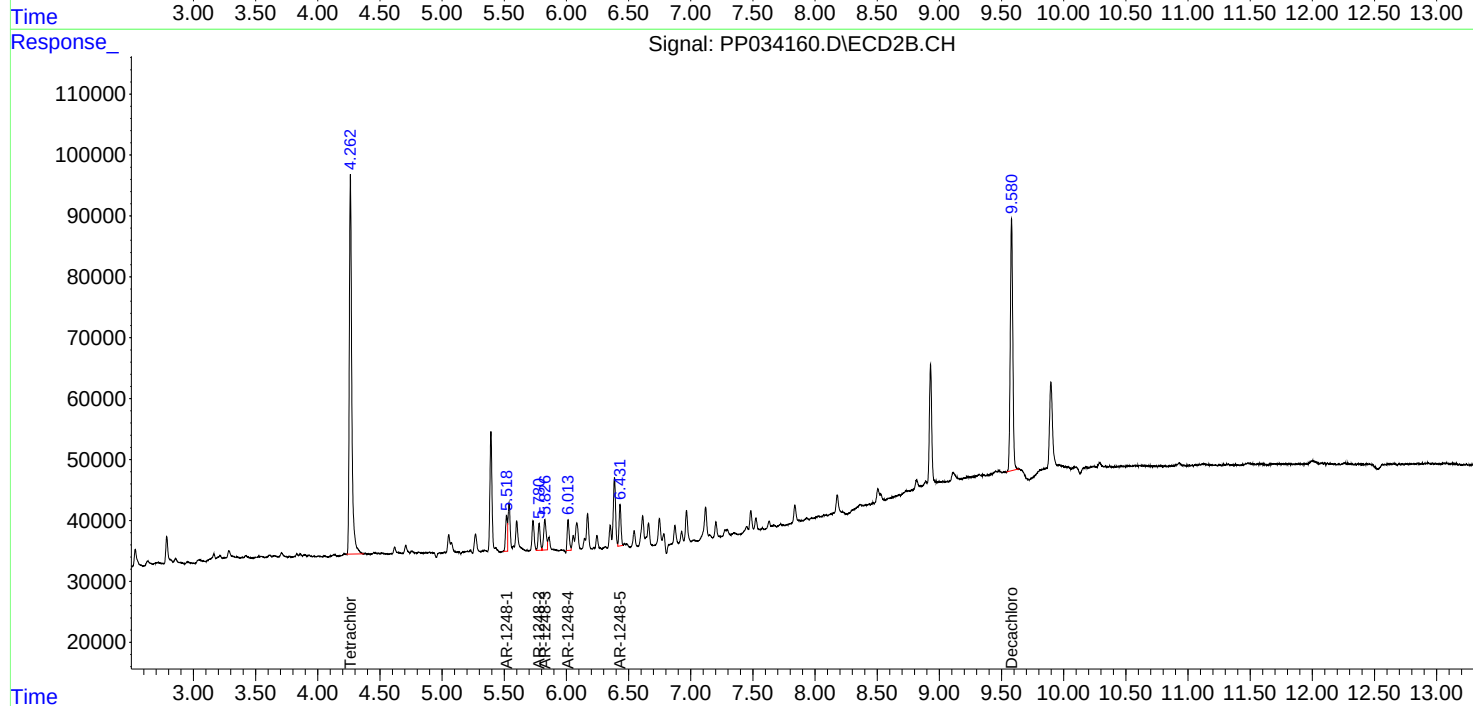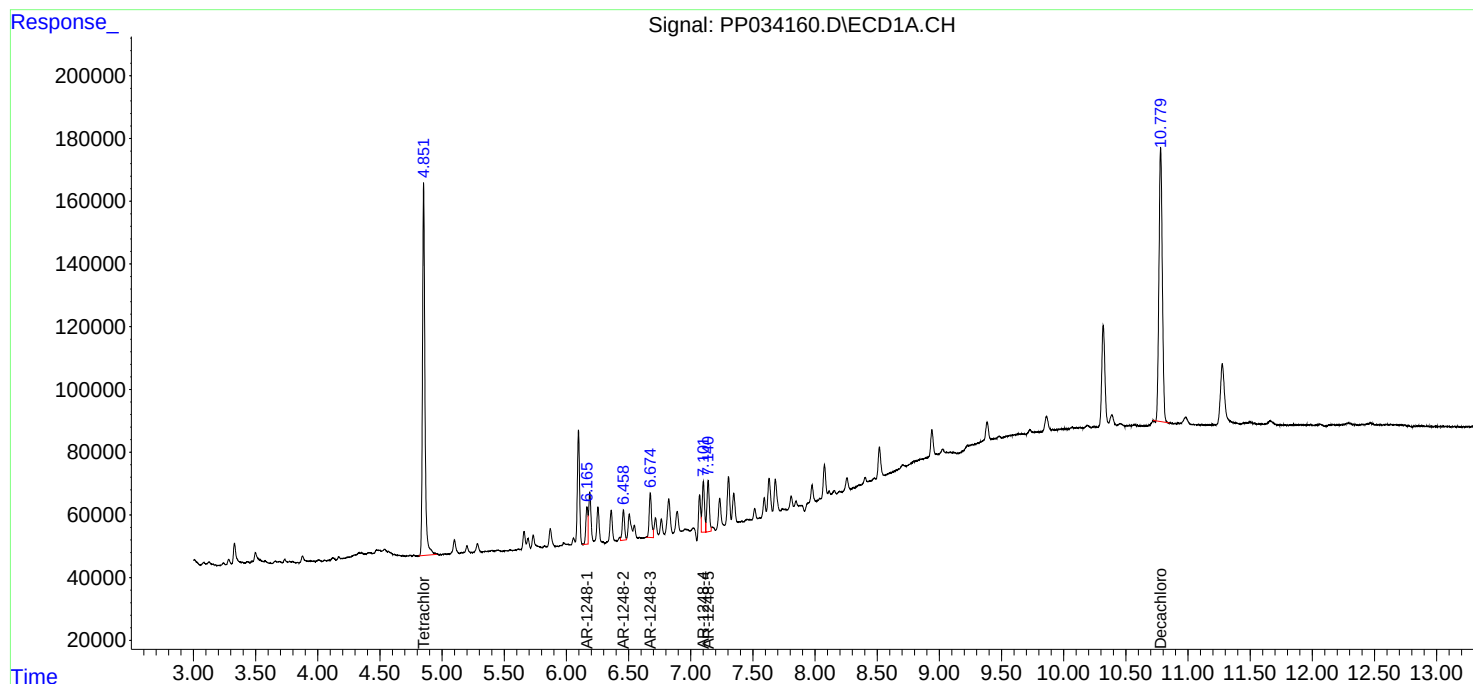

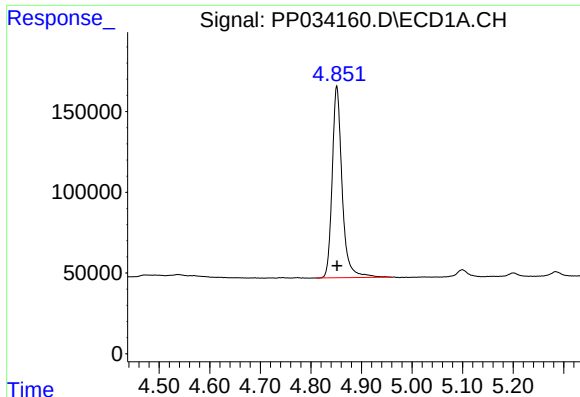


#1 Tetrachloro-m-xylene

R.T.: 4.851 min
Delta R.T.: 0.000 min
Response: 1621396
Conc: 19.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
CT-3


Manual Integrations
APPROVED

Ankita
3/22/2021 2:40:59 PM

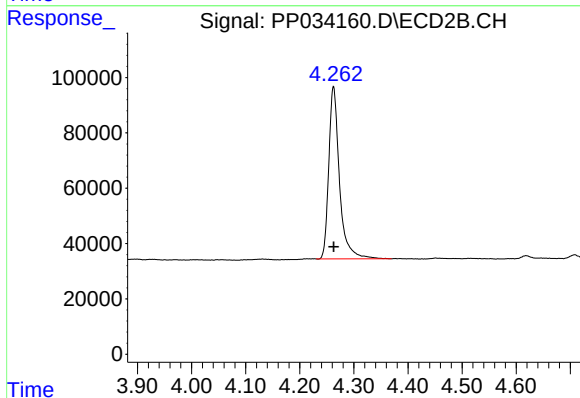


#1 Tetrachloro-m-xylene

R.T.: 4.262 min
Delta R.T.: 0.000 min
Response: 856611
Conc: 19.36 ng/ml

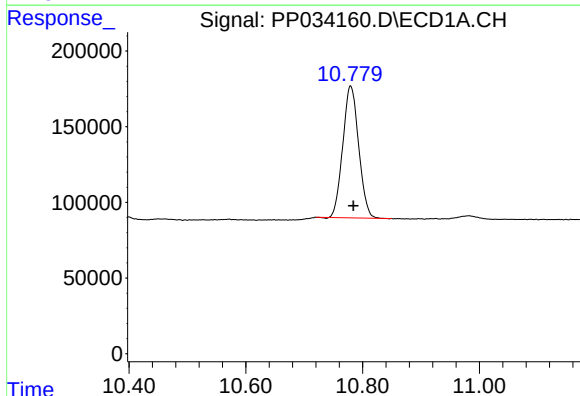


#2 Decachlorobiphenyl

R.T.: 10.779 min
Delta R.T.: -0.005 min
Response: 1643438
Conc: 20.94 ng/ml

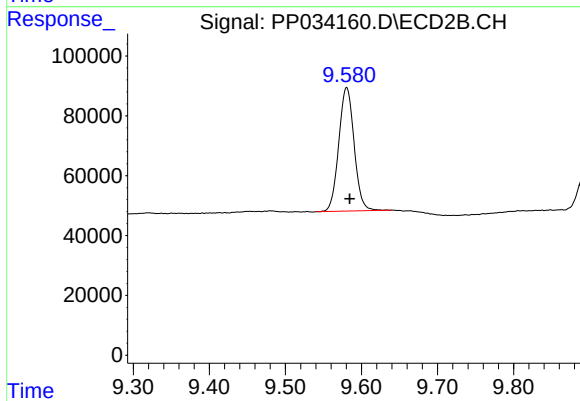

#2 Decachlorobiphenyl

R.T.: 9.581 min
Delta R.T.: -0.004 min
Response: 579480
Conc: 21.96 ng/ml

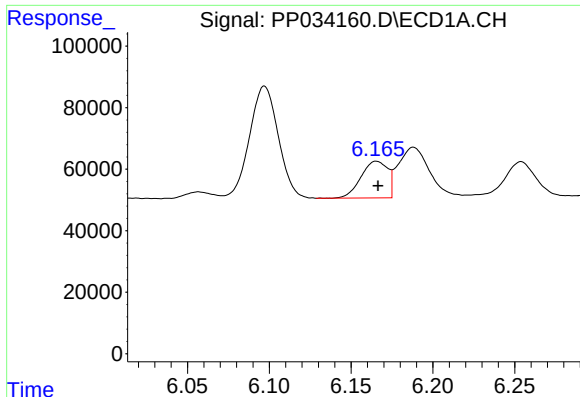


#21 AR-1248-1

R.T.: 6.166 min
Delta R.T.: 0.000 min
Response: 135896
Conc: 90.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
CT-3


Manual Integrations
APPROVED

Ankita
3/22/2021 2:40:59 PM

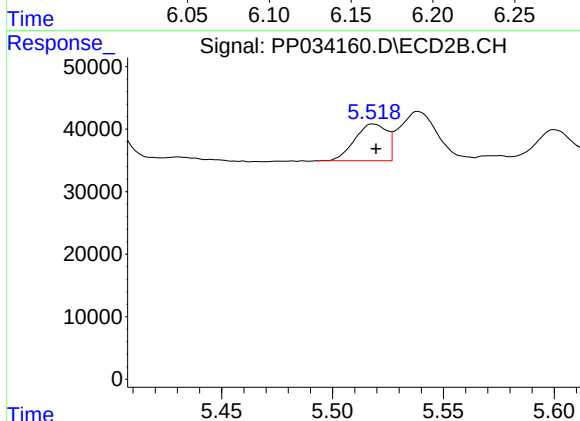


#21 AR-1248-1

R.T.: 5.518 min
Delta R.T.: -0.001 min
Response: 59692
Conc: 86.78 ng/ml

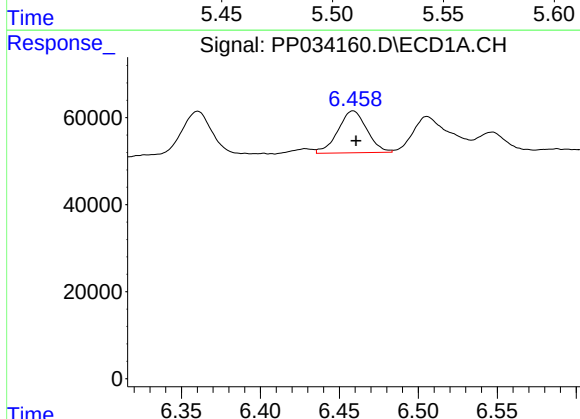


#22 AR-1248-2

R.T.: 6.459 min
Delta R.T.: -0.002 min
Response: 123281
Conc: 58.75 ng/ml

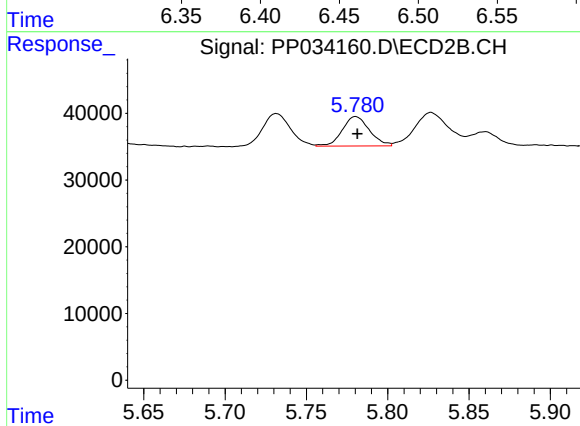

#22 AR-1248-2

R.T.: 5.780 min
Delta R.T.: -0.001 min
Response: 51299
Conc: 51.37 ng/ml

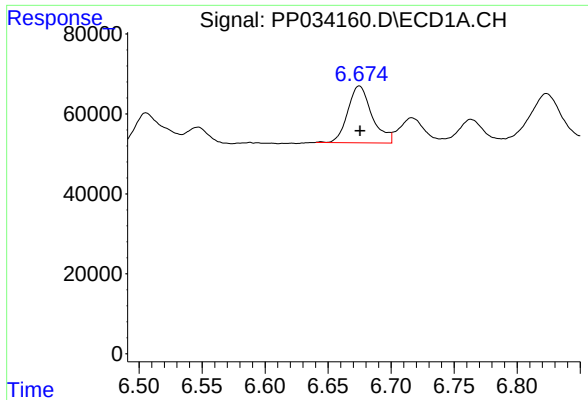


#23 AR-1248-3

R.T.: 6.675 min
Delta R.T.: 0.000 min
Response: 190068
Conc: 74.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
CT-3


Manual Integrations
APPROVED

Ankita
3/22/2021 2:40:59 PM

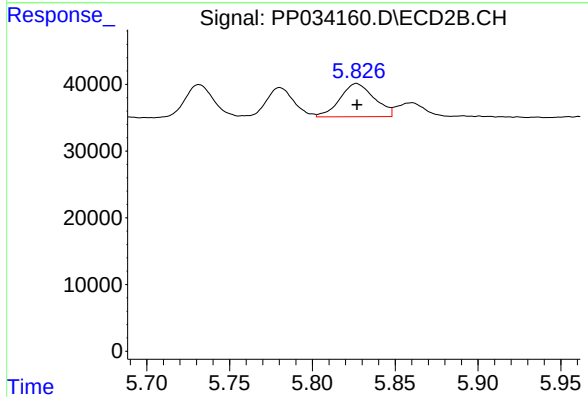


#23 AR-1248-3

R.T.: 5.827 min
Delta R.T.: 0.000 min
Response: 72064
Conc: 68.33 ng/ml

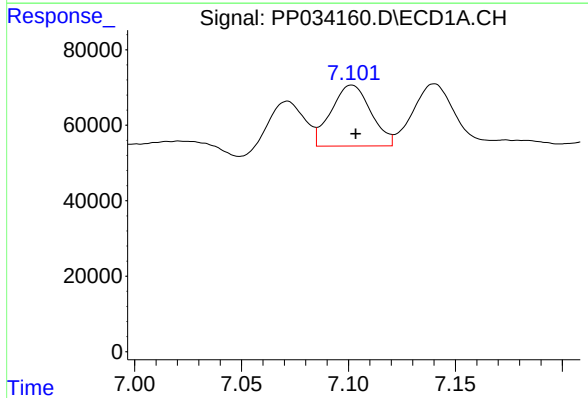


#24 AR-1248-4

R.T.: 7.101 min
Delta R.T.: -0.002 min
Response: 209150
Conc: 80.95 ng/ml m

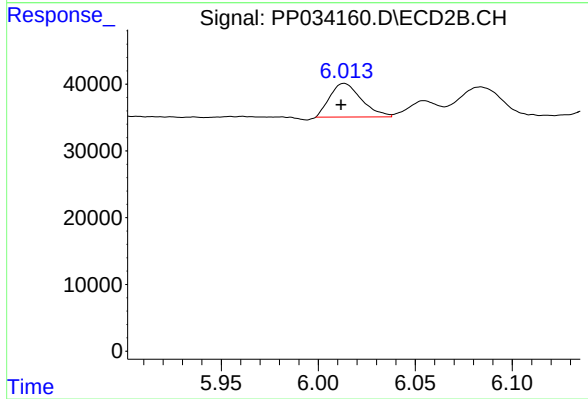

#24 AR-1248-4

R.T.: 6.013 min
Delta R.T.: 0.001 min
Response: 57276
Conc: 46.67 ng/ml m

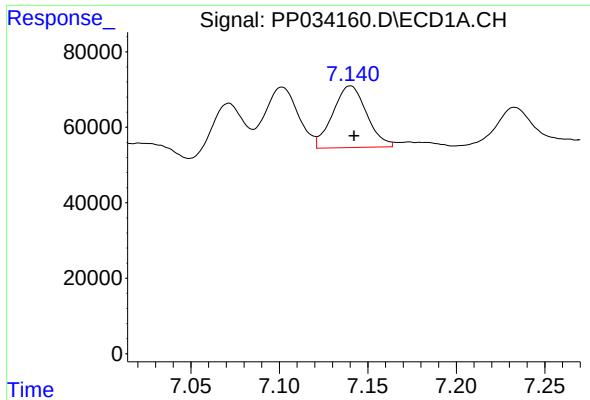


#25 AR-1248-5

R.T.: 7.140 min
Delta R.T.: -0.002 min
Response: 217629
Conc: 83.86 ng/ml m

Instrument :
ECD_P
ClientSampleId :
CT-3

Manual Integrations
APPROVED

Ankita
3/22/2021 2:40:59 PM

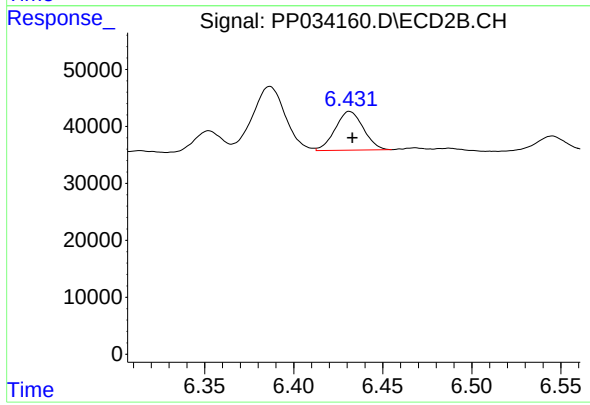

#25 AR-1248-5

R.T.: 6.431 min
Delta R.T.: -0.002 min
Response: 74713
Conc: 74.00 ng/ml