

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031921\
 Data File : PP034161.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Mar 2021 11:28
 Operator : DD\AJ
 Sample : M1702-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CT-4

Manual Integrations
 APPROVED

Ankita
 3/22/2021 2:41:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 02:36:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.851	4.262	1777069	939791	21.154	21.237
2) SA Decachlor...	10.777	9.579	1877114	641075	23.919	24.293
Target Compounds						
21) L5 AR-1248-1	6.164	5.518	408981	184624	273.542	268.391
22) L5 AR-1248-2	6.458	5.780	394621	170099	188.055	170.339
23) L5 AR-1248-3	6.673	5.825	576693	205385	226.450	194.757
24) L5 AR-1248-4	7.101	6.010	554089	268462	214.455	218.763m
25) L5 AR-1248-5	7.139	6.431	547814	225586	211.097	223.429

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031921\
Data File : PP034161.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Mar 2021 11:28
Operator : DD\AJ
Sample : M1702-04
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CT-4


Manual Integrations
APPROVED

Ankita
3/22/2021 2:41:02 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 02:36:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

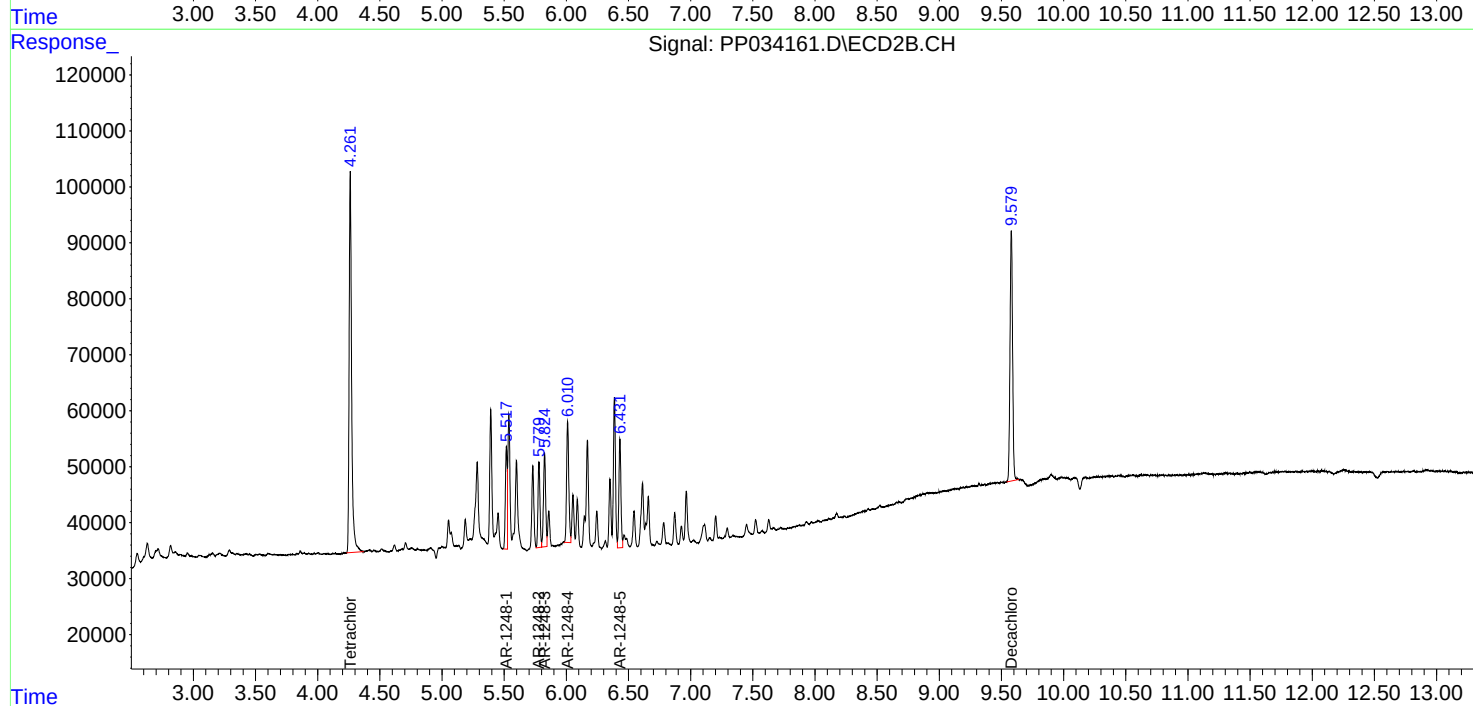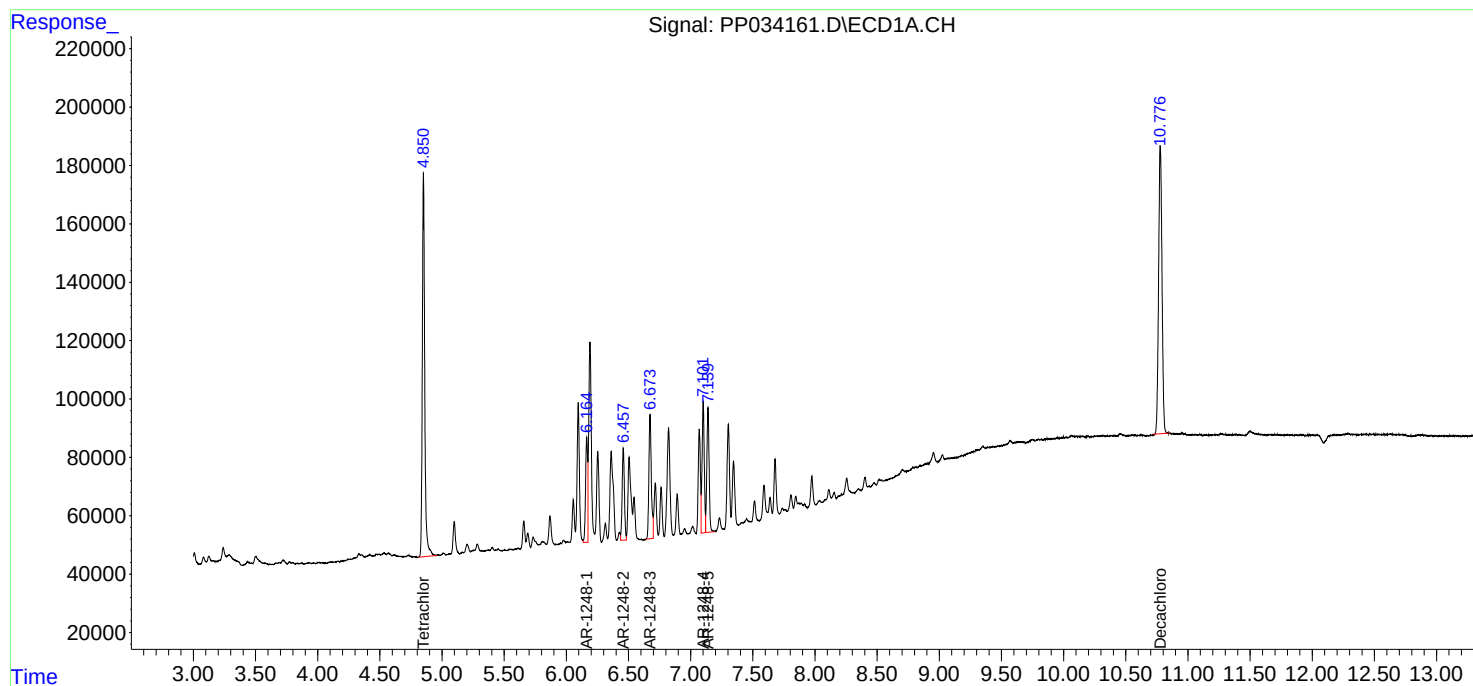

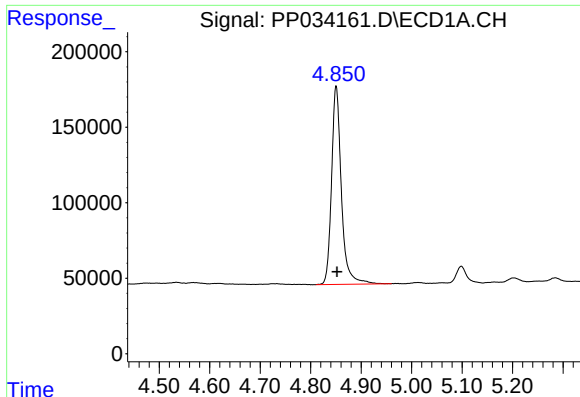


#1 Tetrachloro-m-xylene

R.T.: 4.851 min
Delta R.T.: -0.001 min
Response: 1777069
Conc: 21.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
CT-4


Manual Integrations
APPROVED

Ankita
3/22/2021 2:41:02 PM

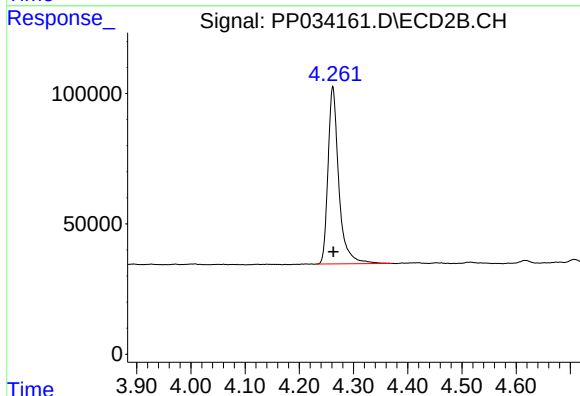


#1 Tetrachloro-m-xylene

R.T.: 4.262 min
Delta R.T.: 0.000 min
Response: 939791
Conc: 21.24 ng/ml

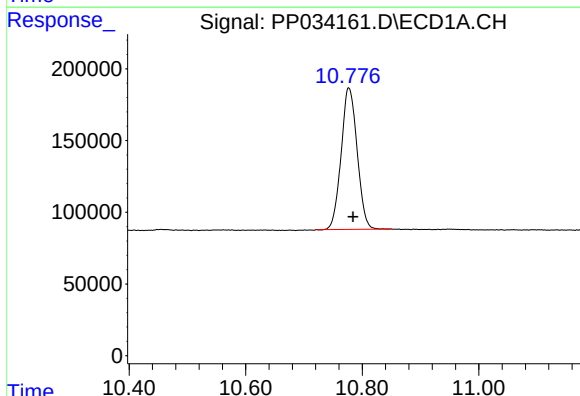


#2 Decachlorobiphenyl

R.T.: 10.777 min
Delta R.T.: -0.007 min
Response: 1877114
Conc: 23.92 ng/ml

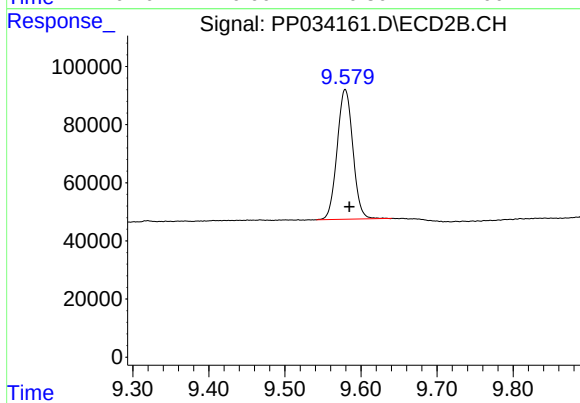

#2 Decachlorobiphenyl

R.T.: 9.579 min
Delta R.T.: -0.005 min
Response: 641075
Conc: 24.29 ng/ml

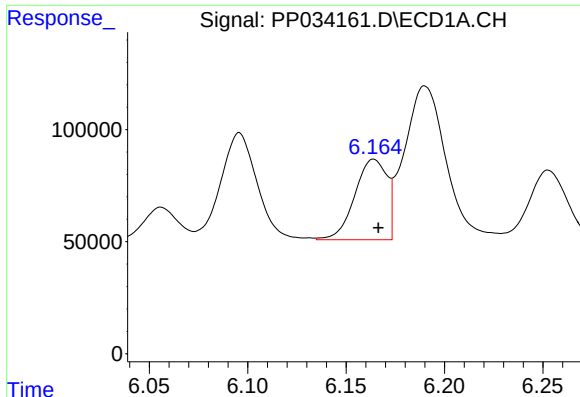


#21 AR-1248-1

R.T.: 6.164 min
Delta R.T.: -0.002 min
Response: 408981
Conc: 273.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
CT-4


Manual Integrations
APPROVED

Ankita
3/22/2021 2:41:02 PM

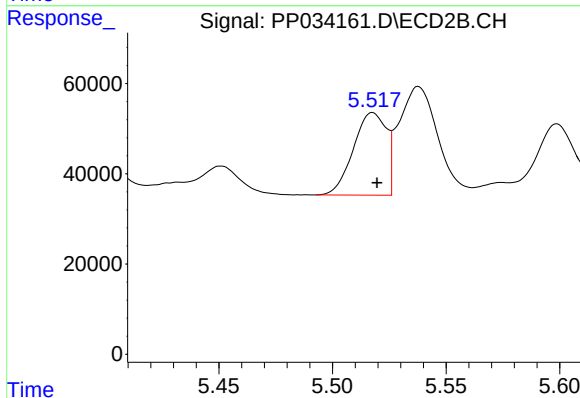


#21 AR-1248-1

R.T.: 5.518 min
Delta R.T.: -0.002 min
Response: 184624
Conc: 268.39 ng/ml

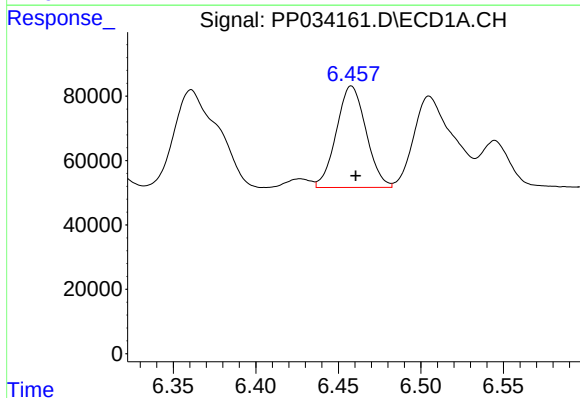


#22 AR-1248-2

R.T.: 6.458 min
Delta R.T.: -0.003 min
Response: 394621
Conc: 188.05 ng/ml

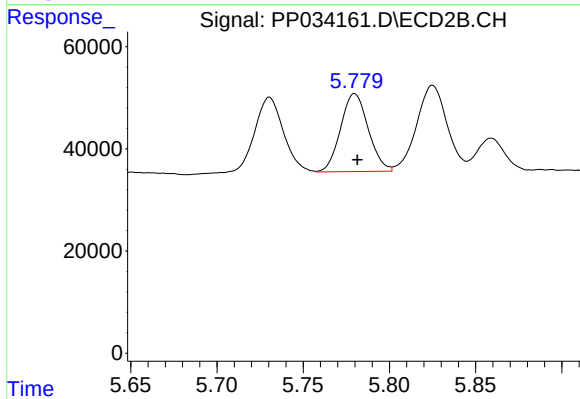

#22 AR-1248-2

R.T.: 5.780 min
Delta R.T.: -0.002 min
Response: 170099
Conc: 170.34 ng/ml

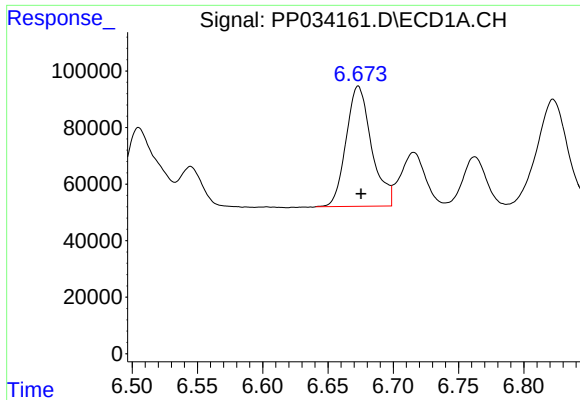


#23 AR-1248-3

R.T.: 6.673 min
Delta R.T.: -0.002 min
Response: 576693
Conc: 226.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
CT-4


Manual Integrations
APPROVED

Ankita
3/22/2021 2:41:02 PM

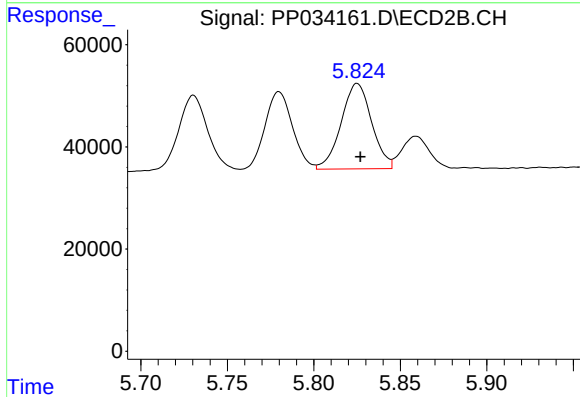


#23 AR-1248-3

R.T.: 5.825 min
Delta R.T.: -0.002 min
Response: 205385
Conc: 194.76 ng/ml

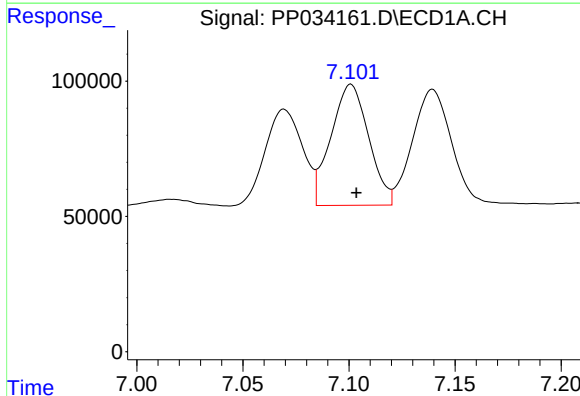


#24 AR-1248-4

R.T.: 7.101 min
Delta R.T.: -0.002 min
Response: 554089
Conc: 214.45 ng/ml

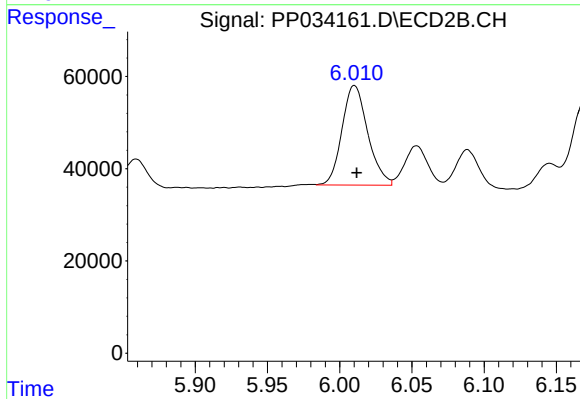

#24 AR-1248-4

R.T.: 6.010 min
Delta R.T.: -0.002 min
Response: 268462
Conc: 218.76 ng/ml m

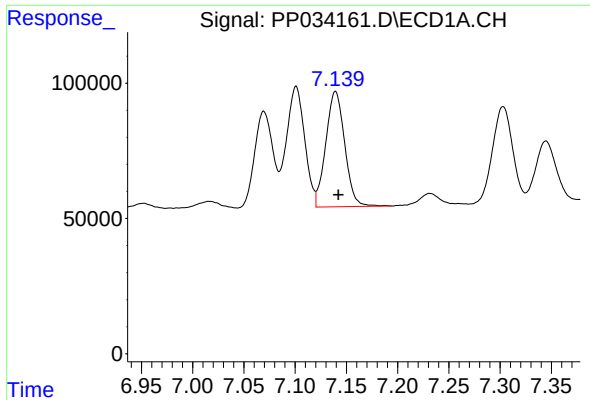


#25 AR-1248-5

R.T.: 7.139 min
Delta R.T.: -0.003 min
Response: 547814
Conc: 211.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
CT-4

Manual Integrations
APPROVED

Ankita
3/22/2021 2:41:02 PM

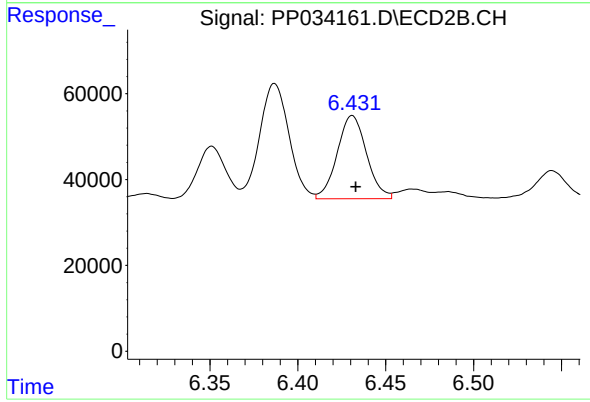

#25 AR-1248-5

R.T.: 6.431 min
Delta R.T.: -0.002 min
Response: 225586
Conc: 223.43 ng/ml