

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031921\
 Data File : PP034164.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Mar 2021 12:18
 Operator : DD\AJ
 Sample : M1702-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CT-7

Manual Integrations
 APPROVED

Ankita
 3/22/2021 2:41:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 02:37:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.851	4.262	1881639	1022671	22.399	23.110
2) SA Decachlor...	10.776	9.579	1940592	680383	24.728	25.783
Target Compounds						
21) L5 AR-1248-1	6.164	5.517	68761	27807	45.990	40.424
22) L5 AR-1248-2	6.456	5.779	66416	29508	31.650m	29.550
23) L5 AR-1248-3	6.673	5.824	99815	33804	39.194	32.054
24) L5 AR-1248-4	7.100	6.011	141883	40752	54.914	33.208 #
25) L5 AR-1248-5	7.139	6.431	137970	54651	53.166	54.128

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031921\
Data File : PP034164.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Mar 2021 12:18
Operator : DD\AJ
Sample : M1702-07
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CT-7


Manual Integrations
APPROVED

Ankita
3/22/2021 2:41:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 02:37:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

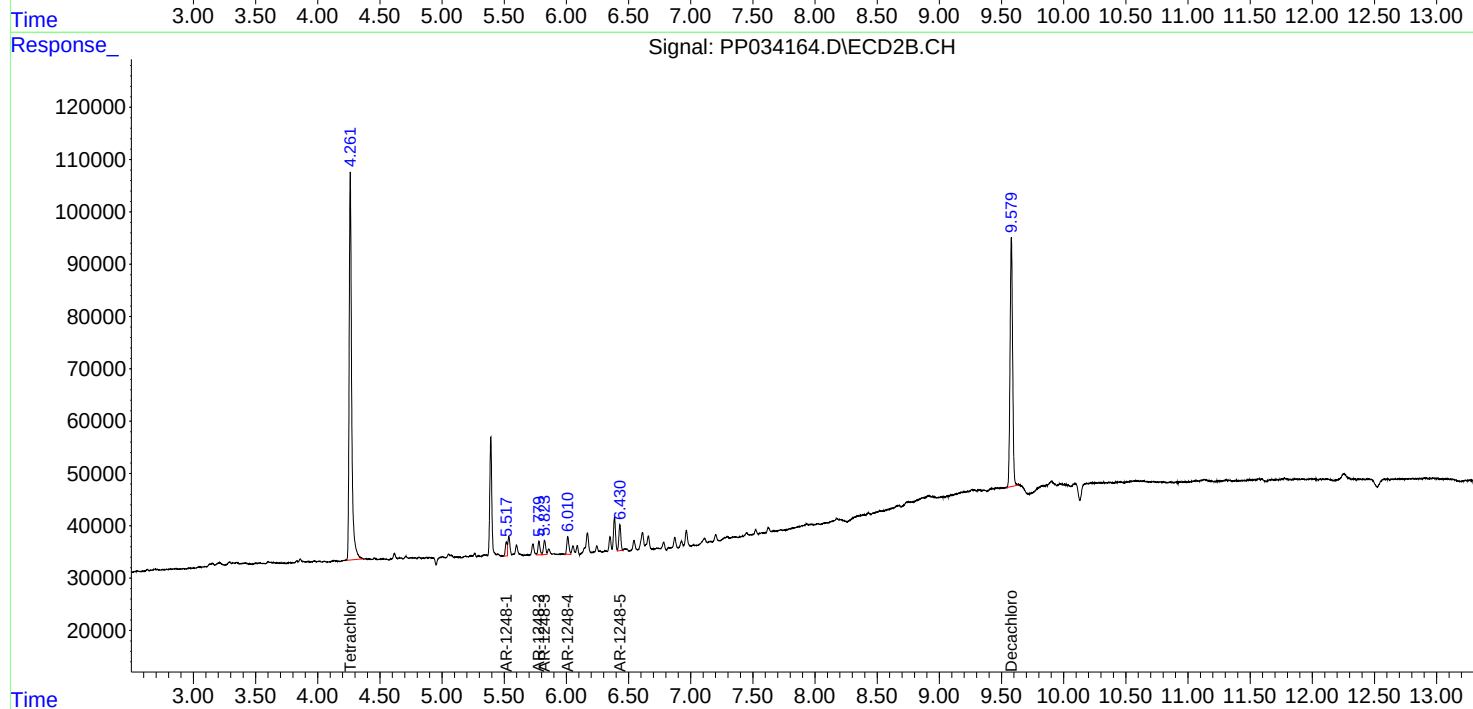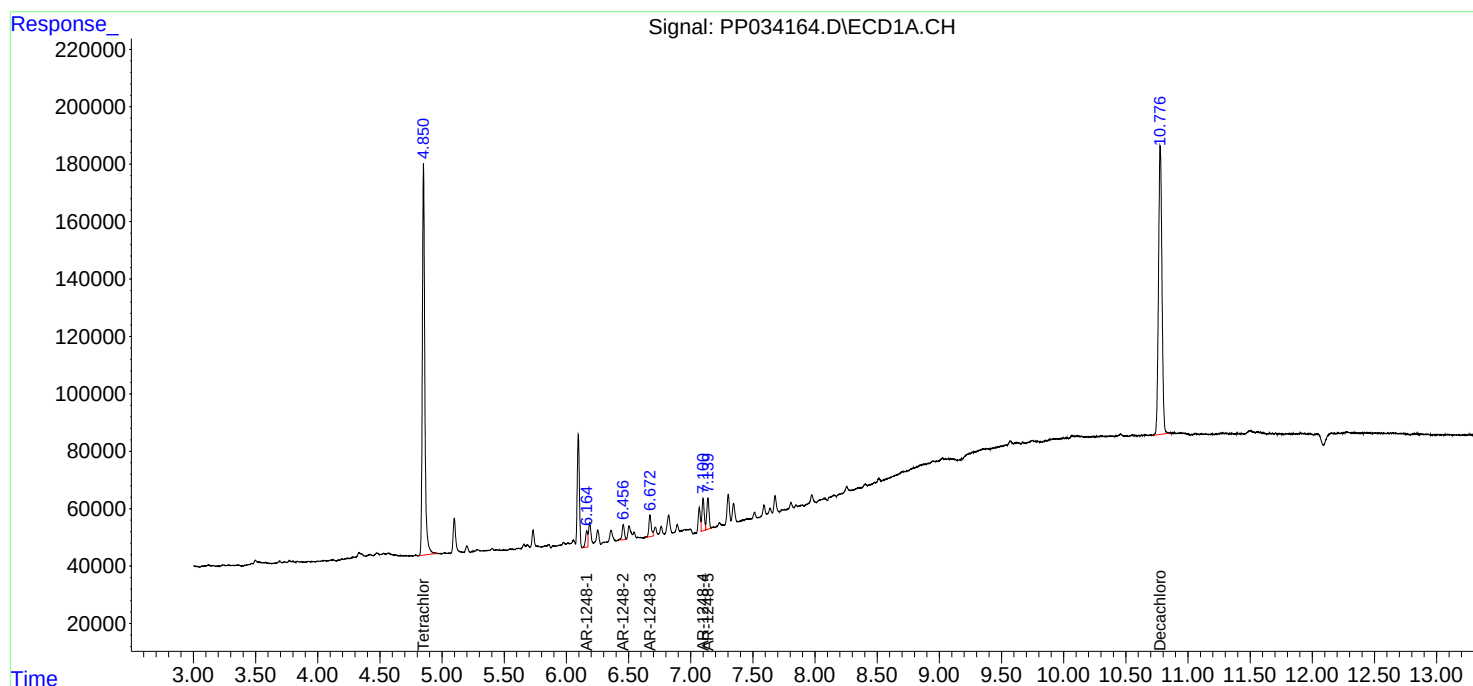

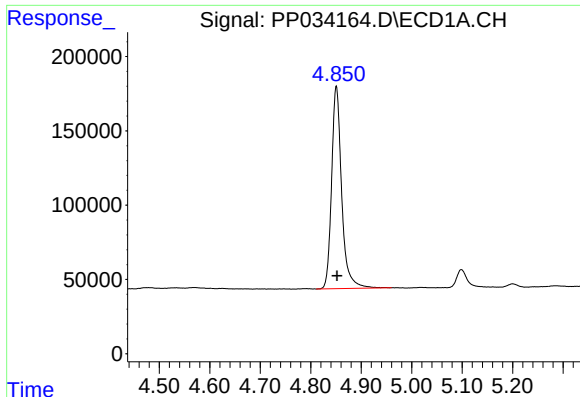


#1 Tetrachloro-m-xylene

R.T.: 4.851 min
Delta R.T.: -0.001 min
Response: 1881639
Conc: 22.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
CT-7


Manual Integrations
APPROVED

Ankita
3/22/2021 2:41:04 PM

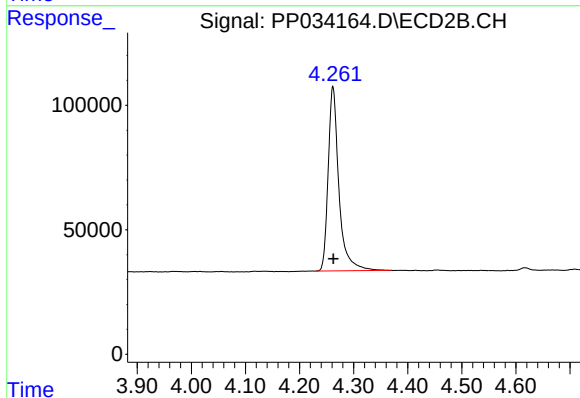


#1 Tetrachloro-m-xylene

R.T.: 4.262 min
Delta R.T.: -0.001 min
Response: 1022671
Conc: 23.11 ng/ml

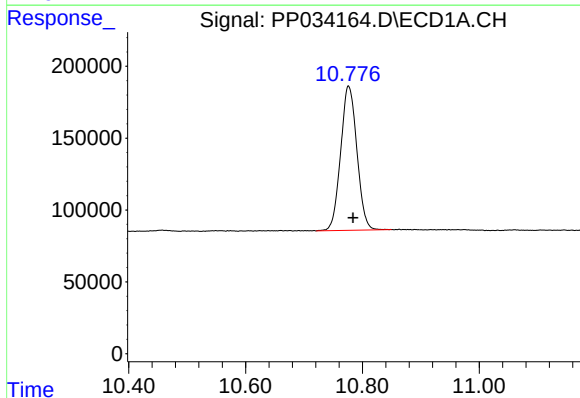


#2 Decachlorobiphenyl

R.T.: 10.776 min
Delta R.T.: -0.008 min
Response: 1940592
Conc: 24.73 ng/ml

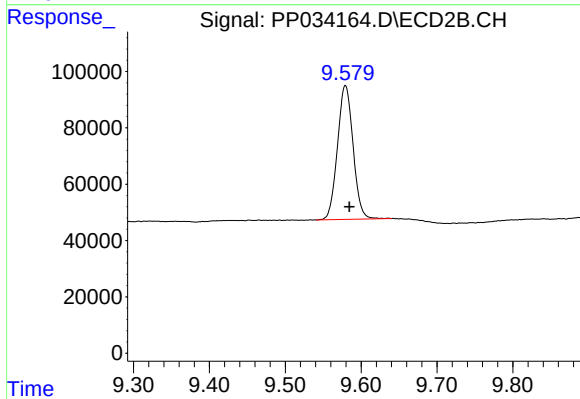

#2 Decachlorobiphenyl

R.T.: 9.579 min
Delta R.T.: -0.005 min
Response: 680383
Conc: 25.78 ng/ml

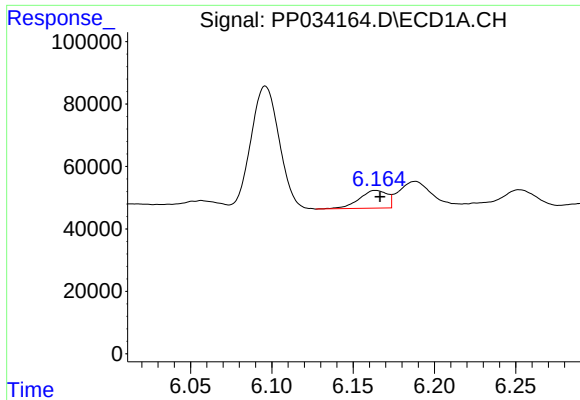


#21 AR-1248-1

R.T.: 6.164 min
Delta R.T.: -0.003 min
Response: 68761
Conc: 45.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
CT-7


Manual Integrations
APPROVED

Ankita
3/22/2021 2:41:04 PM

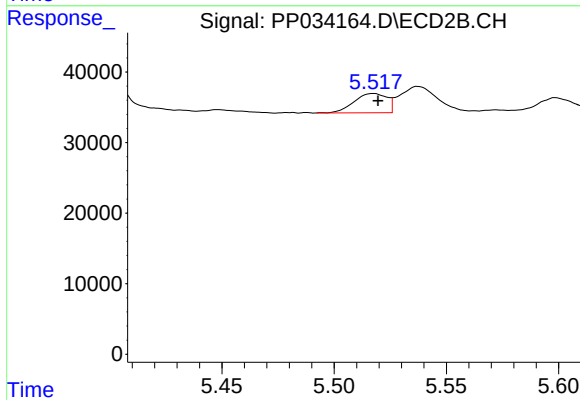


#21 AR-1248-1

R.T.: 5.517 min
Delta R.T.: -0.002 min
Response: 27807
Conc: 40.42 ng/ml

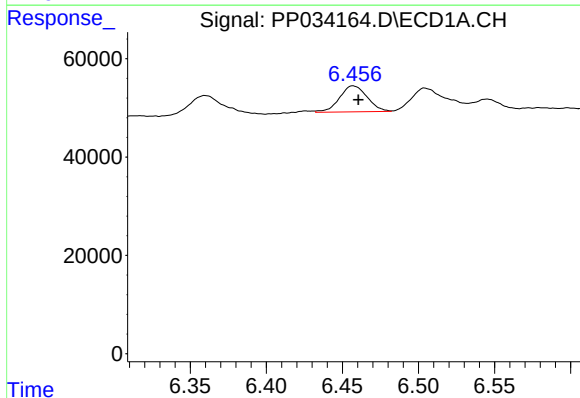


#22 AR-1248-2

R.T.: 6.456 min
Delta R.T.: -0.004 min
Response: 66416
Conc: 31.65 ng/ml m

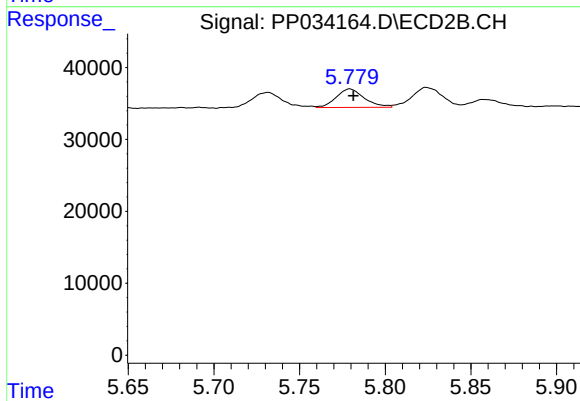

#22 AR-1248-2

R.T.: 5.779 min
Delta R.T.: -0.002 min
Response: 29508
Conc: 29.55 ng/ml

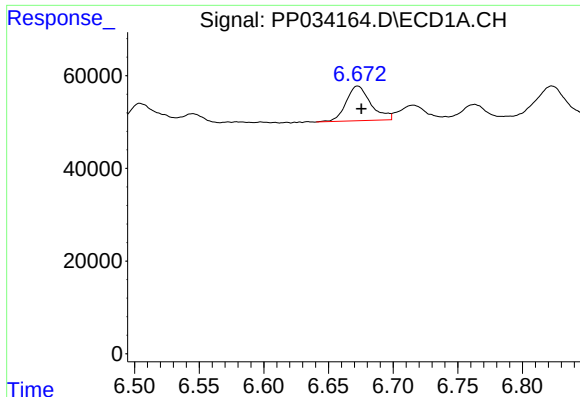


#23 AR-1248-3

R.T.: 6.673 min
Delta R.T.: -0.003 min
Response: 99815
Conc: 39.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
CT-7


Manual Integrations
APPROVED

Ankita
3/22/2021 2:41:04 PM

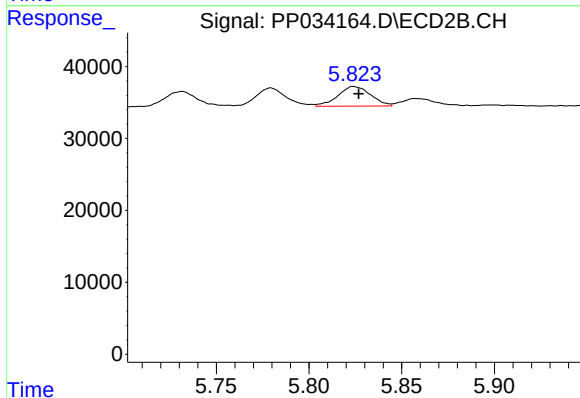


#23 AR-1248-3

R.T.: 5.824 min
Delta R.T.: -0.003 min
Response: 33804
Conc: 32.05 ng/ml

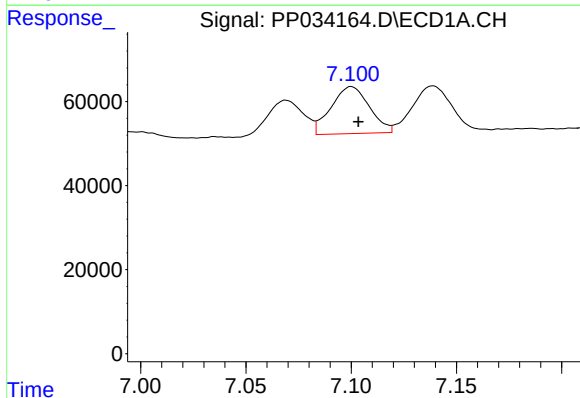


#24 AR-1248-4

R.T.: 7.100 min
Delta R.T.: -0.003 min
Response: 141883
Conc: 54.91 ng/ml

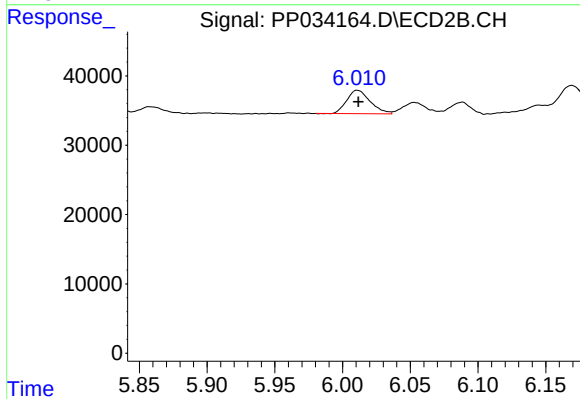

#24 AR-1248-4

R.T.: 6.011 min
Delta R.T.: 0.000 min
Response: 40752
Conc: 33.21 ng/ml

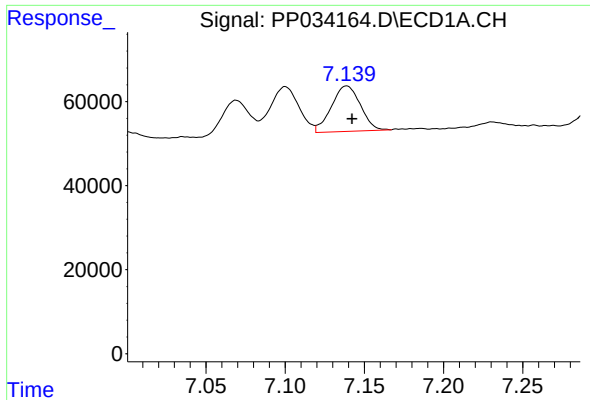


#25 AR-1248-5

R.T.: 7.139 min
Delta R.T.: -0.003 min
Response: 137970
Conc: 53.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
CT-7

Manual Integrations
APPROVED

Ankita
3/22/2021 2:41:04 PM

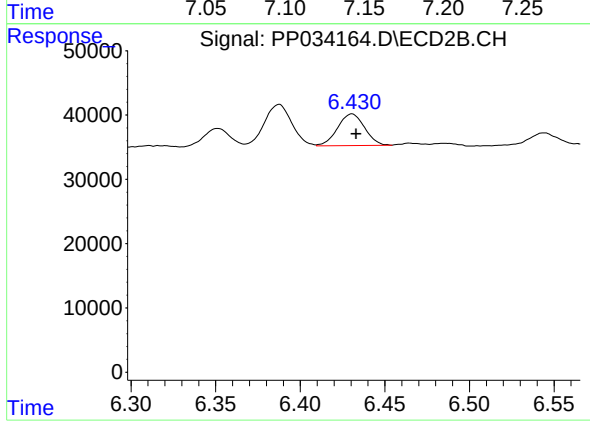

#25 AR-1248-5

R.T.: 6.431 min
Delta R.T.: -0.002 min
Response: 54651
Conc: 54.13 ng/ml