

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031924\
 Data File : PP063578.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2024 23:16
 Operator : YP\AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1268ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/19/2024
 Supervised By :Ankita Jodhani 03/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 05:54:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 19 05:42:33 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.489	3.638	11358676	11157284	4.907	4.669
2) SA Decachlor...	10.364	8.680	22119369	23419037	5.400	5.340
Target Compounds						
41) L9 AR-1268-1	8.795	7.570	16599073	18885307	53.260	50.692m
42) L9 AR-1268-2	8.891	7.634	15087277	17375243	53.286	50.552
43) L9 AR-1268-3	9.131	7.843	13220170	15718000	52.802	52.316
44) L9 AR-1268-4	9.573	8.131	4971188	5686726	48.049	51.709
45) L9 AR-1268-5	10.010	8.424	40092550	41086618	50.710	49.562

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031924\
Data File : PP063578.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2024 23:16
Operator : YP\AJ
Sample : AR1268ICC050
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/19/2024
Supervised By :Ankita Jodhani 03/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 05:54:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 19 05:42:33 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

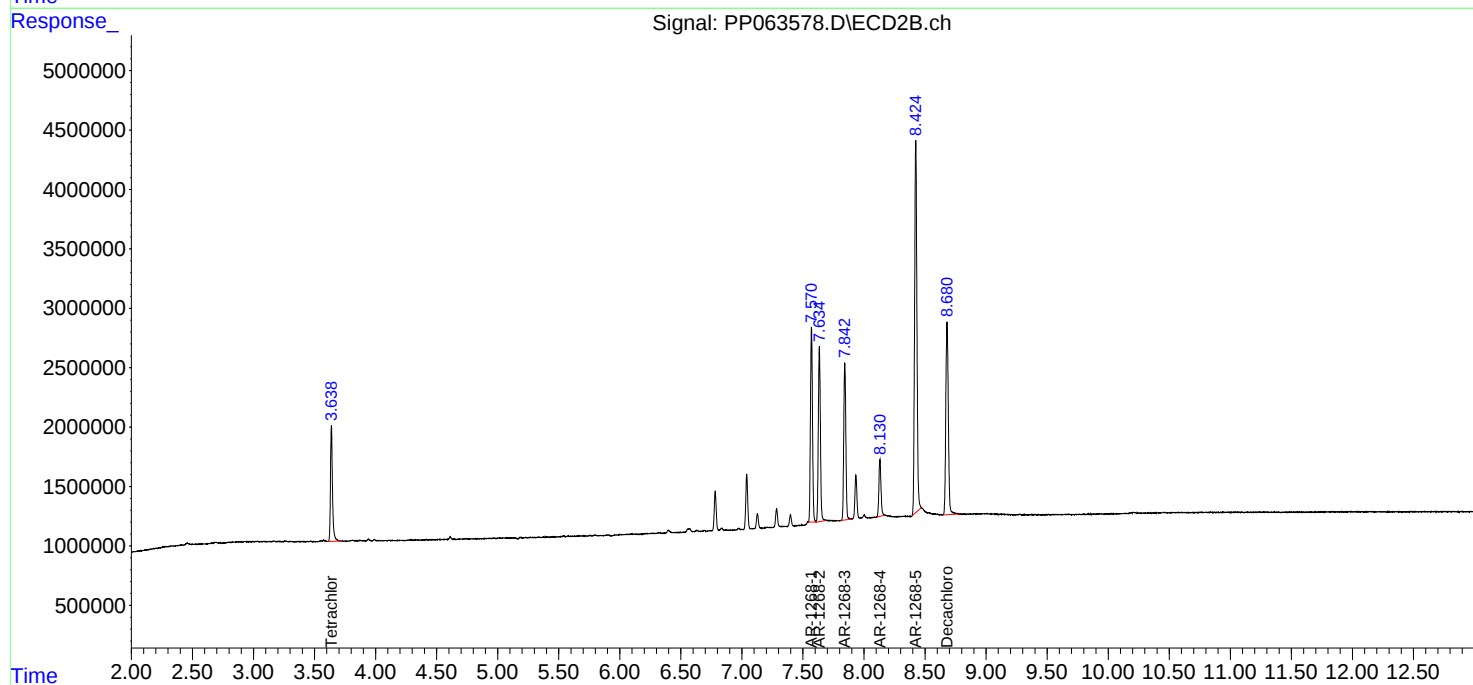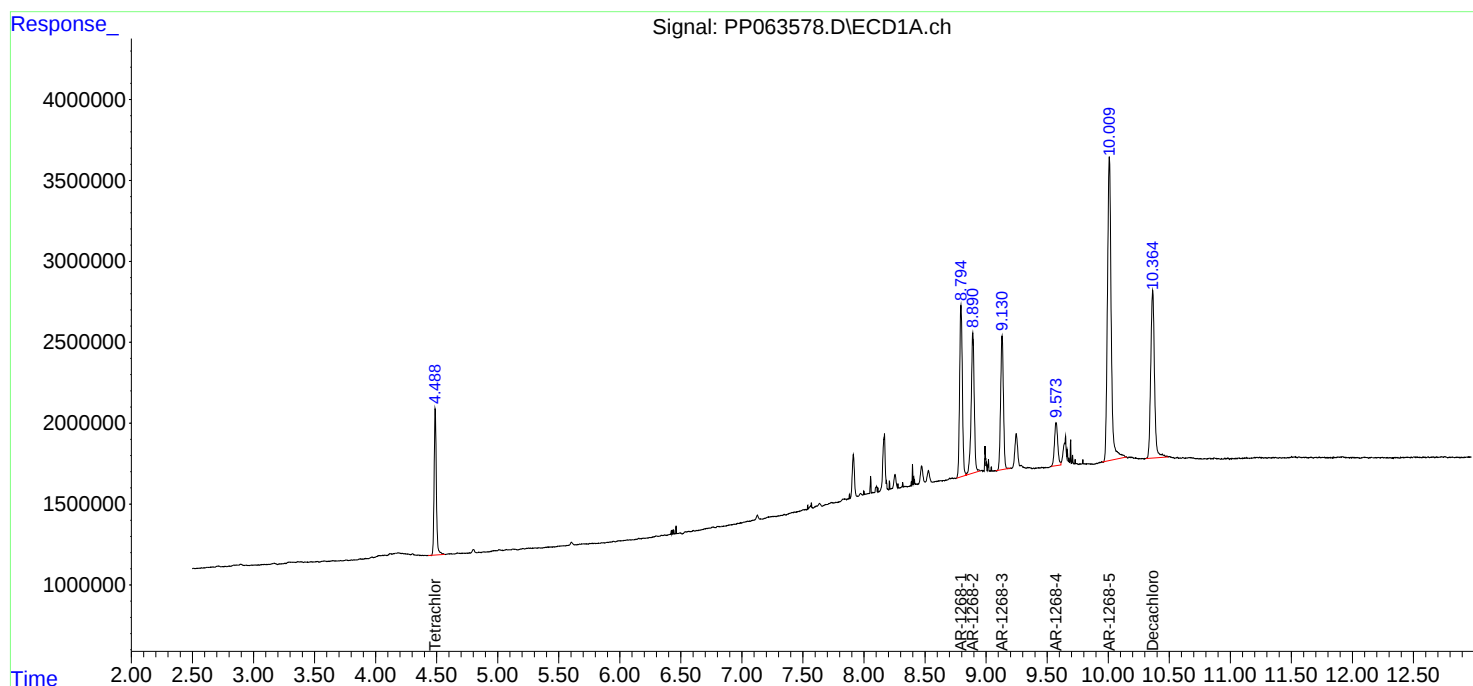

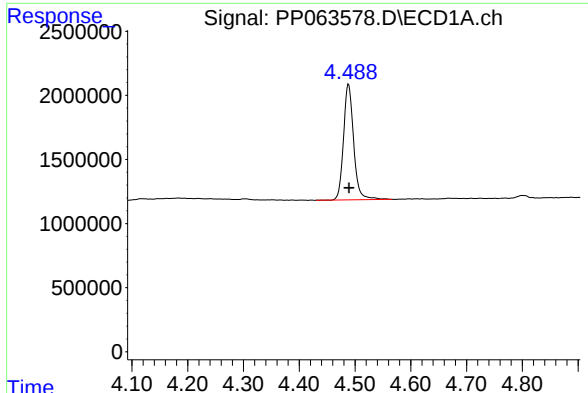


#1 Tetrachloro-m-xylene

R.T.: 4.489 min
Delta R.T.: 0.000 min
Response: 11358676
Conc: 4.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/19/2024
Supervised By :Ankita Jodhani 03/19/2024

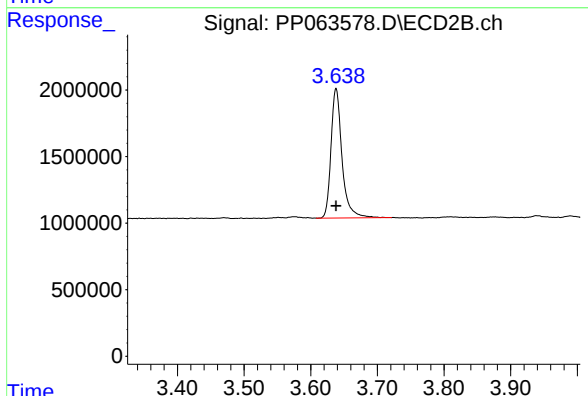


#1 Tetrachloro-m-xylene

R.T.: 3.638 min
Delta R.T.: 0.000 min
Response: 11157284
Conc: 4.67 ng/ml

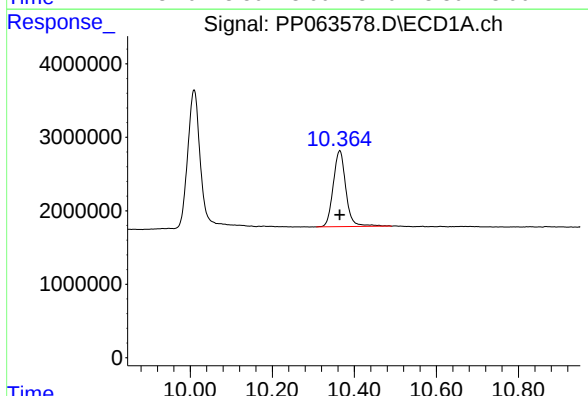


#2 Decachlorobiphenyl

R.T.: 10.364 min
Delta R.T.: 0.000 min
Response: 22119369
Conc: 5.40 ng/ml

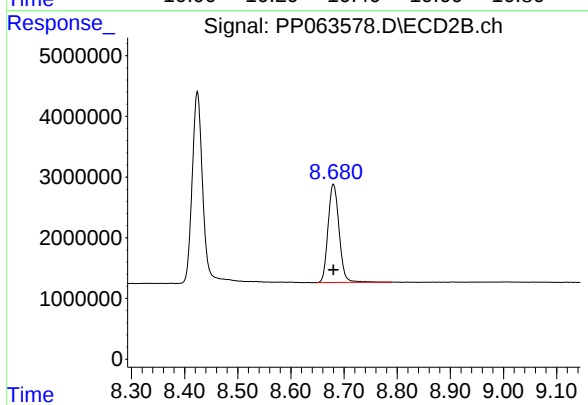

#2 Decachlorobiphenyl

R.T.: 8.680 min
Delta R.T.: 0.000 min
Response: 23419037
Conc: 5.34 ng/ml

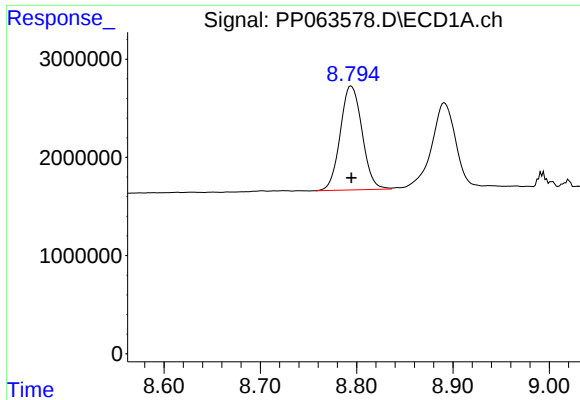


#41 AR-1268-1

R.T.: 8.795 min
Delta R.T.: 0.000 min
Response: 16599073
Conc: 53.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/19/2024
Supervised By :Ankita Jodhani 03/19/2024

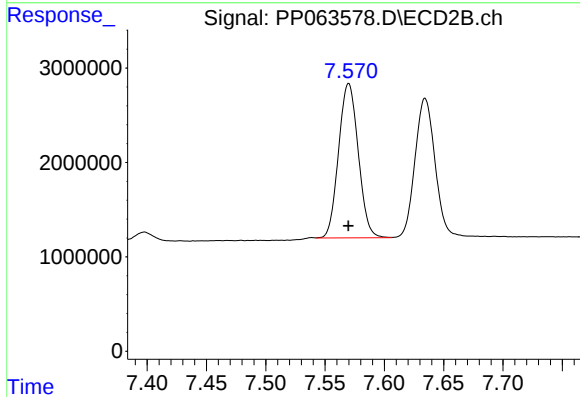


#41 AR-1268-1

R.T.: 7.570 min
Delta R.T.: 0.000 min
Response: 18885307
Conc: 50.69 ng/ml m

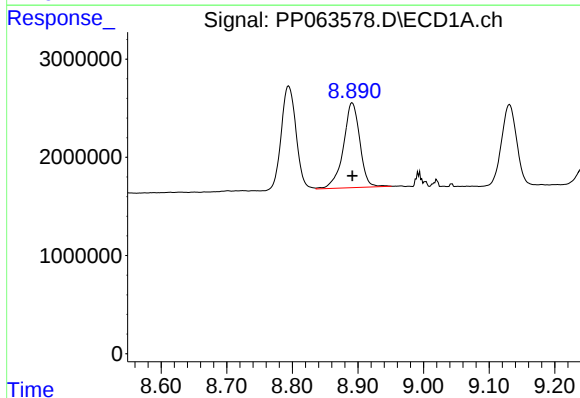


#42 AR-1268-2

R.T.: 8.891 min
Delta R.T.: 0.000 min
Response: 15087277
Conc: 53.29 ng/ml

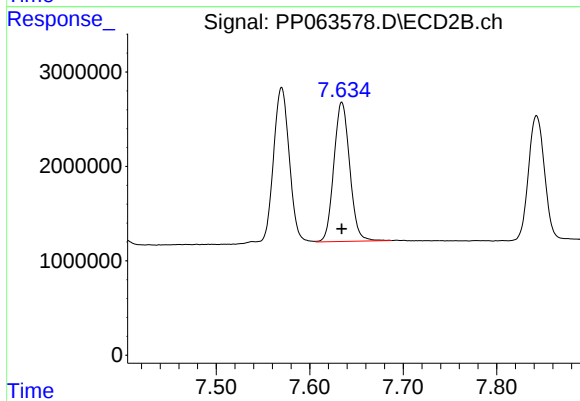

#42 AR-1268-2

R.T.: 7.634 min
Delta R.T.: 0.000 min
Response: 17375243
Conc: 50.55 ng/ml

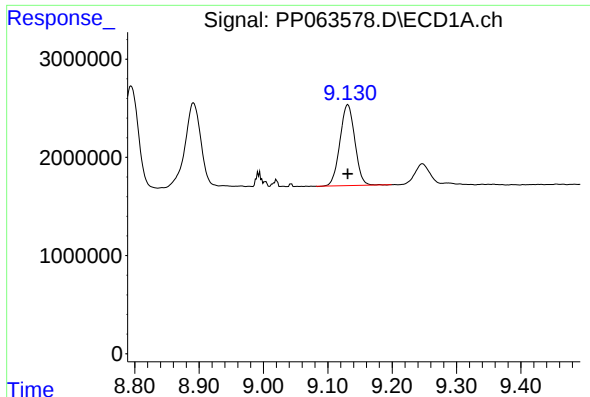


#43 AR-1268-3

R.T.: 9.131 min
Delta R.T.: 0.000 min
Response: 13220170
Conc: 52.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/19/2024
Supervised By :Ankita Jodhani 03/19/2024

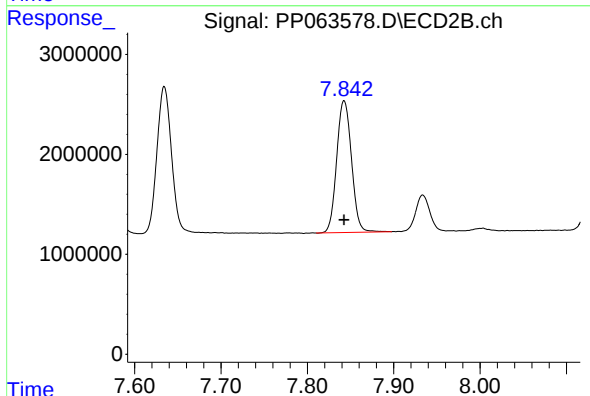


#43 AR-1268-3

R.T.: 7.843 min
Delta R.T.: 0.000 min
Response: 15718000
Conc: 52.32 ng/ml

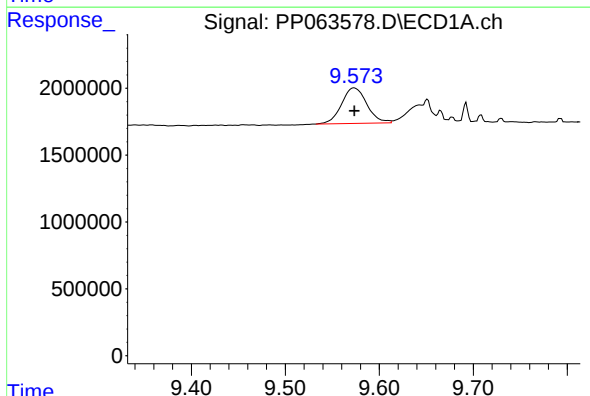


#44 AR-1268-4

R.T.: 9.573 min
Delta R.T.: 0.000 min
Response: 4971188
Conc: 48.05 ng/ml

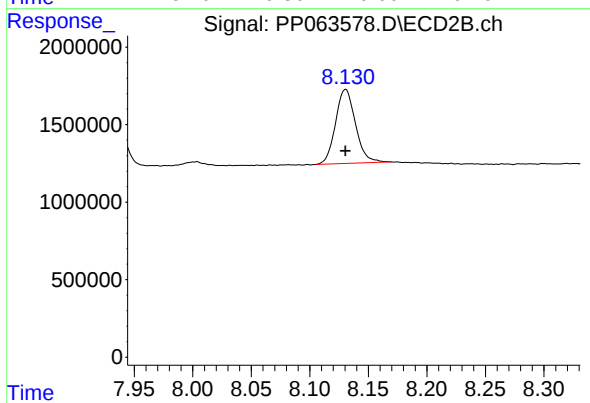

#44 AR-1268-4

R.T.: 8.131 min
Delta R.T.: 0.000 min
Response: 5686726
Conc: 51.71 ng/ml

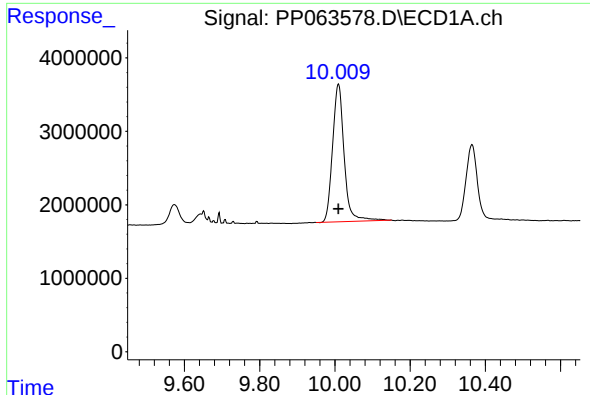


#45 AR-1268-5

R.T.: 10.010 min
Delta R.T.: 0.000 min
Response: 40092550
Conc: 50.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/19/2024
Supervised By :Ankita Jodhani 03/19/2024

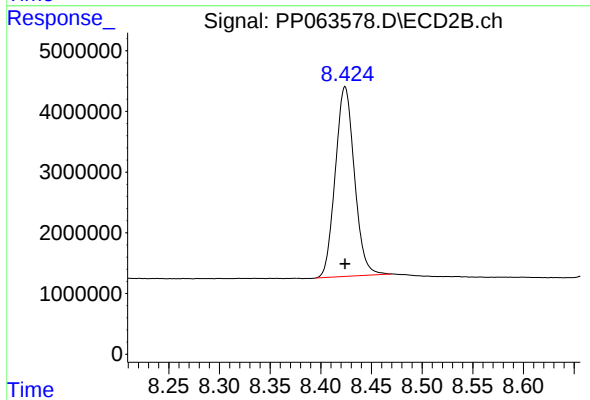

#45 AR-1268-5

R.T.: 8.424 min
Delta R.T.: 0.000 min
Response: 41086618
Conc: 49.56 ng/ml