

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031925\
 Data File : PP070710.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2025 18:36
 Operator : YP\AJ
 Sample : Q1597-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 2-CONCRETE-SLAB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 01:27:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 05:25:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.520	3.823	33734664	22615613	21.689	22.564
2)	SA Decachlor...	10.240	8.868	22963722	19767891	21.616	20.205
Target Compounds							
3)	L1 AR-1016-1	0.000	4.918	0	66371	N.D.	1.846 #
4)	L1 AR-1016-2	0.000	4.936	0	33698	N.D.	0.648 #
5)	L1 AR-1016-3	5.804f	5.159f	409744	116864	8.998	4.107 #
6)	L1 AR-1016-4	5.819f	5.159	450213	116864	11.533	5.220 #
7)	L1 AR-1016-5	0.000	5.382	0	177668	N.D.	5.978 #
8)	L2 AR-1221-1	0.000	3.975f	0	19302	N.D.	1.297 #
9)	L2 AR-1221-2	4.822	4.124	490578	532408	33.581	46.584 #
10)	L2 AR-1221-3	4.822f	4.195	490578	80520	11.058	2.409 #
11)	L3 AR-1232-1	4.822f	4.195	490578	80520	13.797	3.060 #
12)	L3 AR-1232-2	5.371f	4.936	280120	33698	16.606	1.306 #
13)	L3 AR-1232-3	0.000	5.159f	0	116864	N.D.	8.342 #
14)	L3 AR-1232-4	5.819f	5.191	450213	62690	23.703	5.353 #
15)	L3 AR-1232-5	0.000	5.382	0	177668	N.D.	13.596 #
16)	L4 AR-1242-1	0.000	4.918	0	66371	N.D.	2.168 #
17)	L4 AR-1242-2	0.000	4.936	0	33698	N.D.	0.773 #
18)	L4 AR-1242-3	5.804f	5.159f	409744	116864	11.044	4.904 #
19)	L4 AR-1242-4	5.819f	5.191	450213	62690	14.011	2.844 #
20)	L4 AR-1242-5	0.000	5.723	0	420759	N.D.	15.070 #
21)	L5 AR-1248-1	5.606f	4.918	4668396	66371	136.679	2.827 #
22)	L5 AR-1248-2	0.000	5.159	0	116864	N.D.	3.733 #
23)	L5 AR-1248-3	0.000	5.191	0	62690	N.D.	1.976 #
24)	L5 AR-1248-4	0.000	5.382	0	177668	N.D.	4.559 #
25)	L5 AR-1248-5	0.000	5.757	0	314770	N.D.	8.265 #
26)	L6 AR-1254-1	6.468f	5.723	736098	420759	12.855	7.470 #
27)	L6 AR-1254-2	0.000	5.864	0	343040	N.D.	7.014 #
28)	L6 AR-1254-3	0.000	6.293	0	321700	N.D.	4.266 #
29)	L6 AR-1254-4	0.000	6.517	0	48251	N.D.	0.915 #
30)	L6 AR-1254-5	0.000	6.921	0	194799	N.D.	2.821 #
31)	L7 AR-1260-1	0.000	6.402	0	58554	N.D.	1.176 #
32)	L7 AR-1260-2	0.000	6.603	0	46040	N.D.	0.697 #
33)	L7 AR-1260-3	0.000	6.750	0	273048	N.D.	4.774 #
34)	L7 AR-1260-4	0.000	7.215	0	104343	N.D.	2.039 #
35)	L7 AR-1260-5	0.000	7.465	0	229005	N.D.	1.778 #
36)	L8 AR-1262-1	0.000	6.970	0	41073	N.D.	0.491 #
37)	L8 AR-1262-2	0.000	7.215	0	104343	N.D.	1.518 #
38)	L8 AR-1262-3	0.000	7.751	0	383429	N.D.	5.811 #
39)	L8 AR-1262-4	0.000	7.809	0	72358	N.D.	0.693 #
40)	L8 AR-1262-5	9.557f	8.338	1393190	653796	23.655	12.683 #
41)	L9 AR-1268-1	0.000	7.751	0	383429	N.D.	2.190 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031925\
Data File : PP070710.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2025 18:36
Operator : YP\AJ
Sample : Q1597-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
2-CONCRETE-SLAB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 01:27:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 05:25:31 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	0.000	7.809	0	72358	N.D.	0.495 #
43)	L9 AR-1268-3	0.000	8.013	0	120242	N.D.	0.937 #
44)	L9 AR-1268-4	0.000	8.338	0	653796	N.D.	11.891 #
45)	L9 AR-1268-5	0.000	8.604	0	154147	N.D.	0.419 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031925\
Data File : PP070710.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2025 18:36
Operator : YP\AJ
Sample : Q1597-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
2-CONCRETE-SLAB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 01:27:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 05:25:31 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

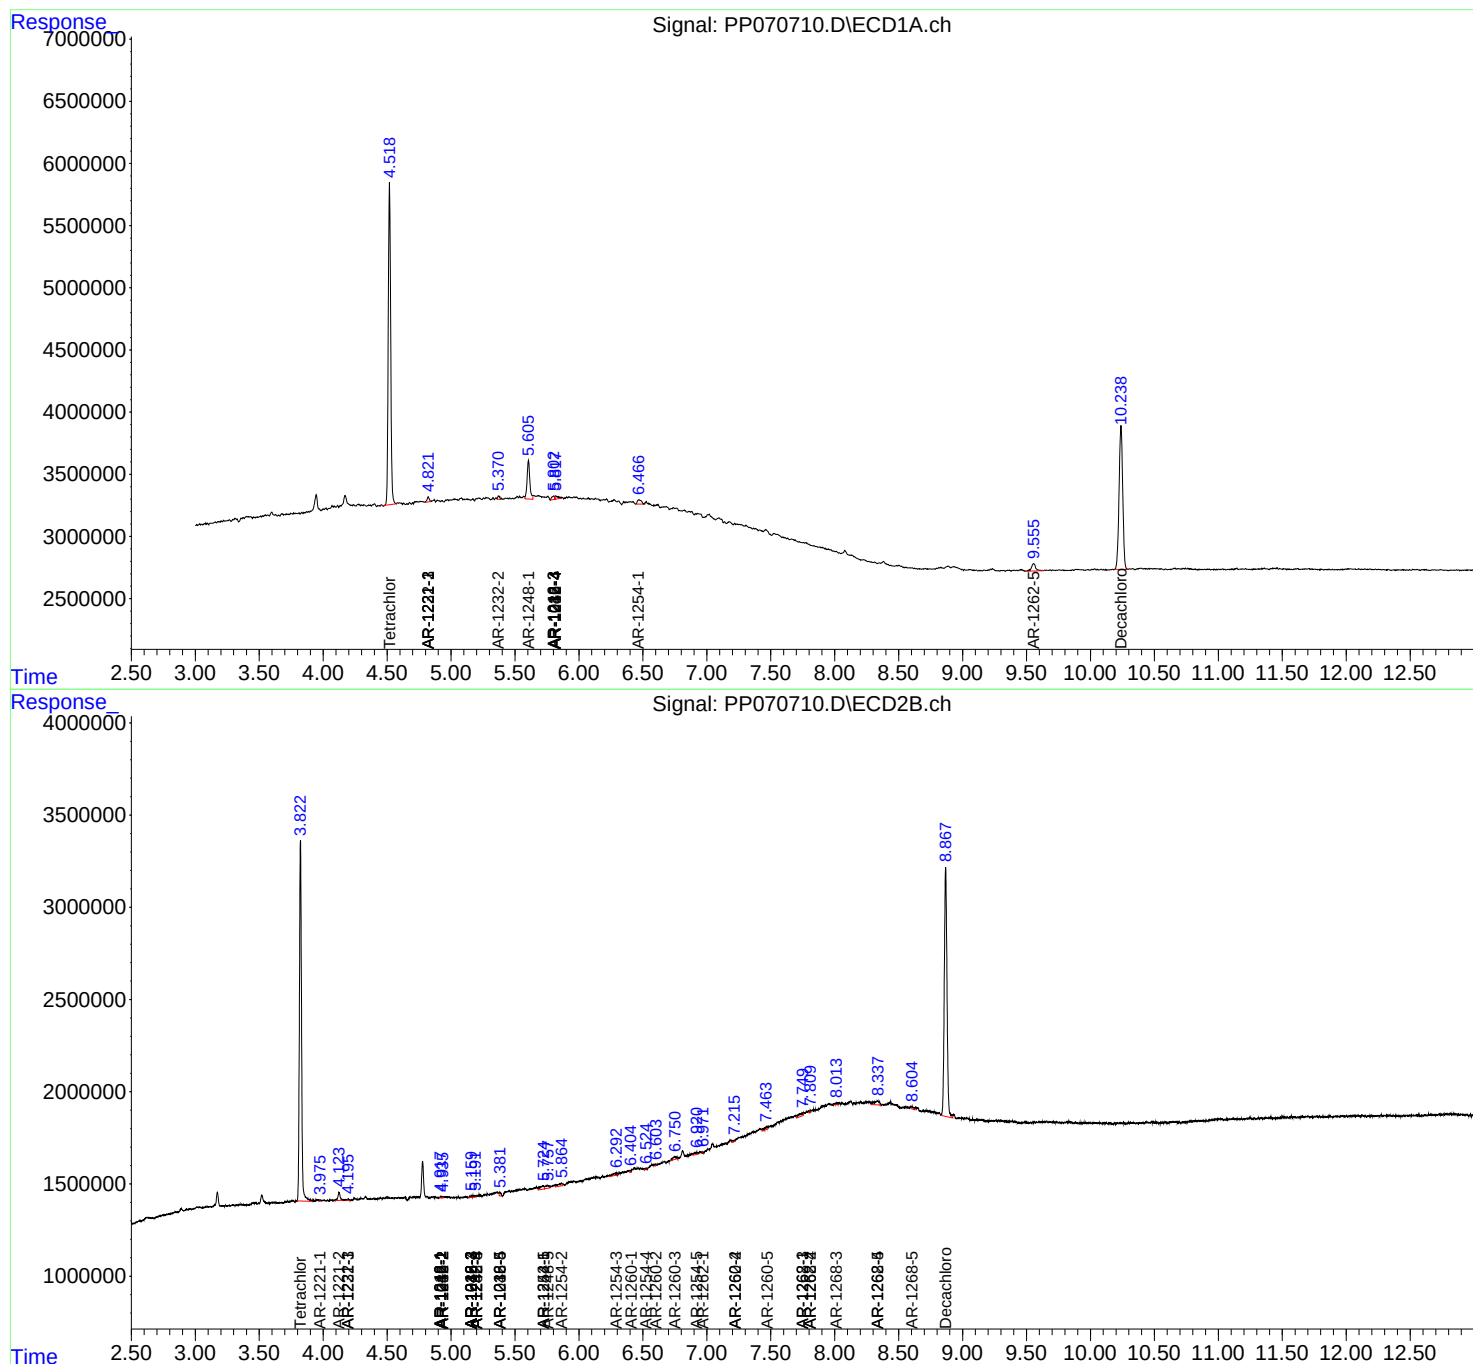


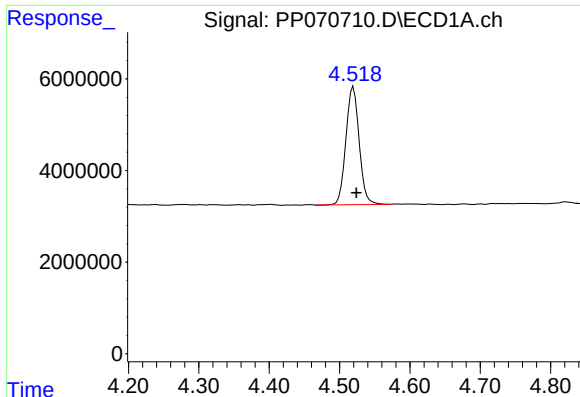

#1 Tetrachloro-m-xylene


R.T.: 4.520 min
Delta R.T.: -0.004 min
Response: 33734664
Conc: 21.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
2-CONCRETE-SLAB

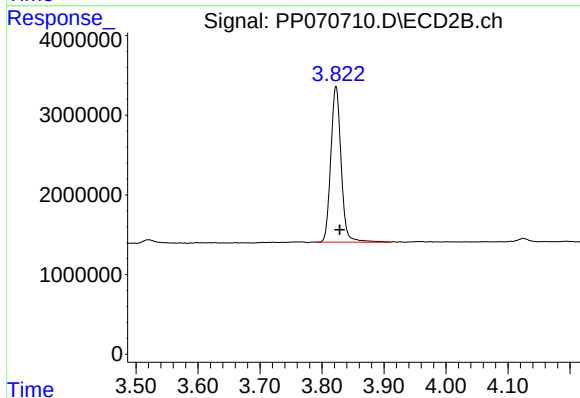


#1 Tetrachloro-m-xylene

R.T.: 3.823 min
Delta R.T.: -0.006 min
Response: 22615613
Conc: 22.56 ng/ml

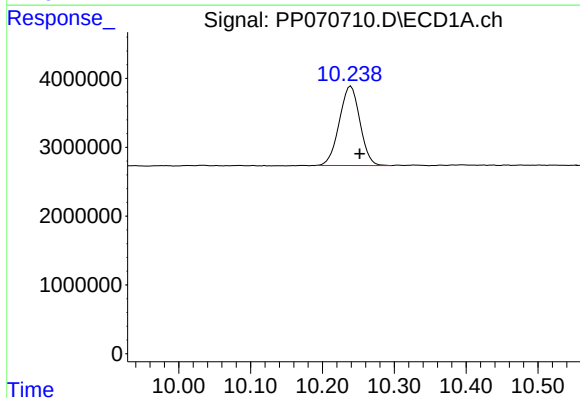


#2 Decachlorobiphenyl

R.T.: 10.240 min
Delta R.T.: -0.012 min
Response: 22963722
Conc: 21.62 ng/ml

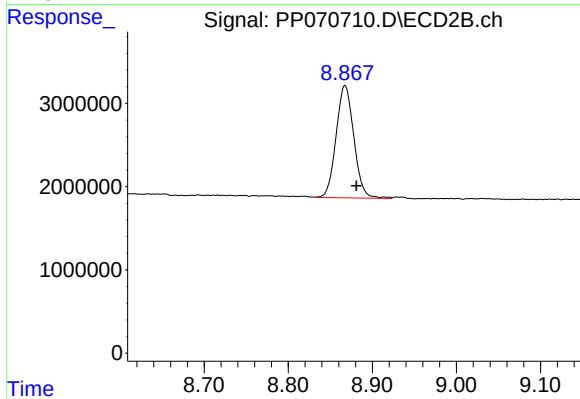

#2 Decachlorobiphenyl


R.T.: 8.868 min
Delta R.T.: -0.014 min
Response: 19767891
Conc: 20.21 ng/ml

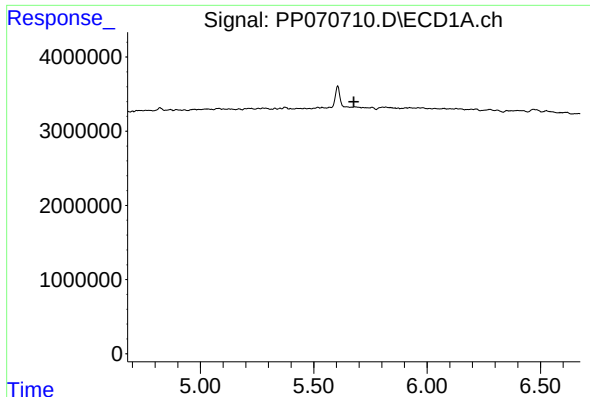

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.677 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
2-CONCRETE-SLAB

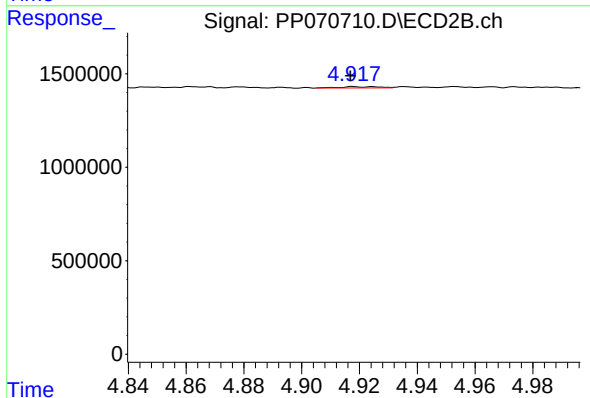


#3 AR-1016-1

R.T.: 4.918 min
Delta R.T.: 0.001 min
Response: 66371
Conc: 1.85 ng/ml

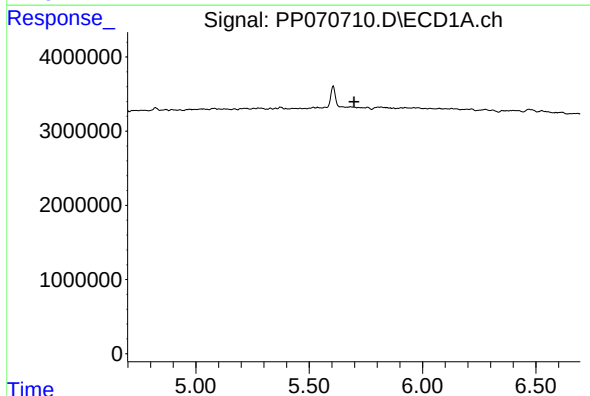


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.699 min
Response: 0
Conc: N.D.

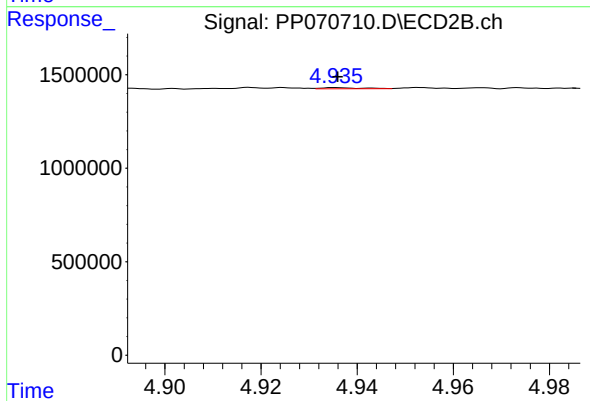

#4 AR-1016-2


R.T.: 4.936 min
Delta R.T.: 0.000 min
Response: 33698
Conc: 0.65 ng/ml

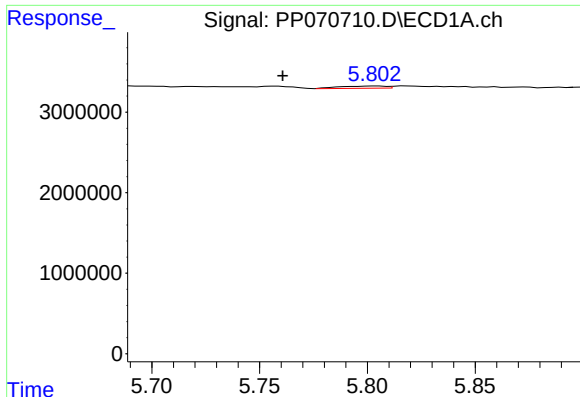

#5 AR-1016-3


R.T.: 5.804 min
Delta R.T.: 0.043 min
Response: 409744
Conc: 9.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
2-CONCRETE-SLAB

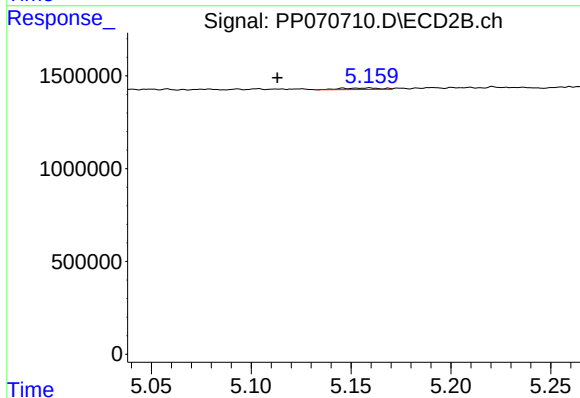


#5 AR-1016-3

R.T.: 5.159 min
Delta R.T.: 0.046 min
Response: 116864
Conc: 4.11 ng/ml

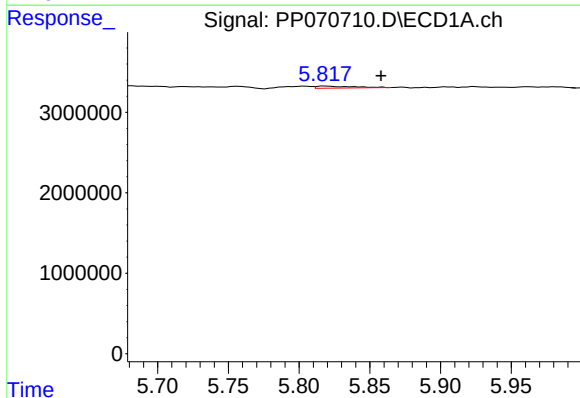


#6 AR-1016-4

R.T.: 5.819 min
Delta R.T.: -0.039 min
Response: 450213
Conc: 11.53 ng/ml

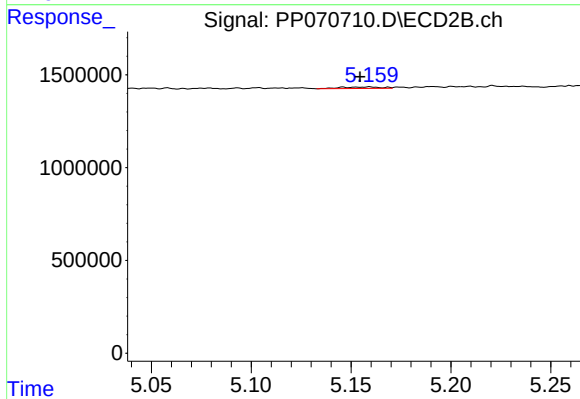

#6 AR-1016-4


R.T.: 5.159 min
Delta R.T.: 0.005 min
Response: 116864
Conc: 5.22 ng/ml

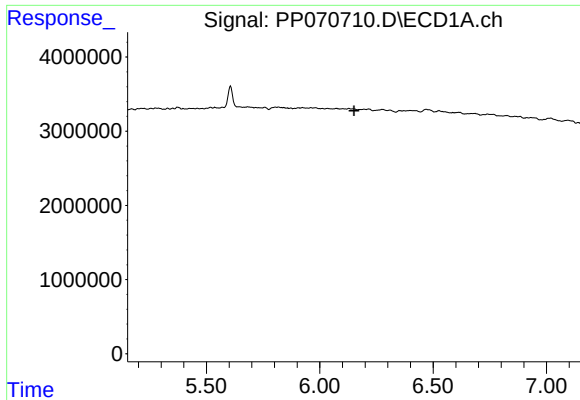

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.151 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
2-CONCRETE-SLAB

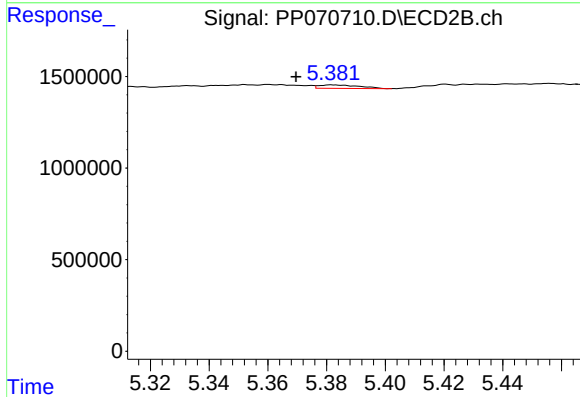


#7 AR-1016-5

R.T.: 5.382 min
Delta R.T.: 0.013 min
Response: 177668
Conc: 5.98 ng/ml

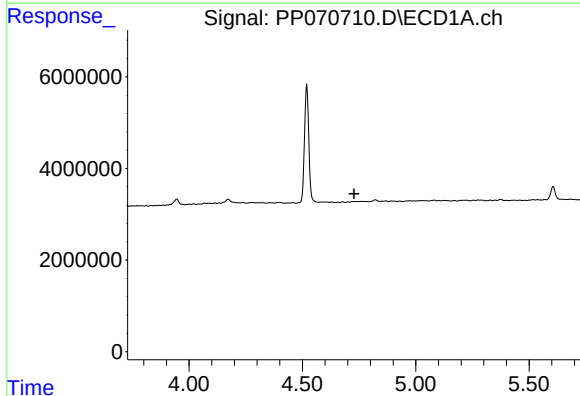


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T.: 4.728 min
Response: 0
Conc: N.D.

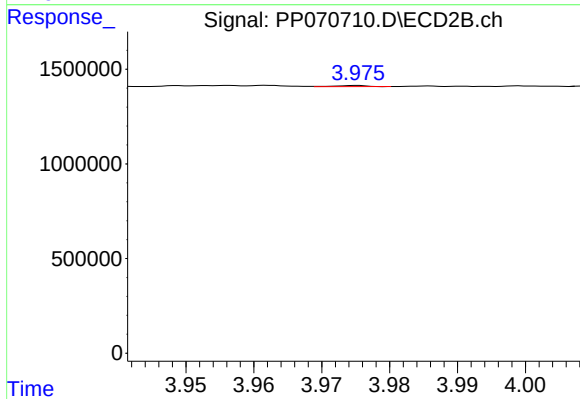

#8 AR-1221-1


R.T.: 3.975 min
Delta R.T.: -0.065 min
Response: 19302
Conc: 1.30 ng/ml

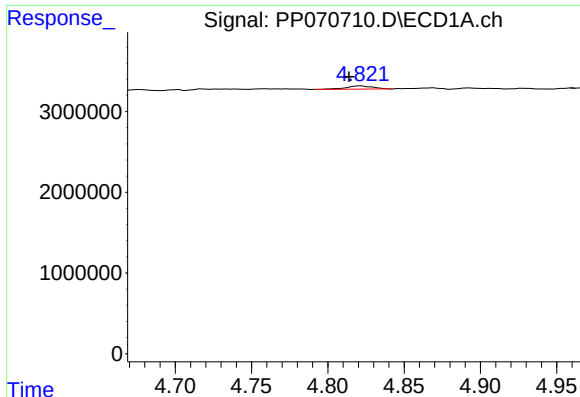

#9 AR-1221-2


R.T.: 4.822 min
Delta R.T.: 0.008 min
Response: 490578
Conc: 33.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
2-CONCRETE-SLAB

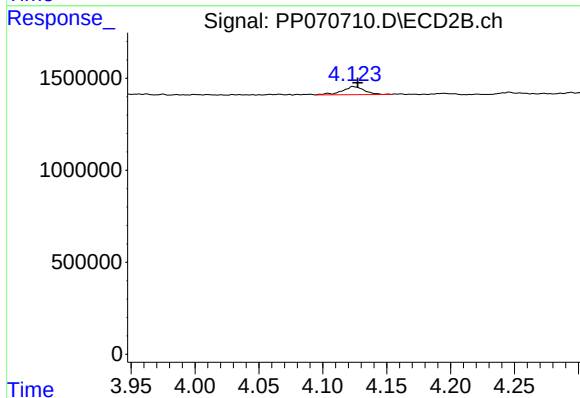


#9 AR-1221-2

R.T.: 4.124 min
Delta R.T.: -0.003 min
Response: 532408
Conc: 46.58 ng/ml

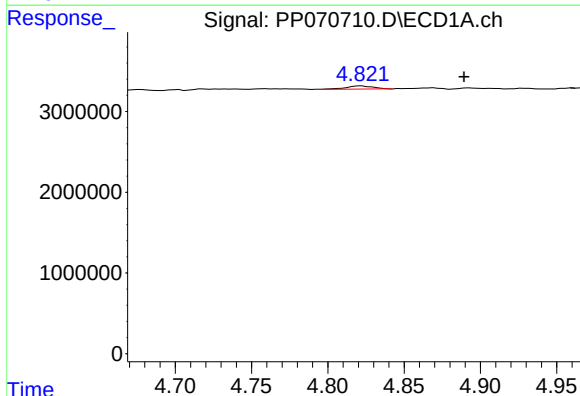


#10 AR-1221-3

R.T.: 4.822 min
Delta R.T.: -0.067 min
Response: 490578
Conc: 11.06 ng/ml

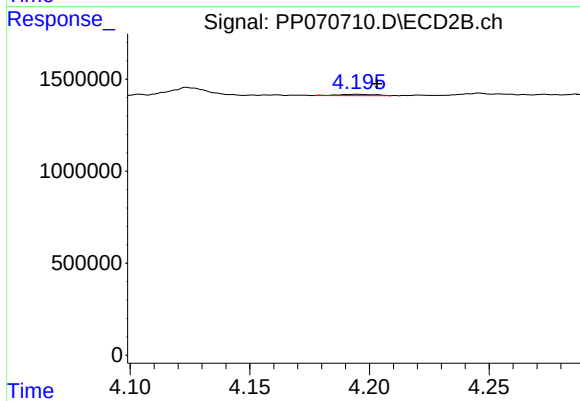

#10 AR-1221-3


R.T.: 4.195 min
Delta R.T.: -0.008 min
Response: 80520
Conc: 2.41 ng/ml

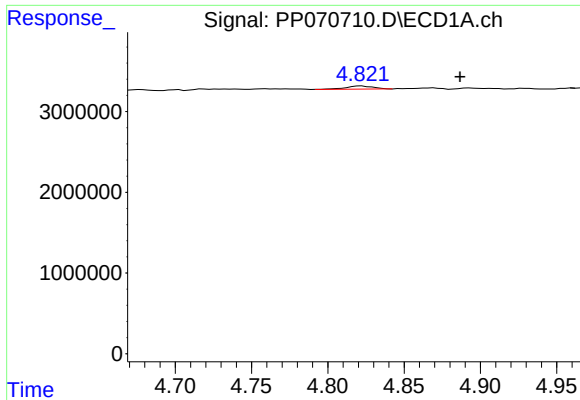

#11 AR-1232-1


R.T.: 4.822 min
Delta R.T.: -0.064 min
Response: 490578
Conc: 13.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
2-CONCRETE-SLAB

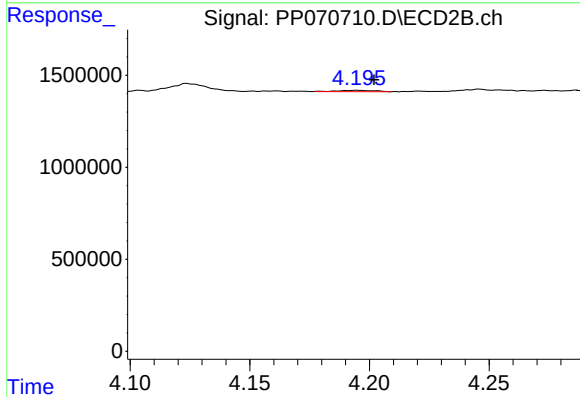


#11 AR-1232-1

R.T.: 4.195 min
Delta R.T.: -0.007 min
Response: 80520
Conc: 3.06 ng/ml

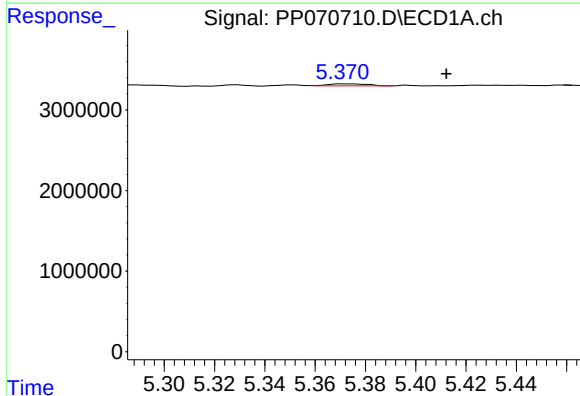


#12 AR-1232-2

R.T.: 5.371 min
Delta R.T.: -0.041 min
Response: 280120
Conc: 16.61 ng/ml

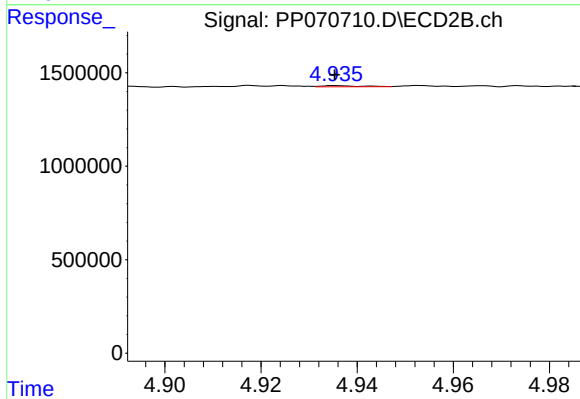

#12 AR-1232-2


R.T.: 4.936 min
Delta R.T.: 0.000 min
Response: 33698
Conc: 1.31 ng/ml

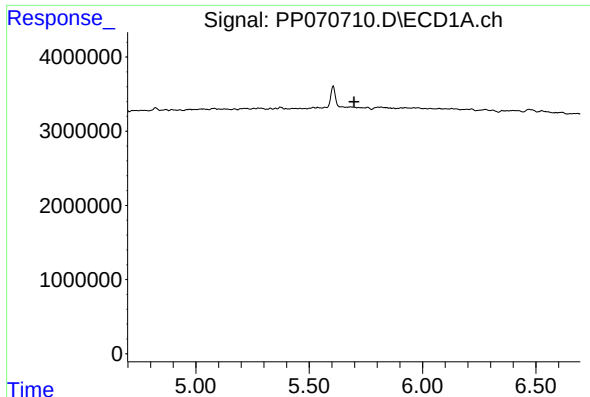

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 5.698 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
2-CONCRETE-SLAB

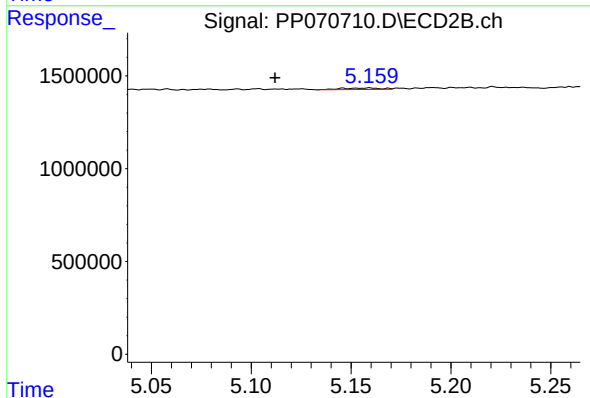


#13 AR-1232-3

R.T.: 5.159 min
Delta R.T.: 0.047 min
Response: 116864
Conc: 8.34 ng/ml

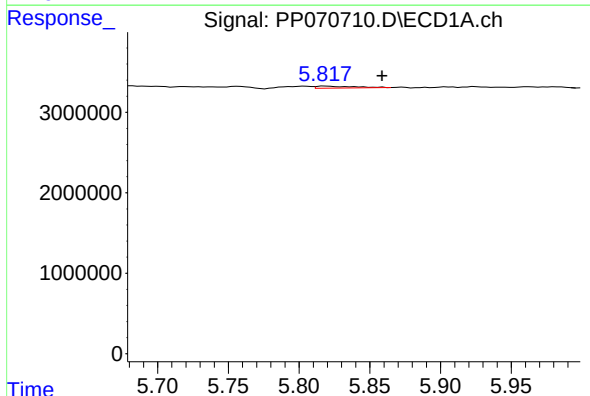


#14 AR-1232-4

R.T.: 5.819 min
Delta R.T.: -0.040 min
Response: 450213
Conc: 23.70 ng/ml

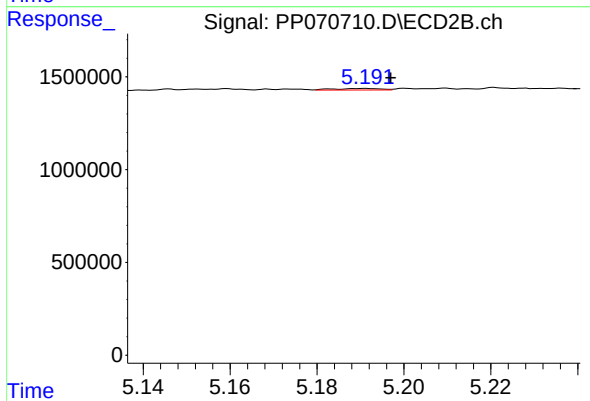

#14 AR-1232-4


R.T.: 5.191 min
Delta R.T.: -0.006 min
Response: 62690
Conc: 5.35 ng/ml

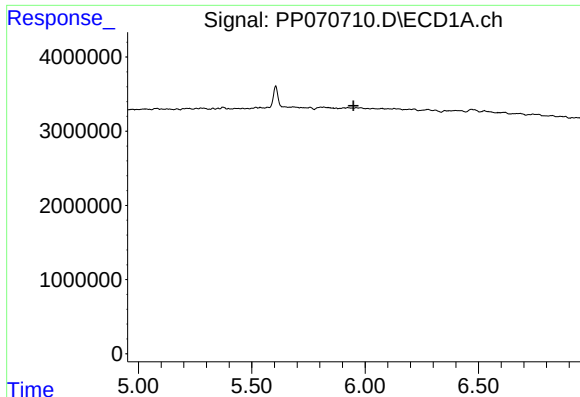

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 5.949 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
2-CONCRETE-SLAB

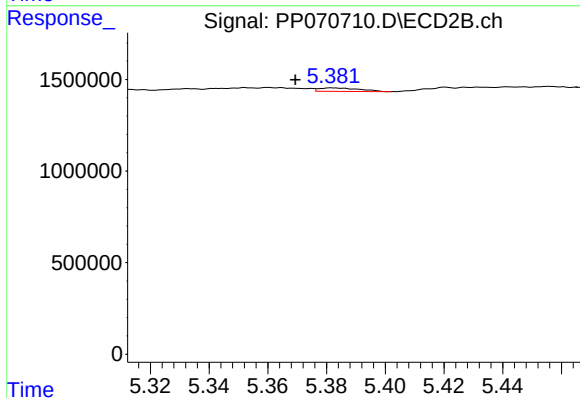


#15 AR-1232-5

R.T.: 5.382 min
Delta R.T.: 0.013 min
Response: 177668
Conc: 13.60 ng/ml

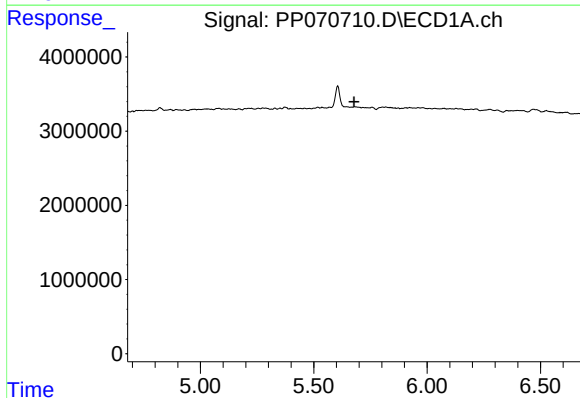


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T.: 5.678 min
Response: 0
Conc: N.D.

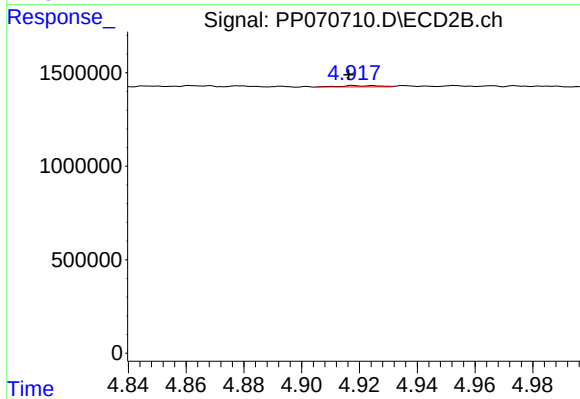

#16 AR-1242-1


R.T.: 4.918 min
Delta R.T.: 0.002 min
Response: 66371
Conc: 2.17 ng/ml

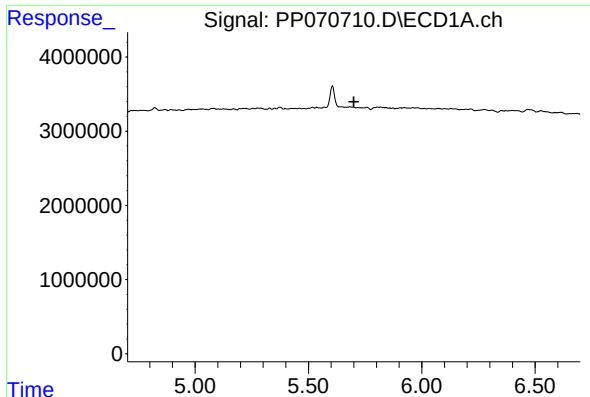

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 5.700 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
2-CONCRETE-SLAB

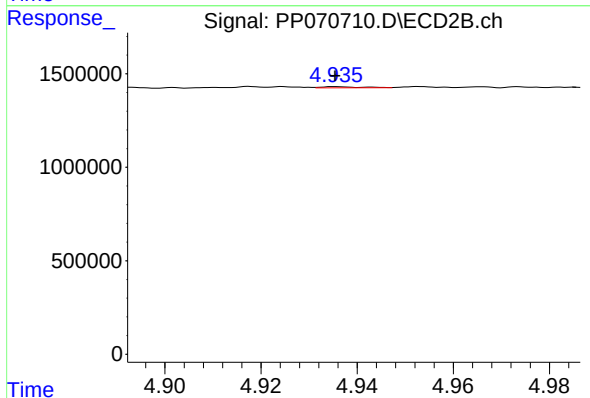


#17 AR-1242-2

R.T.: 4.936 min
Delta R.T.: 0.000 min
Response: 33698
Conc: 0.77 ng/ml

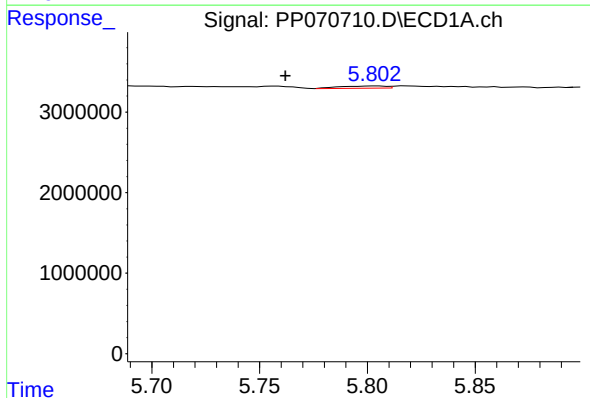


#18 AR-1242-3

R.T.: 5.804 min
Delta R.T.: 0.042 min
Response: 409744
Conc: 11.04 ng/ml

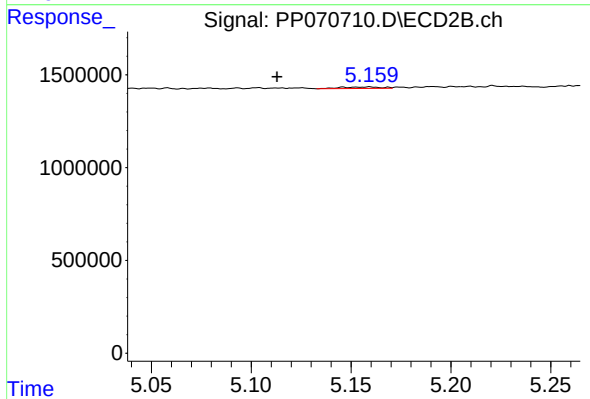

#18 AR-1242-3


R.T.: 5.159 min
Delta R.T.: 0.046 min
Response: 116864
Conc: 4.90 ng/ml

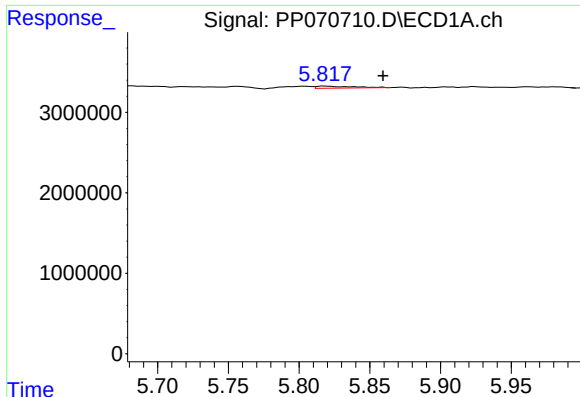

#19 AR-1242-4


R.T.: 5.819 min
Delta R.T.: -0.041 min
Response: 450213
Conc: 14.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
2-CONCRETE-SLAB

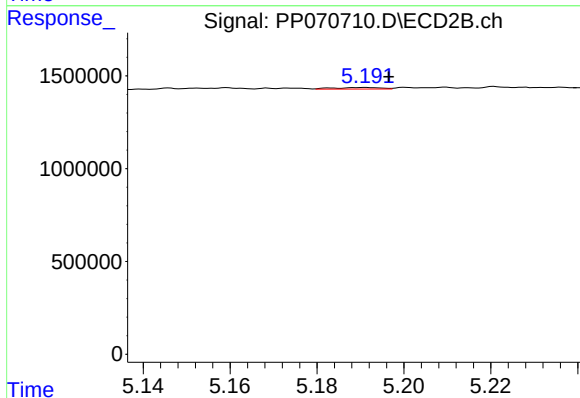


#19 AR-1242-4

R.T.: 5.191 min
Delta R.T.: -0.006 min
Response: 62690
Conc: 2.84 ng/ml

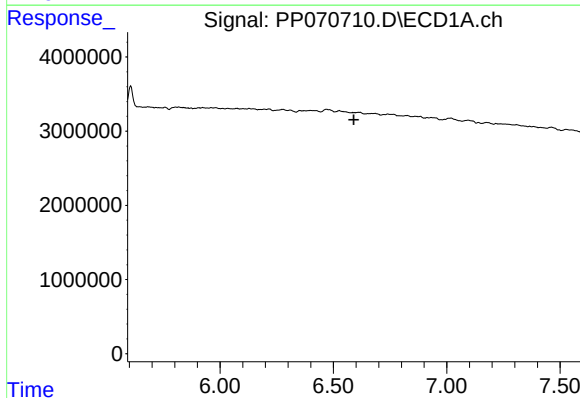


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.590 min
Response: 0
Conc: N.D.

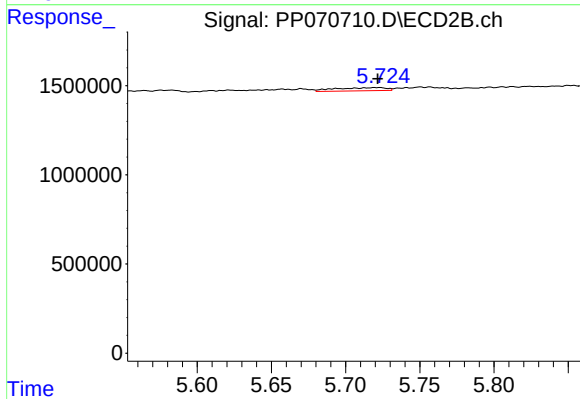

#20 AR-1242-5


R.T.: 5.723 min
Delta R.T.: 0.000 min
Response: 420759
Conc: 15.07 ng/ml

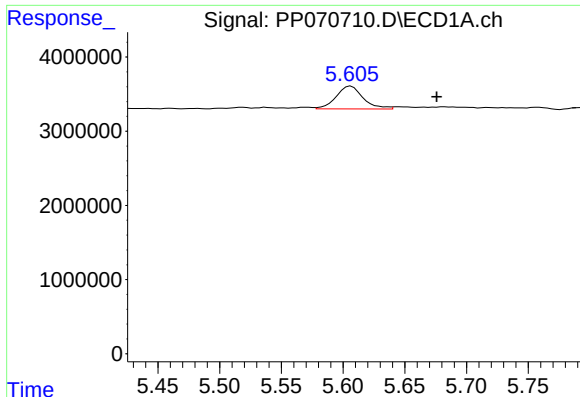

#21 AR-1248-1


R.T.: 5.606 min
Delta R.T.: -0.070 min
Response: 4668396
Conc: 136.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
2-CONCRETE-SLAB

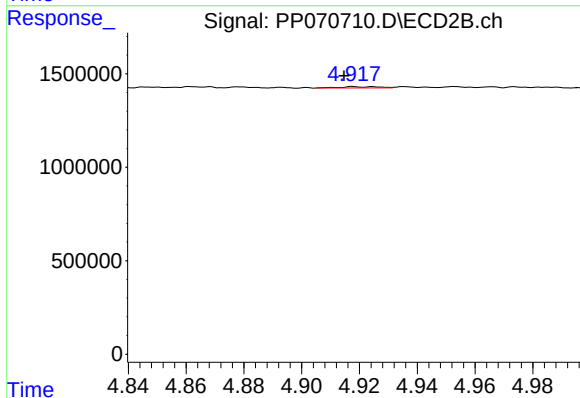


#21 AR-1248-1

R.T.: 4.918 min
Delta R.T.: 0.003 min
Response: 66371
Conc: 2.83 ng/ml

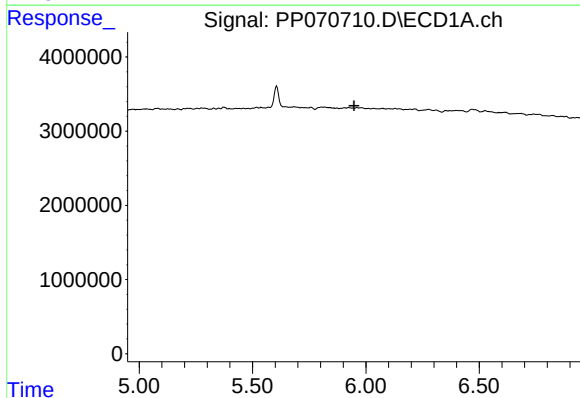


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T. : 5.948 min
Response: 0
Conc: N.D.

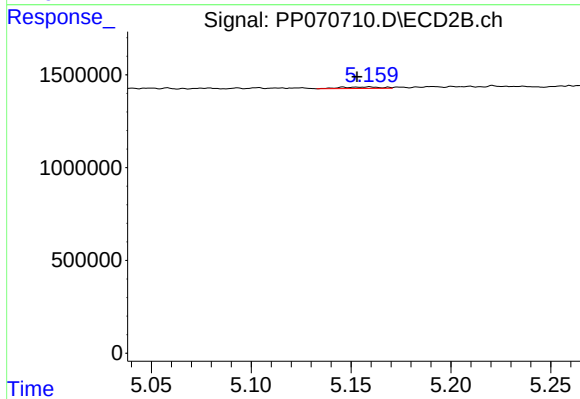

#22 AR-1248-2


R.T.: 5.159 min
Delta R.T.: 0.006 min
Response: 116864
Conc: 3.73 ng/ml

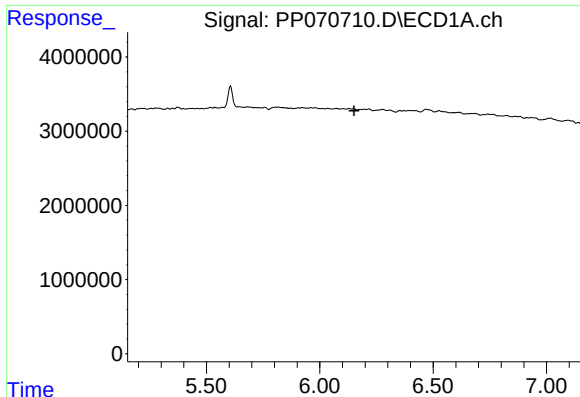

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 6.151 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
2-CONCRETE-SLAB

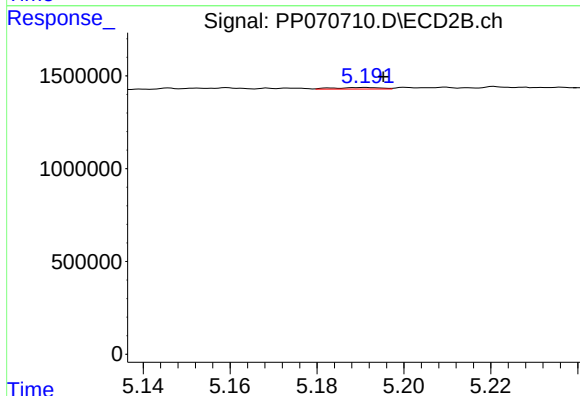


#23 AR-1248-3

R.T.: 5.191 min
Delta R.T.: -0.004 min
Response: 62690
Conc: 1.98 ng/ml

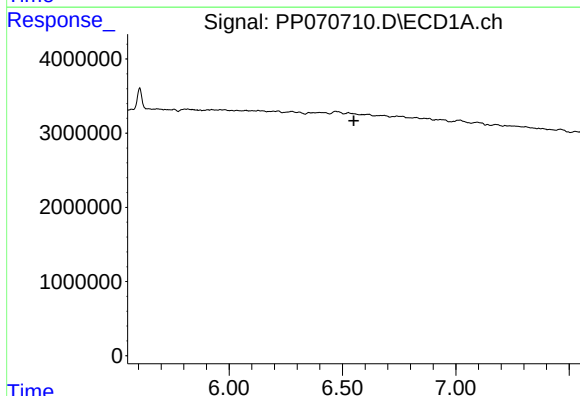


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 6.550 min
Response: 0
Conc: N.D.

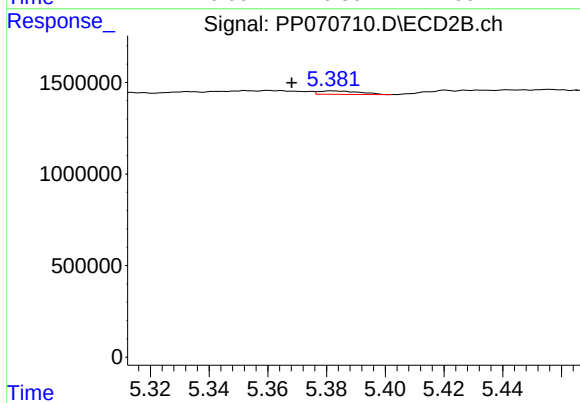

#24 AR-1248-4


R.T.: 5.382 min
Delta R.T.: 0.014 min
Response: 177668
Conc: 4.56 ng/ml

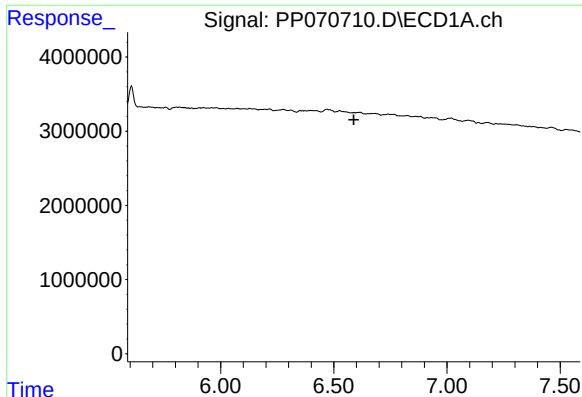

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.589 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
2-CONCRETE-SLAB

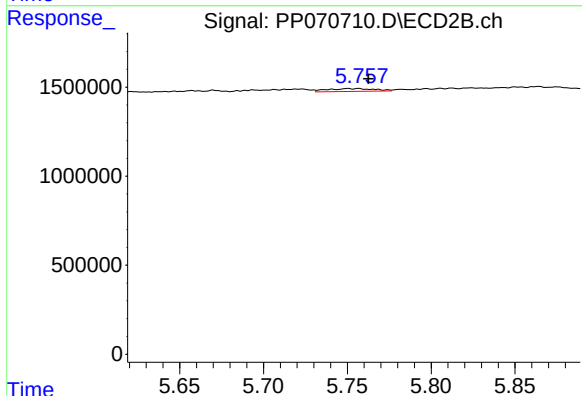


#25 AR-1248-5

R.T.: 5.757 min
Delta R.T.: -0.006 min
Response: 314770
Conc: 8.26 ng/ml

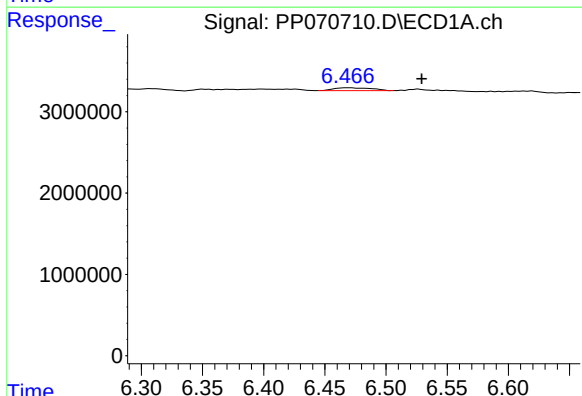


#26 AR-1254-1

R.T.: 6.468 min
Delta R.T.: -0.061 min
Response: 736098
Conc: 12.86 ng/ml

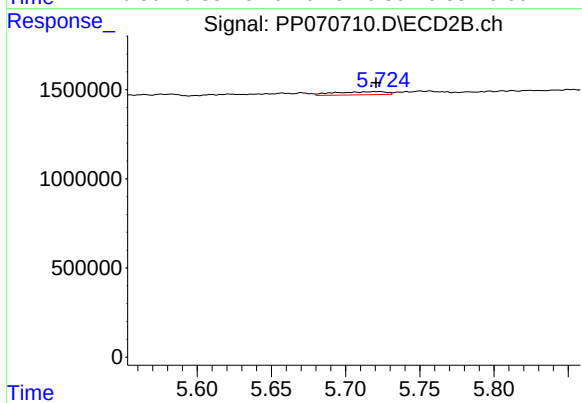

#26 AR-1254-1


R.T.: 5.723 min
Delta R.T.: 0.002 min
Response: 420759
Conc: 7.47 ng/ml

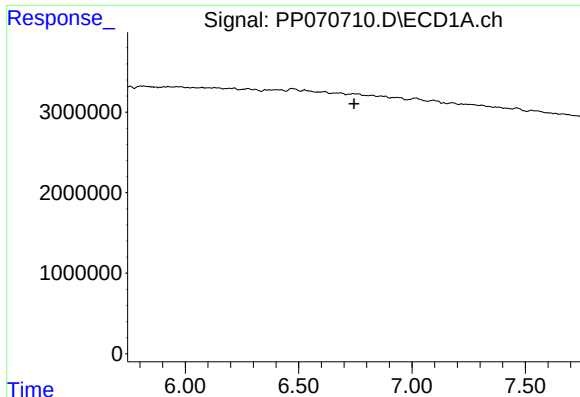

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 6.745 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
2-CONCRETE-SLAB

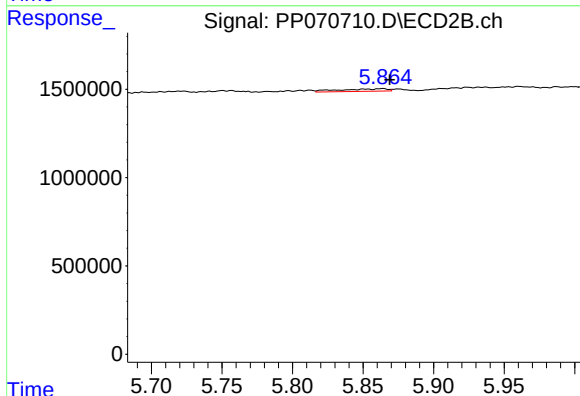


#27 AR-1254-2

R.T.: 5.864 min
Delta R.T.: -0.005 min
Response: 343040
Conc: 7.01 ng/ml

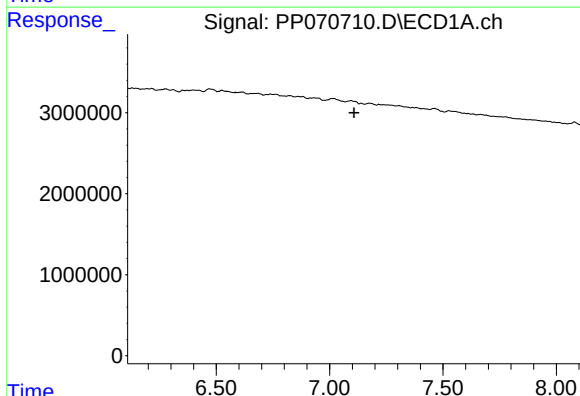


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T.: 7.108 min
Response: 0
Conc: N.D.

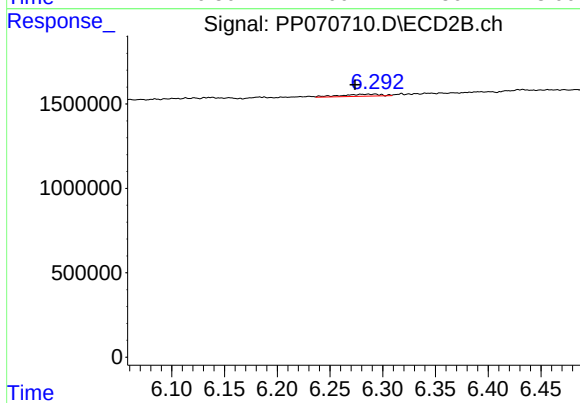

#28 AR-1254-3


R.T.: 6.293 min
Delta R.T.: 0.019 min
Response: 321700
Conc: 4.27 ng/ml

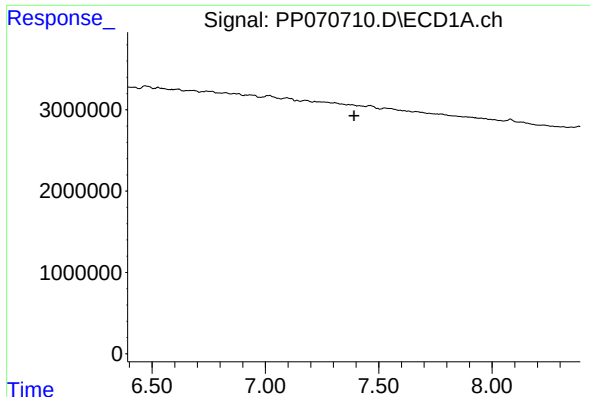

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.391 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
2-CONCRETE-SLAB

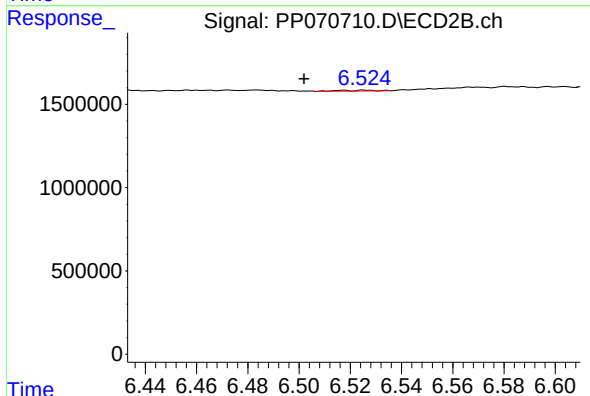


#29 AR-1254-4

R.T.: 6.517 min
Delta R.T.: 0.015 min
Response: 48251
Conc: 0.91 ng/ml

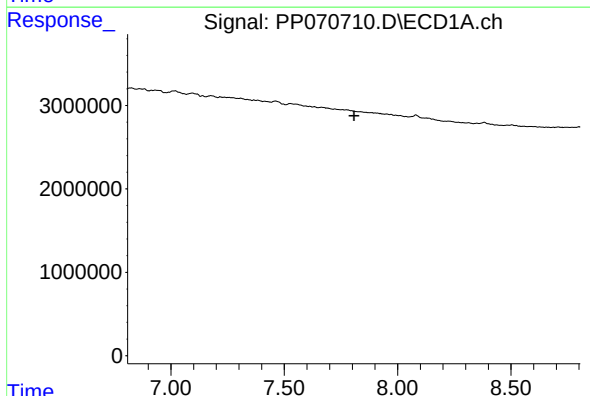


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T.: 7.808 min
Response: 0
Conc: N.D.

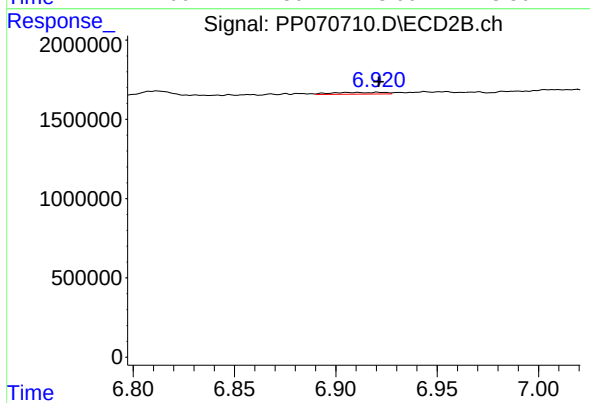

#30 AR-1254-5


R.T.: 6.921 min
Delta R.T.: 0.000 min
Response: 194799
Conc: 2.82 ng/ml

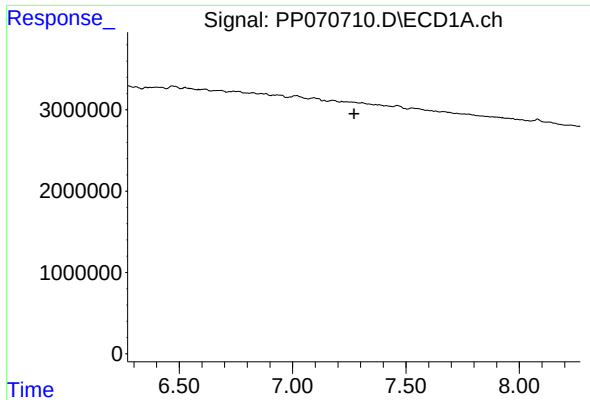

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.271 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
2-CONCRETE-SLAB

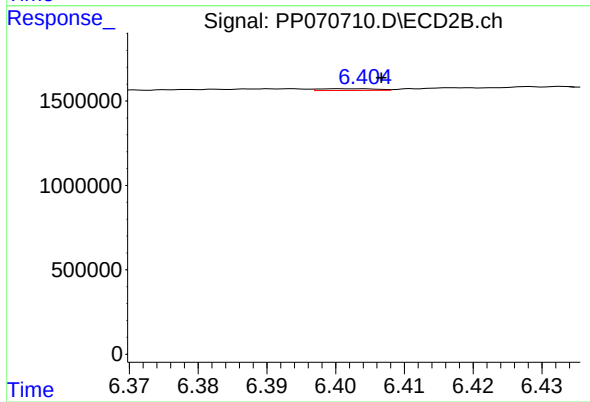


#31 AR-1260-1

R.T.: 6.402 min
Delta R.T.: -0.005 min
Response: 58554
Conc: 1.18 ng/ml

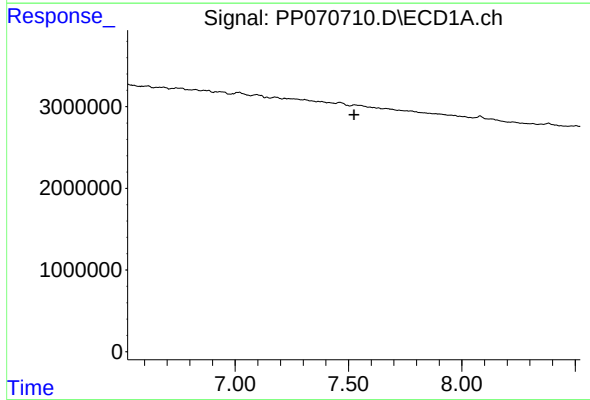


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.525 min
Response: 0
Conc: N.D.

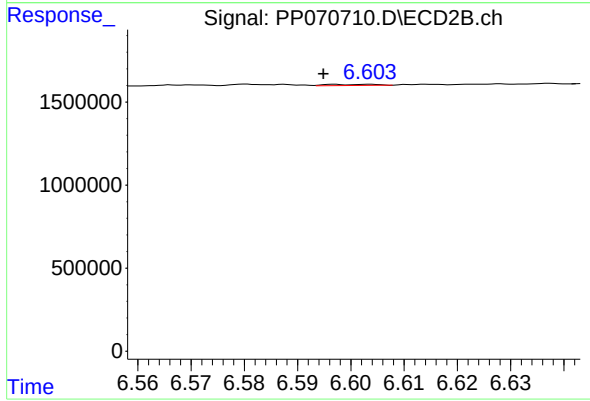

#32 AR-1260-2


R.T.: 6.603 min
Delta R.T.: 0.008 min
Response: 46040
Conc: 0.70 ng/ml

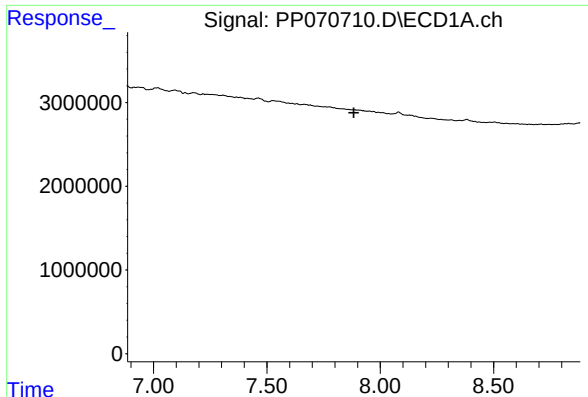

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.883 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
2-CONCRETE-SLAB

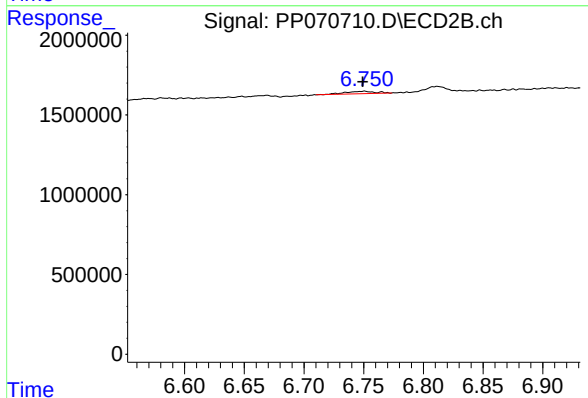


#33 AR-1260-3

R.T.: 6.750 min
Delta R.T.: 0.001 min
Response: 273048
Conc: 4.77 ng/ml

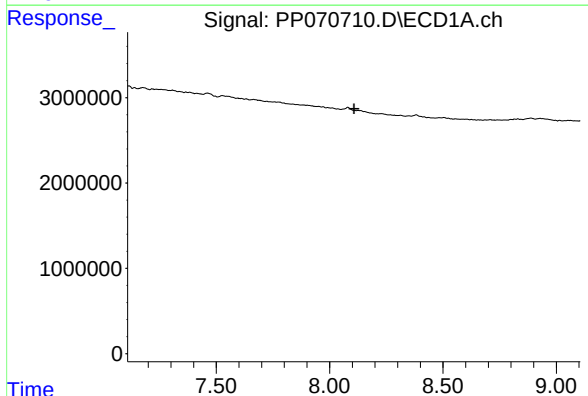


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 8.108 min
Response: 0
Conc: N.D.

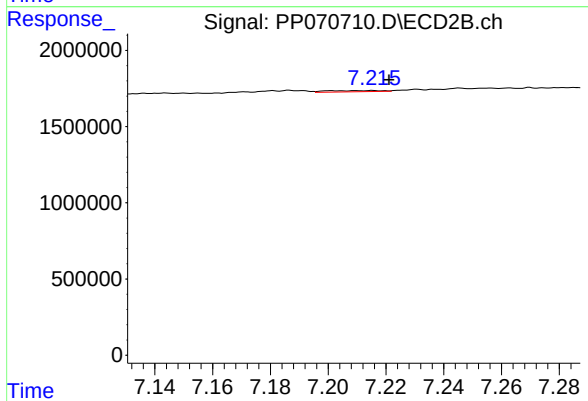

#34 AR-1260-4


R.T.: 7.215 min
Delta R.T.: -0.006 min
Response: 104343
Conc: 2.04 ng/ml

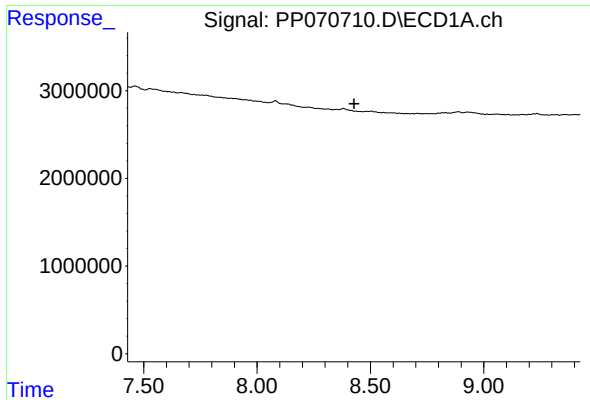

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 8.428 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
2-CONCRETE-SLAB

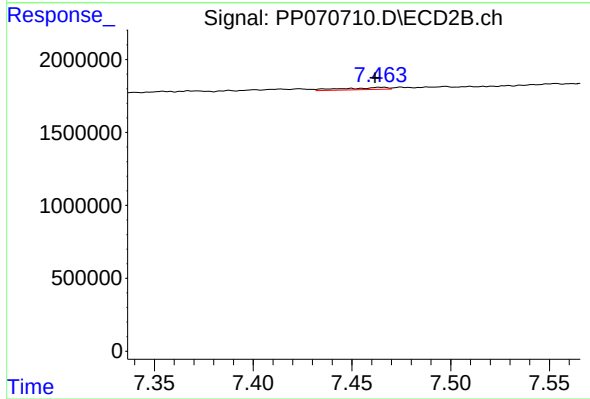


#35 AR-1260-5

R.T.: 7.465 min
Delta R.T.: 0.003 min
Response: 229005
Conc: 1.78 ng/ml

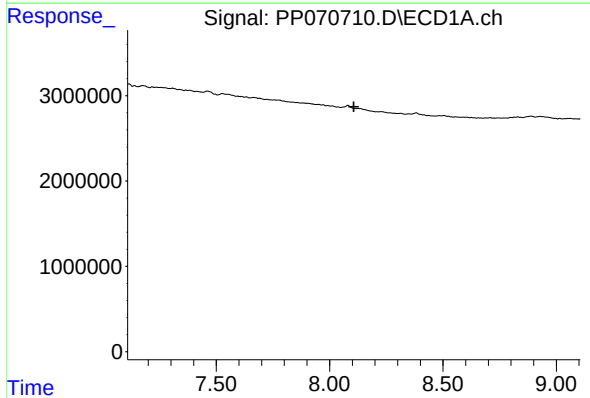


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 8.107 min
Response: 0
Conc: N.D.

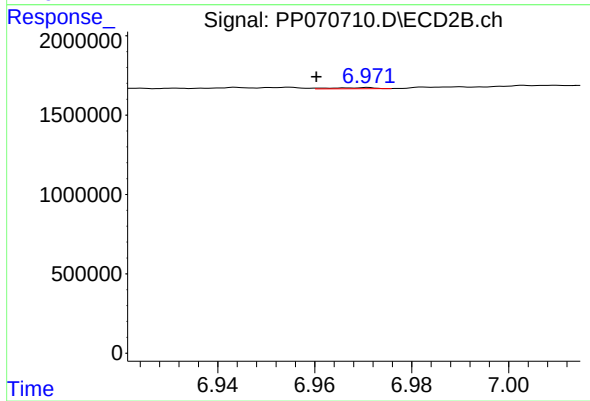

#36 AR-1262-1


R.T.: 6.970 min
Delta R.T.: 0.010 min
Response: 41073
Conc: 0.49 ng/ml

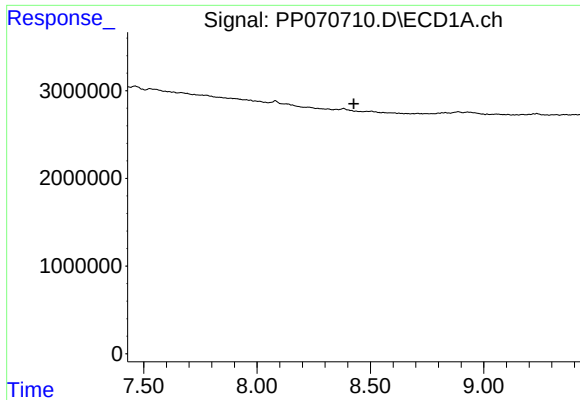

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.427 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
2-CONCRETE-SLAB

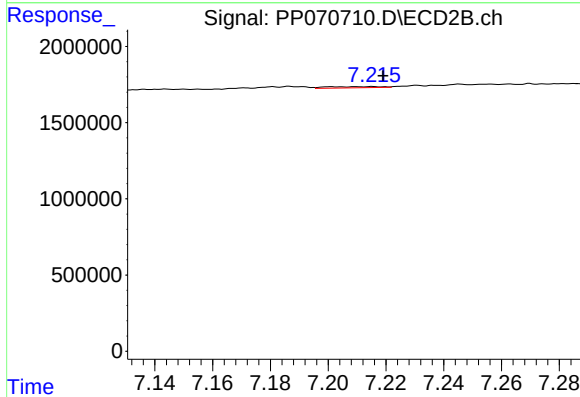


#37 AR-1262-2

R.T.: 7.215 min
Delta R.T.: -0.004 min
Response: 104343
Conc: 1.52 ng/ml

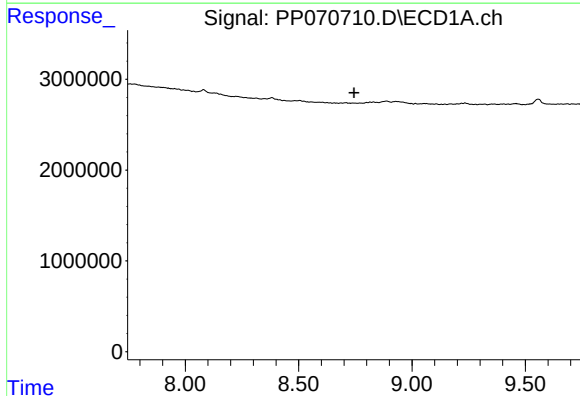


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.745 min
Response: 0
Conc: N.D.

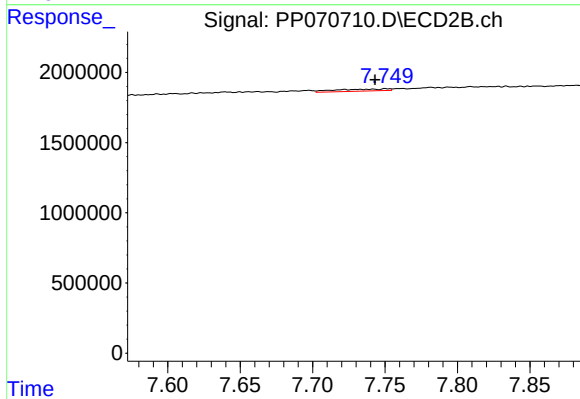

#38 AR-1262-3


R.T.: 7.751 min
Delta R.T.: 0.008 min
Response: 383429
Conc: 5.81 ng/ml

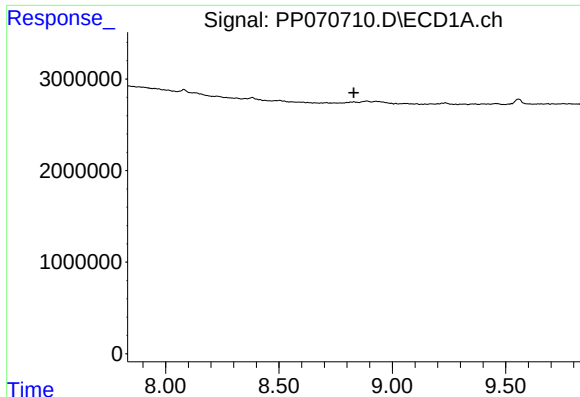

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.830 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
2-CONCRETE-SLAB

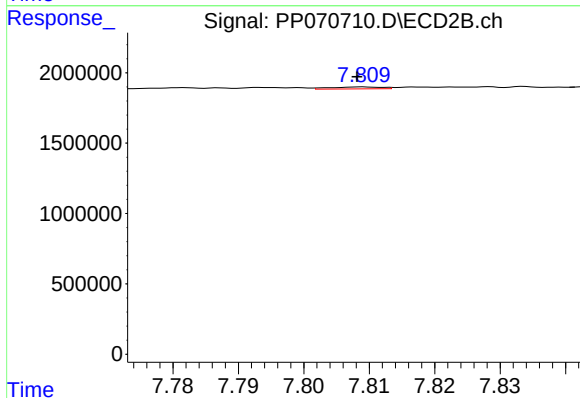


#39 AR-1262-4

R.T.: 7.809 min
Delta R.T.: 0.000 min
Response: 72358
Conc: 0.69 ng/ml

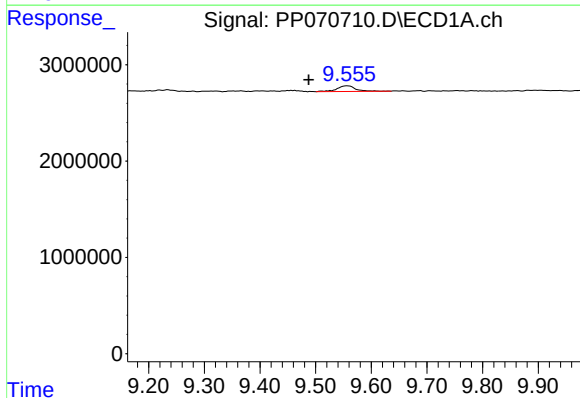


#40 AR-1262-5

R.T.: 9.557 min
Delta R.T.: 0.069 min
Response: 1393190
Conc: 23.65 ng/ml

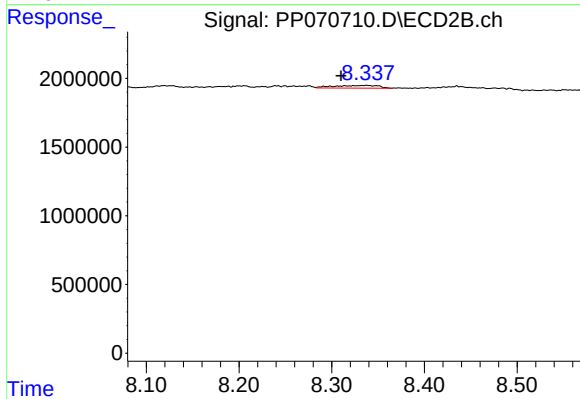

#40 AR-1262-5


R.T.: 8.338 min
Delta R.T.: 0.027 min
Response: 653796
Conc: 12.68 ng/ml

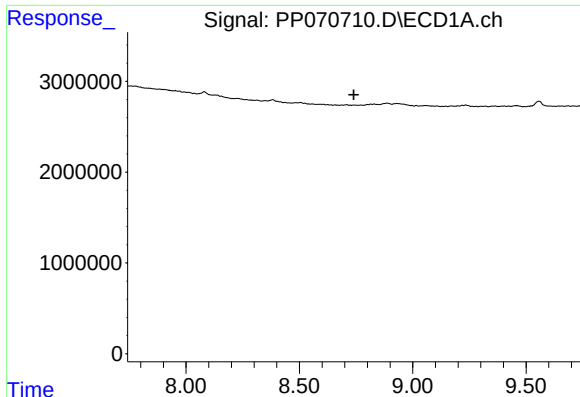

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.740 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
2-CONCRETE-SLAB

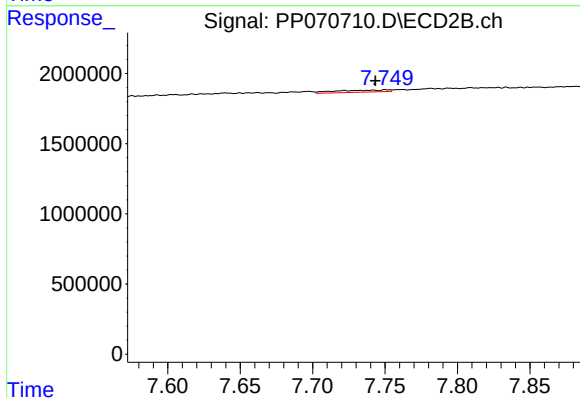


#41 AR-1268-1

R.T.: 7.751 min
Delta R.T.: 0.007 min
Response: 383429
Conc: 2.19 ng/ml

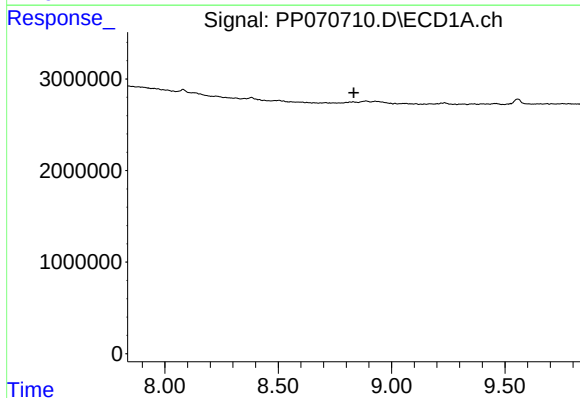


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.833 min
Response: 0
Conc: N.D.

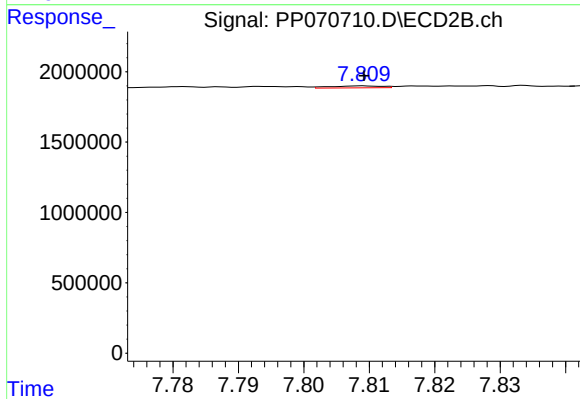

#42 AR-1268-2


R.T.: 7.809 min
Delta R.T.: 0.000 min
Response: 72358
Conc: 0.50 ng/ml

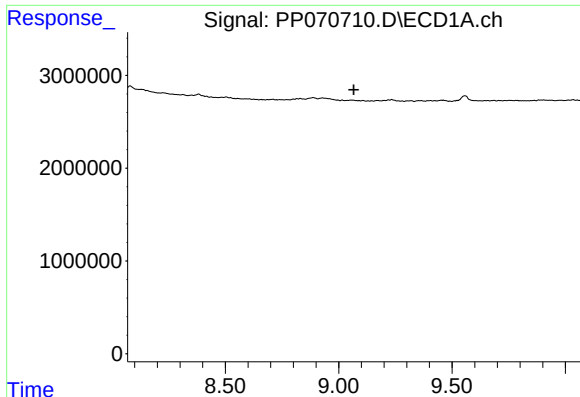

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.066 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
2-CONCRETE-SLAB

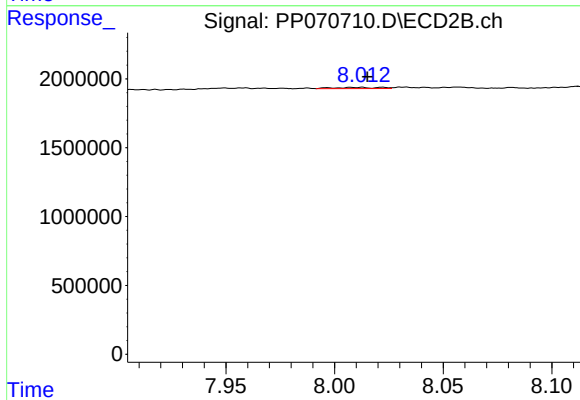


#43 AR-1268-3

R.T.: 8.013 min
Delta R.T.: -0.002 min
Response: 120242
Conc: 0.94 ng/ml

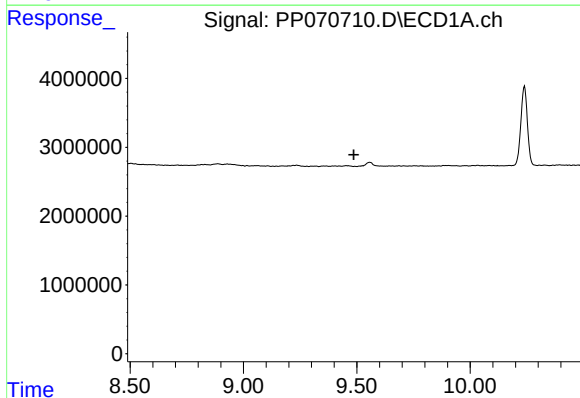


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.487 min
Response: 0
Conc: N.D.

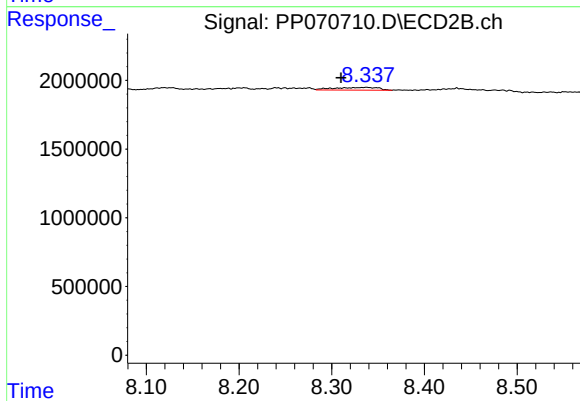

#44 AR-1268-4


R.T.: 8.338 min
Delta R.T.: 0.028 min
Response: 653796
Conc: 11.89 ng/ml

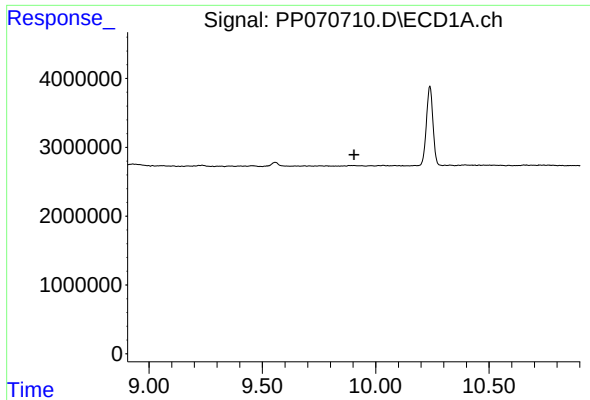

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
2-CONCRETE-SLAB

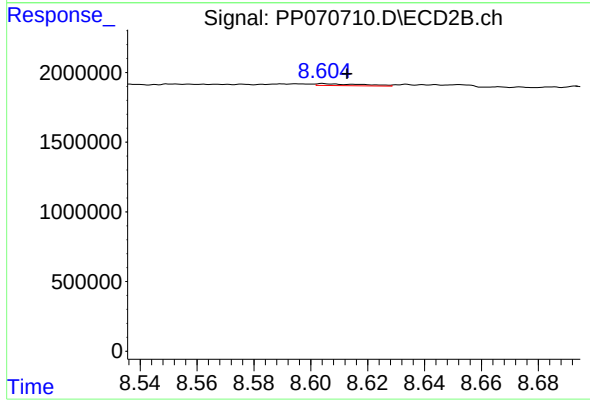

#45 AR-1268-5

R.T.: 8.604 min
Delta R.T.: -0.008 min
Response: 154147
Conc: 0.42 ng/ml