

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032019\
 Data File : PP029446.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Mar 2019 19:43
 Operator : EI\MA
 Sample : K1688-26
 Misc : hexane
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 JC-02-031919-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 21 13:08:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 22 02:24:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.925	12.124	8372386	11957824	278.556	315.073
Target Compounds							
8) T	DICHLORPROP	0.000	13.558	0	406896	N.D.	12.035 #
10) T	Pentachlo...	0.000	14.644	0	264574	N.D.	0.514 #
11) T	2,4,5-TP ...	0.000	15.187	0	12073901	N.D.	59.358 #
12) T	2,4,5-T	0.000	15.865	0	1025714	N.D.	6.195 #
13) T	2,4-DB	16.226	16.462	212993	1164186	11.150	51.681 #
14) T	DINOSEB	17.678	0.000	151537	0	1.041	N.D. #
15) T	Picloram	17.460	18.255	915585	2046414	3.293	9.094 #
16) T	DCPA	18.052	18.143	210999	2266741	0.747	9.754 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032019\
Data File : PP029446.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Mar 2019 19:43
Operator : EI\MA
Sample : K1688-26
Misc : hexane
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
JC-02-031919-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 21 13:08:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
Quant Title : 8080.M
QLast Update : Fri Feb 22 02:24:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

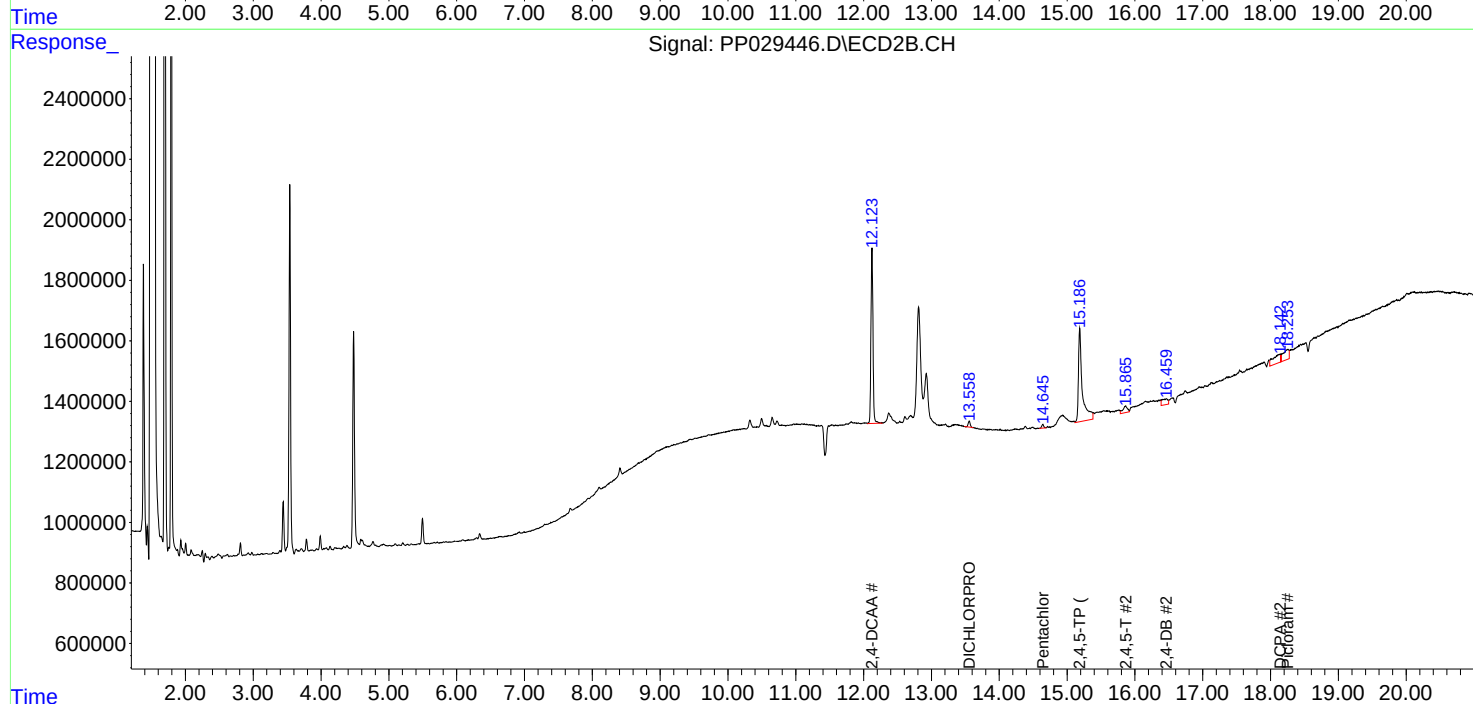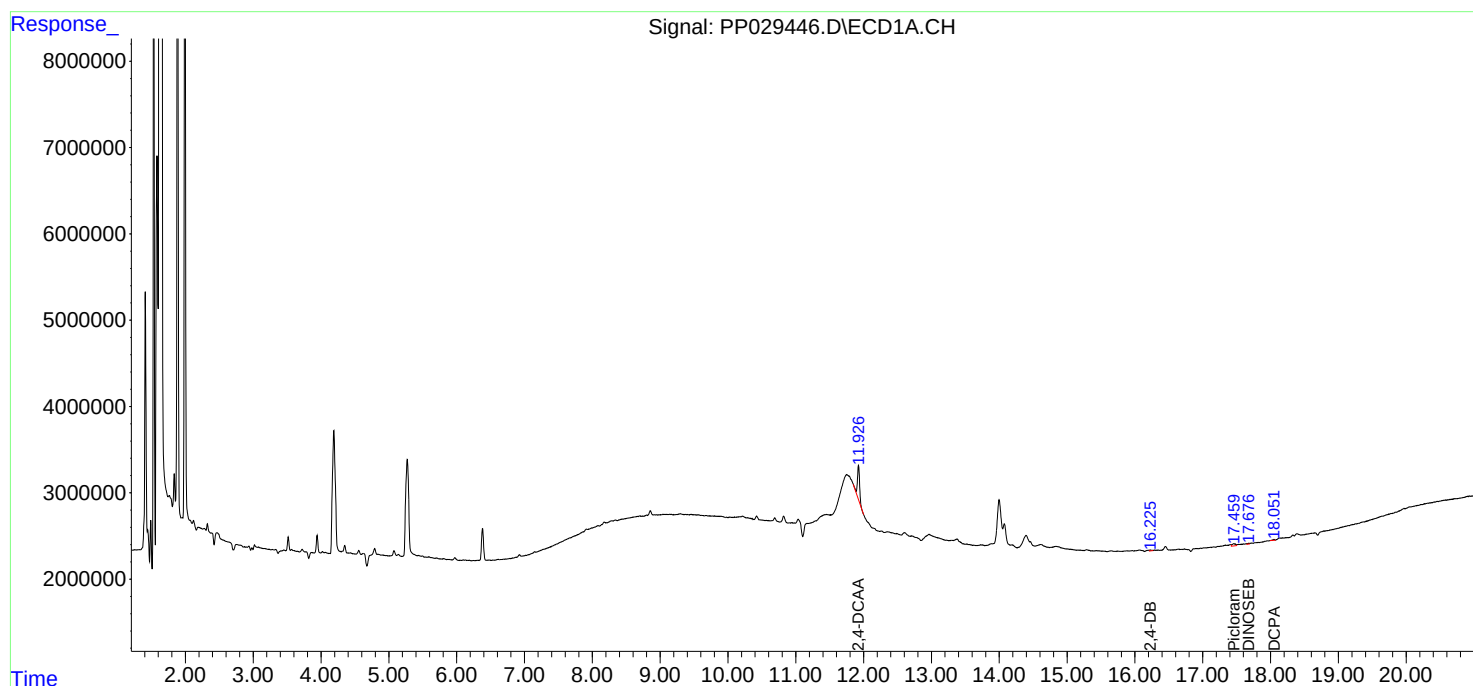


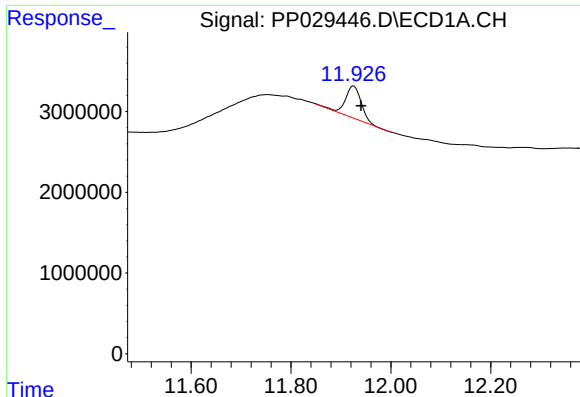

#4 2,4-DCAA


R.T.: 11.925 min
Delta R.T.: -0.015 min
Response: 8372386
Conc: 278.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
JC-02-031919-C

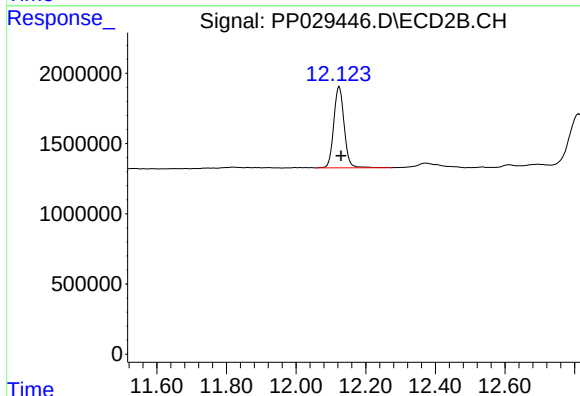


#4 2,4-DCAA

R.T.: 12.124 min
Delta R.T.: -0.005 min
Response: 11957824
Conc: 315.07 ng/ml

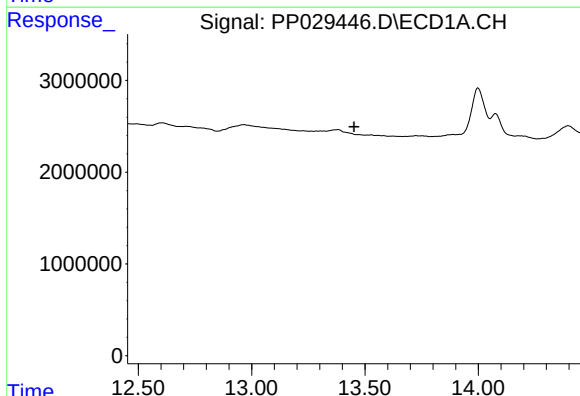


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.452 min
Response: 0
Conc: N.D.

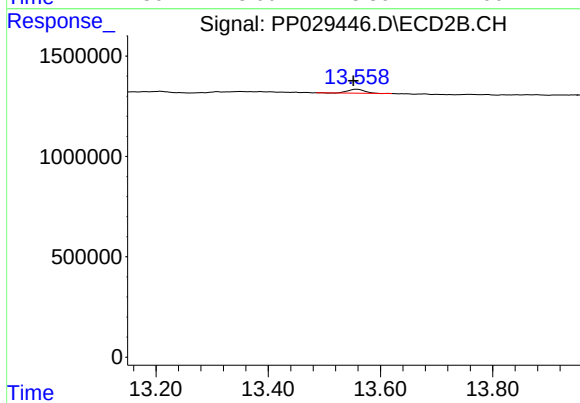

#8 DICHLORPROP


R.T.: 13.558 min
Delta R.T.: 0.007 min
Response: 406896
Conc: 12.04 ng/ml

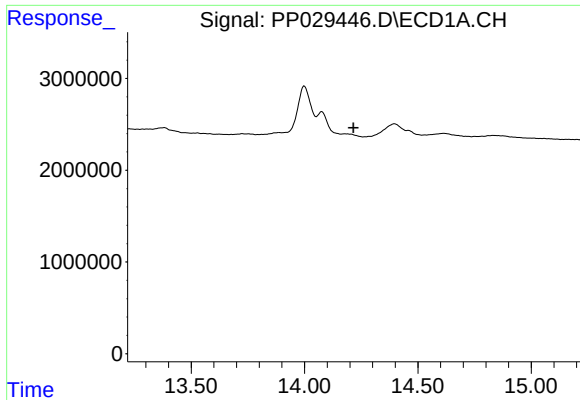

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 14.216 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
JC-02-031919-C

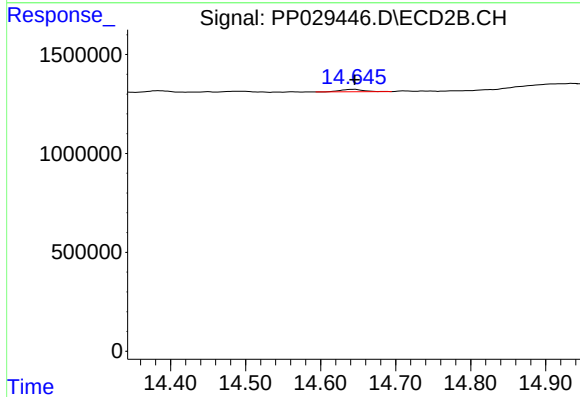


#10 Pentachlorophenol

R.T.: 14.644 min
Delta R.T.: 0.000 min
Response: 264574
Conc: 0.51 ng/ml

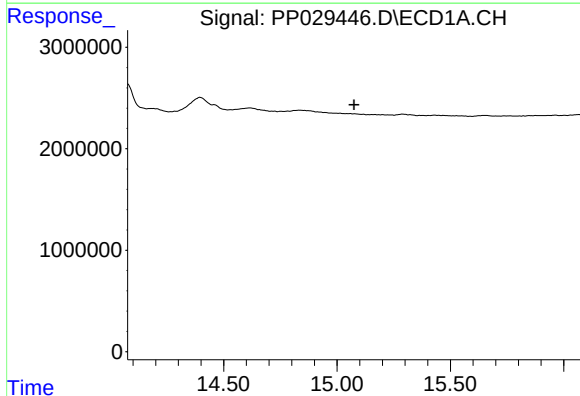


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 15.075 min
Response: 0
Conc: N.D.

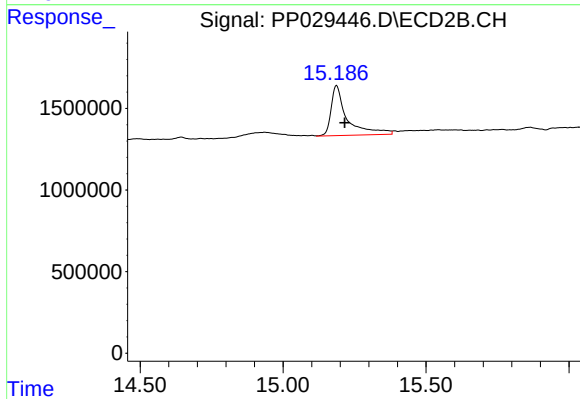

#11 2,4,5-TP (SILVEX)


R.T.: 15.187 min
Delta R.T.: -0.028 min
Response: 12073901
Conc: 59.36 ng/ml

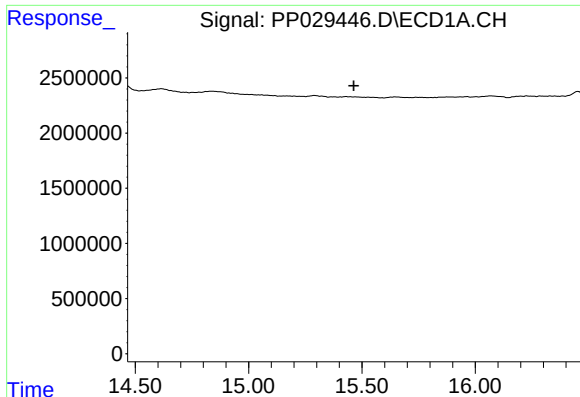

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.464 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
JC-02-031919-C

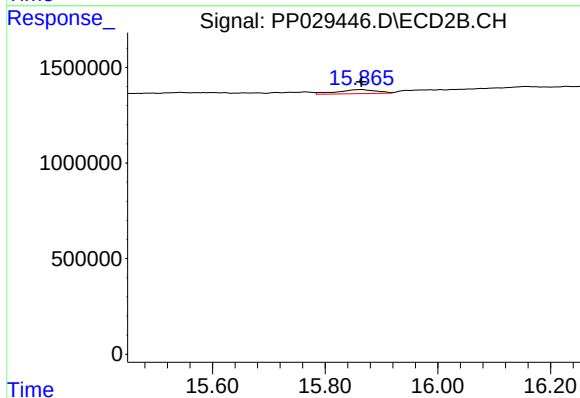


#12 2,4,5-T

R.T.: 15.865 min
Delta R.T.: 0.000 min
Response: 1025714
Conc: 6.19 ng/ml

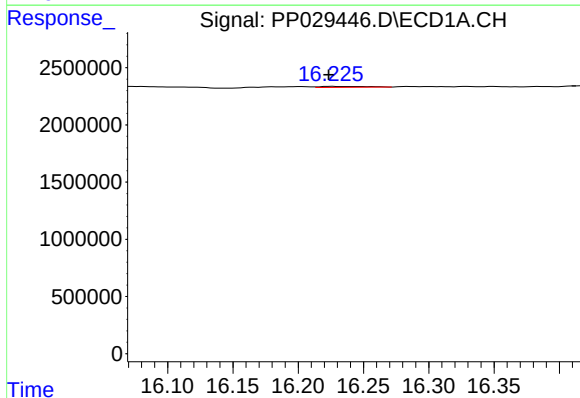


#13 2,4-DB

R.T.: 16.226 min
Delta R.T.: 0.002 min
Response: 212993
Conc: 11.15 ng/ml

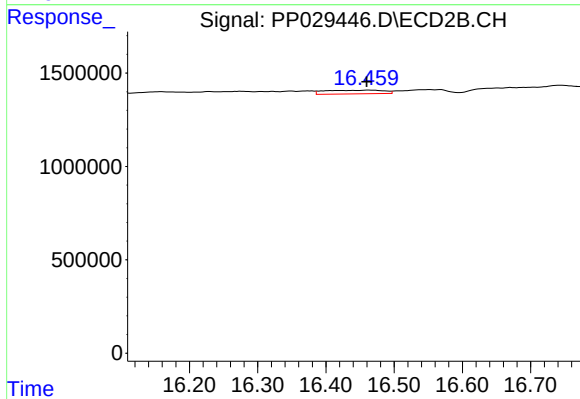

#13 2,4-DB


R.T.: 16.462 min
Delta R.T.: 0.003 min
Response: 1164186
Conc: 51.68 ng/ml

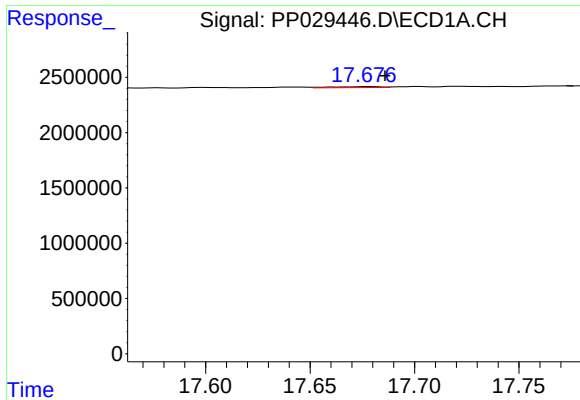

#14 DINOSEB


R.T.: 17.678 min
Delta R.T.: -0.008 min
Response: 151537
Conc: 1.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
JC-02-031919-C

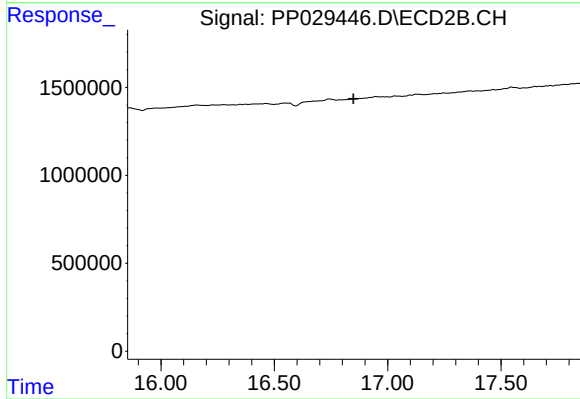


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 16.849 min
Response: 0
Conc: N.D.

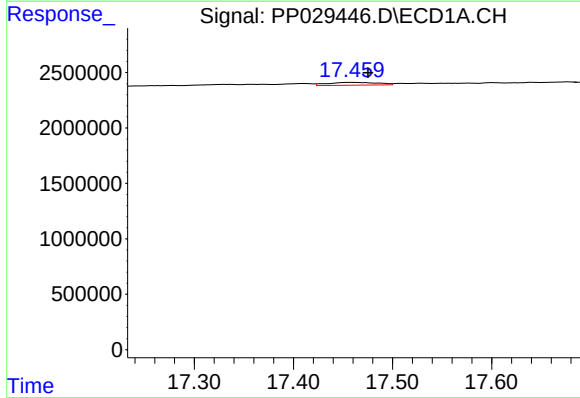


#15 Picloram

R.T.: 17.460 min
Delta R.T.: -0.015 min
Response: 915585
Conc: 3.29 ng/ml

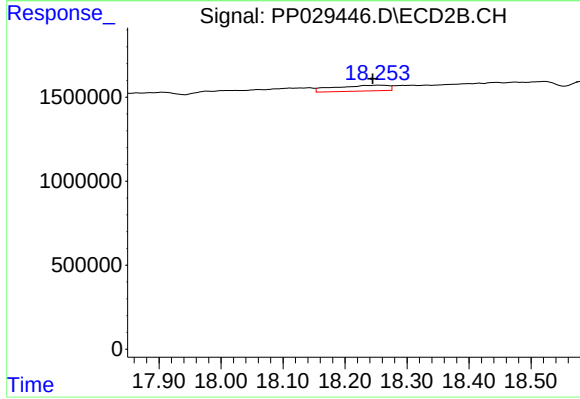

#15 Picloram


R.T.: 18.255 min
Delta R.T.: 0.010 min
Response: 2046414
Conc: 9.09 ng/ml

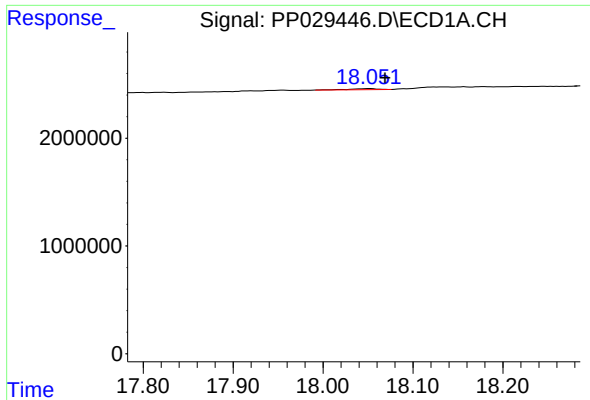

#16 DCPA

R.T.: 18.052 min
Delta R.T.: -0.017 min
Response: 210999
Conc: 0.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
JC-02-031919-C

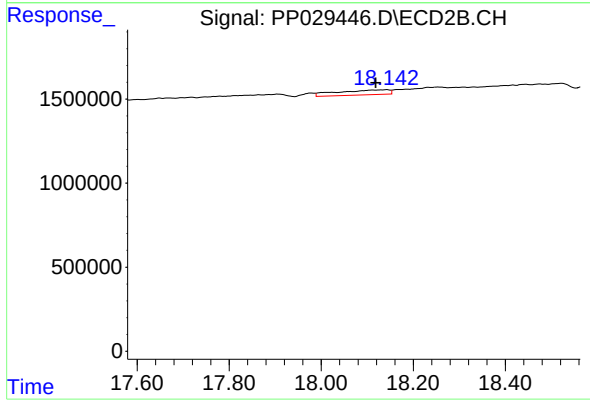

#16 DCPA

R.T.: 18.143 min
Delta R.T.: 0.024 min
Response: 2266741
Conc: 9.75 ng/ml