

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032024\
 Data File : PP063614.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2024 16:36
 Operator : YP\AJ
 Sample : P1788-02RE
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PEZOMETER-206RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/20/2024
 Supervised By :Ankita Jodhani 03/20/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 01:33:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 19 06:23:02 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.488	3.638	24405305	23869727	10.228m	9.998m
2) SA Decachlor...	10.365	8.680	18960927	20437497	7.468m	7.562m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032024\
Data File : PP063614.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2024 16:36
Operator : YP\AJ
Sample : P1788-02RE
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PEZOMETER-206RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/20/2024
Supervised By :Ankita Jodhani 03/20/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 01:33:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 19 06:23:02 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

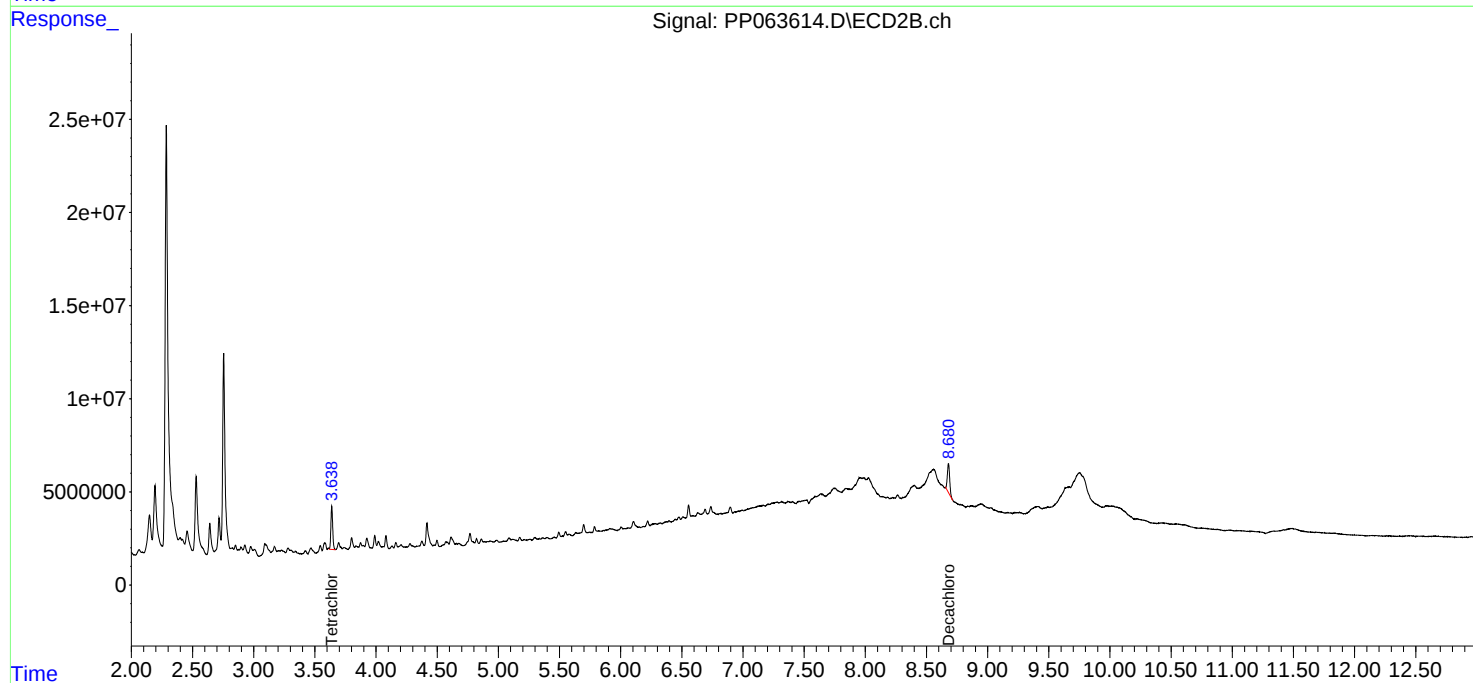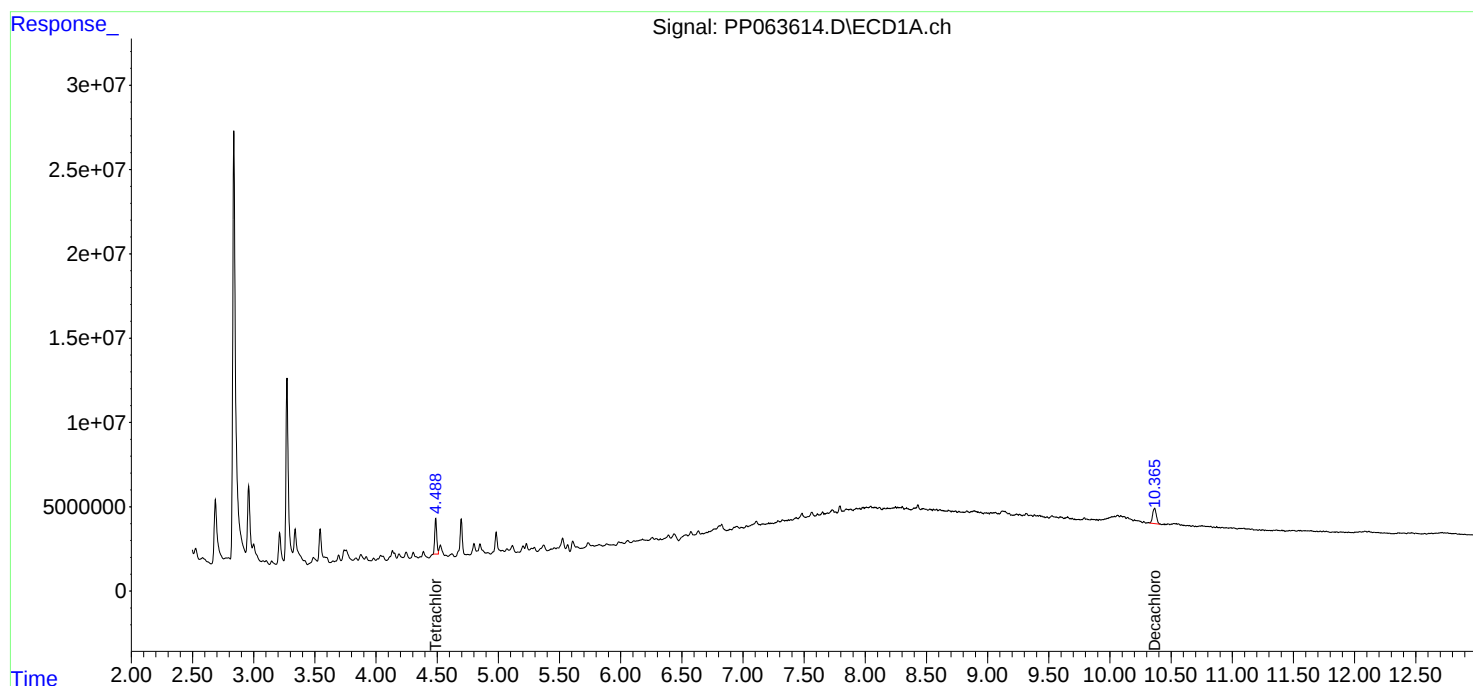

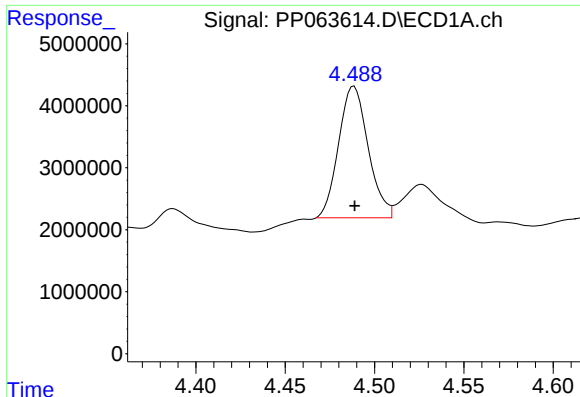


#1 Tetrachloro-m-xylene

R.T.: 4.488 min
Delta R.T.: -0.001 min
Response: 24405305
Conc: 10.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
PEZOMETER-206RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/20/2024
Supervised By :Ankita Jodhani 03/20/2024

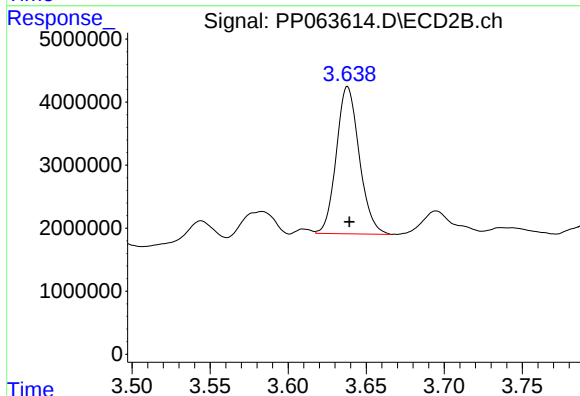


#1 Tetrachloro-m-xylene

R.T.: 3.638 min
Delta R.T.: -0.002 min
Response: 23869727
Conc: 10.00 ng/ml m

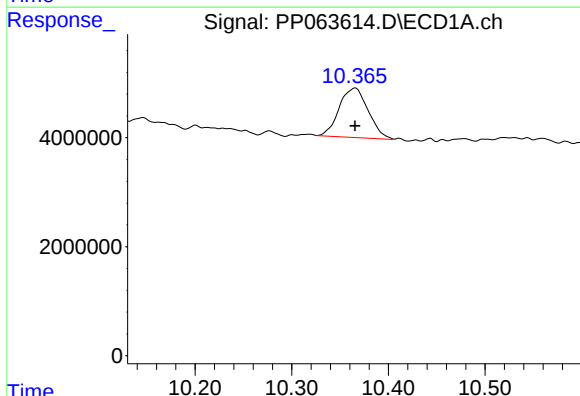

#2 Decachlorobiphenyl

R.T.: 10.365 min
Delta R.T.: 0.000 min
Response: 18960927
Conc: 7.47 ng/ml m

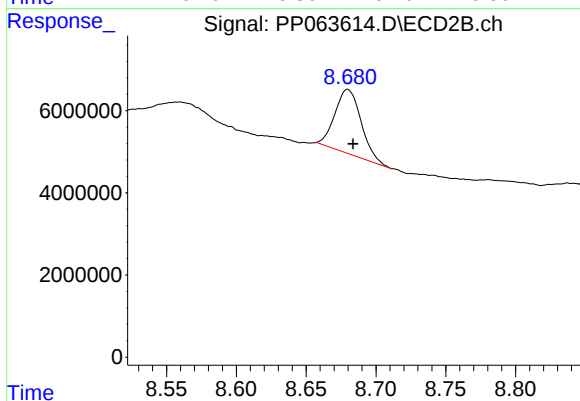

#2 Decachlorobiphenyl

R.T.: 8.680 min
Delta R.T.: -0.004 min
Response: 20437497
Conc: 7.56 ng/ml m