

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032025\
 Data File : PP070784.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Mar 2025 01:59
 Operator : YP\AJ
 Sample : Q1613-01 10X
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LAW-25-0051

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/21/2025
 Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 21 04:29:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 05:25:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.519	3.821	2818433	2326712	1.812	2.321 #
2) SA Decachlor...	10.241	8.868	3376181	2638624	3.178m	2.697

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032025\
Data File : PP070784.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Mar 2025 01:59
Operator : YP\AJ
Sample : Q1613-01 10X
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
LAW-25-0051


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/21/2025
Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 21 04:29:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 05:25:31 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

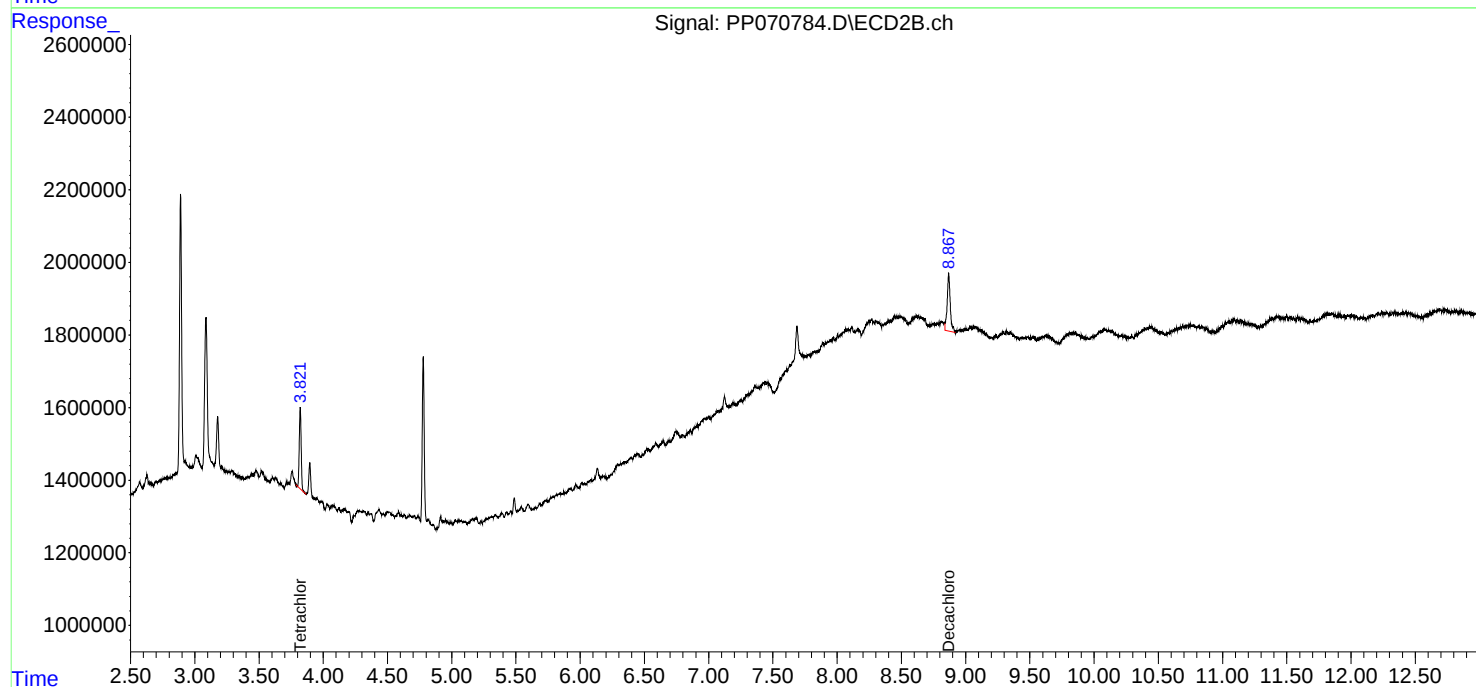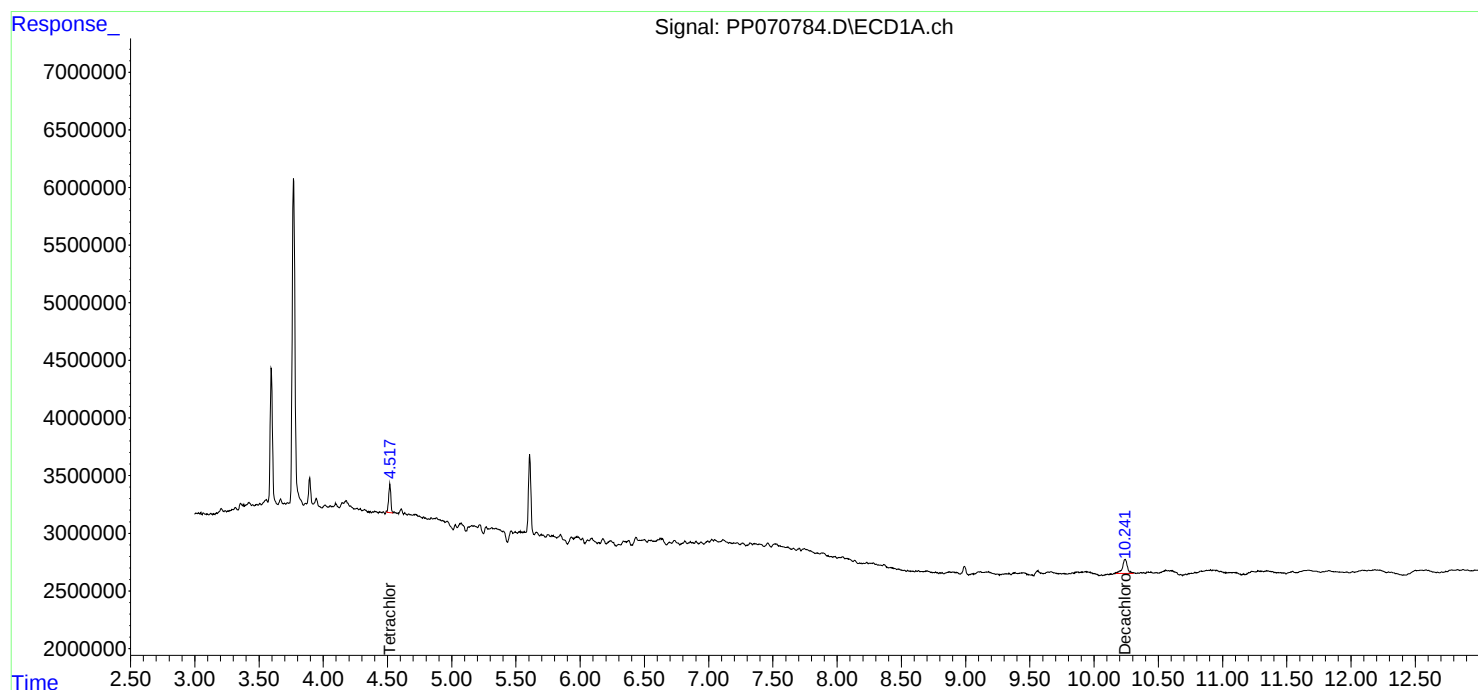

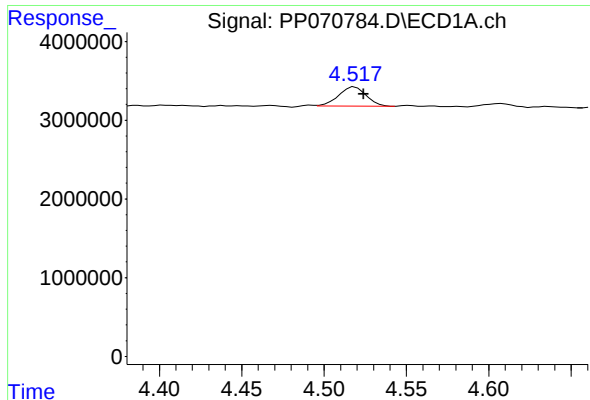


#1 Tetrachloro-m-xylene

R.T.: 4.519 min
Delta R.T.: -0.005 min
Response: 2818433
Conc: 1.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-25-0051


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/21/2025
Supervised By :mohammad ahmed 03/24/2025

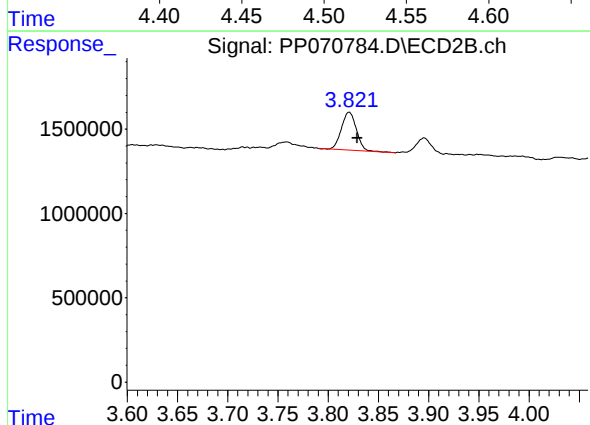


#1 Tetrachloro-m-xylene

R.T.: 3.821 min
Delta R.T.: -0.008 min
Response: 2326712
Conc: 2.32 ng/ml

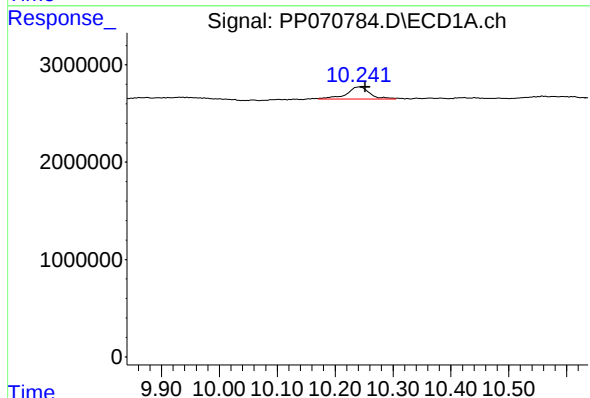

#2 Decachlorobiphenyl

R.T.: 10.241 min
Delta R.T.: -0.011 min
Response: 3376181
Conc: 3.18 ng/ml m

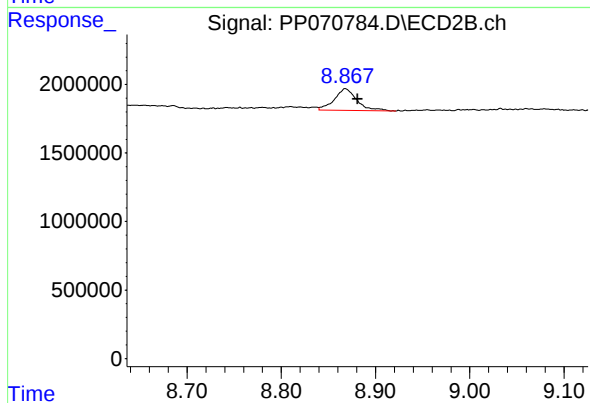

#2 Decachlorobiphenyl

R.T.: 8.868 min
Delta R.T.: -0.013 min
Response: 2638624
Conc: 2.70 ng/ml