

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032122\
 Data File : PP044933.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Mar 2022 19:23
 Operator : YP\AJ
 Sample : N2021-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MHQ-SP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/22/2022
 Supervised By :mohammad ahmed 03/23/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 05:58:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 17 04:32:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.896	3.154	39105359	29696196	21.462	22.534
2) SA Decachlor...	10.018	8.512	23138234	25616199	17.975m	19.714m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032122\
Data File : PP044933.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Mar 2022 19:23
Operator : YP\AJ
Sample : N2021-03
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MHQ-SP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/22/2022
Supervised By :mohammad ahmed 03/23/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 05:58:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 17 04:32:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

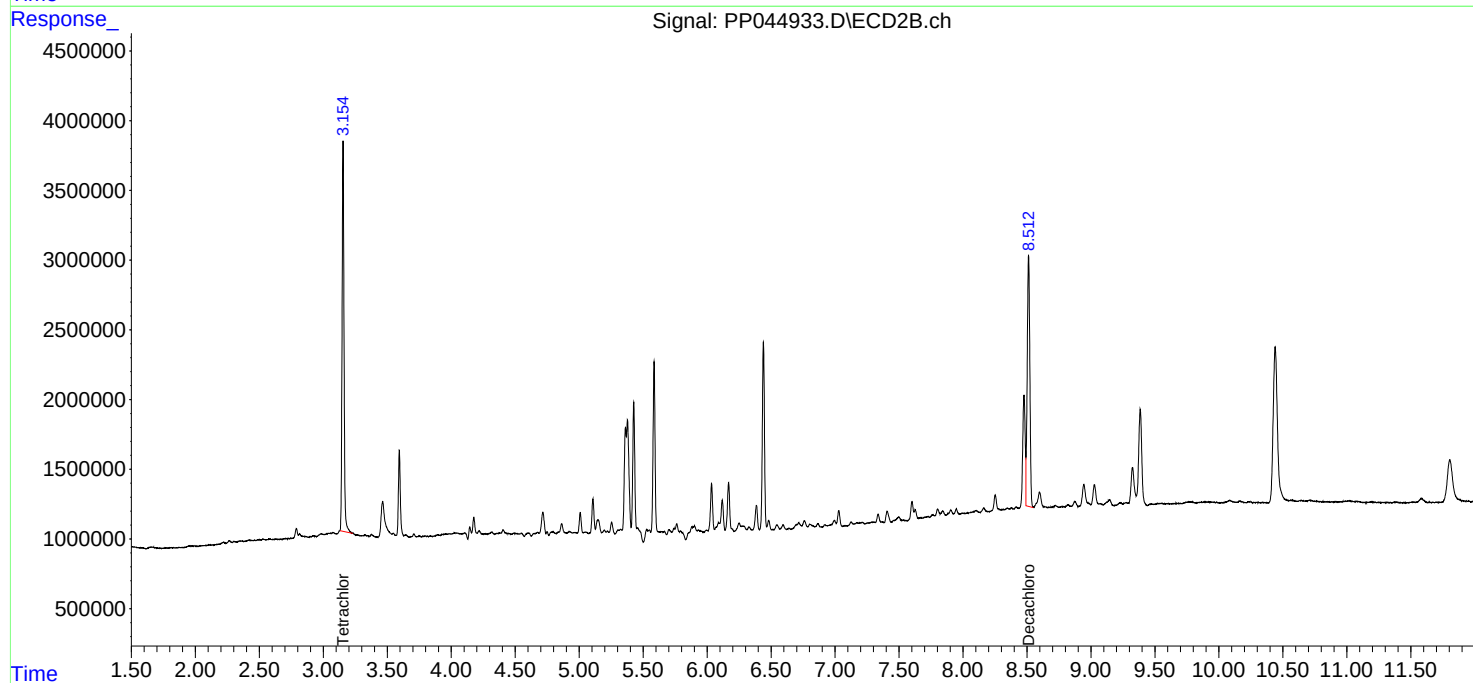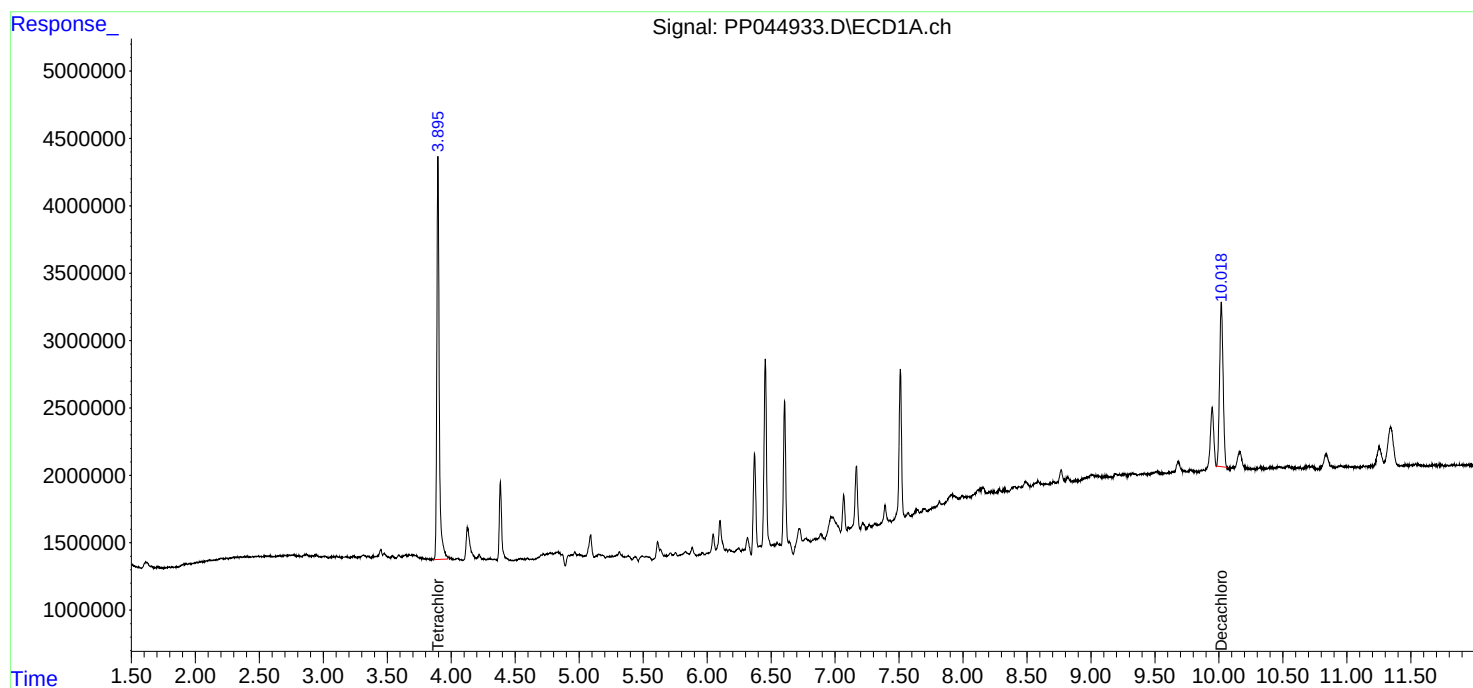

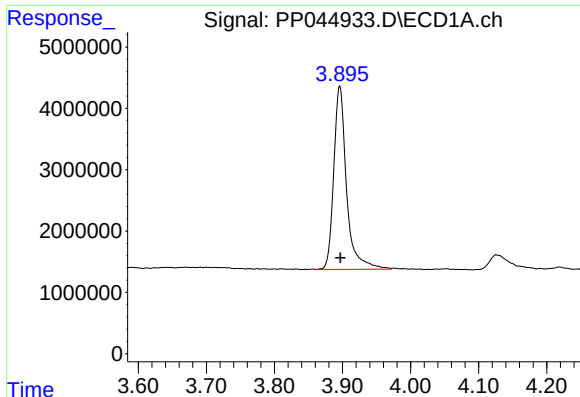


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 39105359
Conc: 21.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
MHQ-SP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/22/2022
Supervised By :mohammad ahmed 03/23/2022

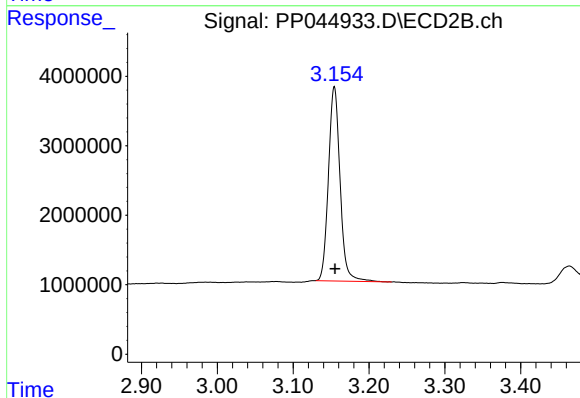


#1 Tetrachloro-m-xylene

R.T.: 3.154 min
Delta R.T.: 0.000 min
Response: 29696196
Conc: 22.53 ng/ml

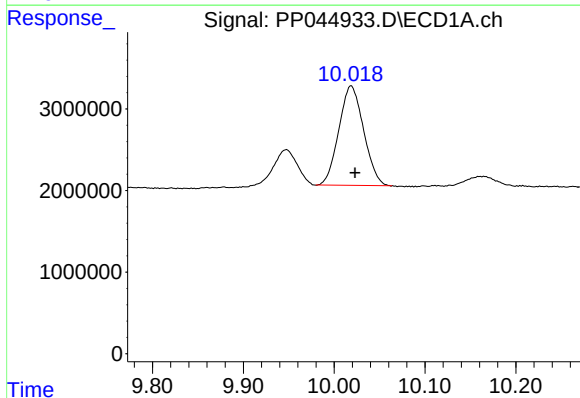

#2 Decachlorobiphenyl

R.T.: 10.018 min
Delta R.T.: -0.005 min
Response: 23138234
Conc: 17.97 ng/ml m

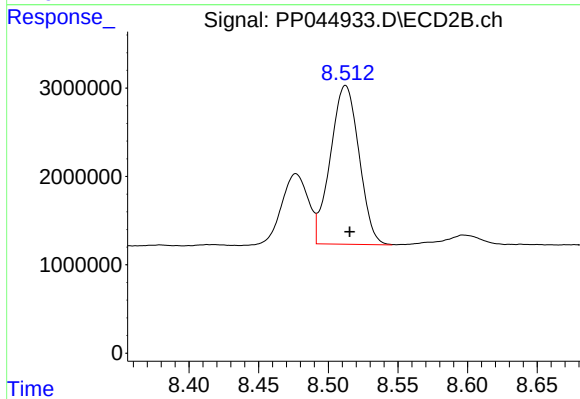

#2 Decachlorobiphenyl

R.T.: 8.512 min
Delta R.T.: -0.003 min
Response: 25616199
Conc: 19.71 ng/ml m