

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032122\
 Data File : PP044953.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2022 02:11
 Operator : YP\AJ
 Sample : N2032-03 10X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FDA47D-2-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/22/2022
 Supervised By :mohammad ahmed 03/23/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 06:19:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 17 04:32:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.897	3.155	2637456	2599786	1.448m	1.973m#
2) SA Decachlor...	10.019	8.512	3629011	3251723	2.819	2.503
Target Compounds						
31) L7 AR-1260-1	6.890	5.881	12290187	14170147	178.518	201.249
32) L7 AR-1260-2	7.173	6.088	15579230	17506448	200.661m	195.758
33) L7 AR-1260-3	7.568	6.250	8493053	14204863	134.968	166.784
34) L7 AR-1260-4	7.815	6.762	12015128	8828067	163.792	131.356
35) L7 AR-1260-5	8.157	7.029	21580990	23964570	154.113	153.367

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032122\
Data File : PP044953.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2022 02:11
Operator : YP\AJ
Sample : N2032-03 10X
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
FDA47D-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/22/2022
Supervised By :mohammad ahmed 03/23/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 06:19:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 17 04:32:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

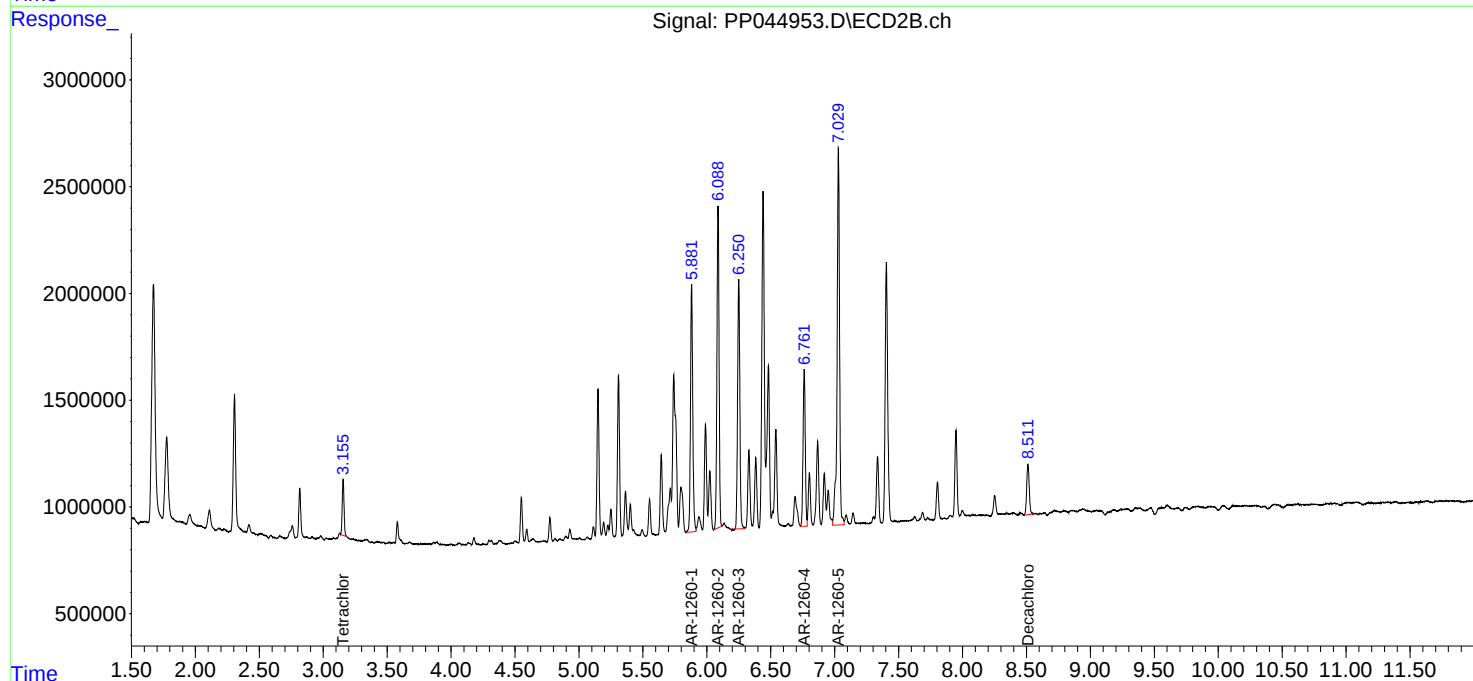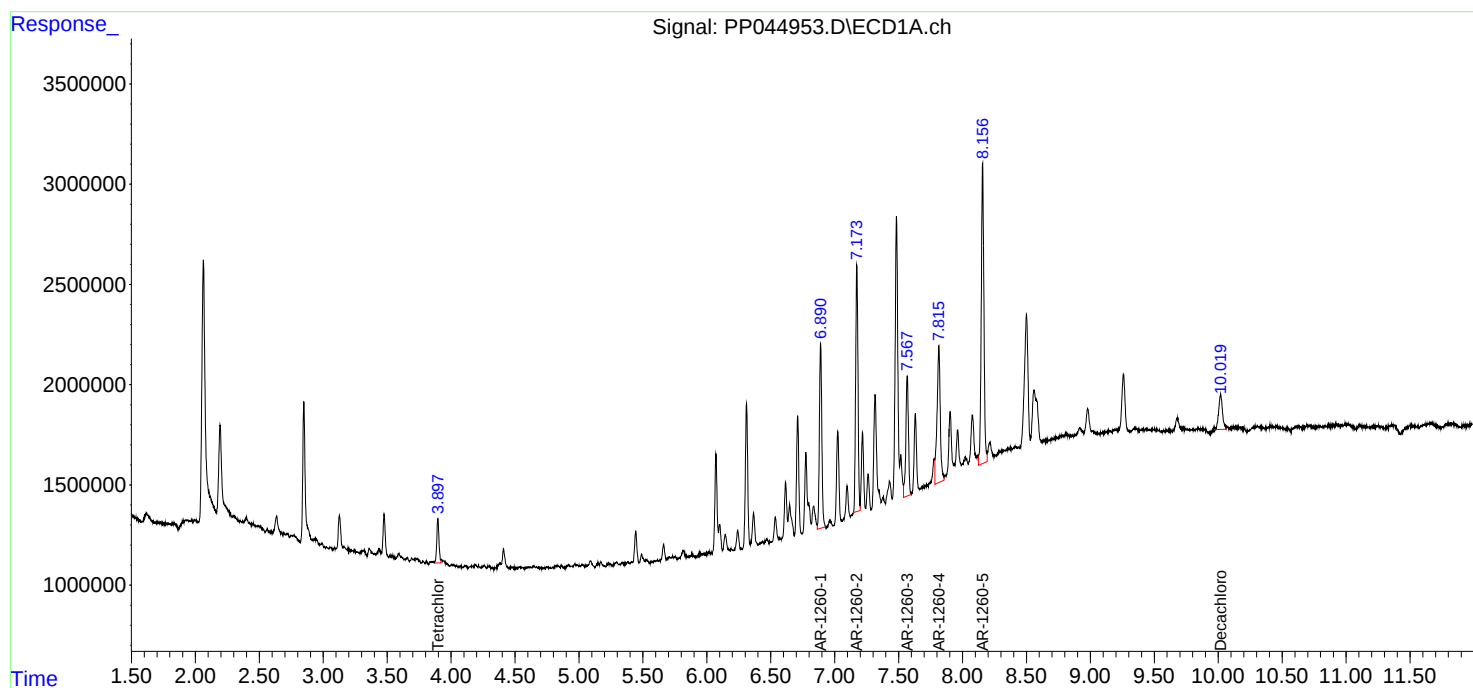

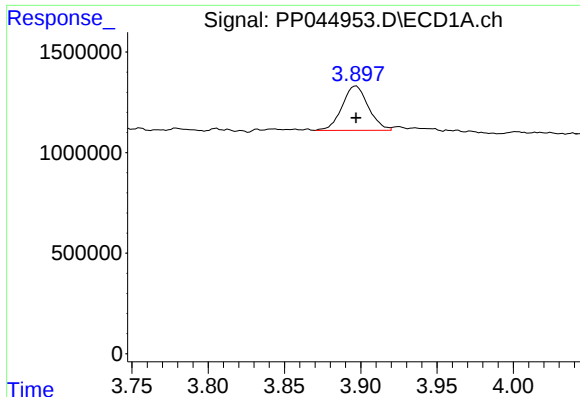


#1 Tetrachloro-m-xylene

R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 2637456
Conc: 1.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
FDA47D-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/22/2022
Supervised By :mohammad ahmed 03/23/2022

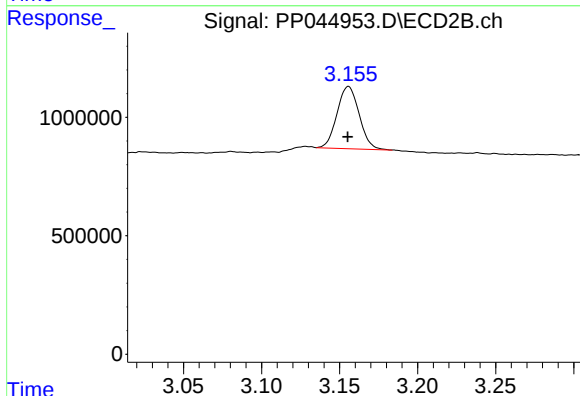


#1 Tetrachloro-m-xylene

R.T.: 3.155 min
Delta R.T.: 0.000 min
Response: 2599786
Conc: 1.97 ng/ml m

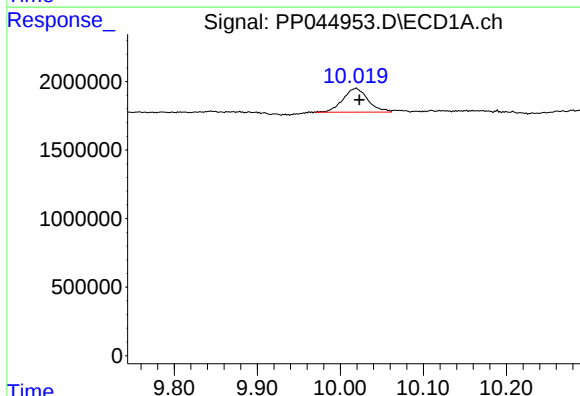


#2 Decachlorobiphenyl

R.T.: 10.019 min
Delta R.T.: -0.004 min
Response: 3629011
Conc: 2.82 ng/ml

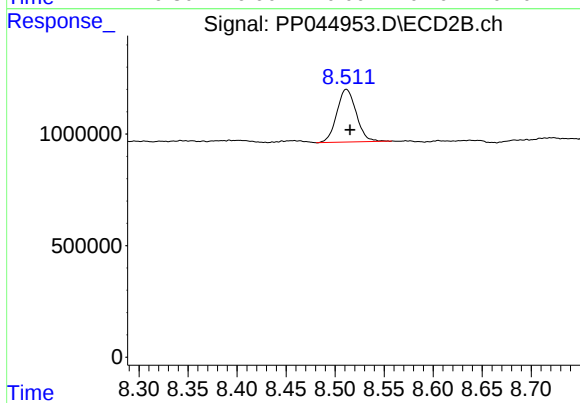

#2 Decachlorobiphenyl

R.T.: 8.512 min
Delta R.T.: -0.004 min
Response: 3251723
Conc: 2.50 ng/ml

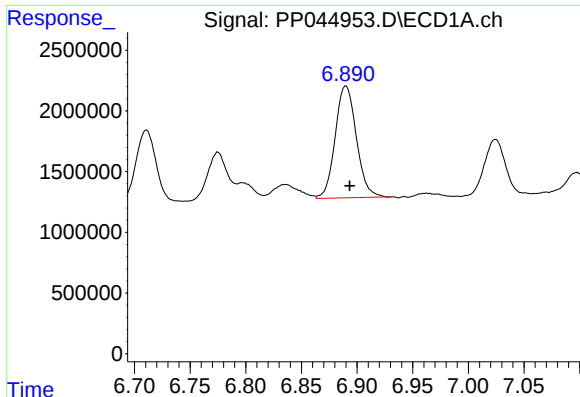


#31 AR-1260-1

R.T.: 6.890 min
Delta R.T.: -0.003 min
Response: 12290187
Conc: 178.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
FDA47D-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/22/2022
Supervised By :mohammad ahmed 03/23/2022

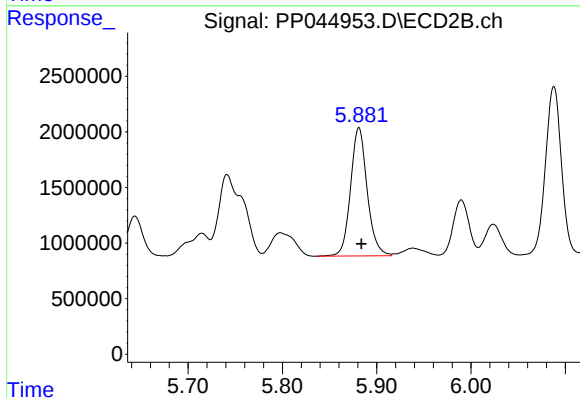


#31 AR-1260-1

R.T.: 5.881 min
Delta R.T.: -0.002 min
Response: 14170147
Conc: 201.25 ng/ml

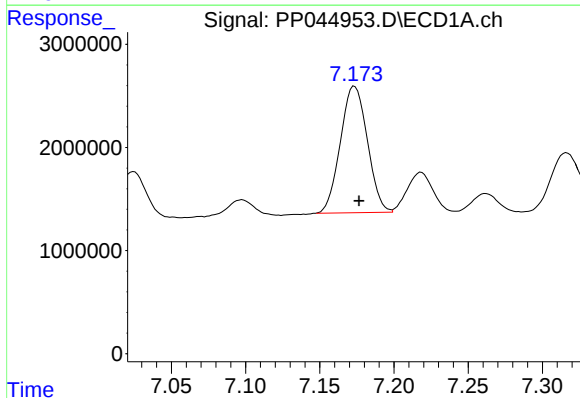


#32 AR-1260-2

R.T.: 7.173 min
Delta R.T.: -0.004 min
Response: 15579230
Conc: 200.66 ng/ml m

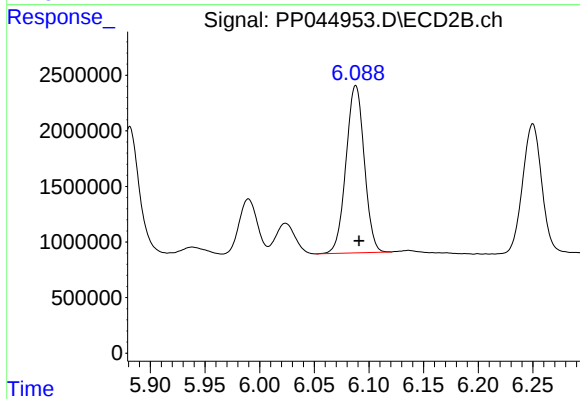

#32 AR-1260-2

R.T.: 6.088 min
Delta R.T.: -0.003 min
Response: 17506448
Conc: 195.76 ng/ml

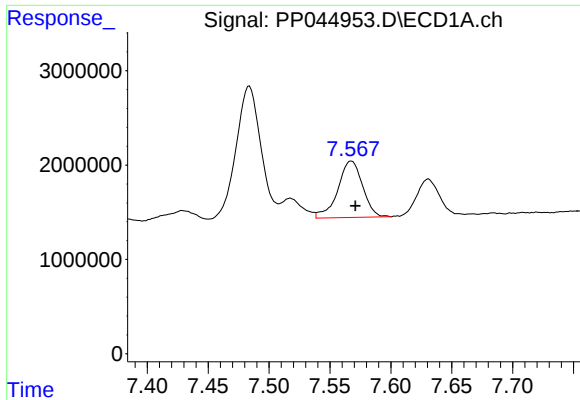


#33 AR-1260-3

R.T.: 7.568 min
Delta R.T.: -0.003 min
Response: 8493053
Conc: 134.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
FDA47D-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/22/2022
Supervised By :mohammad ahmed 03/23/2022

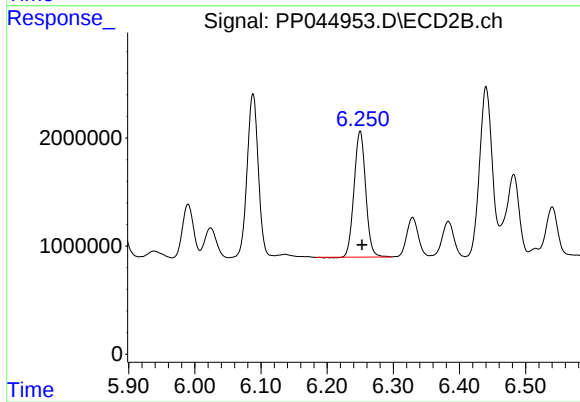


#33 AR-1260-3

R.T.: 6.250 min
Delta R.T.: -0.003 min
Response: 14204863
Conc: 166.78 ng/ml

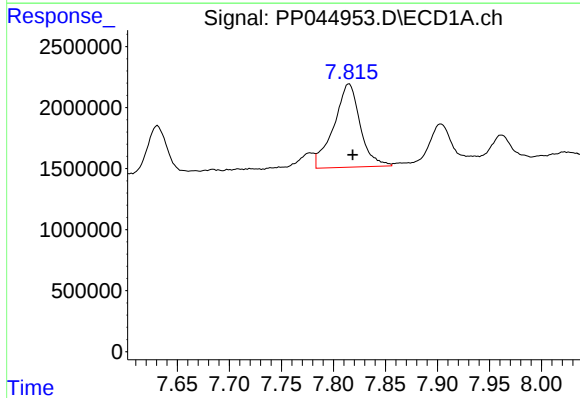


#34 AR-1260-4

R.T.: 7.815 min
Delta R.T.: -0.003 min
Response: 12015128
Conc: 163.79 ng/ml

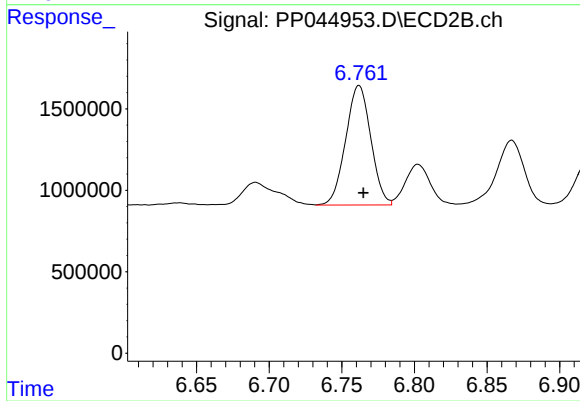

#34 AR-1260-4

R.T.: 6.762 min
Delta R.T.: -0.003 min
Response: 8828067
Conc: 131.36 ng/ml

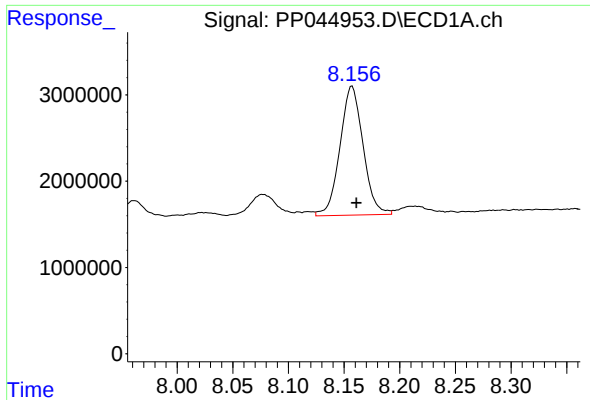


#35 AR-1260-5

R.T.: 8.157 min
Delta R.T.: -0.004 min
Response: 21580990
Conc: 154.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
FDA47D-2-1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/22/2022
Supervised By :mohammad ahmed 03/23/2022

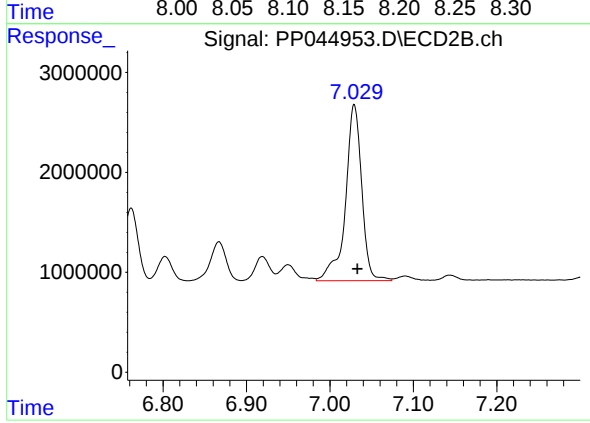

#35 AR-1260-5

R.T.: 7.029 min
Delta R.T.: -0.004 min
Response: 23964570
Conc: 153.37 ng/ml