

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032124\
 Data File : PP063637.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Mar 2024 17:07
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 17:54:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 19 06:23:02 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.489	3.639	40189993	40636800	16.843	17.020
2) SA Decachlor...	10.365	8.680	45899177	45932303	18.078	16.996
Target Compounds						
9) L2 AR-1221-2	0.000	3.941	0	611501	N.D.	29.838 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032124\
Data File : PP063637.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Mar 2024 17:07
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 17:54:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 19 06:23:02 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

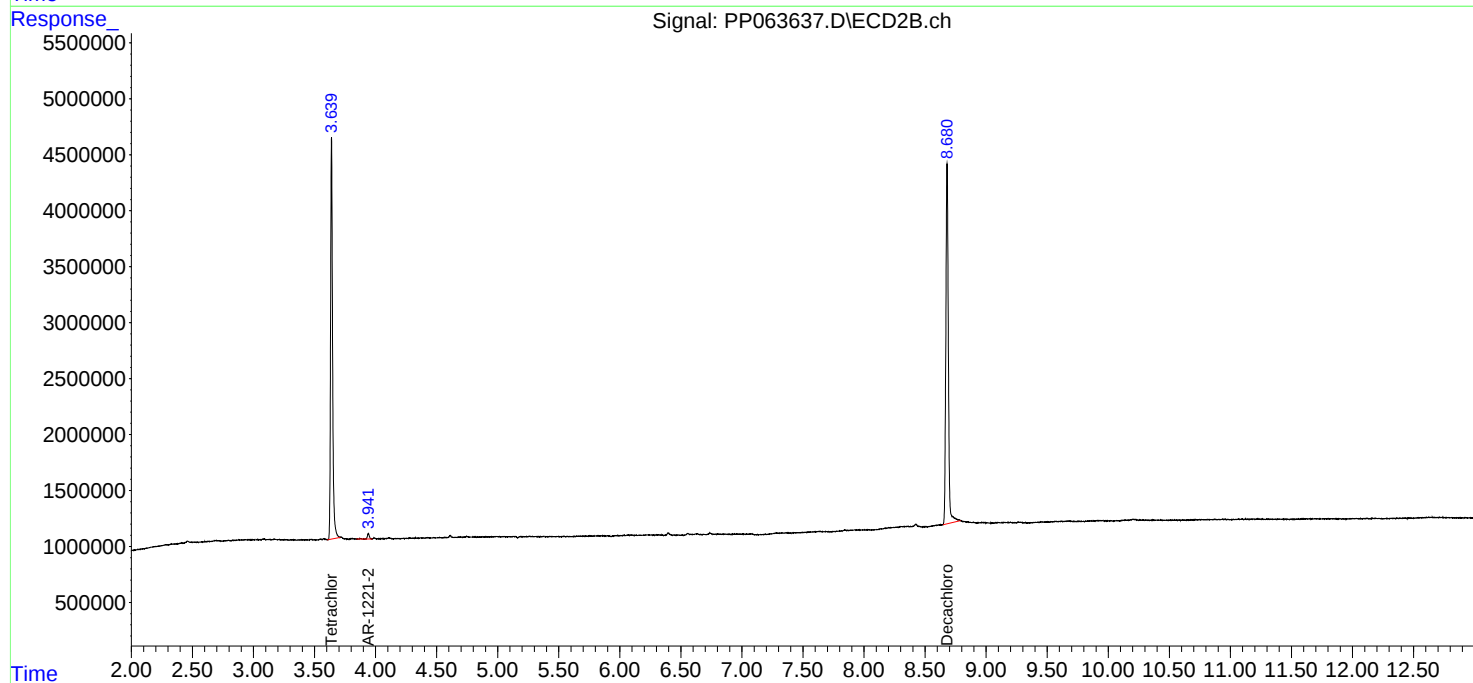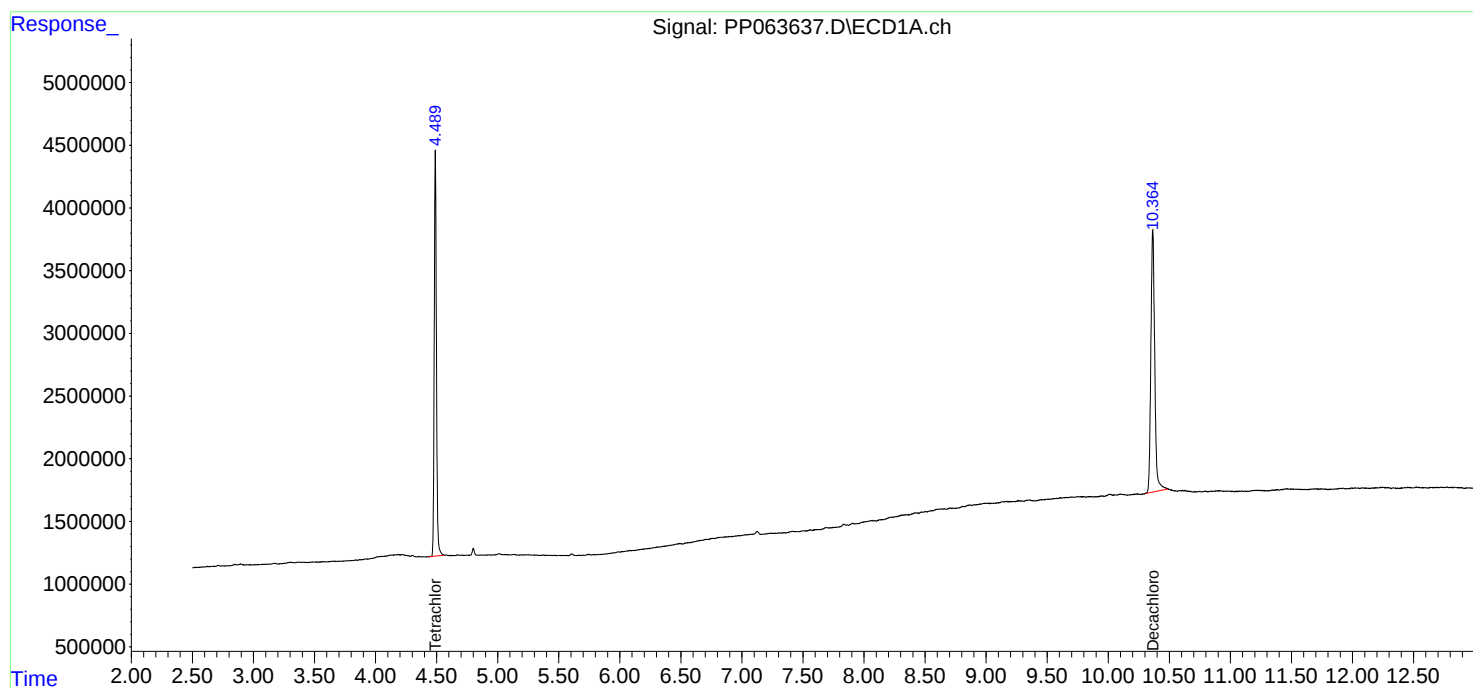


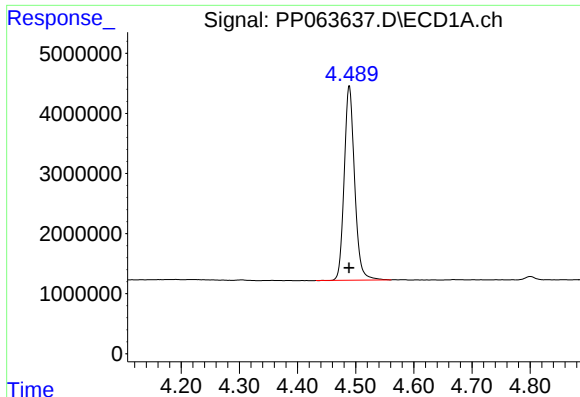

#1 Tetrachloro-m-xylene


R.T.: 4.489 min
Delta R.T.: 0.000 min
Response: 40189993
Conc: 16.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

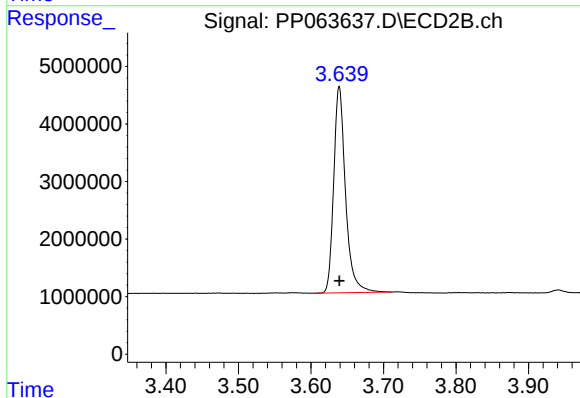


#1 Tetrachloro-m-xylene

R.T.: 3.639 min
Delta R.T.: 0.000 min
Response: 40636800
Conc: 17.02 ng/ml

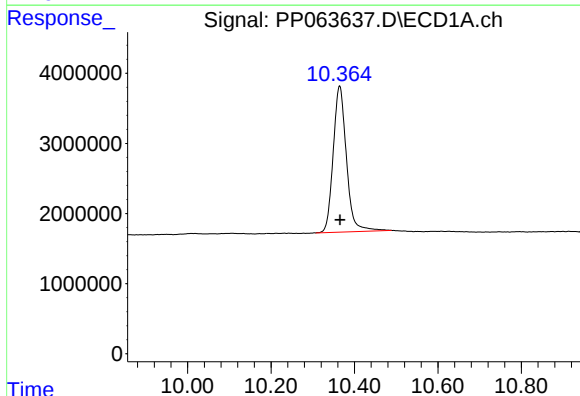


#2 Decachlorobiphenyl

R.T.: 10.365 min
Delta R.T.: 0.000 min
Response: 45899177
Conc: 18.08 ng/ml

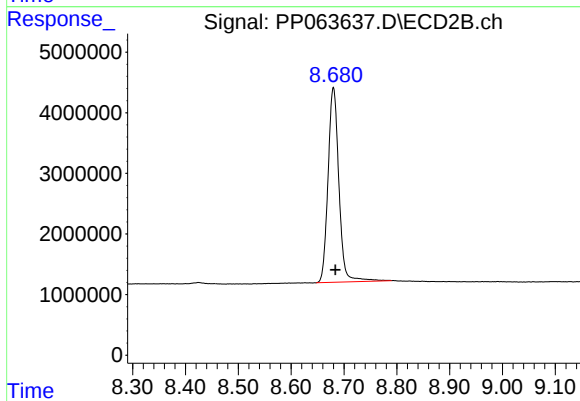

#2 Decachlorobiphenyl


R.T.: 8.680 min
Delta R.T.: -0.004 min
Response: 45932303
Conc: 17.00 ng/ml

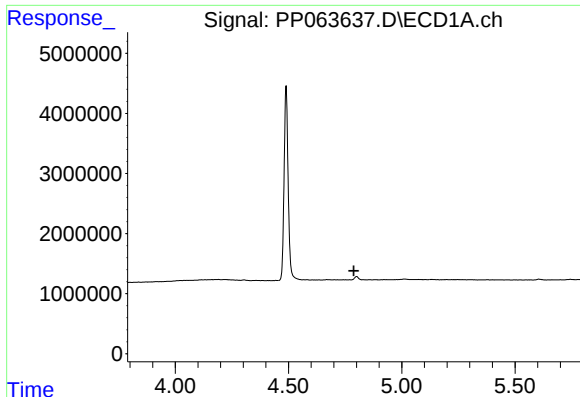

#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 4.789 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

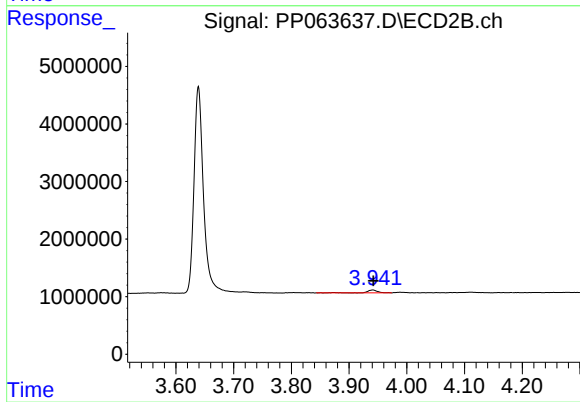

#9 AR-1221-2

R.T.: 3.941 min
Delta R.T.: 0.000 min
Response: 611501
Conc: 29.84 ng/ml