

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032219\
 Data File : PP029469.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Mar 2019 17:18
 Operator : EI\MA
 Sample : K1694-02
 Misc : hexane
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 EO-02-032019-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 23:17:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 22 09:23:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.927	12.117	5216249	7238544	159.445	168.568
Target Compounds							
5) T	DICAMBA	12.266	0.000	300287	0	2.032	N.D. #
8) T	DICHLORPROP	0.000	13.548	0	885770	N.D.	21.873 #
9) T	2,4-D	13.719	0.000	430749	0	11.138	N.D. #
11) T	2,4,5-TP ...	0.000	15.145	0	62220	N.D.	0.301 #
12) T	2,4,5-T	0.000	15.847	0	792200	N.D.	4.779 #
13) T	2,4-DB	16.211	0.000	750438	0	36.089	N.D. #
14) T	DINOSEB	17.695	16.887	327482	1638611	1.943	10.846 #
15) T	Picloram	17.467	0.000	150783	0	0.460	N.D. #
16) T	DCPA	18.039	0.000	1939095	0	6.112	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032219\
Data File : PP029469.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Mar 2019 17:18
Operator : EI\MA
Sample : K1694-02
Misc : hexane
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
EO-02-032019-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 23:17:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
Quant Title : 8080.M
QLast Update : Fri Mar 22 09:23:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

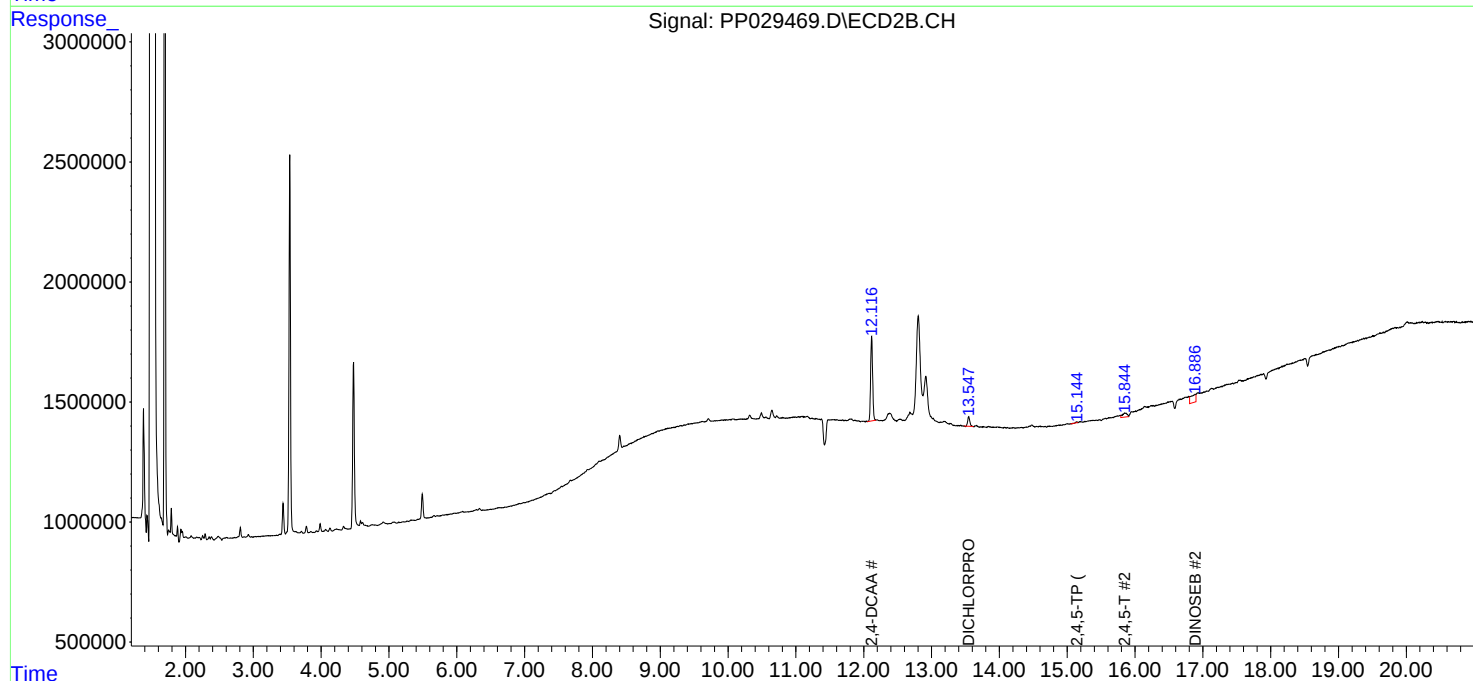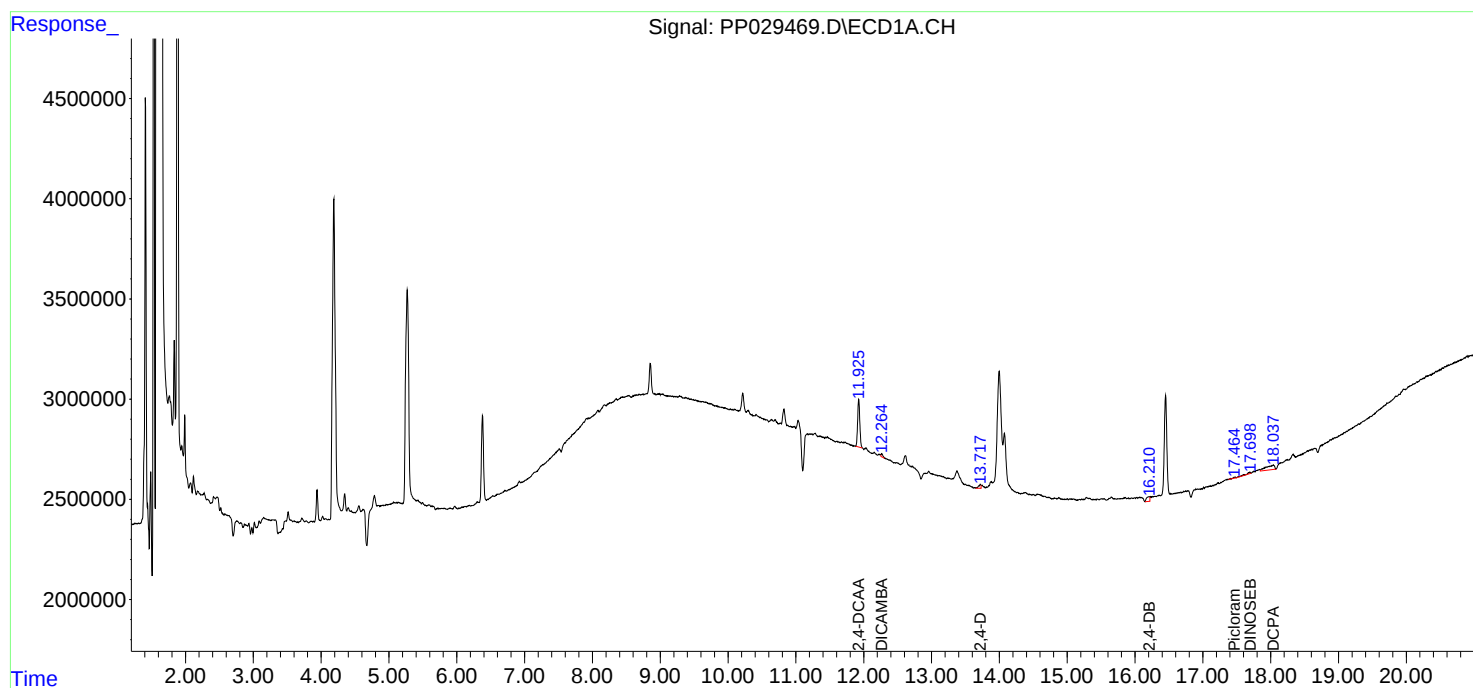


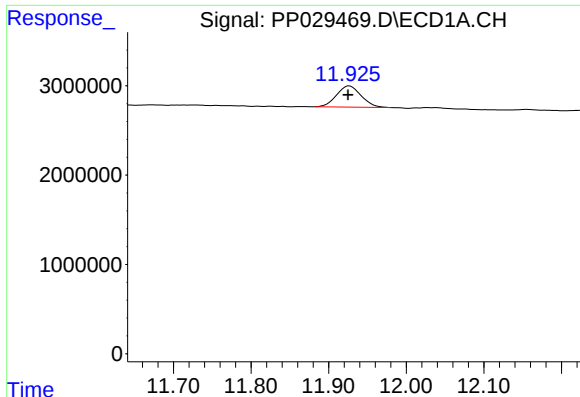

#4 2,4-DCAA


R.T.: 11.927 min
Delta R.T.: 0.002 min
Response: 5216249
Conc: 159.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
EO-02-032019-A

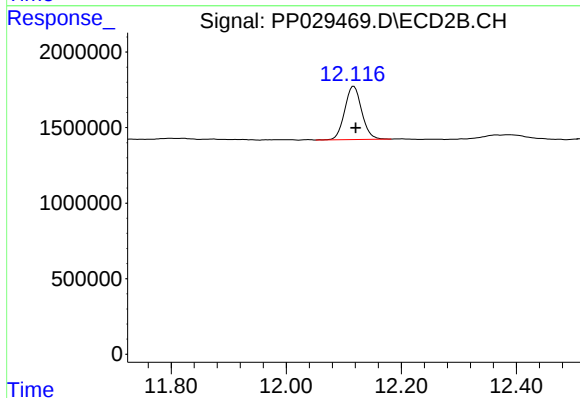


#4 2,4-DCAA

R.T.: 12.117 min
Delta R.T.: -0.004 min
Response: 7238544
Conc: 168.57 ng/ml

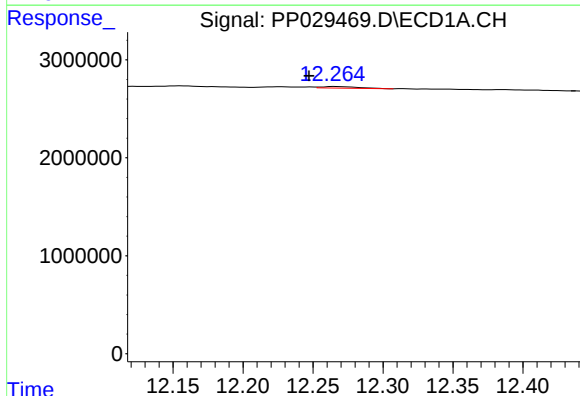


#5 DICAMBA

R.T.: 12.266 min
Delta R.T.: 0.019 min
Response: 300287
Conc: 2.03 ng/ml

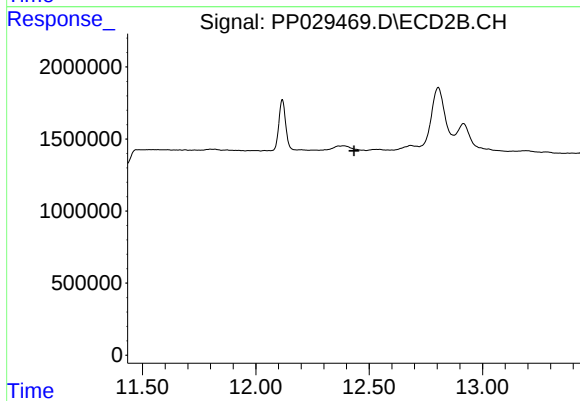

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 12.433 min
Response: 0
Conc: N.D.

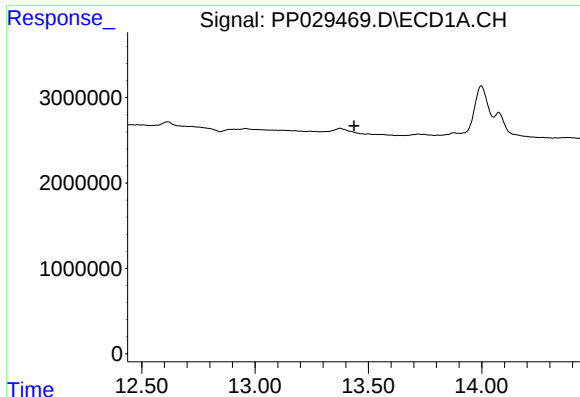

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.438 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
EO-02-032019-A

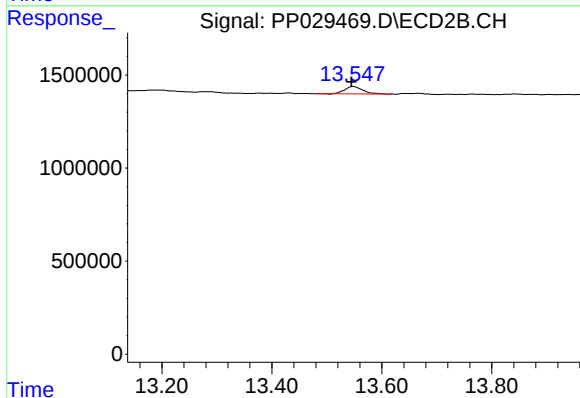


#8 DICHLORPROP

R.T.: 13.548 min
Delta R.T.: 0.003 min
Response: 885770
Conc: 21.87 ng/ml

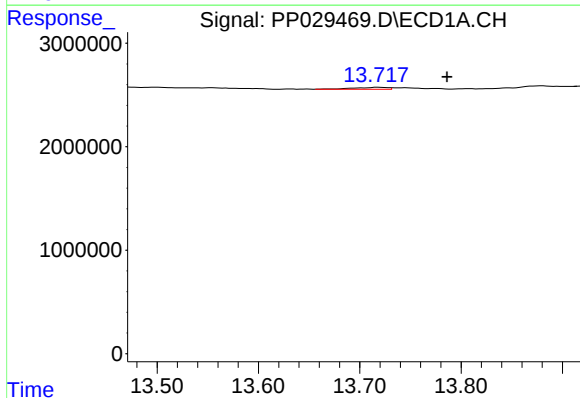


#9 2,4-D

R.T.: 13.719 min
Delta R.T.: -0.068 min
Response: 430749
Conc: 11.14 ng/ml

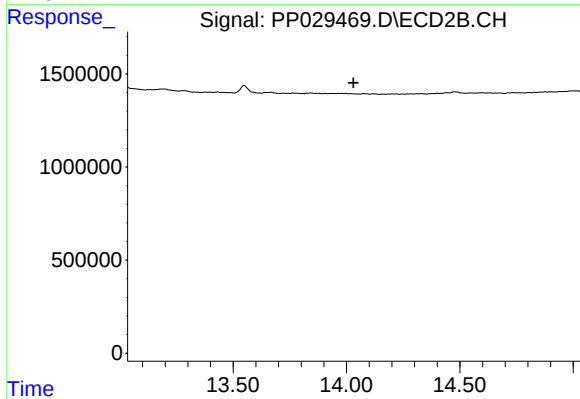

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 14.031 min
Response: 0
Conc: N.D.

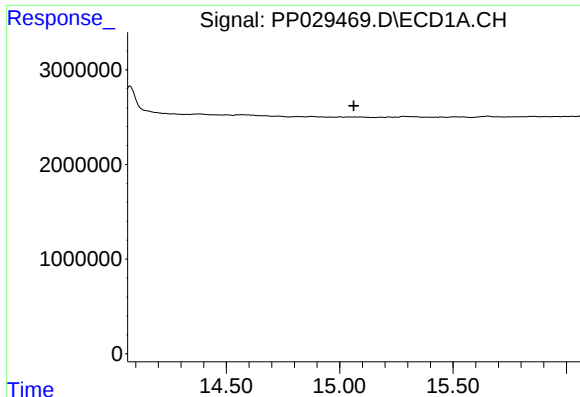

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 15.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
EO-02-032019-A

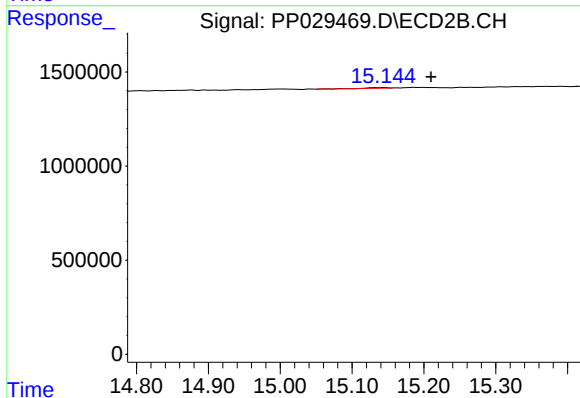


#11 2,4,5-TP (SILVEX)

R.T.: 15.145 min
Delta R.T.: -0.065 min
Response: 62220
Conc: 0.30 ng/ml

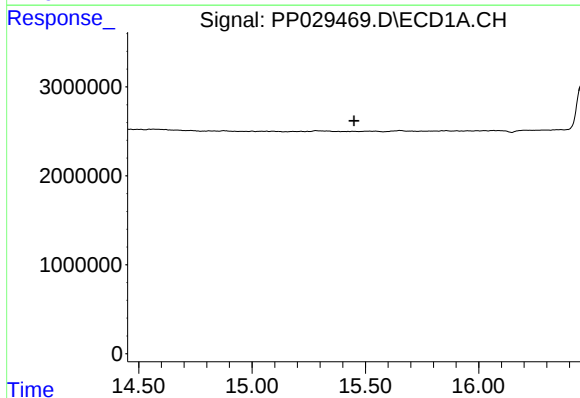


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 15.451 min
Response: 0
Conc: N.D.

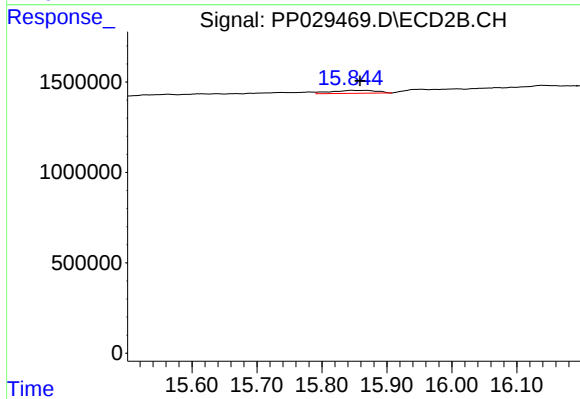

#12 2,4,5-T


R.T.: 15.847 min
Delta R.T.: -0.012 min
Response: 792200
Conc: 4.78 ng/ml

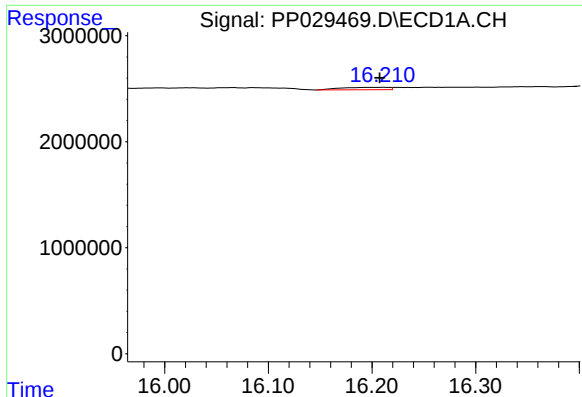

#13 2,4-DB


R.T.: 16.211 min
Delta R.T.: 0.003 min
Response: 750438
Conc: 36.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
EO-02-032019-A

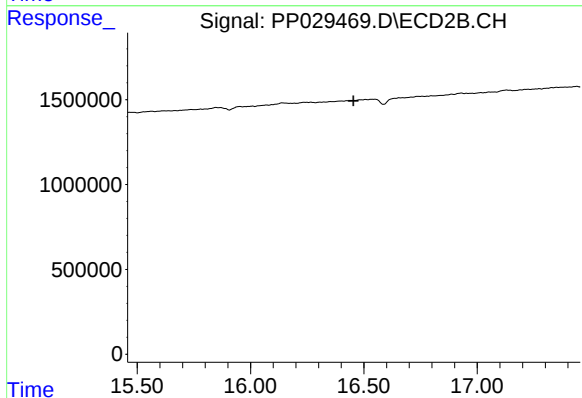


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 16.455 min
Response: 0
Conc: N.D.

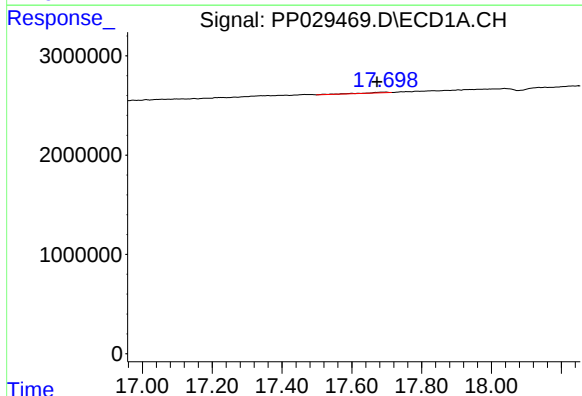


#14 DINOSEB

R.T.: 17.695 min
Delta R.T.: 0.023 min
Response: 327482
Conc: 1.94 ng/ml

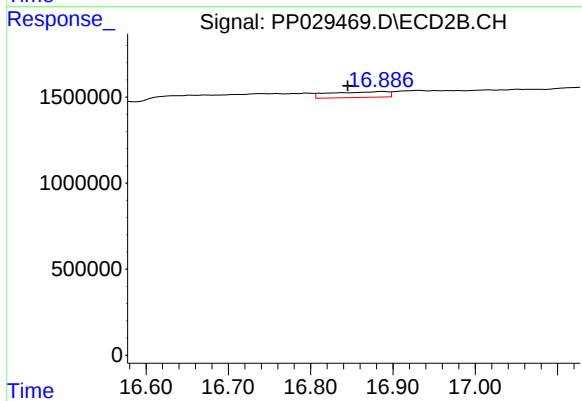

#14 DINOSEB


R.T.: 16.887 min
Delta R.T.: 0.042 min
Response: 1638611
Conc: 10.85 ng/ml

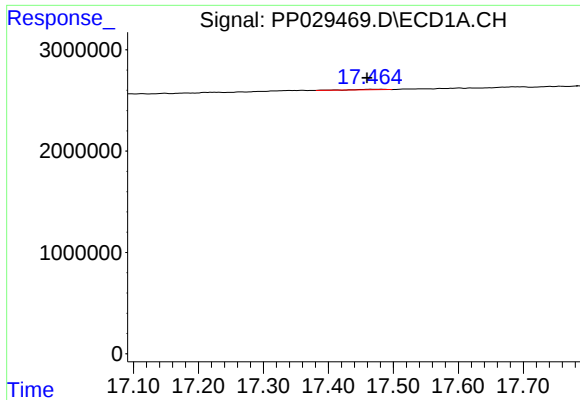

#15 Picloram


R.T.: 17.467 min
Delta R.T.: 0.007 min
Response: 150783
Conc: 0.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
EO-02-032019-A

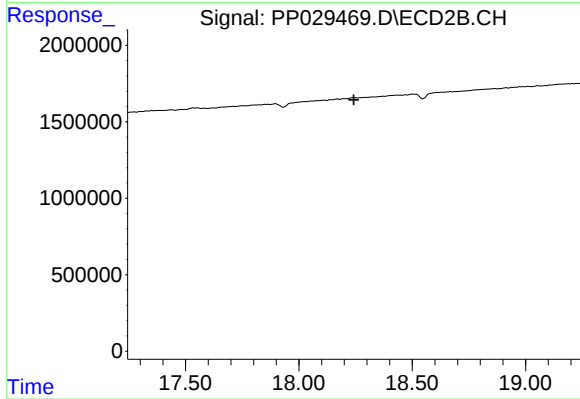


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 18.242 min
Response: 0
Conc: N.D.

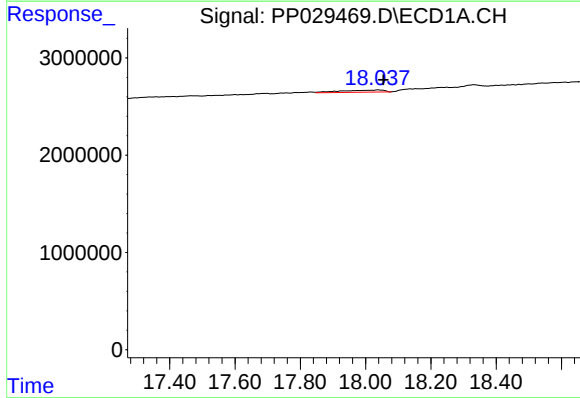

#16 DCPA

R.T.: 18.039 min
Delta R.T.: -0.016 min
Response: 1939095
Conc: 6.11 ng/ml

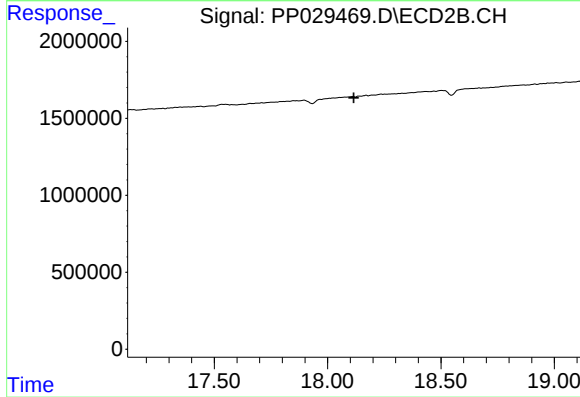

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 18.116 min
Response: 0
Conc: N.D.