

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032221\
 Data File : PP034219.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Mar 2021 16:22
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 02:00:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.850	4.261	1723218	992128	20.513	22.420
2)	SA Decachlor...	10.772	9.576	1810755	667760	23.074	25.304
Target Compounds							
9)	L2 AR-1221-2	5.198	4.616	18525	15501	26.917	43.711 #
28)	L6 AR-1254-3	7.695	0.000	12881	0	2.966	N.D. #
32)	L7 AR-1260-2	0.000	7.276f	0	3316	N.D.	1.853 #
34)	L7 AR-1260-4	0.000	7.931	0	3244	N.D.	2.278 #
35)	L7 AR-1260-5	0.000	8.181	0	4436	N.D.	1.429 #
37)	L8 AR-1262-2	0.000	8.181	0	4436	N.D.	1.374 #
45)	L9 AR-1268-5	10.456	0.000	238915	0	8.646	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032221\
Data File : PP034219.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Mar 2021 16:22
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 02:00:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

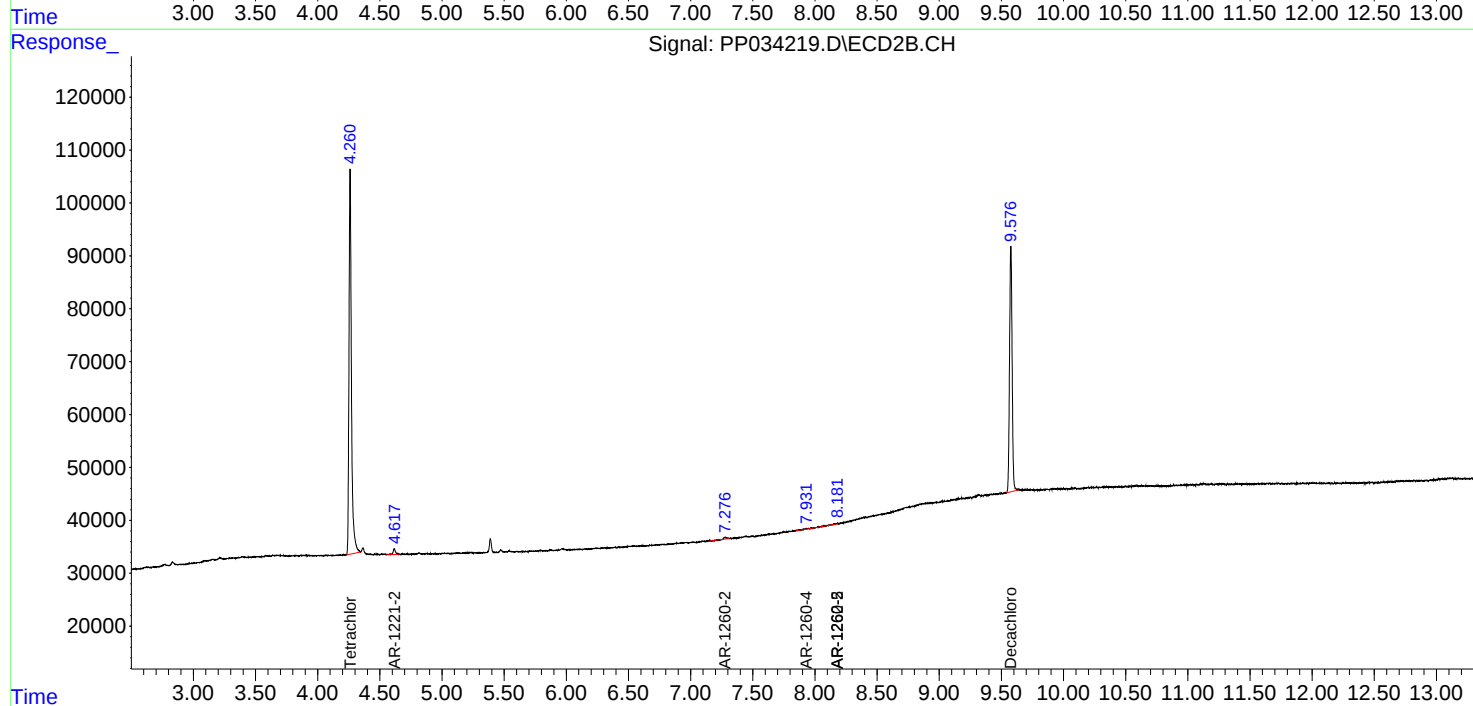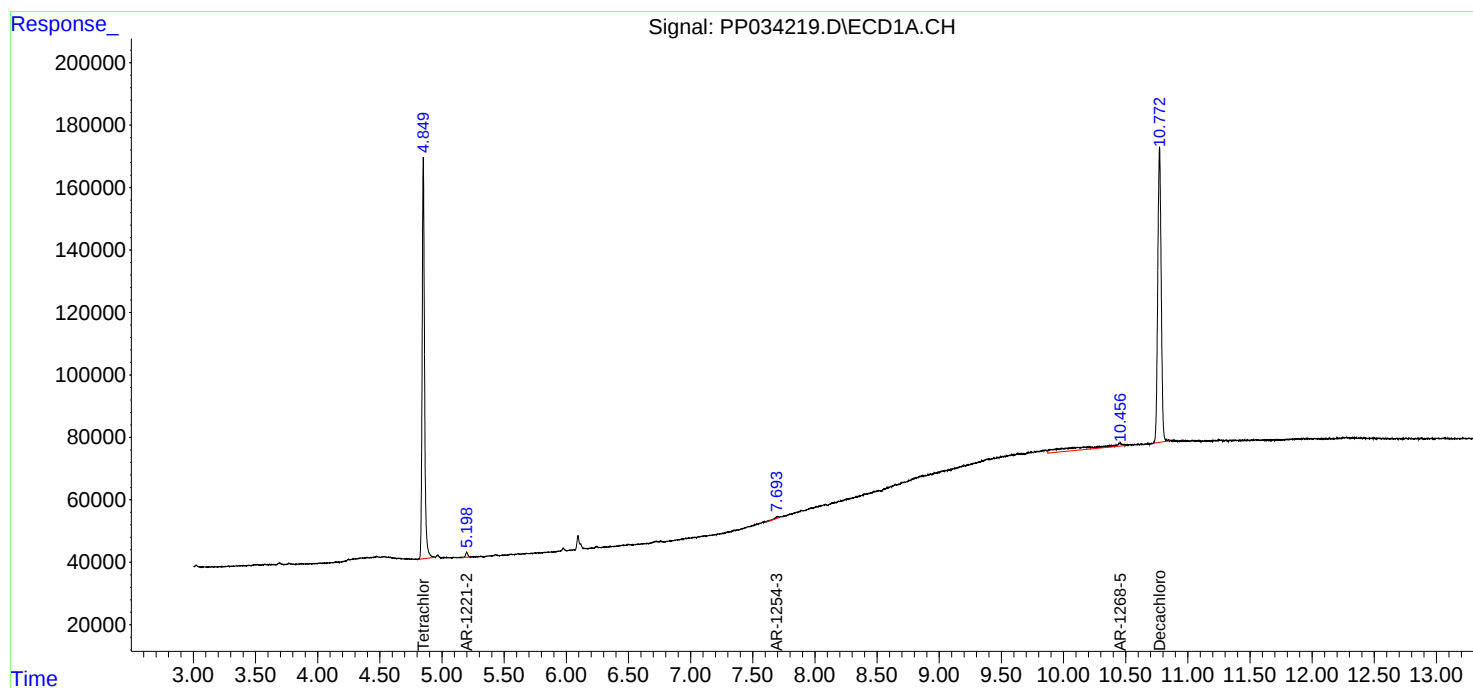


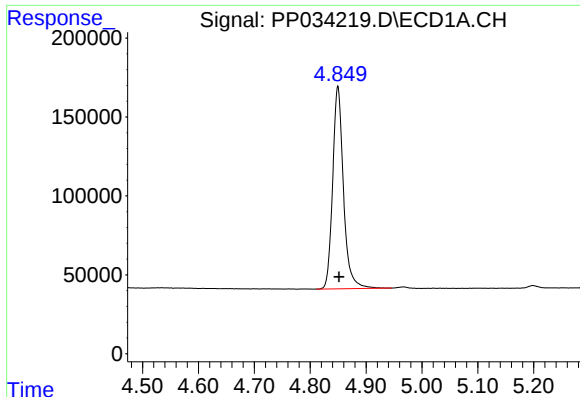

#1 Tetrachloro-m-xylene


R.T.: 4.850 min
Delta R.T.: -0.002 min
Response: 1723218
Conc: 20.51 ng/ml

Instrument :
ECD_P
ClientSampleId :

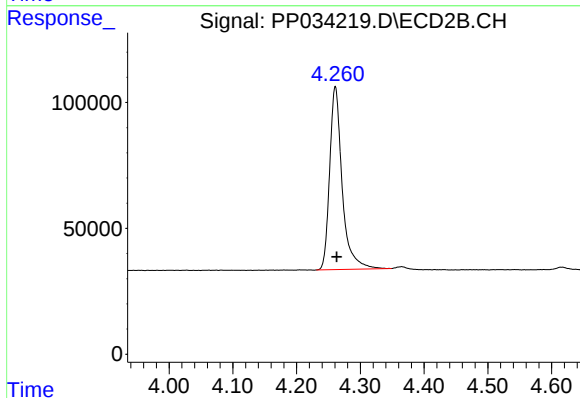


#1 Tetrachloro-m-xylene

R.T.: 4.261 min
Delta R.T.: -0.002 min
Response: 992128
Conc: 22.42 ng/ml

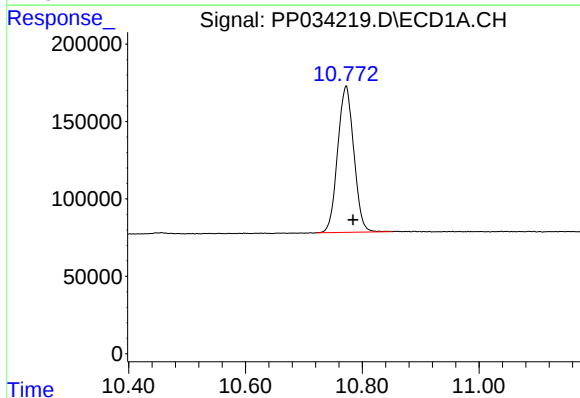


#2 Decachlorobiphenyl

R.T.: 10.772 min
Delta R.T.: -0.012 min
Response: 1810755
Conc: 23.07 ng/ml

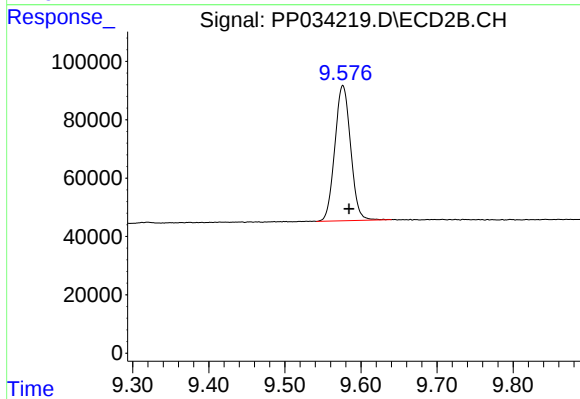

#2 Decachlorobiphenyl


R.T.: 9.576 min
Delta R.T.: -0.008 min
Response: 667760
Conc: 25.30 ng/ml

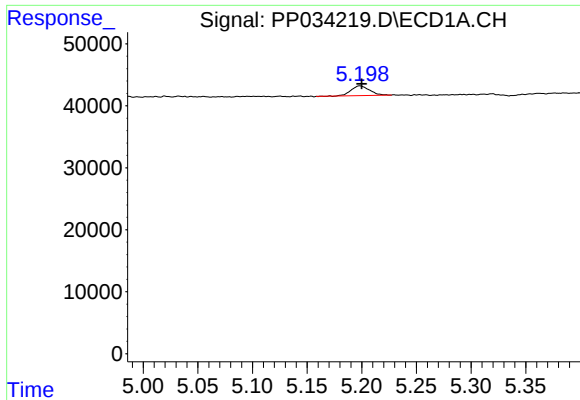

#9 AR-1221-2


R.T.: 5.198 min
Delta R.T.: -0.002 min
Response: 18525
Conc: 26.92 ng/ml

Instrument :
ECD_P
ClientSampleId :

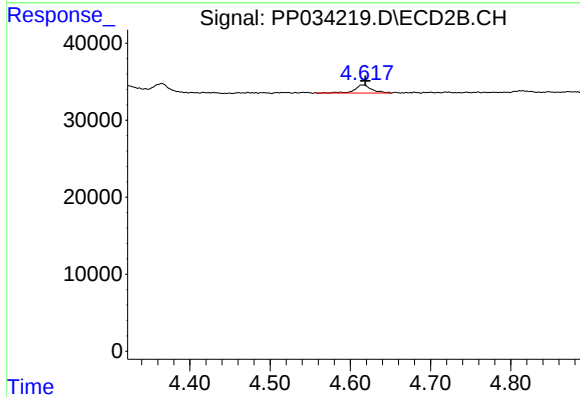


#9 AR-1221-2

R.T.: 4.616 min
Delta R.T.: -0.003 min
Response: 15501
Conc: 43.71 ng/ml

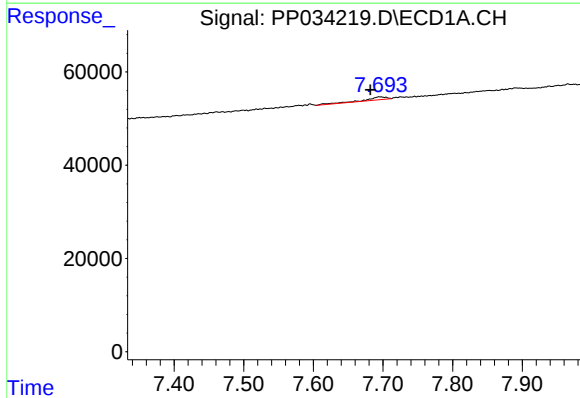


#28 AR-1254-3

R.T.: 7.695 min
Delta R.T.: 0.013 min
Response: 12881
Conc: 2.97 ng/ml

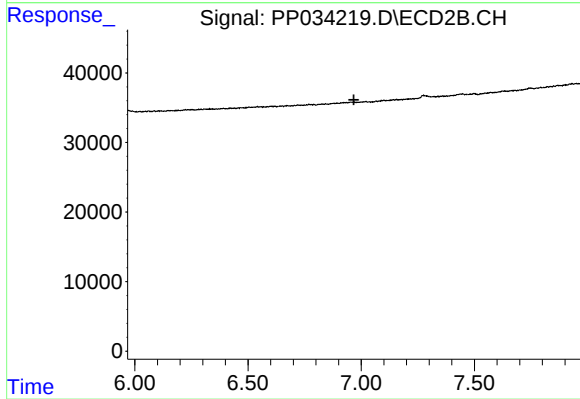

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 6.968 min
Response: 0
Conc: N.D.

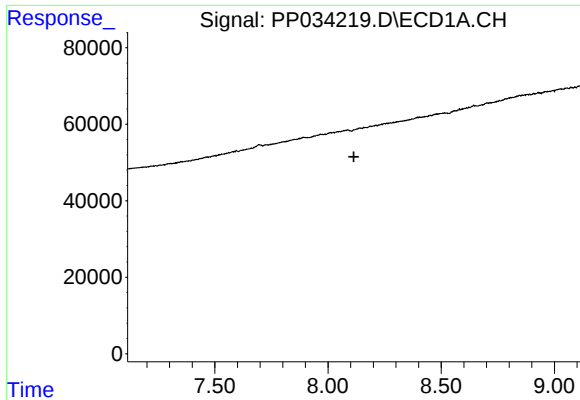

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 8.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

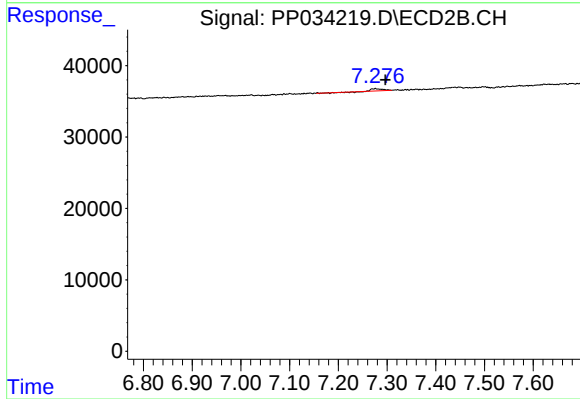


#32 AR-1260-2

R.T.: 7.276 min
Delta R.T.: -0.021 min
Response: 3316
Conc: 1.85 ng/ml

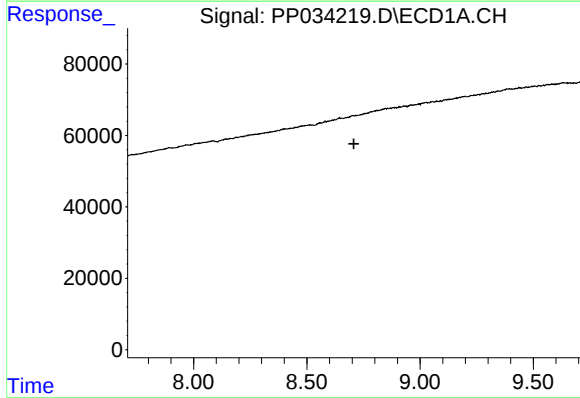


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 8.708 min
Response: 0
Conc: N.D.

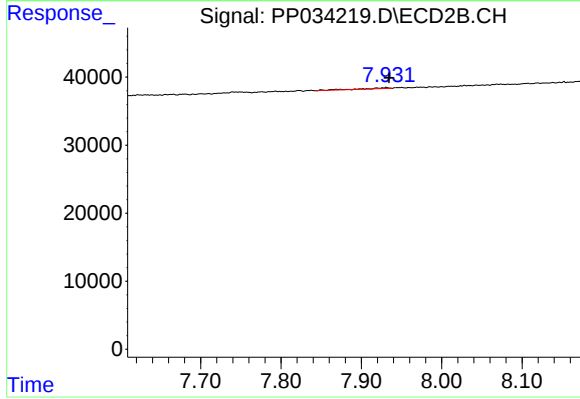

#34 AR-1260-4


R.T.: 7.931 min
Delta R.T.: -0.003 min
Response: 3244
Conc: 2.28 ng/ml

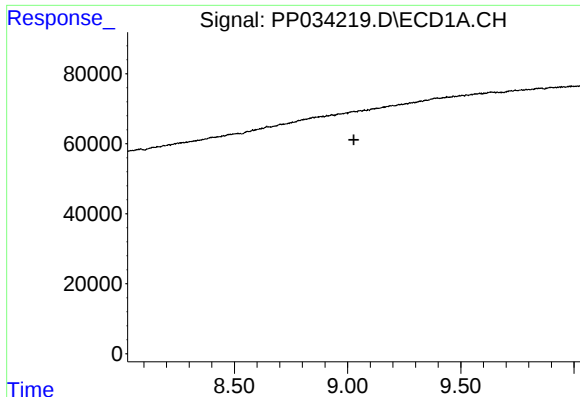

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 9.028 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

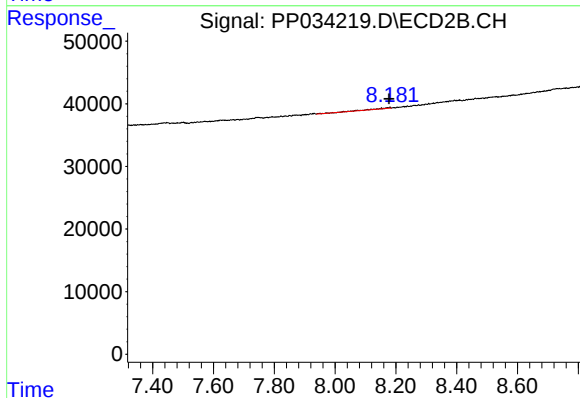


#35 AR-1260-5

R.T.: 8.181 min
Delta R.T.: 0.003 min
Response: 4436
Conc: 1.43 ng/ml

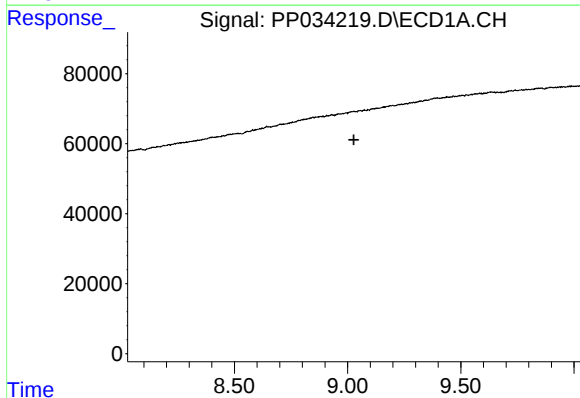


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 9.028 min
Response: 0
Conc: N.D.

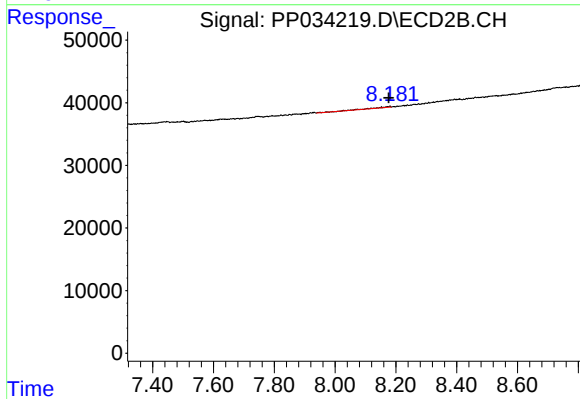

#37 AR-1262-2


R.T.: 8.181 min
Delta R.T.: 0.004 min
Response: 4436
Conc: 1.37 ng/ml

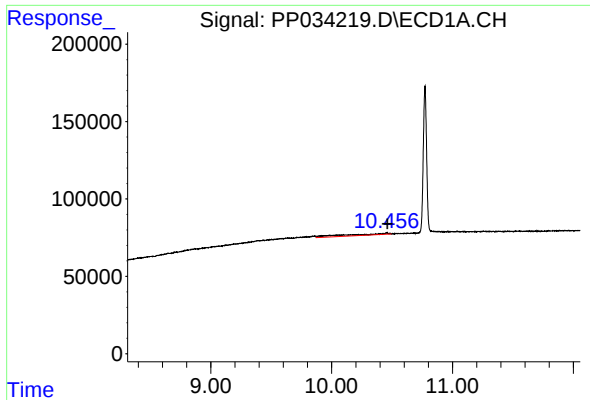

#45 AR-1268-5

R.T.: 10.456 min
Delta R.T.: -0.005 min
Response: 238915
Conc: 8.65 ng/ml

Instrument :
ECD_P
ClientSampleId :

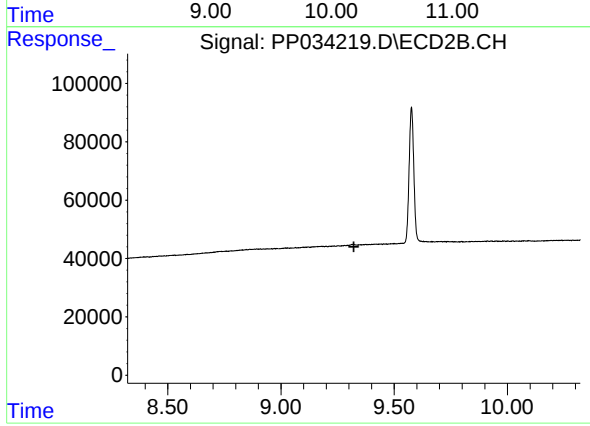

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.322 min
Response: 0
Conc: N.D.