

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032221\
 Data File : PP034241.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Mar 2021 23:24
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 02:11:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.849	4.261	1807197	1007572	21.513	22.769
2)	SA Decachlor...	10.772	9.574	1889313	681023	24.075	25.807
Target Compounds							
9)	L2 AR-1221-2	5.198	4.616	21691	14197	31.518	40.033 #
28)	L6 AR-1254-3	7.694	0.000	391029	0	90.032	N.D. #
29)	L6 AR-1254-4	8.006f	0.000	78881	0	27.171	N.D. #
32)	L7 AR-1260-2	8.086f	7.273f	21687	4447	5.771	2.485 #
35)	L7 AR-1260-5	0.000	8.172	0	36750	N.D.	11.835 #
37)	L8 AR-1262-2	0.000	8.172	0	36750	N.D.	11.386 #
40)	L8 AR-1262-5	0.000	8.999f	0	32901	N.D.	31.294 #
44)	L9 AR-1268-4	0.000	8.999f	0	32901	N.D.	27.341 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032221\
Data File : PP034241.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Mar 2021 23:24
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 02:11:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

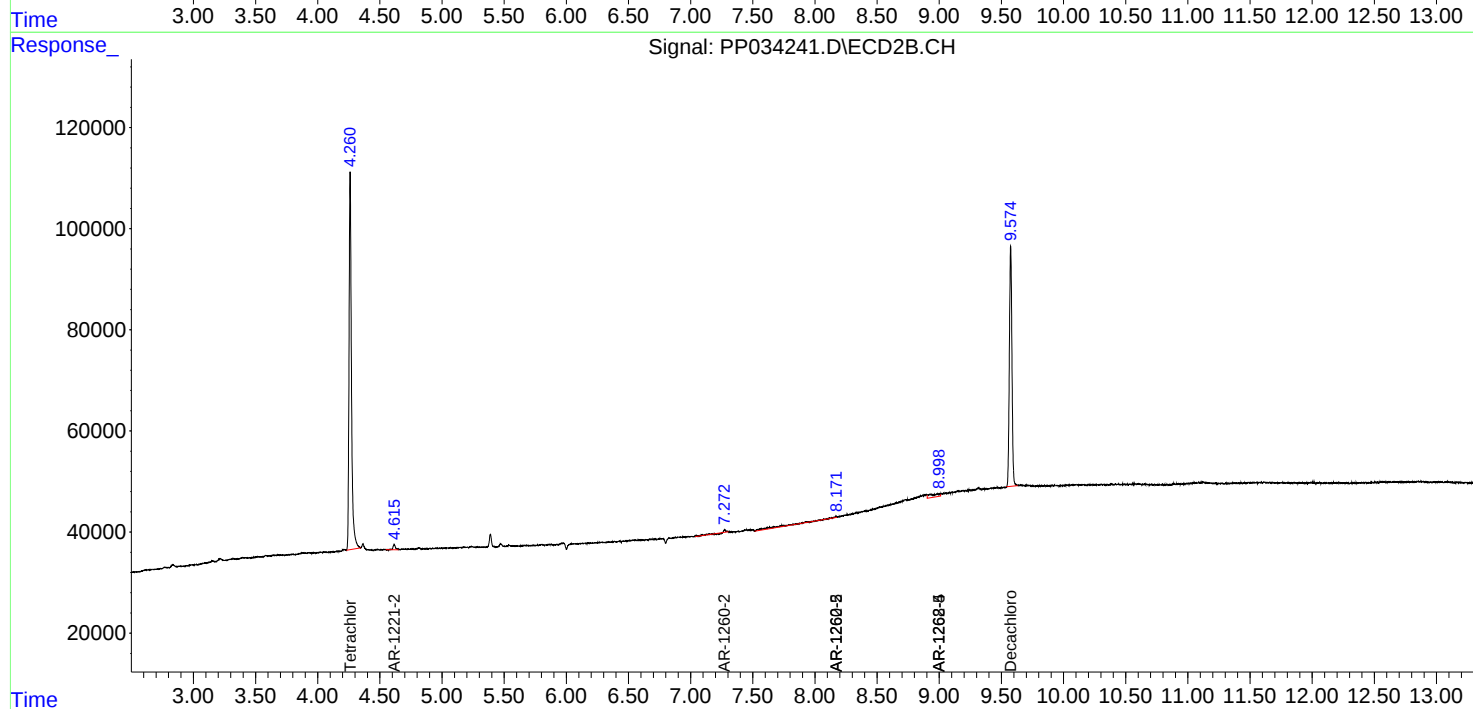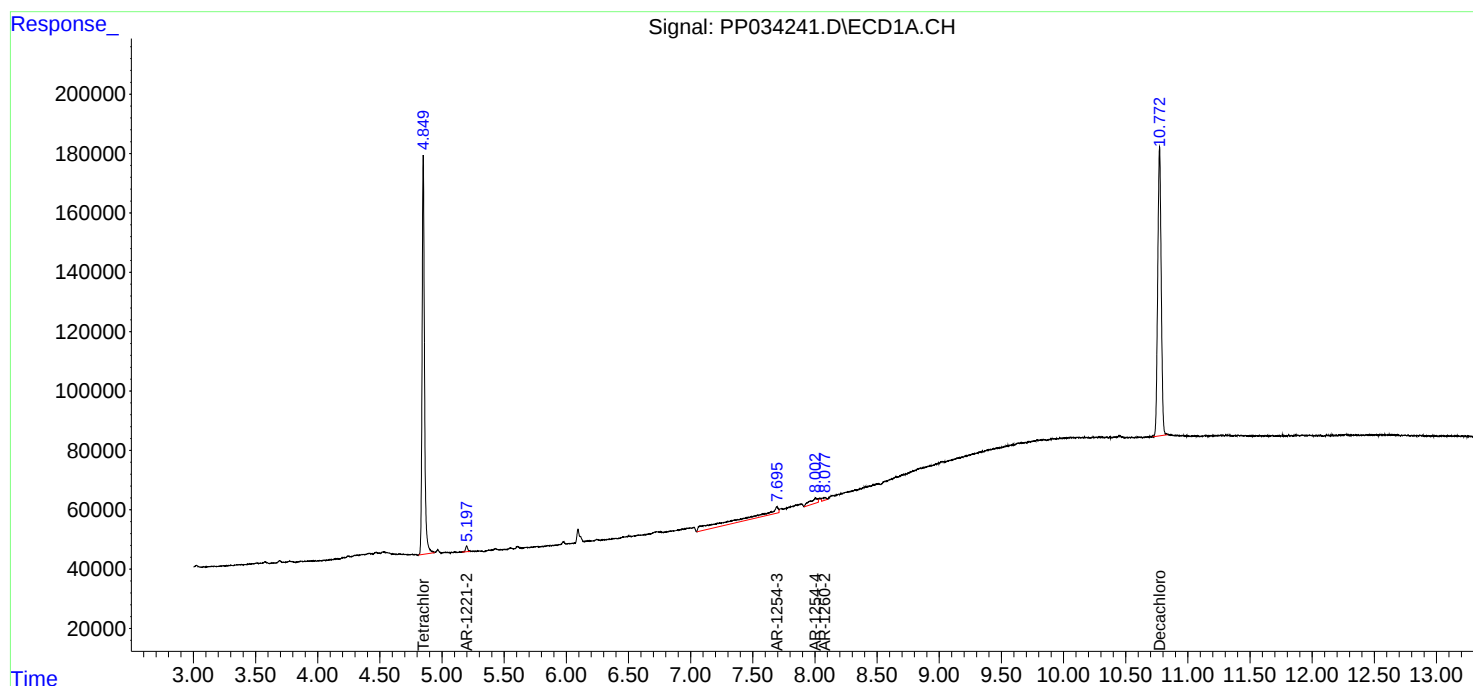


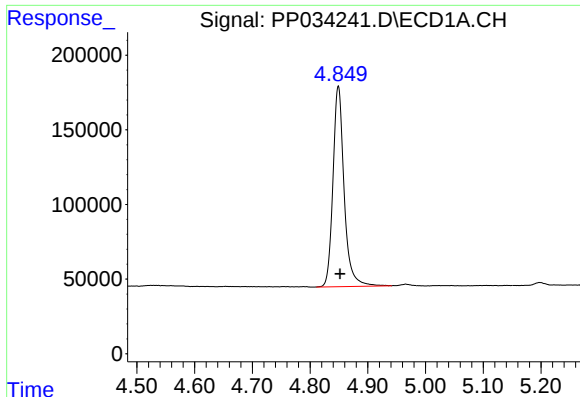

#1 Tetrachloro-m-xylene


R.T.: 4.849 min
Delta R.T.: -0.003 min
Response: 1807197
Conc: 21.51 ng/ml

Instrument :
ECD_P
ClientSampleId :

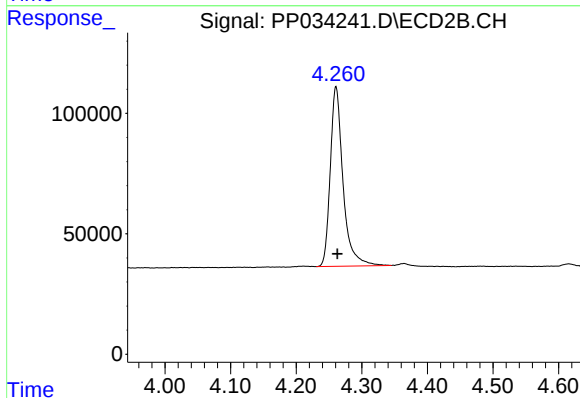


#1 Tetrachloro-m-xylene

R.T.: 4.261 min
Delta R.T.: -0.002 min
Response: 1007572
Conc: 22.77 ng/ml

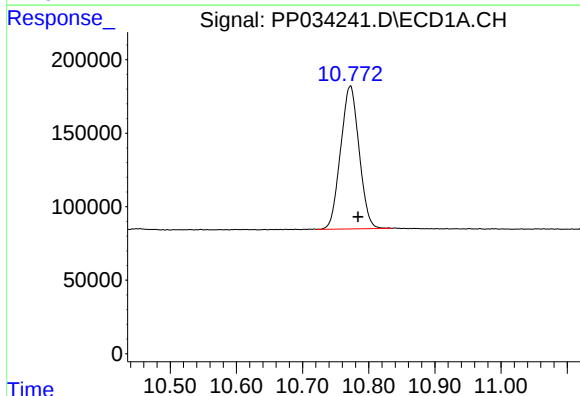


#2 Decachlorobiphenyl

R.T.: 10.772 min
Delta R.T.: -0.012 min
Response: 1889313
Conc: 24.07 ng/ml

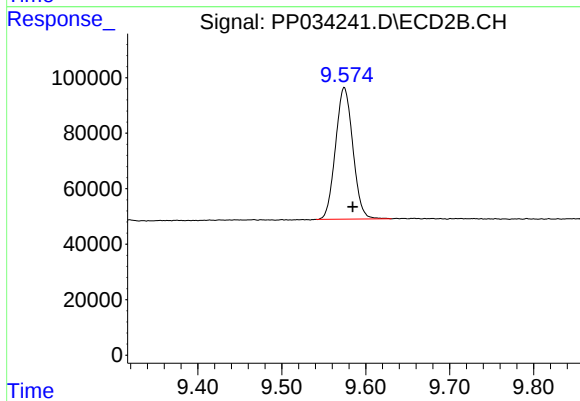

#2 Decachlorobiphenyl


R.T.: 9.574 min
Delta R.T.: -0.010 min
Response: 681023
Conc: 25.81 ng/ml

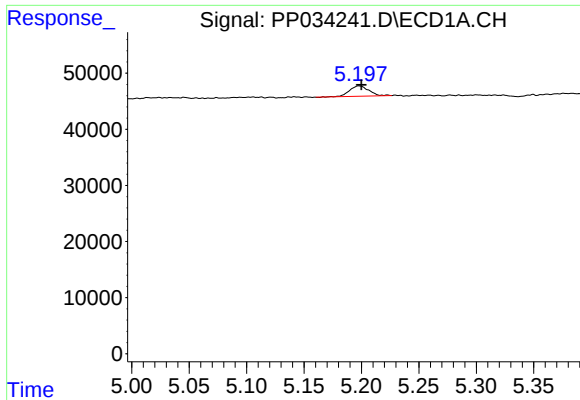

#9 AR-1221-2


R.T.: 5.198 min
Delta R.T.: -0.002 min
Response: 21691
Conc: 31.52 ng/ml

Instrument :
ECD_P
ClientSampleId :

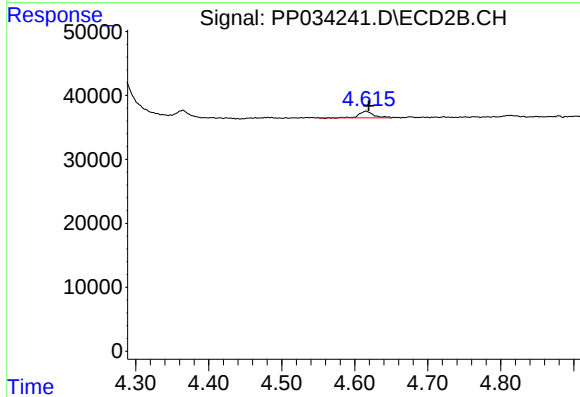


#9 AR-1221-2

R.T.: 4.616 min
Delta R.T.: -0.004 min
Response: 14197
Conc: 40.03 ng/ml

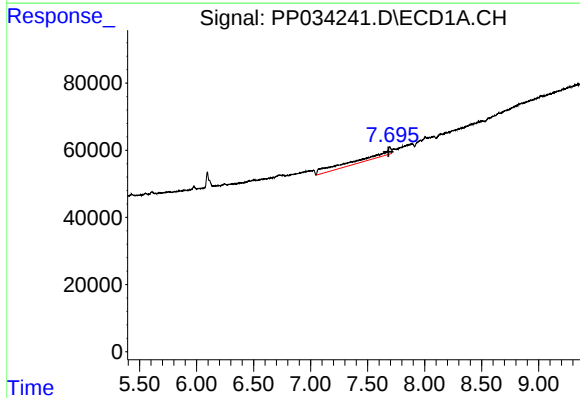


#28 AR-1254-3

R.T.: 7.694 min
Delta R.T.: 0.012 min
Response: 391029
Conc: 90.03 ng/ml

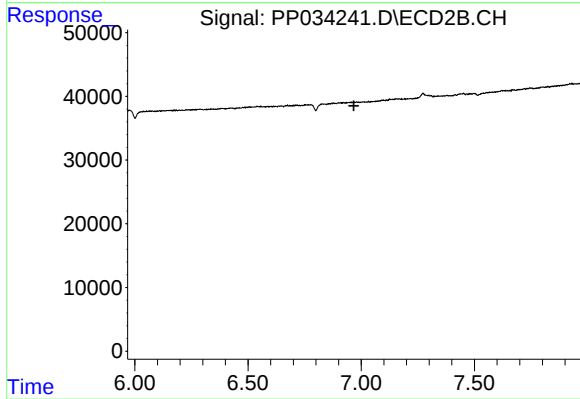

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 6.968 min
Response: 0
Conc: N.D.

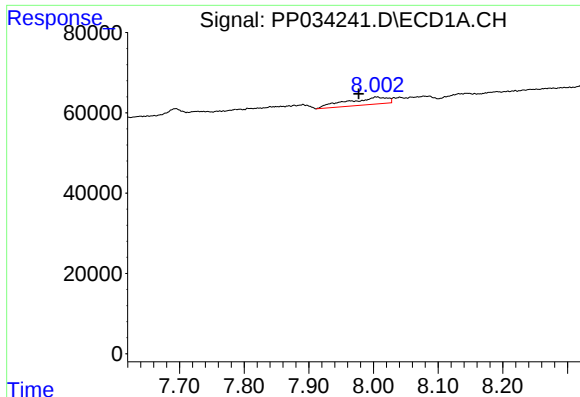

#29 AR-1254-4


R.T.: 8.006 min
Delta R.T.: 0.028 min
Response: 78881
Conc: 27.17 ng/ml

Instrument :
ECD_P
ClientSampleId :

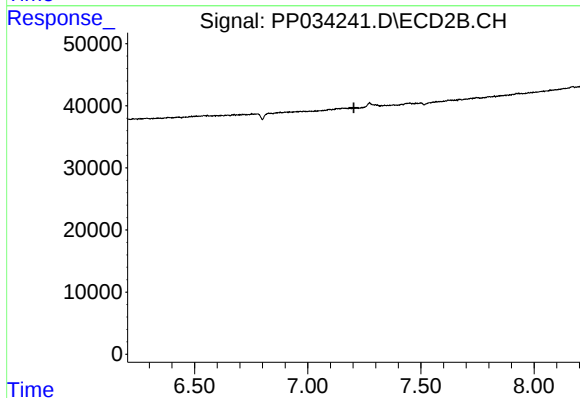


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.204 min
Response: 0
Conc: N.D.

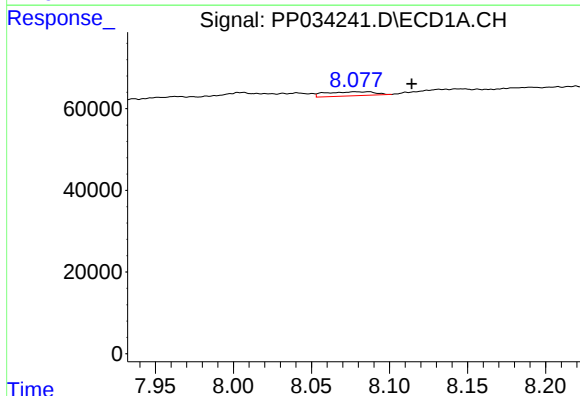


#32 AR-1260-2

R.T.: 8.086 min
Delta R.T.: -0.028 min
Response: 21687
Conc: 5.77 ng/ml

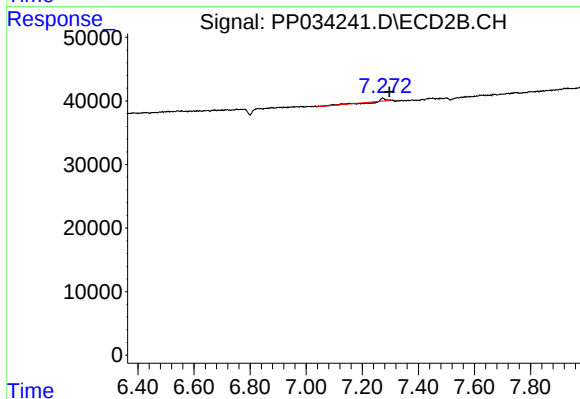

#32 AR-1260-2


R.T.: 7.273 min
Delta R.T.: -0.024 min
Response: 4447
Conc: 2.49 ng/ml

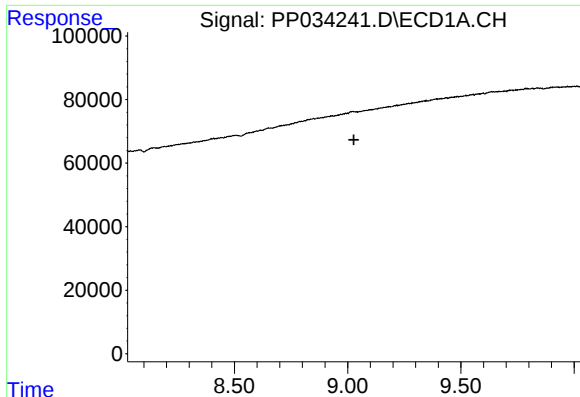

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 9.028 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

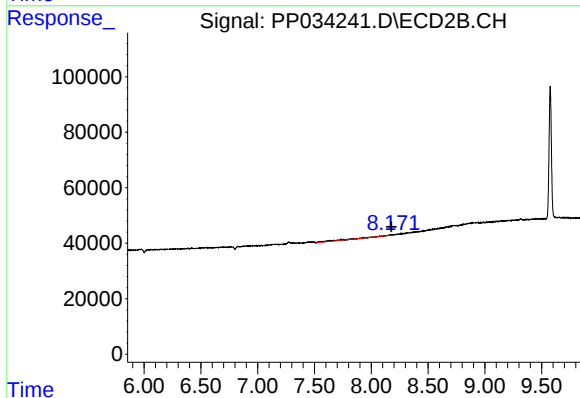


#35 AR-1260-5

R.T.: 8.172 min
Delta R.T.: -0.005 min
Response: 36750
Conc: 11.84 ng/ml

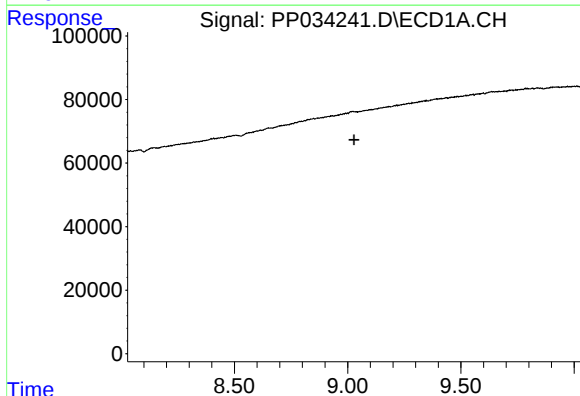


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 9.028 min
Response: 0
Conc: N.D.

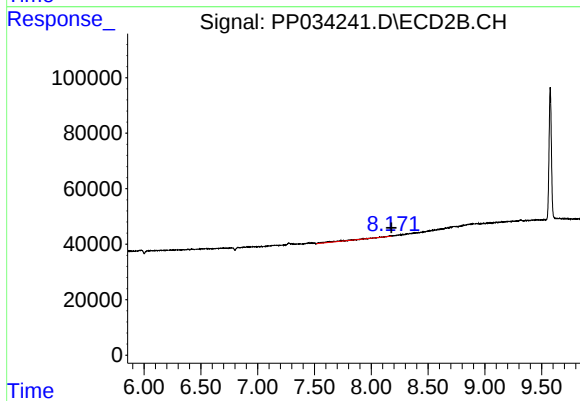

#37 AR-1262-2


R.T.: 8.172 min
Delta R.T.: -0.005 min
Response: 36750
Conc: 11.39 ng/ml

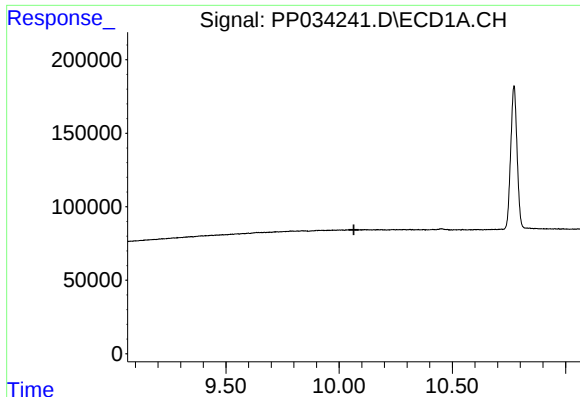

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 10.065 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

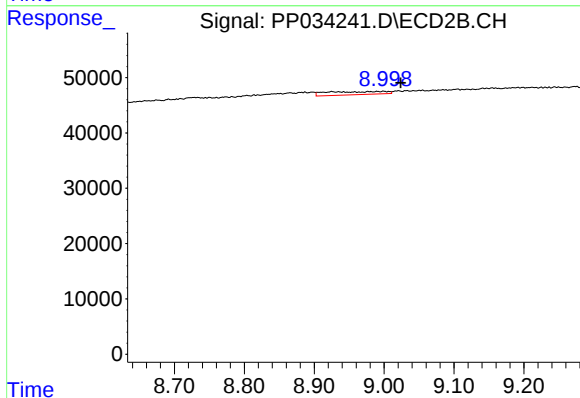


#40 AR-1262-5

R.T.: 8.999 min
Delta R.T.: -0.025 min
Response: 32901
Conc: 31.29 ng/ml

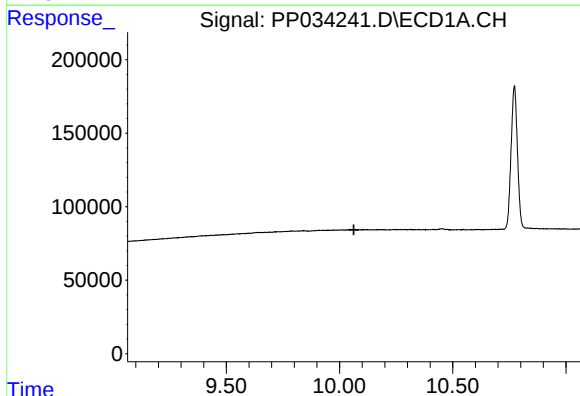

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 10.063 min
Response: 0
Conc: N.D.

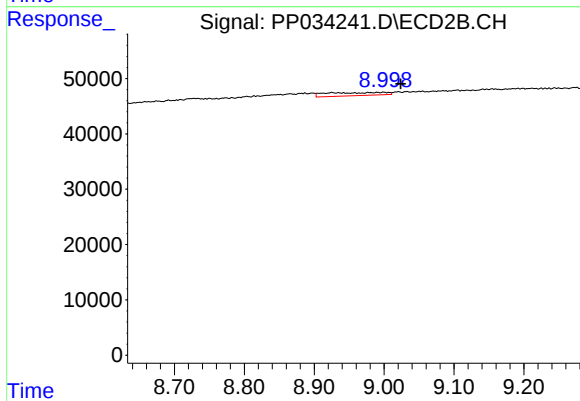

#44 AR-1268-4

R.T.: 8.999 min
Delta R.T.: -0.024 min
Response: 32901
Conc: 27.34 ng/ml