

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032221\
 Data File : PP034224.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Mar 2021 17:46
 Operator : DD\AJ
 Sample : M1660-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-1C

Manual Integrations
 APPROVED

Ankita
 3/23/2021 1:38:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 02:02:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.849	4.261	1386186	821618	16.501	18.567
2) SA Decachlor...	10.773	9.570	1243936	961870	15.851m	36.450 #
Target Compounds						
26) L6 AR-1254-1	7.068	6.387	167082	98165	61.046	58.540
27) L6 AR-1254-2	7.292	6.543	447952	85249	107.576	58.785 #
28) L6 AR-1254-3	7.677	6.963	703017	431521	161.866	188.427
29) L6 AR-1254-4	7.970	7.200	234644	95504	80.824	79.870
30) L6 AR-1254-5	8.399	7.627	1288767	2984310	386.061	1616.236 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032221\
Data File : PP034224.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Mar 2021 17:46
Operator : DD\AJ
Sample : M1660-04
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
X127-1C


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 02:02:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

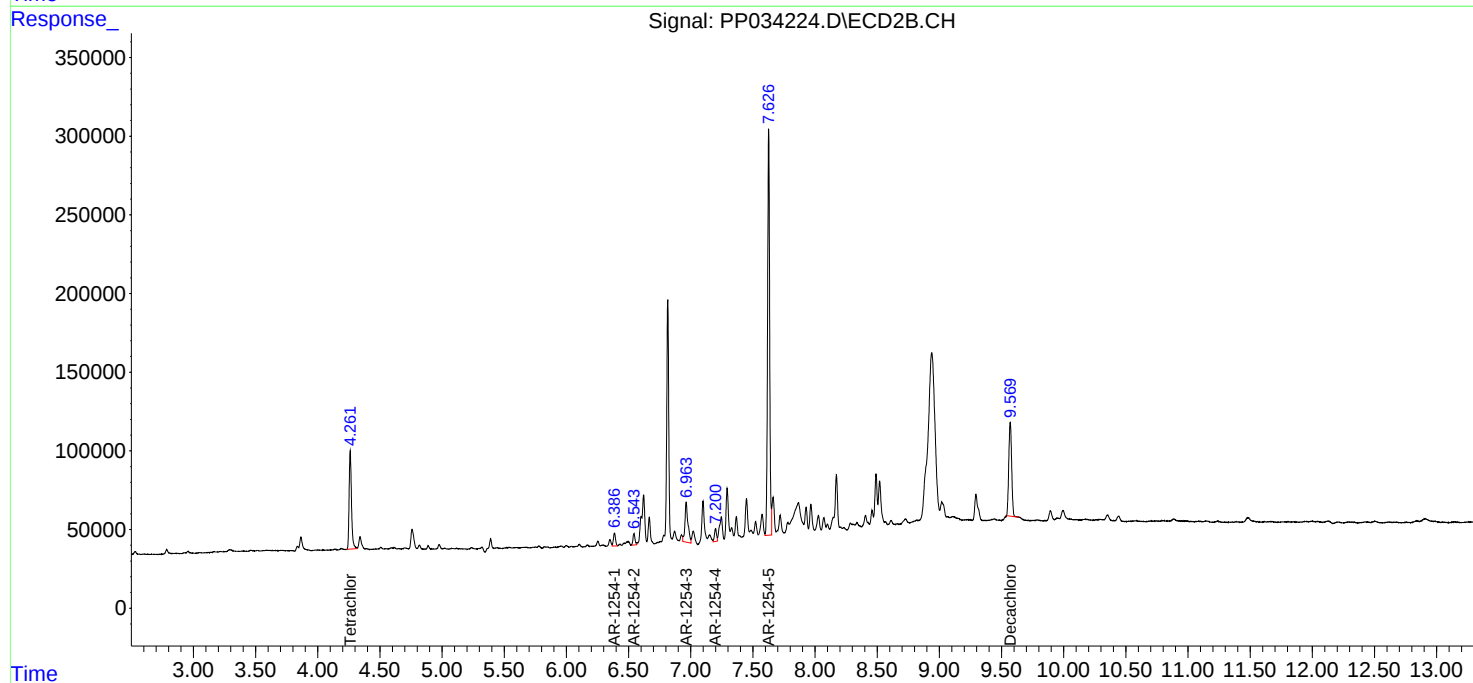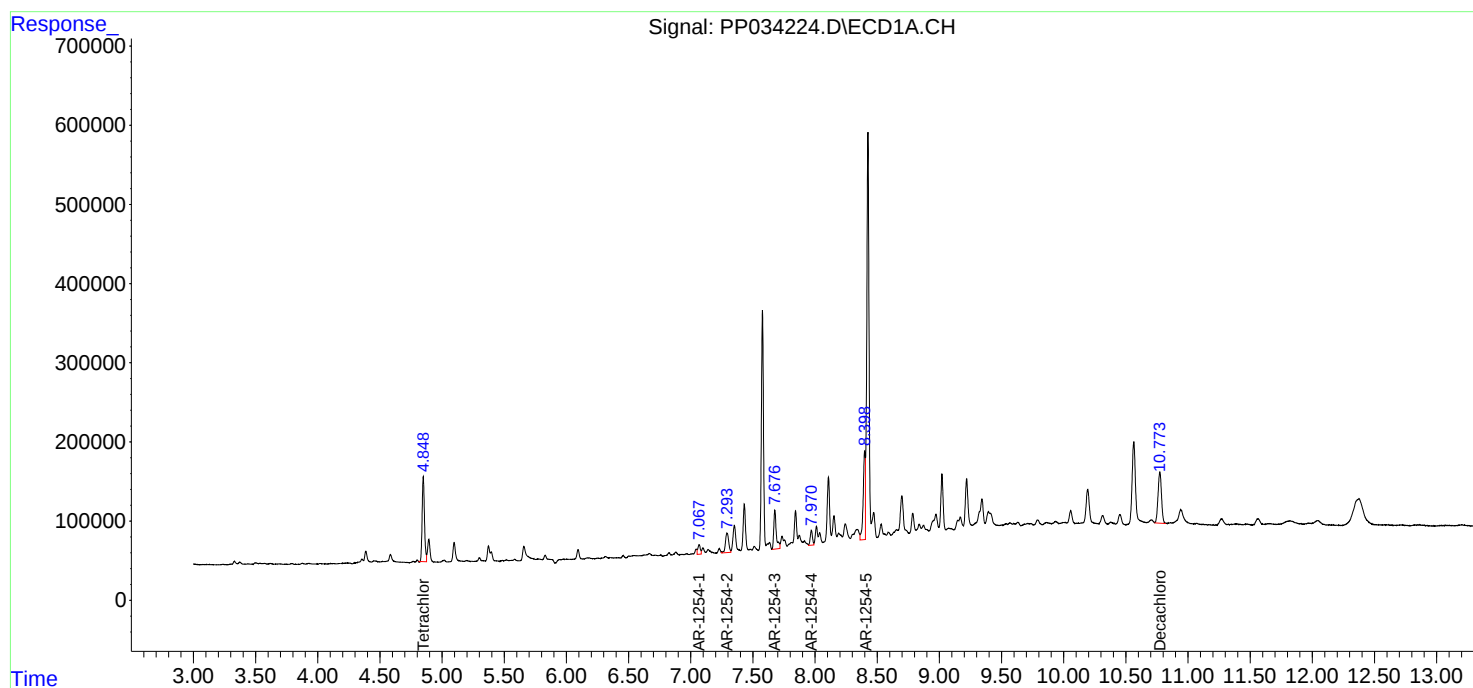

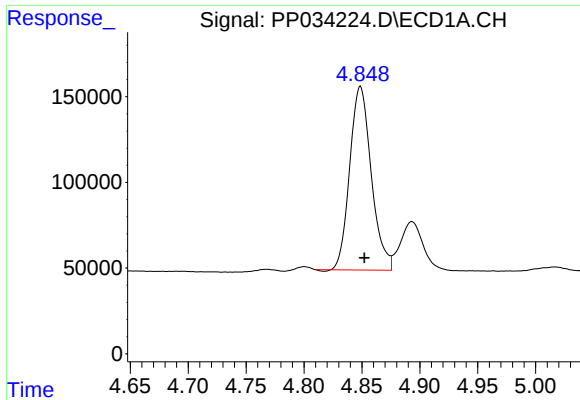


#1 Tetrachloro-m-xylene

R.T.: 4.849 min
Delta R.T.: -0.003 min
Response: 1386186
Conc: 16.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-1C


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:38 PM

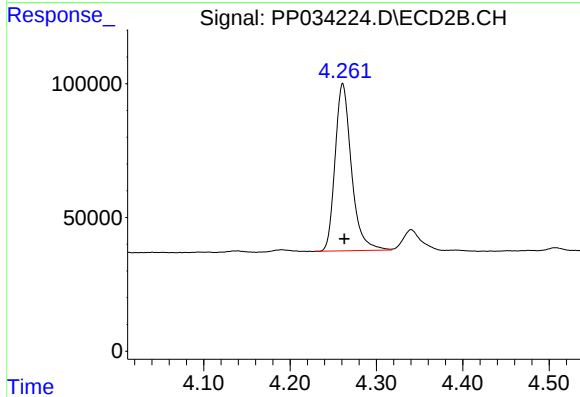


#1 Tetrachloro-m-xylene

R.T.: 4.261 min
Delta R.T.: -0.002 min
Response: 821618
Conc: 18.57 ng/ml

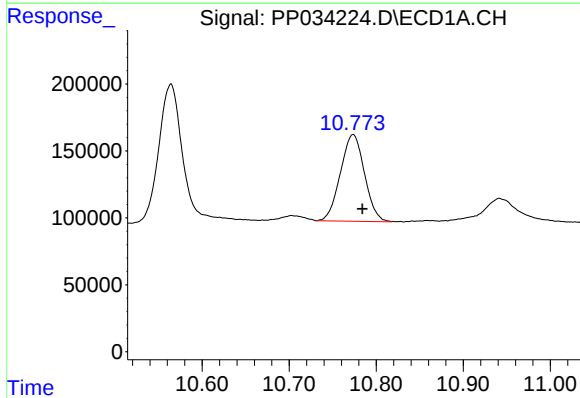


#2 Decachlorobiphenyl

R.T.: 10.773 min
Delta R.T.: -0.011 min
Response: 1243936
Conc: 15.85 ng/ml m

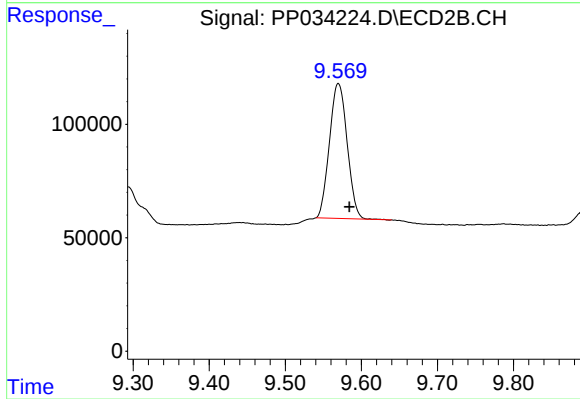

#2 Decachlorobiphenyl

R.T.: 9.570 min
Delta R.T.: -0.015 min
Response: 961870
Conc: 36.45 ng/ml

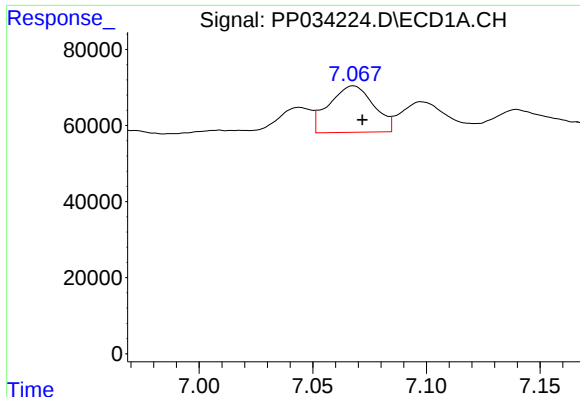


#26 AR-1254-1

R.T.: 7.068 min
Delta R.T.: -0.004 min
Response: 167082
Conc: 61.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-1C


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:38 PM

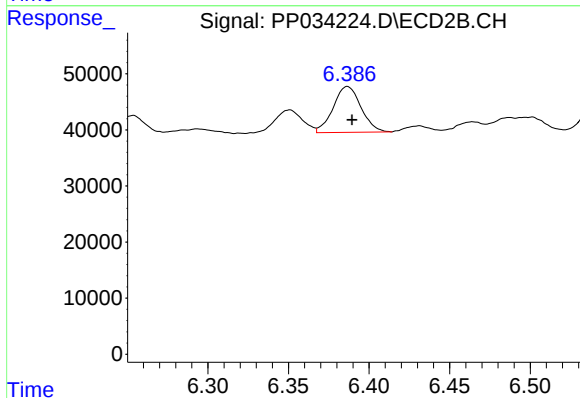


#26 AR-1254-1

R.T.: 6.387 min
Delta R.T.: -0.003 min
Response: 98165
Conc: 58.54 ng/ml

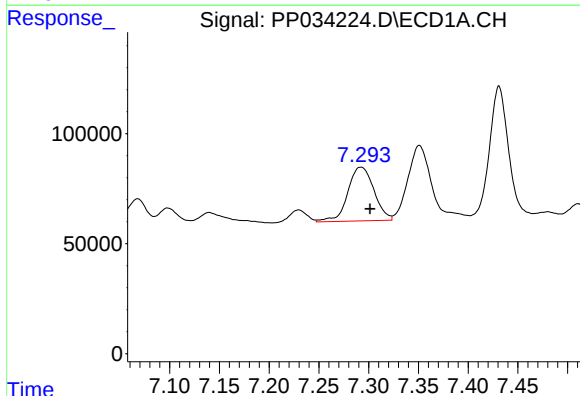


#27 AR-1254-2

R.T.: 7.292 min
Delta R.T.: -0.009 min
Response: 447952
Conc: 107.58 ng/ml

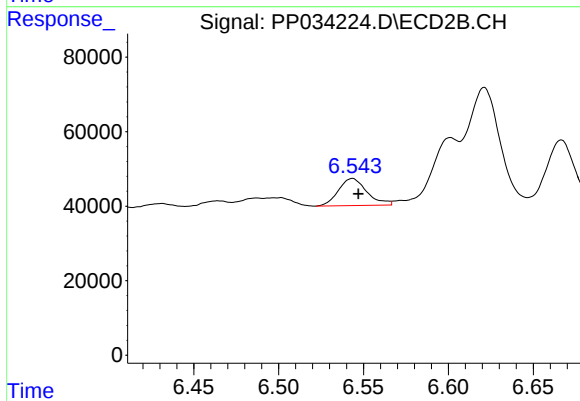

#27 AR-1254-2

R.T.: 6.543 min
Delta R.T.: -0.003 min
Response: 85249
Conc: 58.78 ng/ml

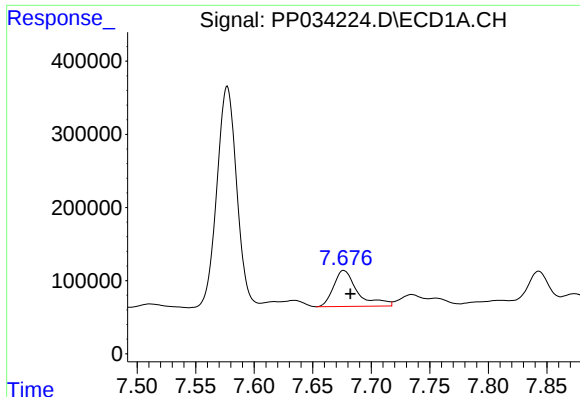


#28 AR-1254-3

R.T.: 7.677 min
Delta R.T.: -0.006 min
Response: 703017
Conc: 161.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-1C


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:38 PM

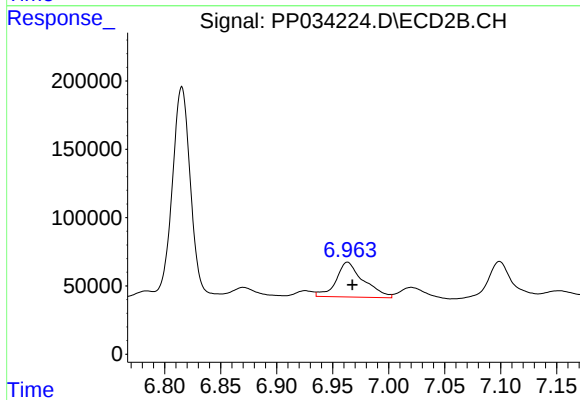


#28 AR-1254-3

R.T.: 6.963 min
Delta R.T.: -0.004 min
Response: 431521
Conc: 188.43 ng/ml

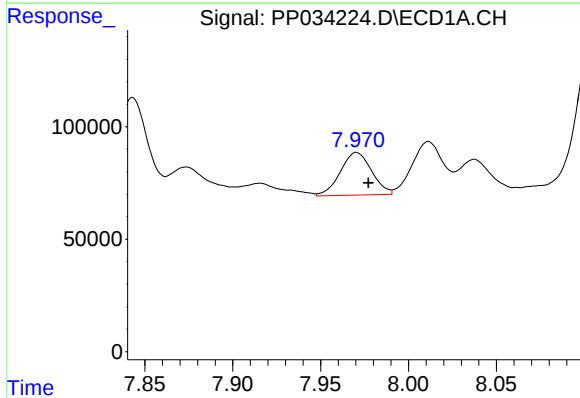


#29 AR-1254-4

R.T.: 7.970 min
Delta R.T.: -0.007 min
Response: 234644
Conc: 80.82 ng/ml

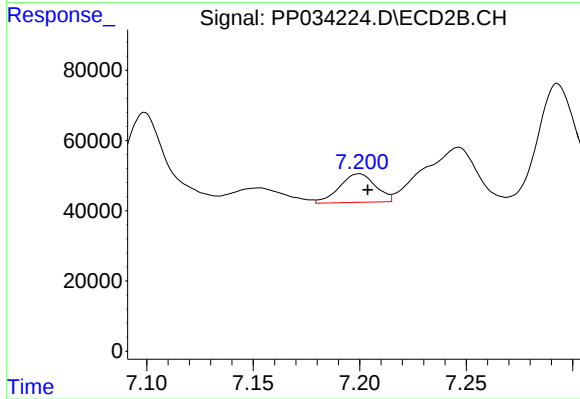

#29 AR-1254-4

R.T.: 7.200 min
Delta R.T.: -0.004 min
Response: 95504
Conc: 79.87 ng/ml

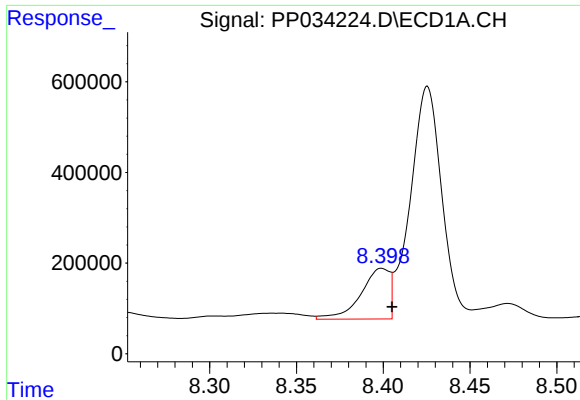


#30 AR-1254-5

R.T.: 8.399 min
Delta R.T.: -0.006 min
Response: 1288767
Conc: 386.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-1C

Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:38 PM

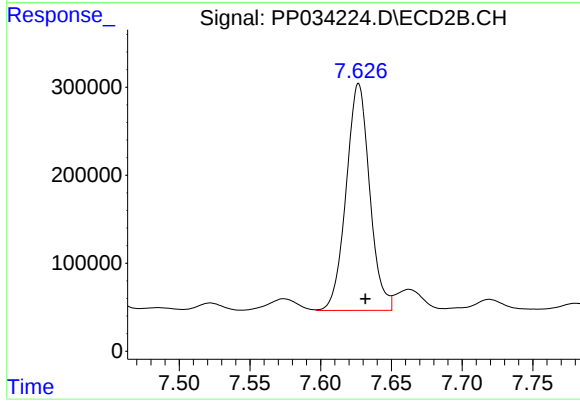

#30 AR-1254-5

R.T.: 7.627 min
Delta R.T.: -0.005 min
Response: 2984310
Conc: 1616.24 ng/ml