

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032221\
 Data File : PP034225.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Mar 2021 18:03
 Operator : DD\AJ
 Sample : M1660-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-2B

Manual Integrations
 APPROVED

Ankita
 3/23/2021 1:38:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 02:03:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.848	4.261	1539404	865963	18.325m	19.569
2) SA Decachlor...	10.772	9.576	1251497	462446	15.947	17.524
Target Compounds						
26) L6 AR-1254-1	7.067	6.386	1789382	1215302	653.781	724.737
27) L6 AR-1254-2	7.296	6.543	5725238	2531352	1374.923	1745.543 #
28) L6 AR-1254-3	7.676	6.964	10389743	4771277	2392.180	2083.414
29) L6 AR-1254-4	7.972	7.200	9499079	3846611	3272.001	3216.892
30) L6 AR-1254-5	8.399	7.627	19738985	12798735	5912.974	6931.513

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032221\
Data File : PP034225.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Mar 2021 18:03
Operator : DD\AJ
Sample : M1660-06
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
X127-2B


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 02:03:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

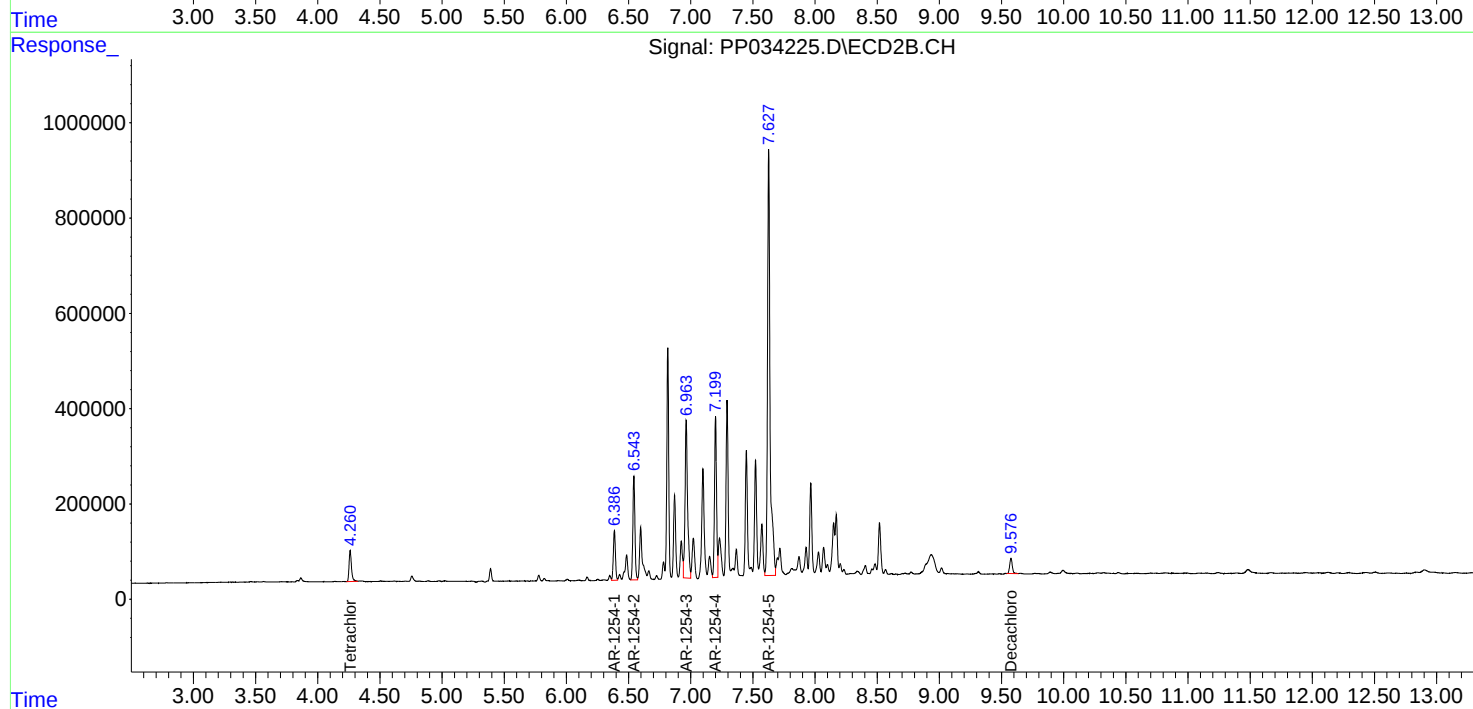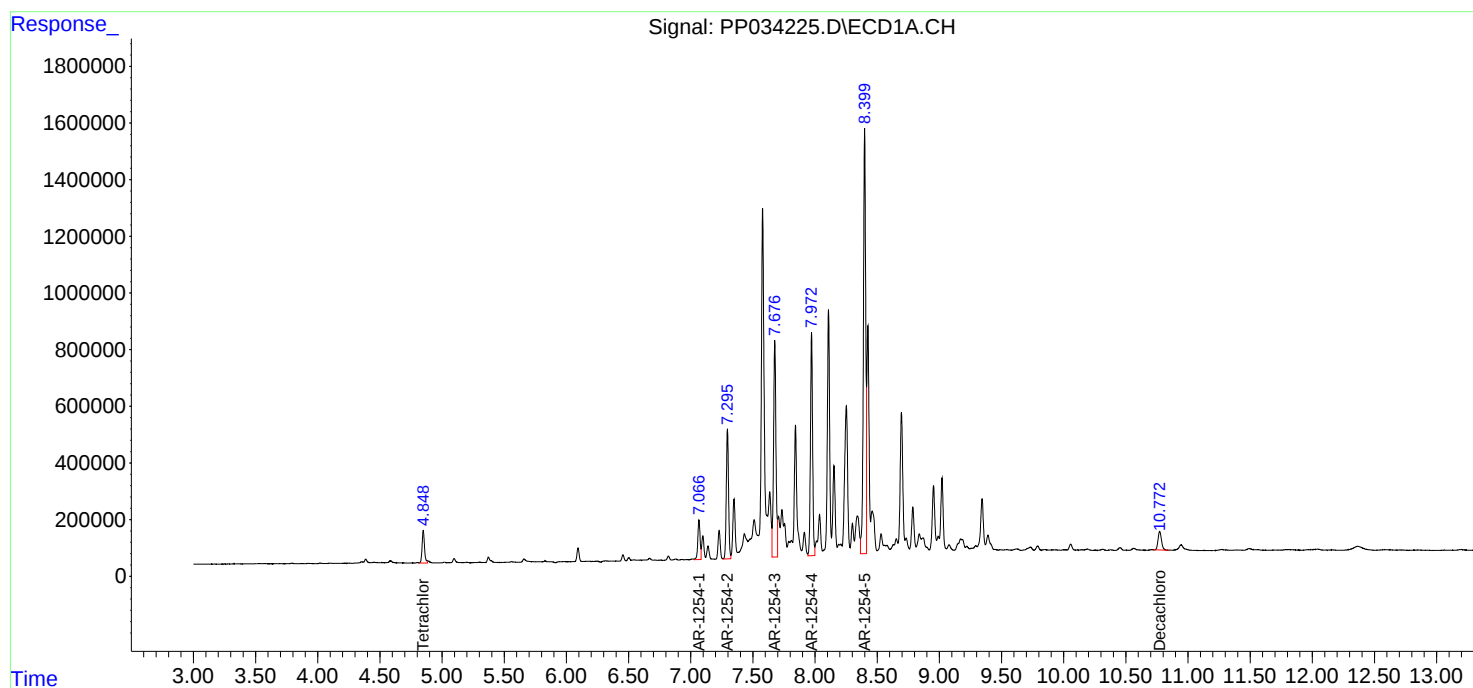

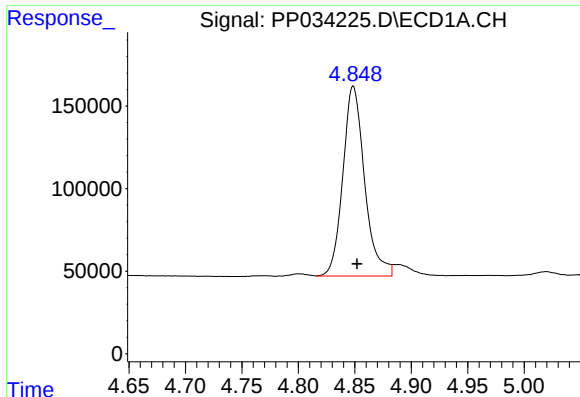


#1 Tetrachloro-m-xylene

R.T.: 4.848 min
Delta R.T.: -0.004 min
Response: 1539404
Conc: 18.32 ng/ml m

Instrument :
ECD_P
ClientSampleId :
X127-2B


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:41 PM

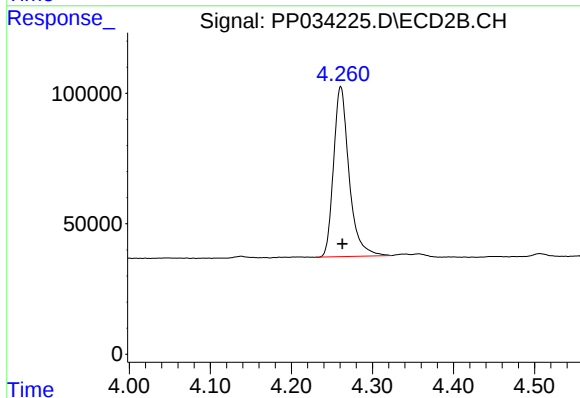


#1 Tetrachloro-m-xylene

R.T.: 4.261 min
Delta R.T.: -0.002 min
Response: 865963
Conc: 19.57 ng/ml

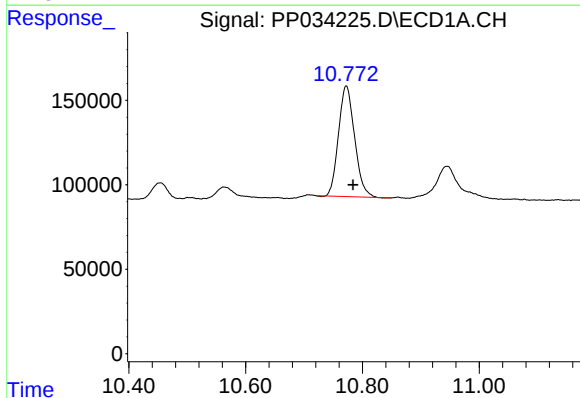


#2 Decachlorobiphenyl

R.T.: 10.772 min
Delta R.T.: -0.012 min
Response: 1251497
Conc: 15.95 ng/ml

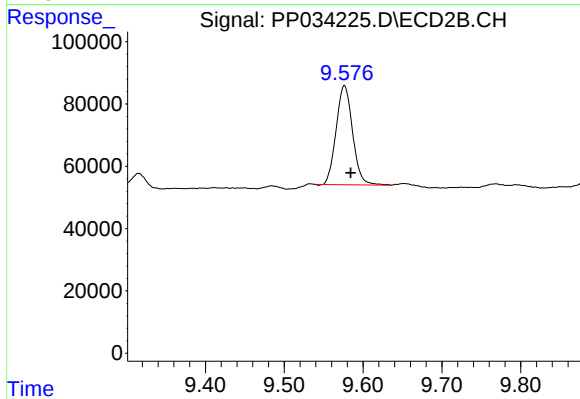

#2 Decachlorobiphenyl

R.T.: 9.576 min
Delta R.T.: -0.008 min
Response: 462446
Conc: 17.52 ng/ml

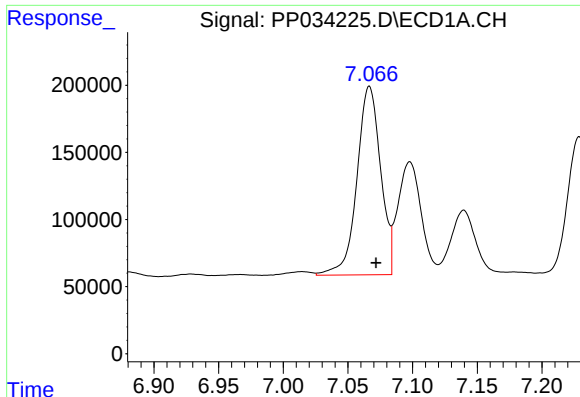


#26 AR-1254-1

R.T.: 7.067 min
Delta R.T.: -0.005 min
Response: 1789382
Conc: 653.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-2B


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:41 PM

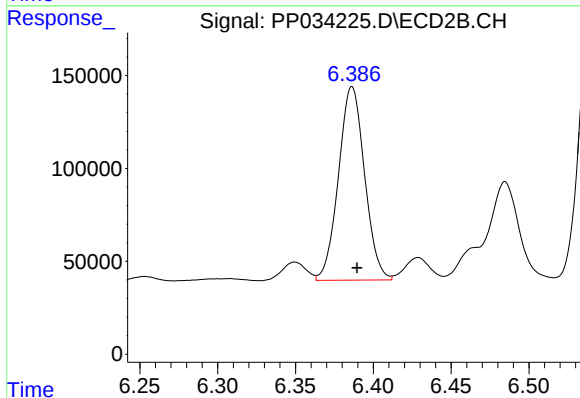


#26 AR-1254-1

R.T.: 6.386 min
Delta R.T.: -0.003 min
Response: 1215302
Conc: 724.74 ng/ml

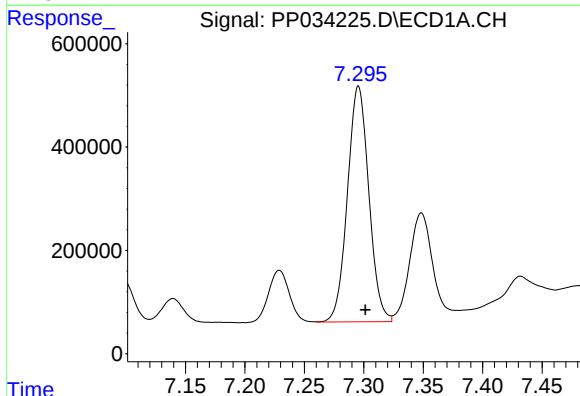


#27 AR-1254-2

R.T.: 7.296 min
Delta R.T.: -0.006 min
Response: 5725238
Conc: 1374.92 ng/ml

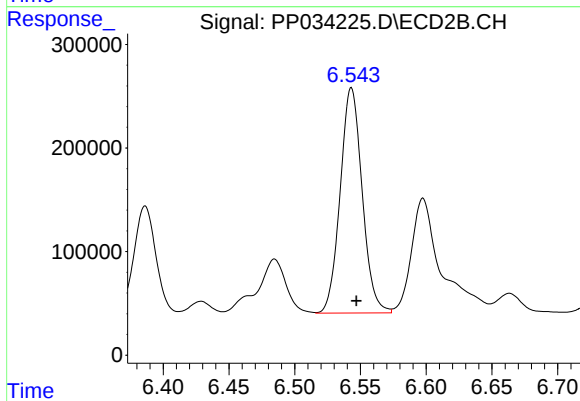

#27 AR-1254-2

R.T.: 6.543 min
Delta R.T.: -0.004 min
Response: 2531352
Conc: 1745.54 ng/ml

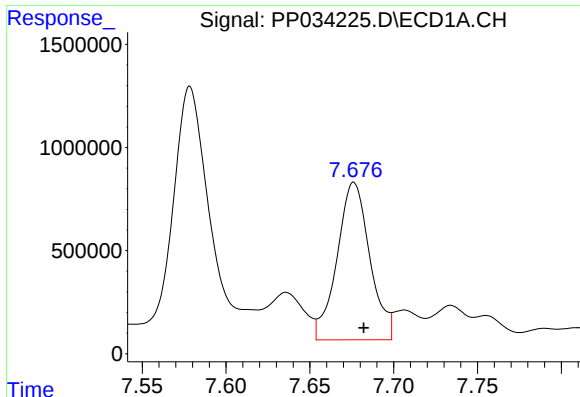


#28 AR-1254-3

R.T.: 7.676 min
Delta R.T.: -0.006 min
Response: 10389743
Conc: 2392.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-2B


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:41 PM

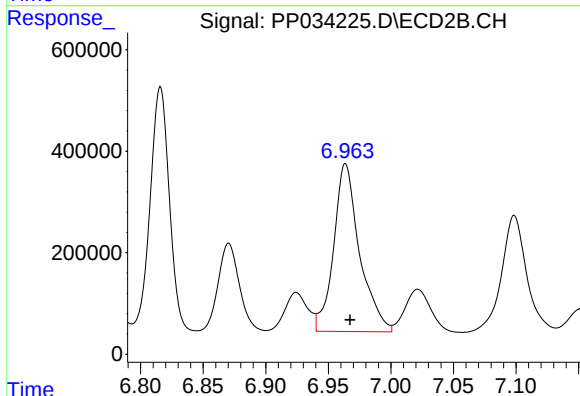


#28 AR-1254-3

R.T.: 6.964 min
Delta R.T.: -0.004 min
Response: 4771277
Conc: 2083.41 ng/ml

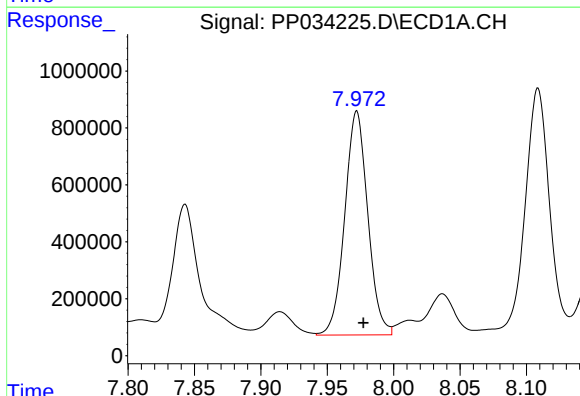


#29 AR-1254-4

R.T.: 7.972 min
Delta R.T.: -0.005 min
Response: 9499079
Conc: 3272.00 ng/ml

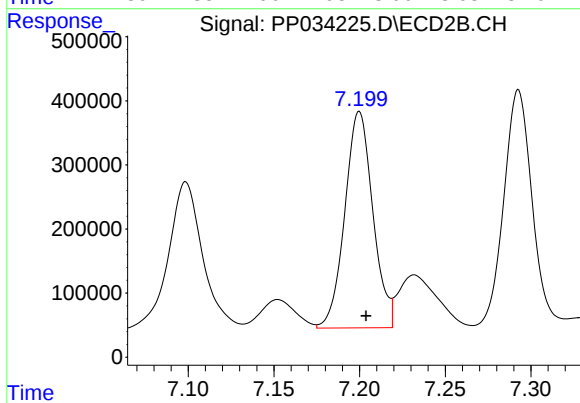

#29 AR-1254-4

R.T.: 7.200 min
Delta R.T.: -0.004 min
Response: 3846611
Conc: 3216.89 ng/ml

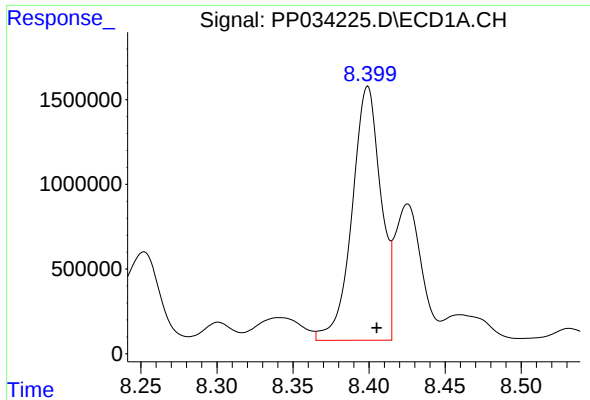


#30 AR-1254-5

R.T.: 8.399 min
Delta R.T.: -0.006 min
Response: 19738985
Conc: 5912.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-2B

Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:41 PM

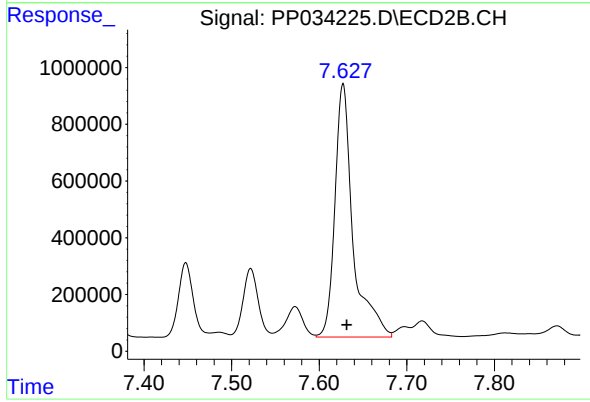

#30 AR-1254-5

R.T.: 7.627 min
Delta R.T.: -0.004 min
Response: 12798735
Conc: 6931.51 ng/ml