

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032221\
 Data File : PP034226.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Mar 2021 18:20
 Operator : DD\AJ
 Sample : M1660-07
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-2C

Manual Integrations
 APPROVED

Ankita
 3/23/2021 1:38:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 02:03:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.849	4.261	2124854	1158253	25.294	26.174
2) SA Decachlor...	10.773	9.575	2000570	848471	25.492	32.152 #
Target Compounds						
26) L6 AR-1254-1	7.067	6.386	306960	195542	112.153m	116.610
27) L6 AR-1254-2	7.296	6.543	821885	377607	197.377	260.386 #
28) L6 AR-1254-3	7.676	6.963	1877100	923675	432.192	403.330
29) L6 AR-1254-4	7.972	7.199	1025863	472674	353.363	395.294
30) L6 AR-1254-5	8.399	7.626	3761301	5164366	1126.728	2796.907 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032221\
Data File : PP034226.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Mar 2021 18:20
Operator : DD\AJ
Sample : M1660-07
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
X127-2C


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 02:03:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

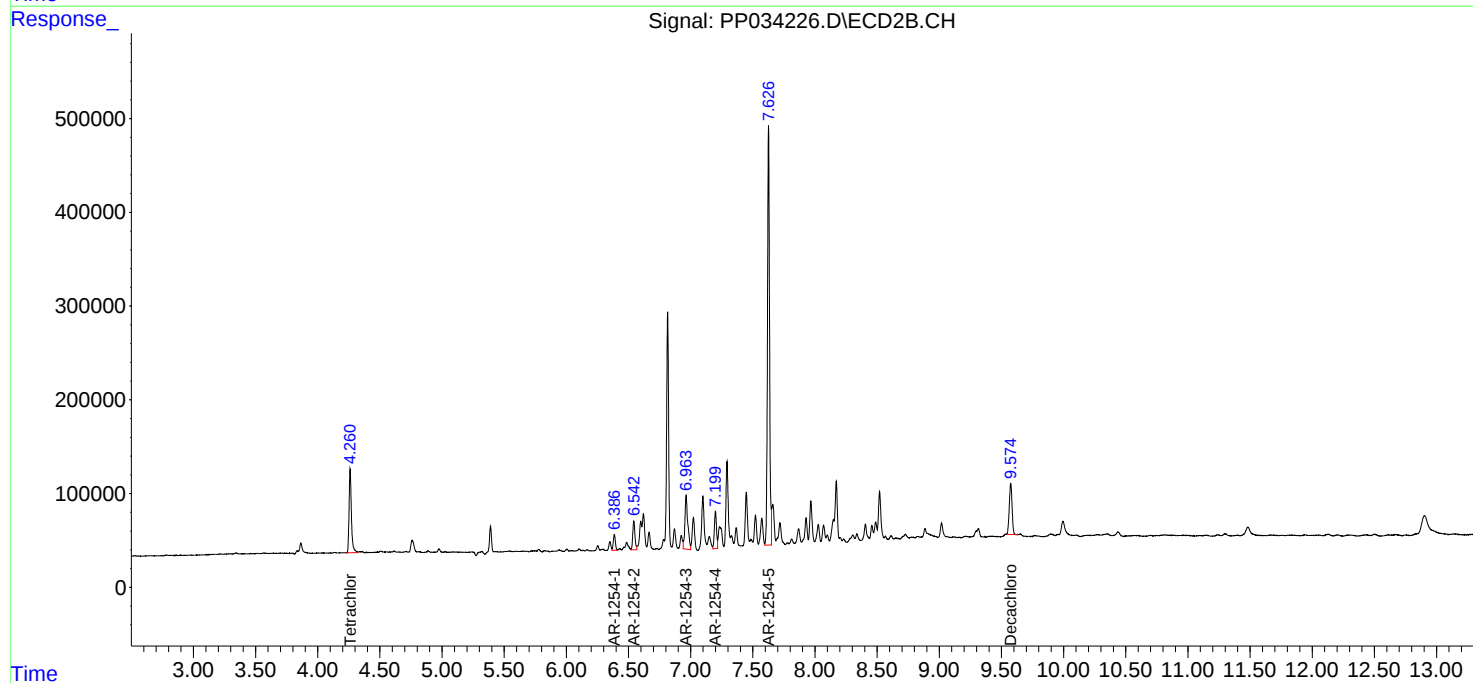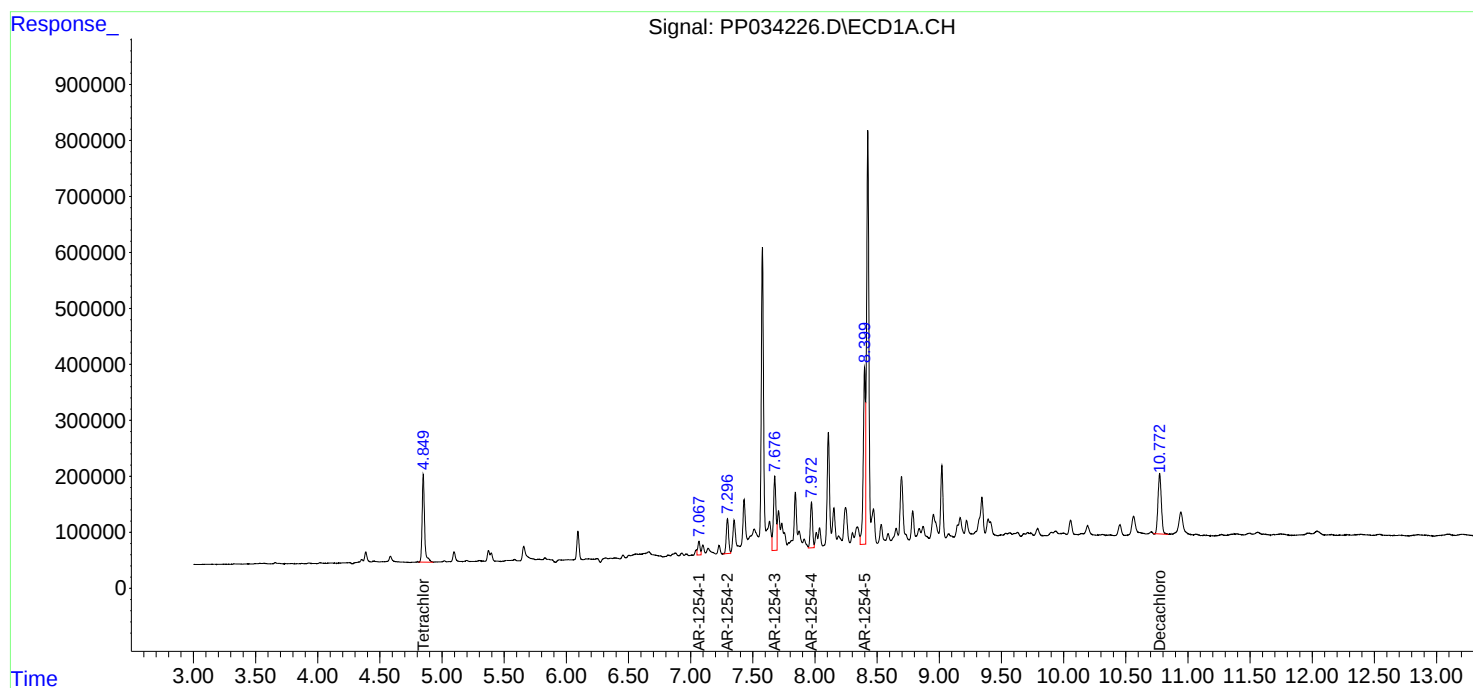

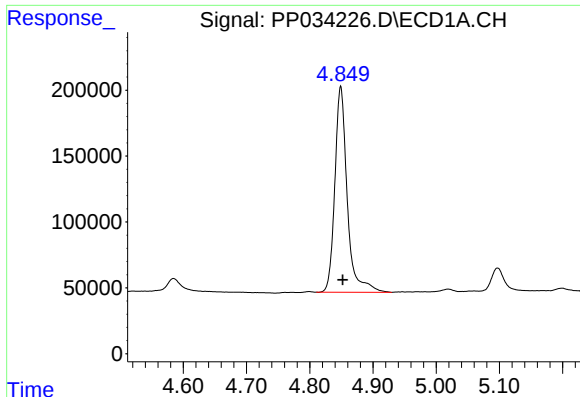


#1 Tetrachloro-m-xylene

R.T.: 4.849 min
Delta R.T.: -0.003 min
Response: 2124854
Conc: 25.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-2C


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:43 PM

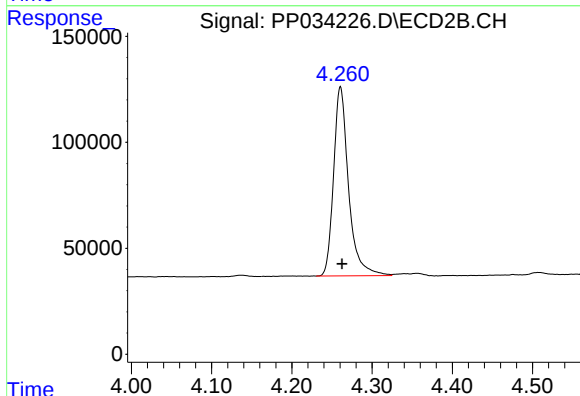


#1 Tetrachloro-m-xylene

R.T.: 4.261 min
Delta R.T.: -0.002 min
Response: 1158253
Conc: 26.17 ng/ml

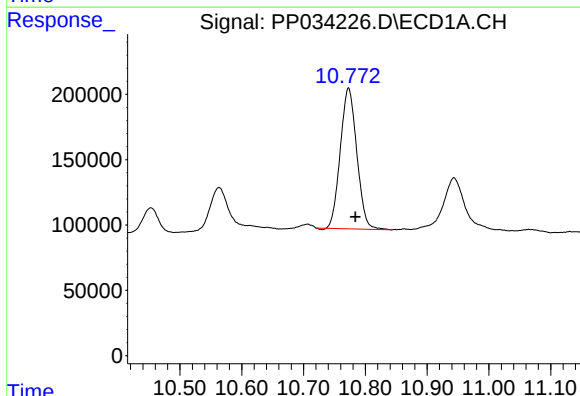


#2 Decachlorobiphenyl

R.T.: 10.773 min
Delta R.T.: -0.011 min
Response: 2000570
Conc: 25.49 ng/ml

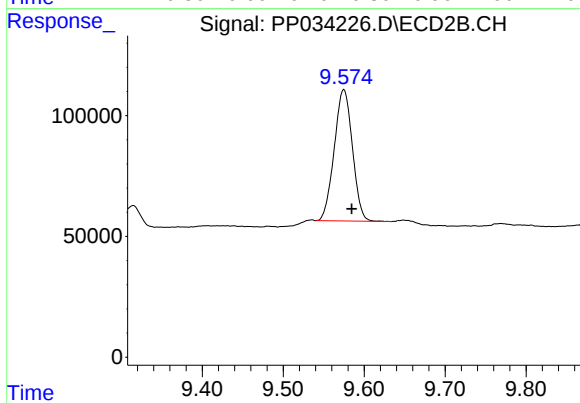

#2 Decachlorobiphenyl

R.T.: 9.575 min
Delta R.T.: -0.010 min
Response: 848471
Conc: 32.15 ng/ml

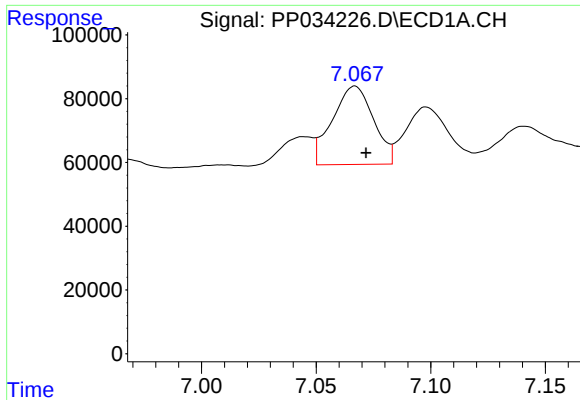


#26 AR-1254-1

R.T.: 7.067 min
Delta R.T.: -0.005 min
Response: 306960
Conc: 112.15 ng/ml m

Instrument :
ECD_P
ClientSampleId :
X127-2C


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:43 PM

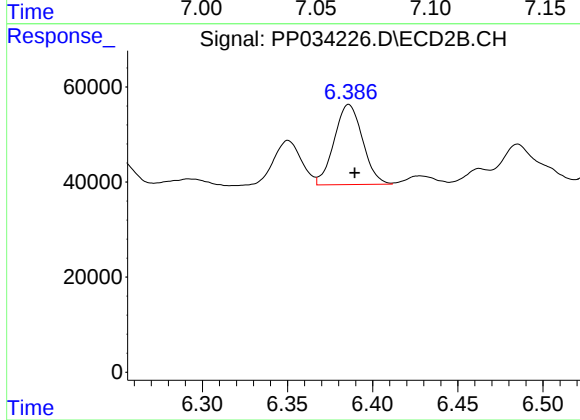


#26 AR-1254-1

R.T.: 6.386 min
Delta R.T.: -0.004 min
Response: 195542
Conc: 116.61 ng/ml

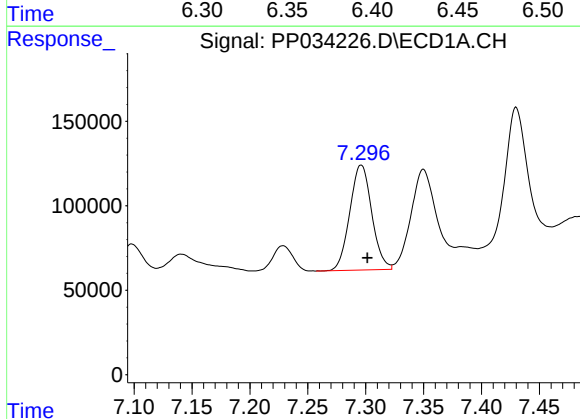


#27 AR-1254-2

R.T.: 7.296 min
Delta R.T.: -0.005 min
Response: 821885
Conc: 197.38 ng/ml

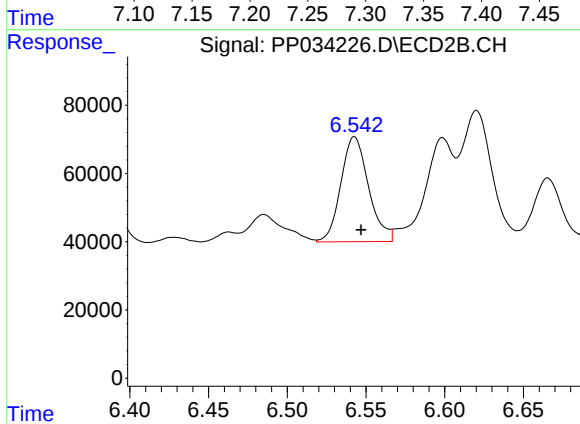

#27 AR-1254-2

R.T.: 6.543 min
Delta R.T.: -0.004 min
Response: 377607
Conc: 260.39 ng/ml

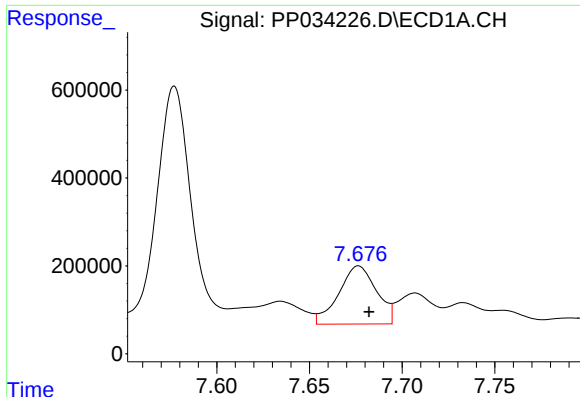


#28 AR-1254-3

R.T.: 7.676 min
Delta R.T.: -0.006 min
Response: 1877100
Conc: 432.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-2C


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:43 PM

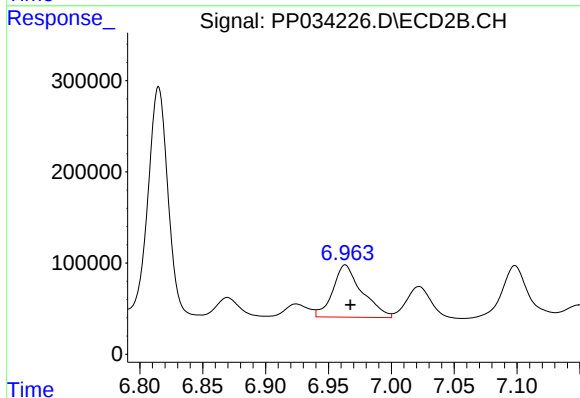


#28 AR-1254-3

R.T.: 6.963 min
Delta R.T.: -0.004 min
Response: 923675
Conc: 403.33 ng/ml

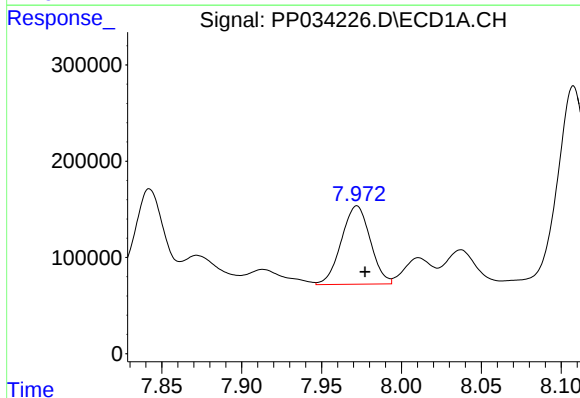


#29 AR-1254-4

R.T.: 7.972 min
Delta R.T.: -0.005 min
Response: 1025863
Conc: 353.36 ng/ml

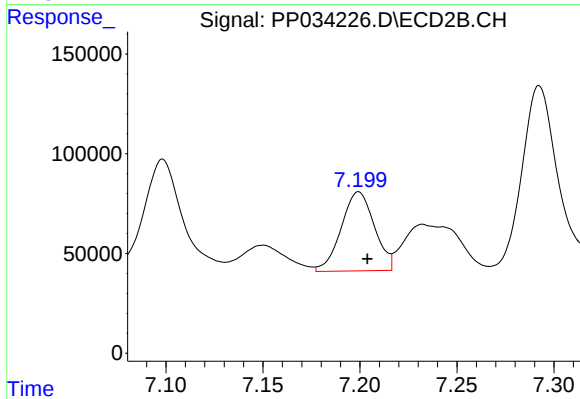

#29 AR-1254-4

R.T.: 7.199 min
Delta R.T.: -0.004 min
Response: 472674
Conc: 395.29 ng/ml

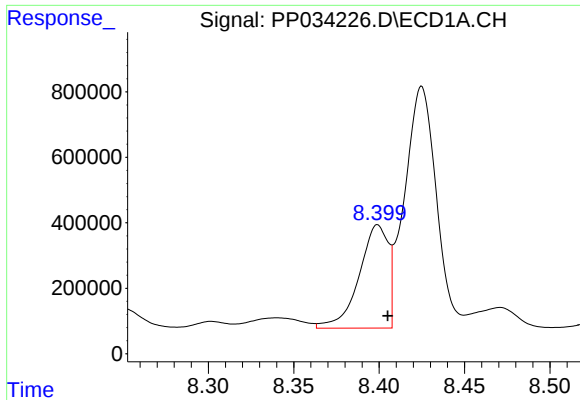


#30 AR-1254-5

R.T.: 8.399 min
Delta R.T.: -0.006 min
Response: 3761301
Conc: 1126.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-2C

Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:43 PM

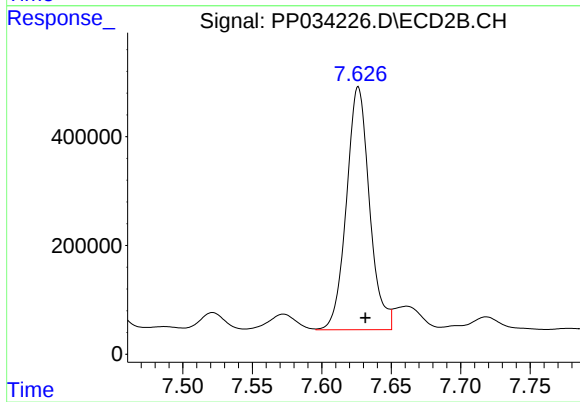

#30 AR-1254-5

R.T.: 7.626 min
Delta R.T.: -0.005 min
Response: 5164366
Conc: 2796.91 ng/ml