

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032221\
 Data File : PP034228.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Mar 2021 18:54
 Operator : DD\AJ
 Sample : M1660-10
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-3C

Manual Integrations
 APPROVED

Ankita
 3/23/2021 1:38:45 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 02:04:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.849	4.261	1315805	769859	15.663	17.397
2) SA Decachlor...	10.773	9.575	1035258	427829	13.192	16.212
Target Compounds						
26) L6 AR-1254-1	7.067	6.386	343665	187856	125.564m	112.027
27) L6 AR-1254-2	7.296	6.543	732634	321250	175.943	221.524 #
28) L6 AR-1254-3	7.676	6.964	1249904	793190	287.783	346.352
29) L6 AR-1254-4	7.971	7.200	734849	332976	253.122	278.466
30) L6 AR-1254-5	8.399	7.627	2531954	4144955	758.468	2244.816 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032221\
Data File : PP034228.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Mar 2021 18:54
Operator : DD\AJ
Sample : M1660-10
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
X127-3C


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:45 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 02:04:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

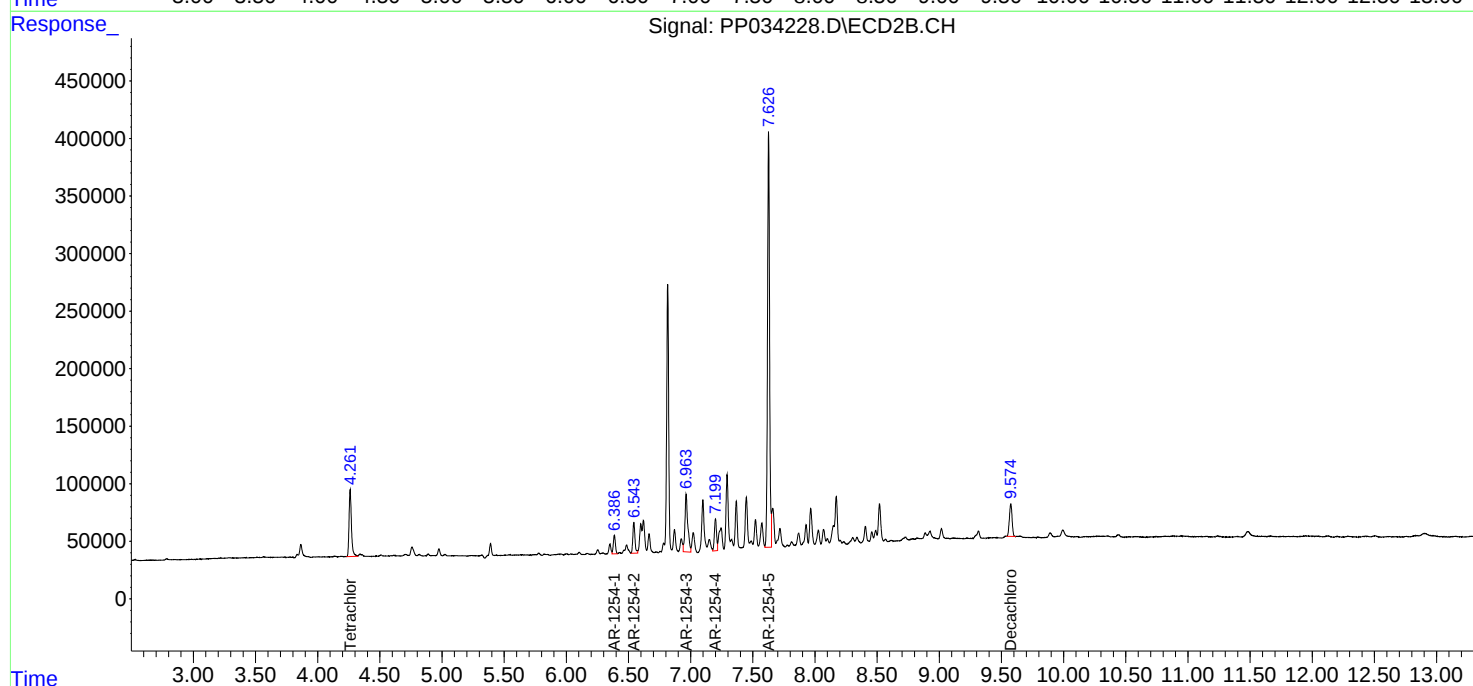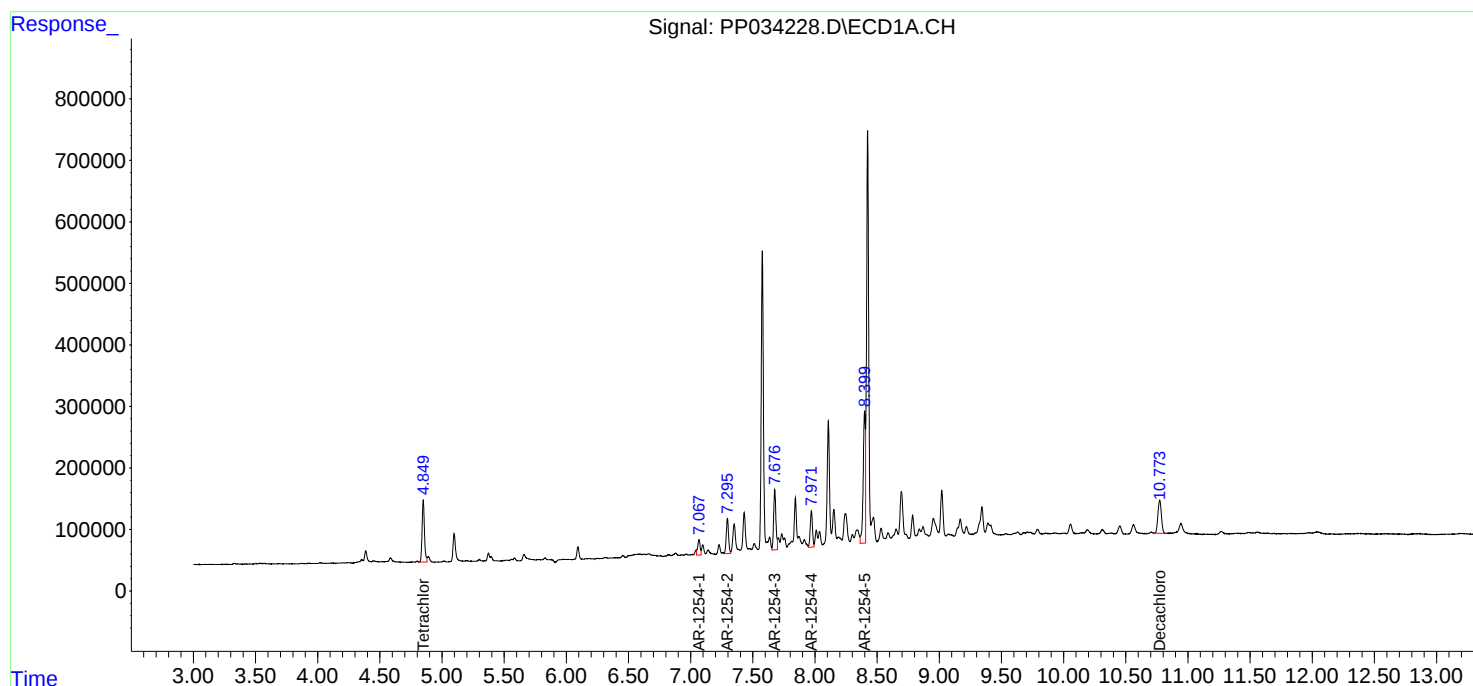

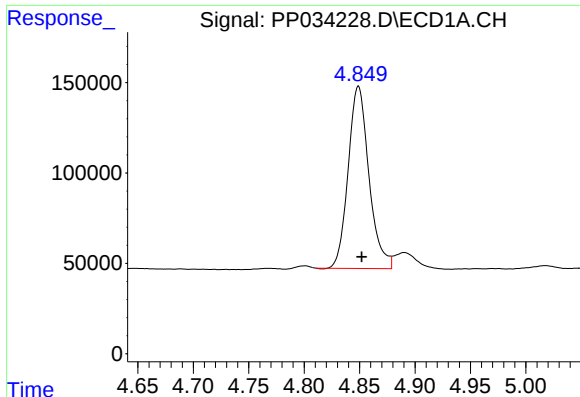


#1 Tetrachloro-m-xylene

R.T.: 4.849 min
Delta R.T.: -0.003 min
Response: 1315805
Conc: 15.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-3C


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:45 PM

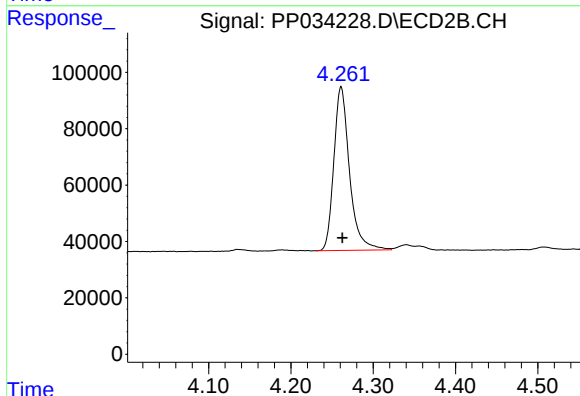


#1 Tetrachloro-m-xylene

R.T.: 4.261 min
Delta R.T.: -0.002 min
Response: 769859
Conc: 17.40 ng/ml

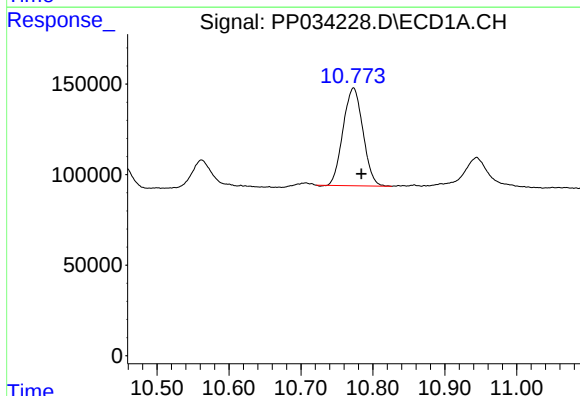


#2 Decachlorobiphenyl

R.T.: 10.773 min
Delta R.T.: -0.011 min
Response: 1035258
Conc: 13.19 ng/ml

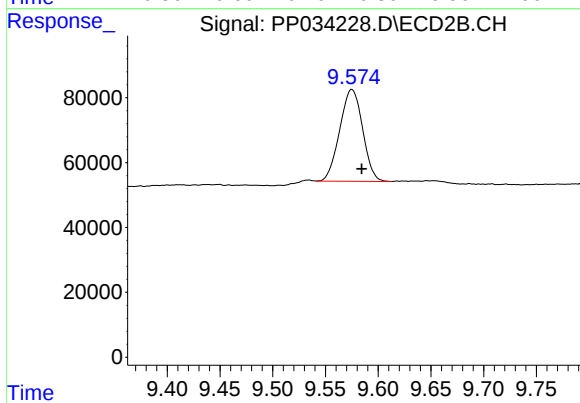

#2 Decachlorobiphenyl

R.T.: 9.575 min
Delta R.T.: -0.010 min
Response: 427829
Conc: 16.21 ng/ml

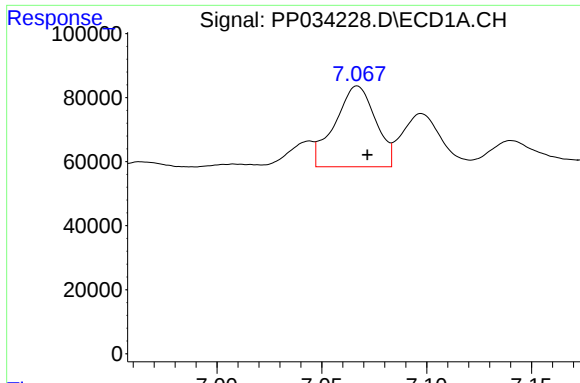


#26 AR-1254-1

R.T.: 7.067 min
Delta R.T.: -0.005 min
Response: 343665
Conc: 125.56 ng/ml m

Instrument :
ECD_P
ClientSampleId :
X127-3C


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:45 PM

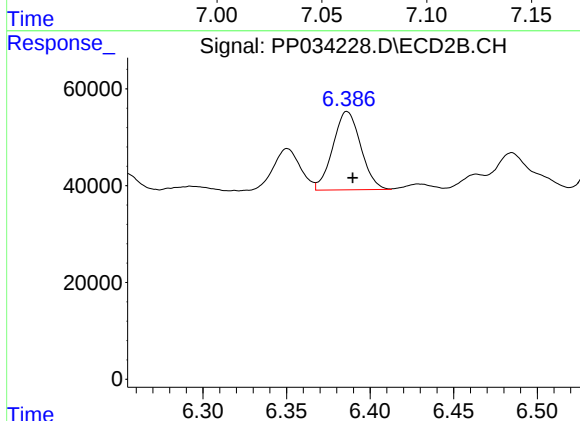


#26 AR-1254-1

R.T.: 6.386 min
Delta R.T.: -0.003 min
Response: 187856
Conc: 112.03 ng/ml

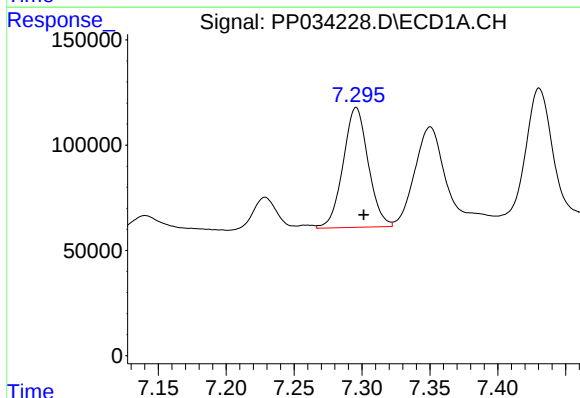


#27 AR-1254-2

R.T.: 7.296 min
Delta R.T.: -0.006 min
Response: 732634
Conc: 175.94 ng/ml

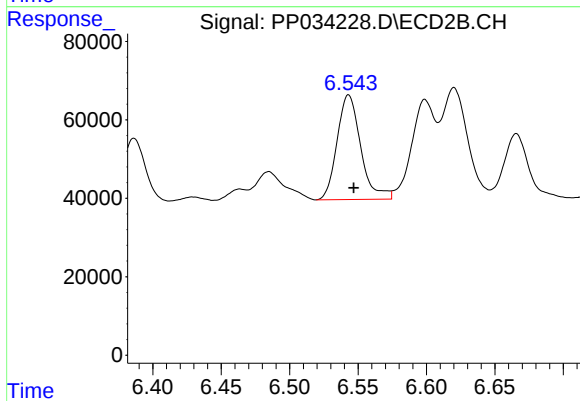

#27 AR-1254-2

R.T.: 6.543 min
Delta R.T.: -0.004 min
Response: 321250
Conc: 221.52 ng/ml

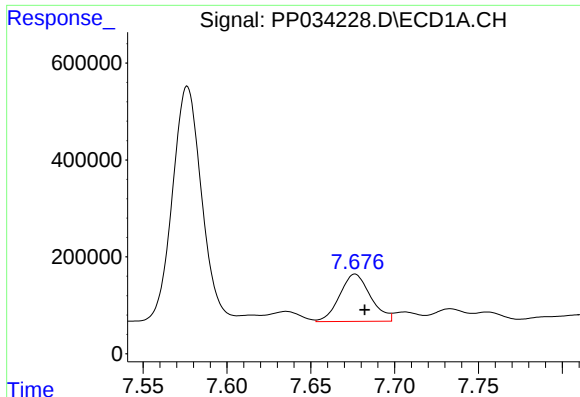


#28 AR-1254-3

R.T.: 7.676 min
Delta R.T.: -0.006 min
Response: 1249904
Conc: 287.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-3C


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:45 PM

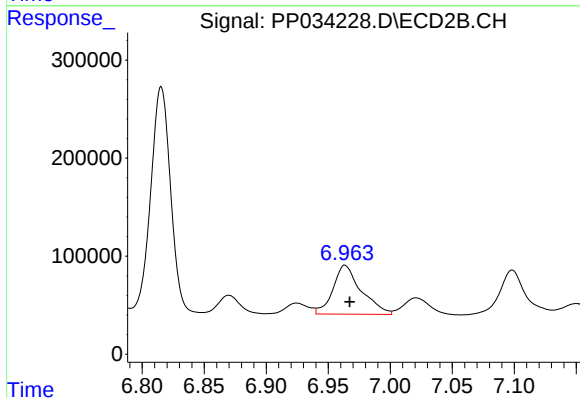


#28 AR-1254-3

R.T.: 6.964 min
Delta R.T.: -0.004 min
Response: 793190
Conc: 346.35 ng/ml

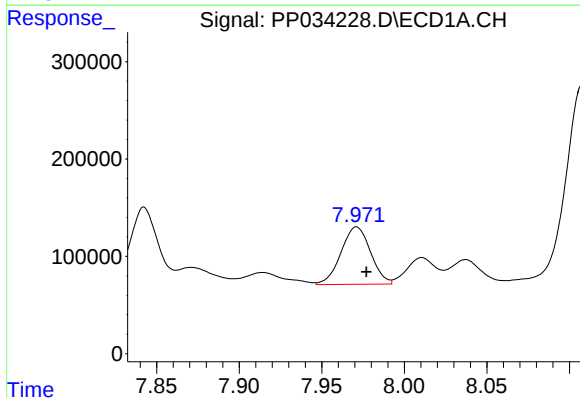


#29 AR-1254-4

R.T.: 7.971 min
Delta R.T.: -0.006 min
Response: 734849
Conc: 253.12 ng/ml

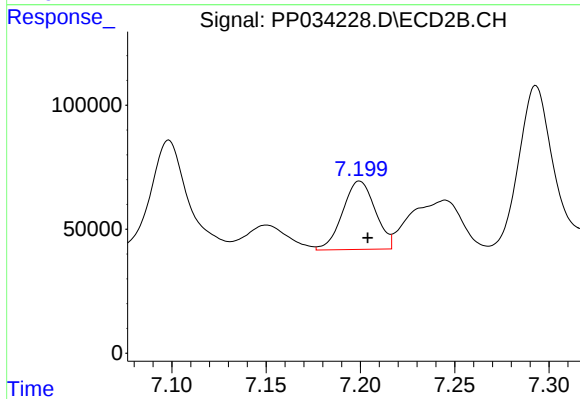

#29 AR-1254-4

R.T.: 7.200 min
Delta R.T.: -0.004 min
Response: 332976
Conc: 278.47 ng/ml

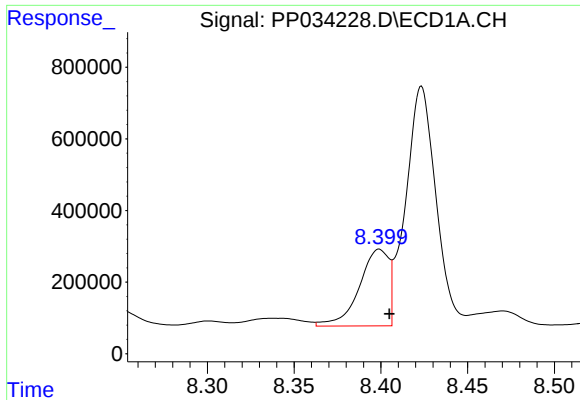


#30 AR-1254-5

R.T.: 8.399 min
Delta R.T.: -0.006 min
Response: 2531954
Conc: 758.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-3C

Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:45 PM

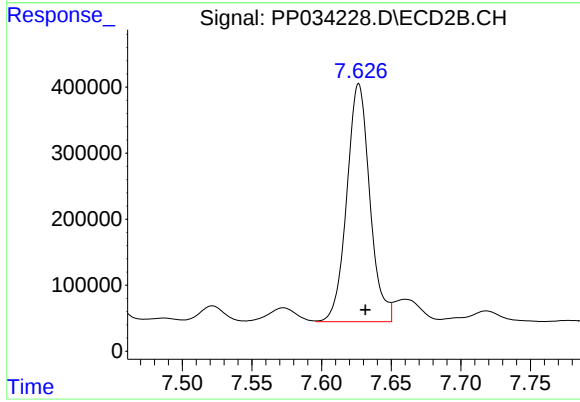

#30 AR-1254-5

R.T.: 7.627 min
Delta R.T.: -0.005 min
Response: 4144955
Conc: 2244.82 ng/ml