

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032221\
 Data File : PP034229.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Mar 2021 19:11
 Operator : DD\AJ
 Sample : M1660-12
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-4B

Manual Integrations
 APPROVED

Ankita
 3/23/2021 1:38:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 02:05:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.849	4.261	1594174	903835	18.977	20.424
2) SA Decachlor...	10.773	9.575	1418339	576480	18.073	21.845m
Target Compounds						
26) L6 AR-1254-1	7.067	6.387	9031423	5290308	3299.784	3154.840
27) L6 AR-1254-2	7.296	6.543	21445200	8334682	5150.092	5747.341
28) L6 AR-1254-3	7.676	6.964	30376894	15700513	6994.109	6855.747
29) L6 AR-1254-4	7.972	7.200	25813336	10051700	8891.521	8406.161
30) L6 AR-1254-5	8.399	7.627	48861520	32694609	14636.867	17706.679

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032221\
Data File : PP034229.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Mar 2021 19:11
Operator : DD\AJ
Sample : M1660-12
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
X127-4B


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 02:05:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

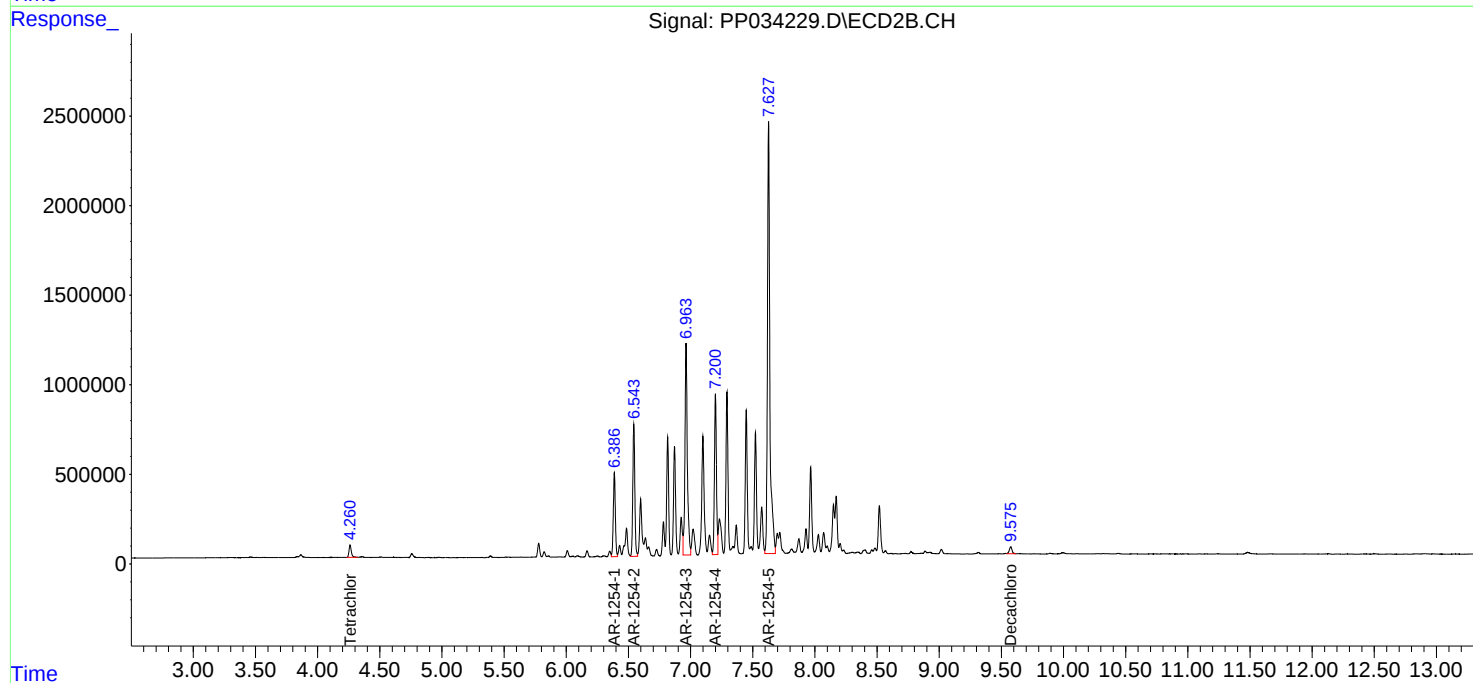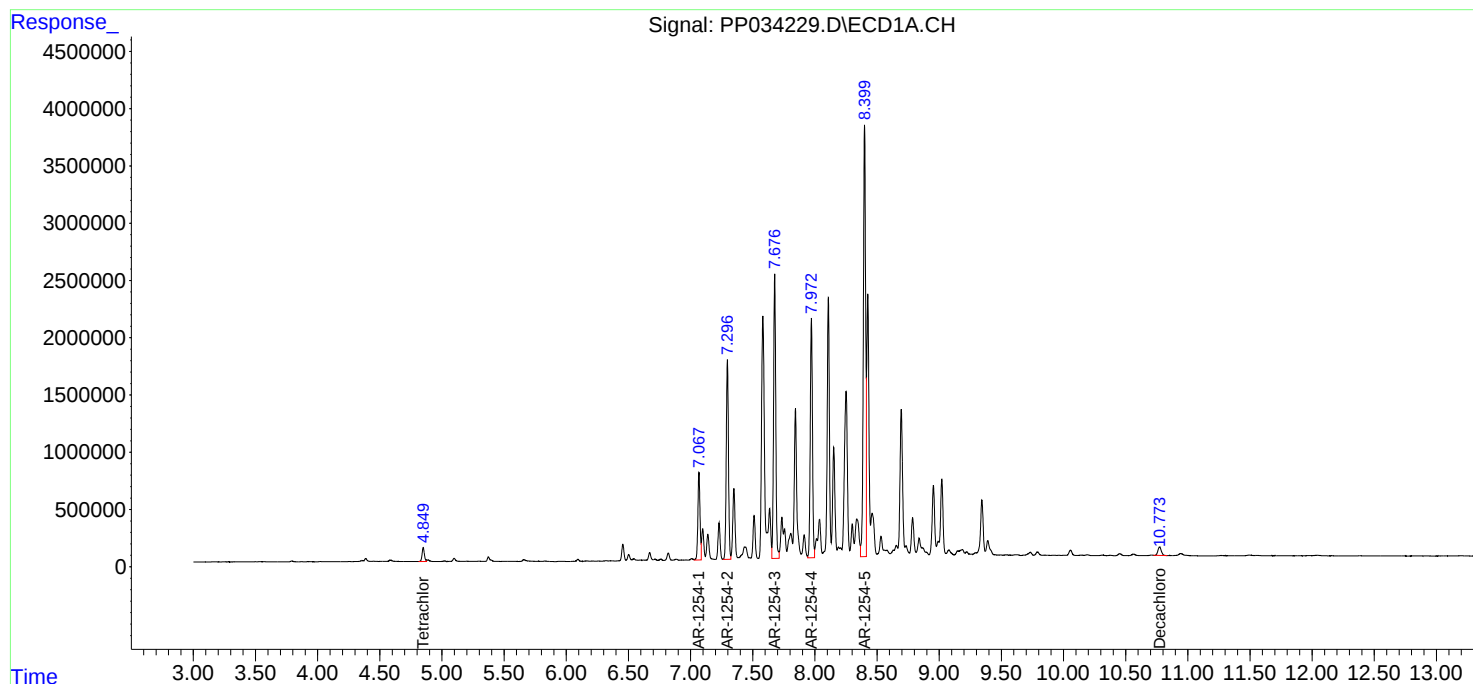

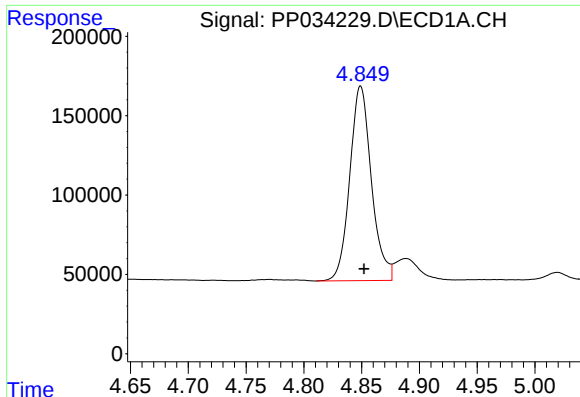


#1 Tetrachloro-m-xylene

R.T.: 4.849 min
Delta R.T.: -0.003 min
Response: 1594174
Conc: 18.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-4B


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:47 PM

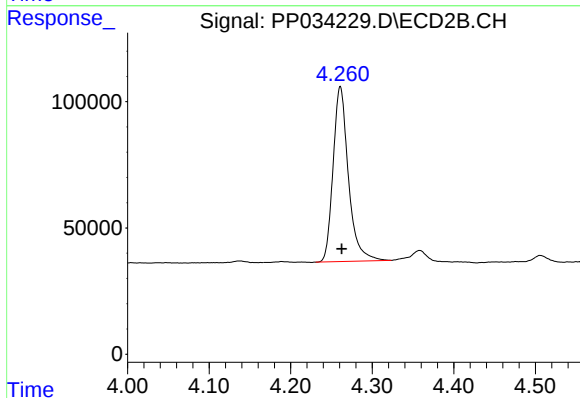


#1 Tetrachloro-m-xylene

R.T.: 4.261 min
Delta R.T.: -0.002 min
Response: 903835
Conc: 20.42 ng/ml

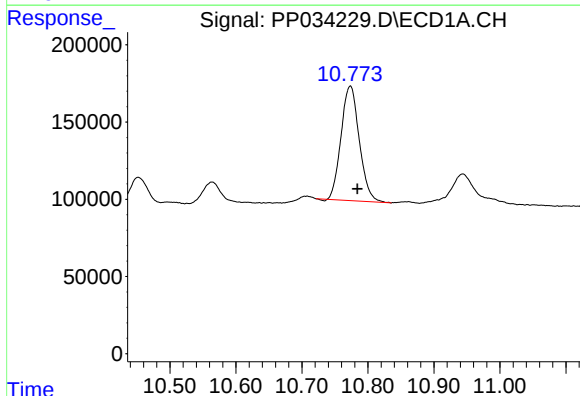


#2 Decachlorobiphenyl

R.T.: 10.773 min
Delta R.T.: -0.011 min
Response: 1418339
Conc: 18.07 ng/ml

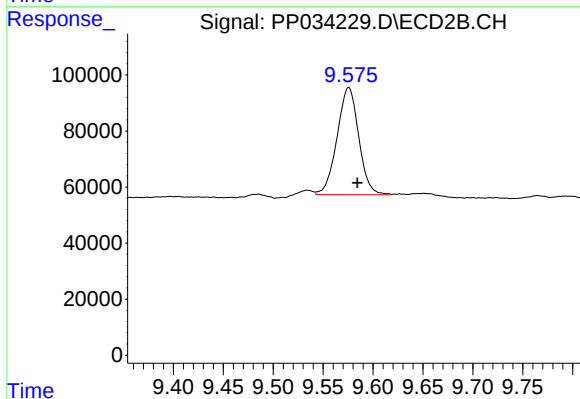

#2 Decachlorobiphenyl

R.T.: 9.575 min
Delta R.T.: -0.009 min
Response: 576480
Conc: 21.85 ng/ml m

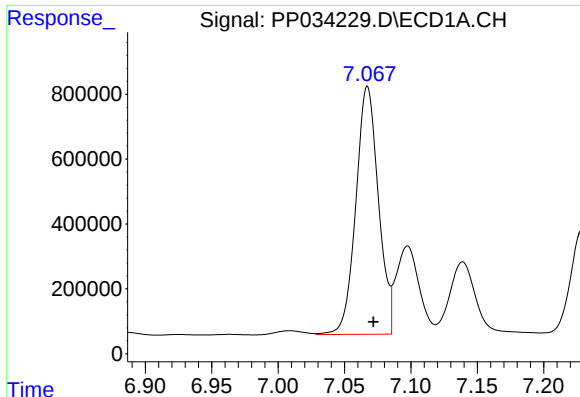


#26 AR-1254-1

R.T.: 7.067 min
Delta R.T.: -0.004 min
Response: 9031423
Conc: 3299.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-4B


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:47 PM

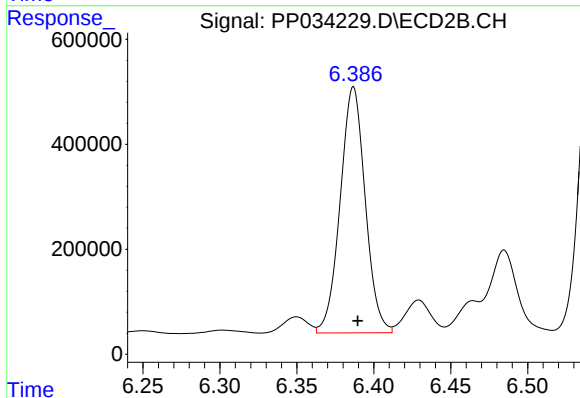


#26 AR-1254-1

R.T.: 6.387 min
Delta R.T.: -0.003 min
Response: 5290308
Conc: 3154.84 ng/ml

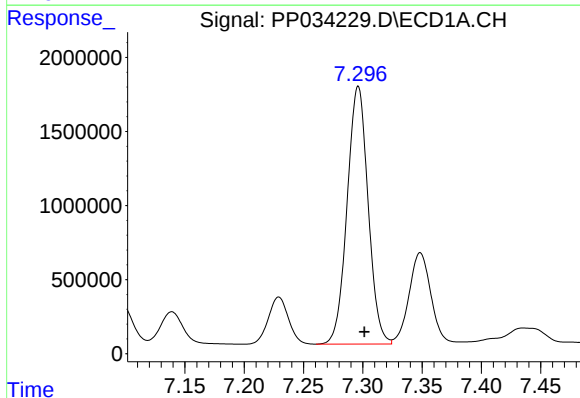


#27 AR-1254-2

R.T.: 7.296 min
Delta R.T.: -0.005 min
Response: 21445200
Conc: 5150.09 ng/ml

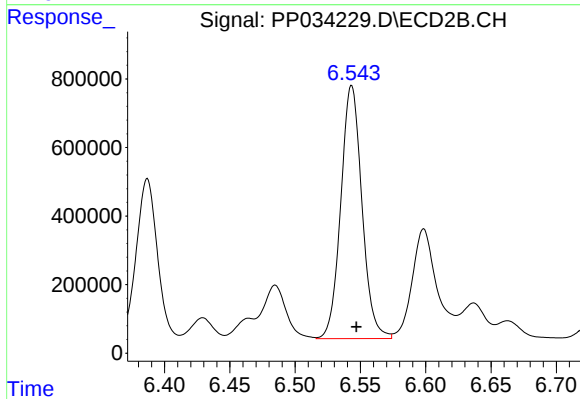

#27 AR-1254-2

R.T.: 6.543 min
Delta R.T.: -0.004 min
Response: 8334682
Conc: 5747.34 ng/ml

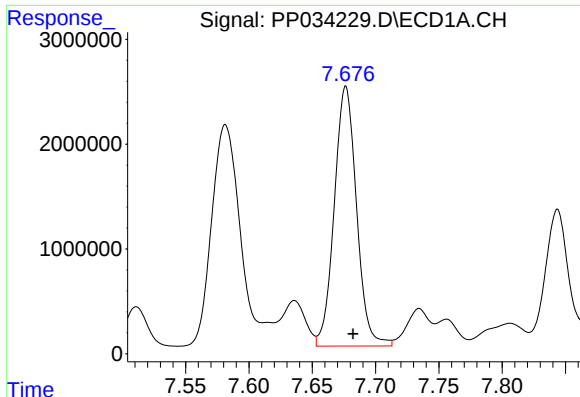


#28 AR-1254-3

R.T.: 7.676 min
Delta R.T.: -0.006 min
Response: 30376894
Conc: 6994.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-4B


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:47 PM

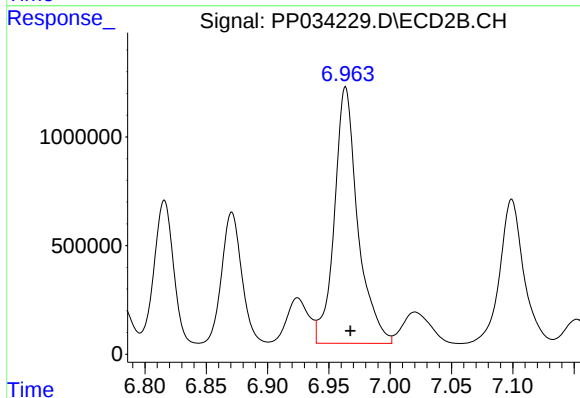


#28 AR-1254-3

R.T.: 6.964 min
Delta R.T.: -0.004 min
Response: 15700513
Conc: 6855.75 ng/ml

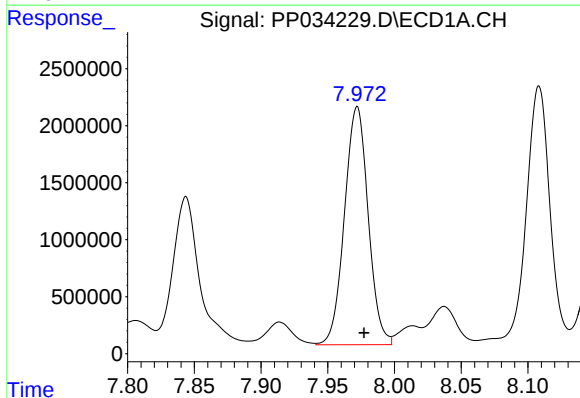


#29 AR-1254-4

R.T.: 7.972 min
Delta R.T.: -0.005 min
Response: 25813336
Conc: 8891.52 ng/ml

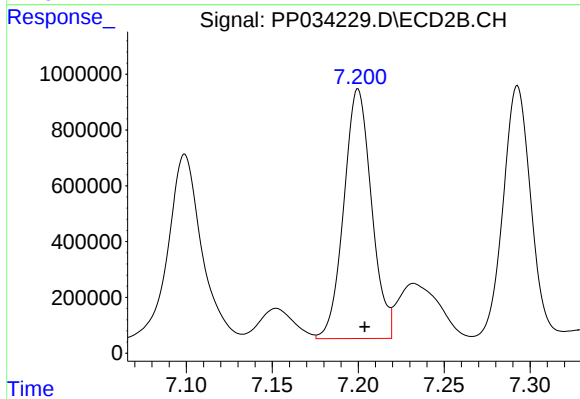

#29 AR-1254-4

R.T.: 7.200 min
Delta R.T.: -0.004 min
Response: 10051700
Conc: 8406.16 ng/ml

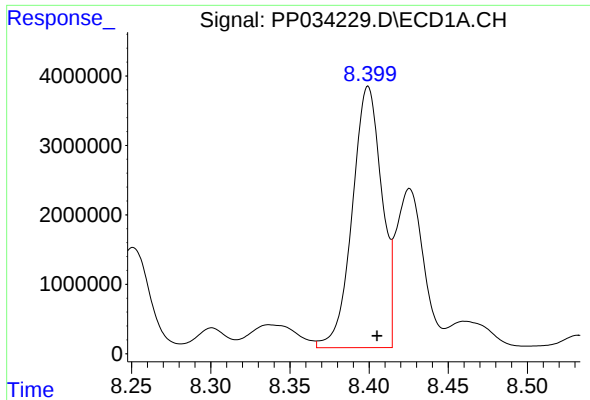


#30 AR-1254-5

R.T.: 8.399 min
Delta R.T.: -0.006 min
Response: 48861520
Conc: 14636.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-4B

Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:47 PM

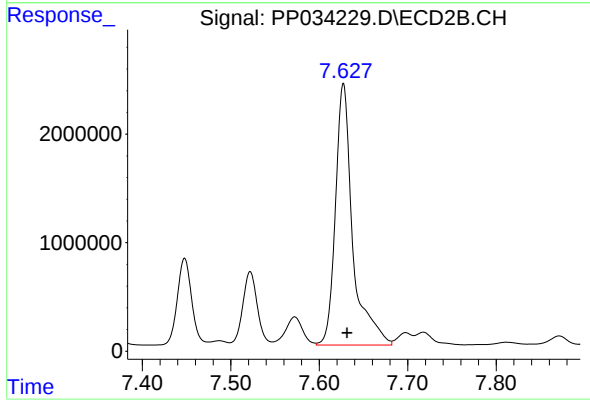

#30 AR-1254-5

R.T.: 7.627 min
Delta R.T.: -0.004 min
Response: 32694609
Conc: 17706.68 ng/ml