

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032221\
 Data File : PP034231.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Mar 2021 19:45
 Operator : DD\AJ
 Sample : M1660-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-5B

Manual Integrations
 APPROVED

Ankita
 3/23/2021 1:38:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 02:06:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.849	4.261	1192931	695950	14.200m	15.727
2) SA Decachlor...	10.774	9.576	1105755	406298	14.090	15.396
Target Compounds						
26) L6 AR-1254-1	7.067	6.387	142224	81761	51.964m	48.758
27) L6 AR-1254-2	7.297	6.542	308315	102784	74.042	70.876
28) L6 AR-1254-3	7.677	6.963	506939	291206	116.720	127.157
29) L6 AR-1254-4	7.971	7.200	294802	153951	101.546	128.748 #
30) L6 AR-1254-5	8.401	7.627	600010	6046568	179.738m	3274.688 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032221\
Data File : PP034231.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Mar 2021 19:45
Operator : DD\AJ
Sample : M1660-15
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
X127-5B


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 02:06:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

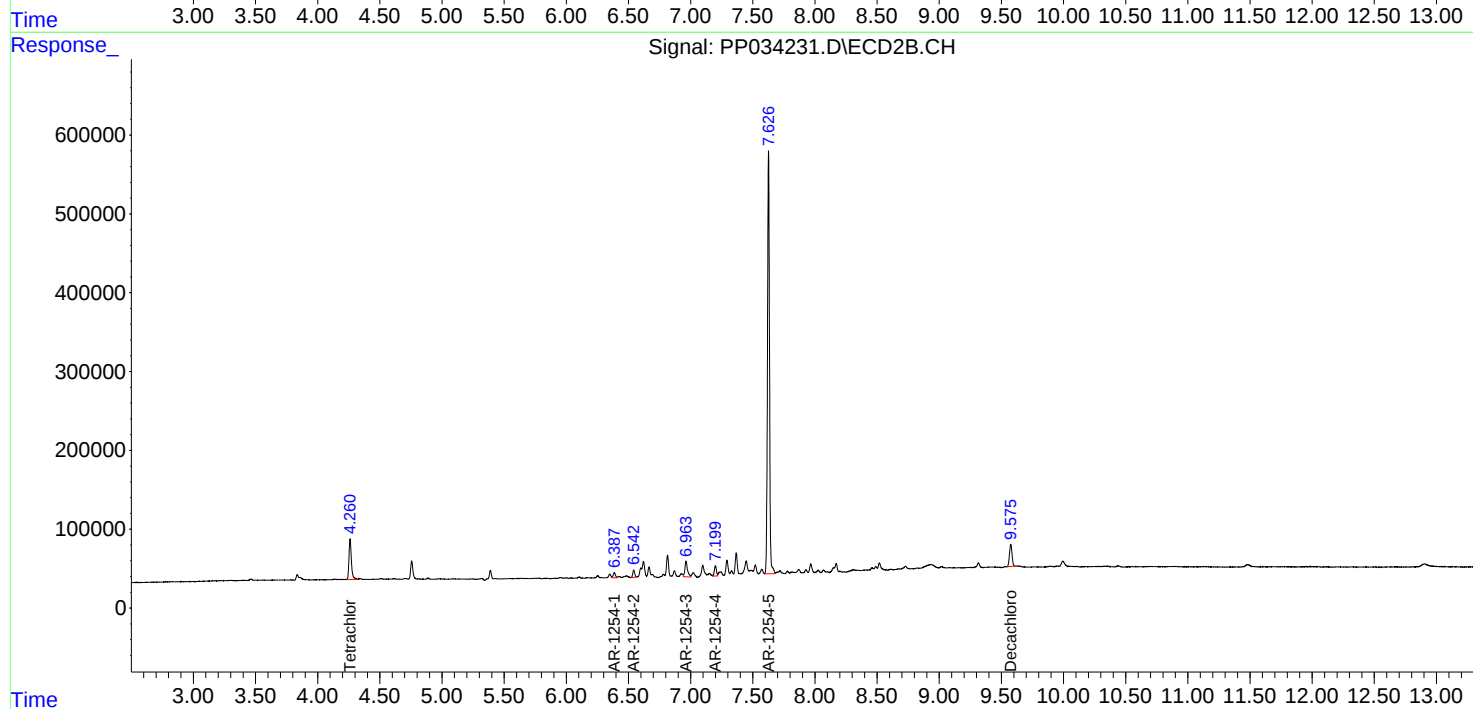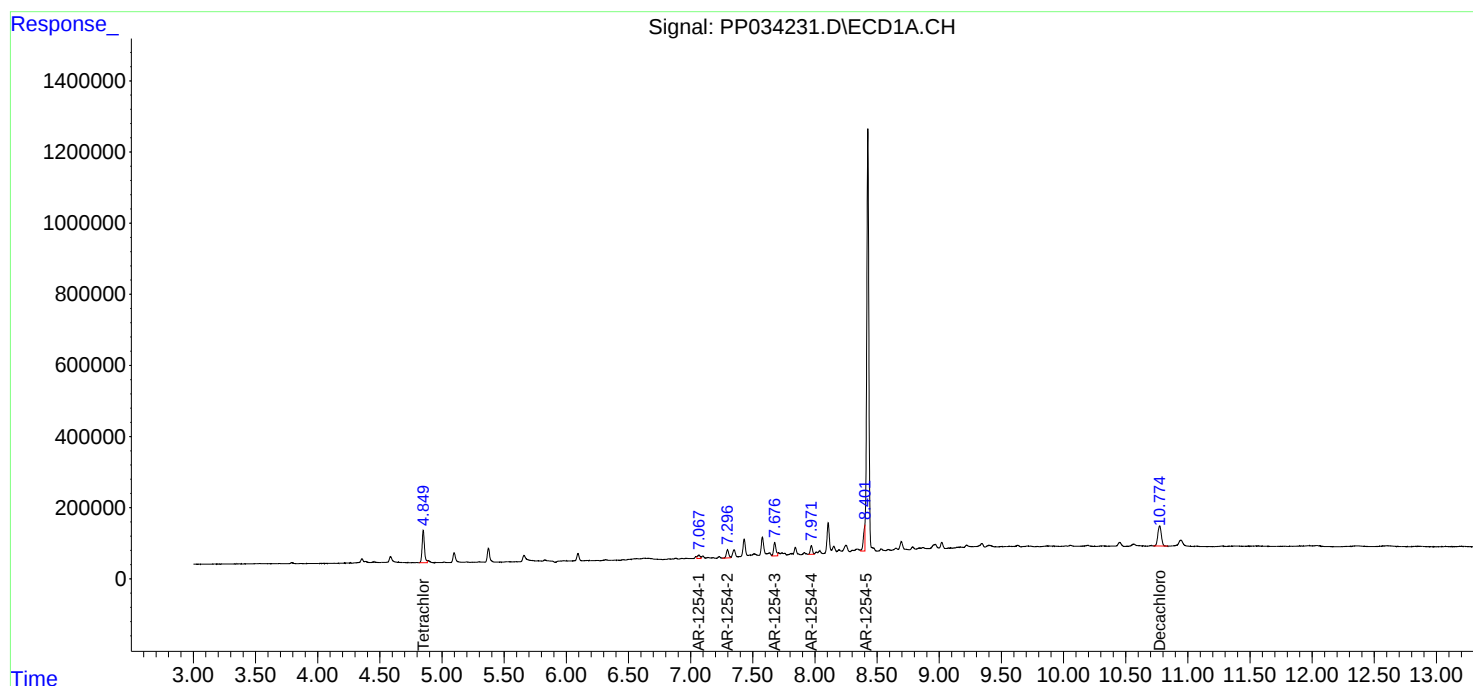

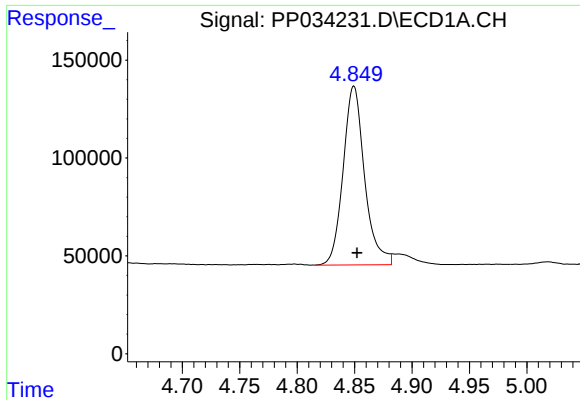


#1 Tetrachloro-m-xylene

R.T.: 4.849 min
Delta R.T.: -0.003 min
Response: 1192931
Conc: 14.20 ng/ml m

Instrument :
ECD_P
ClientSampleId :
X127-5B


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:49 PM

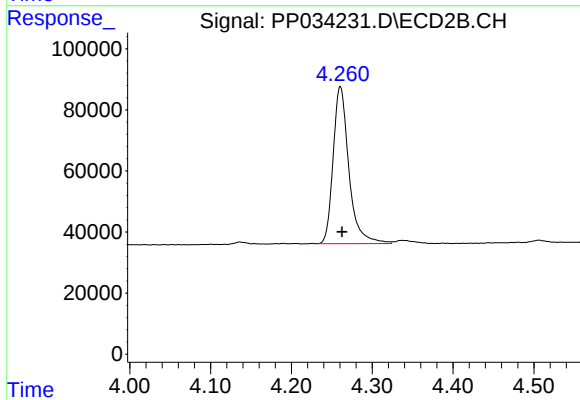


#1 Tetrachloro-m-xylene

R.T.: 4.261 min
Delta R.T.: -0.002 min
Response: 695950
Conc: 15.73 ng/ml

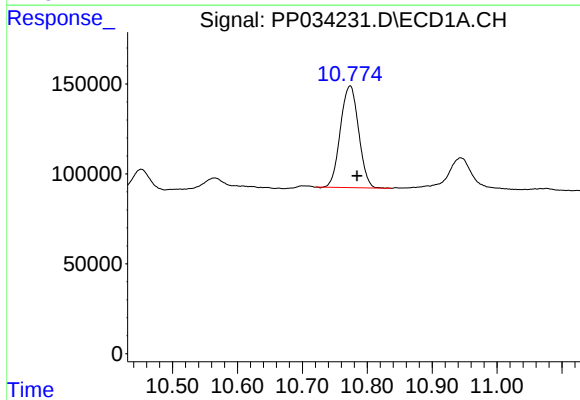


#2 Decachlorobiphenyl

R.T.: 10.774 min
Delta R.T.: -0.010 min
Response: 1105755
Conc: 14.09 ng/ml

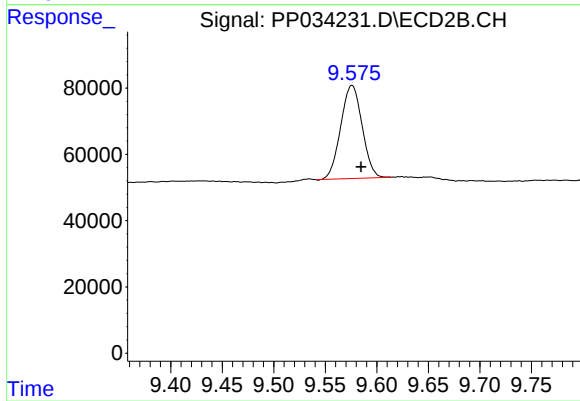

#2 Decachlorobiphenyl

R.T.: 9.576 min
Delta R.T.: -0.009 min
Response: 406298
Conc: 15.40 ng/ml

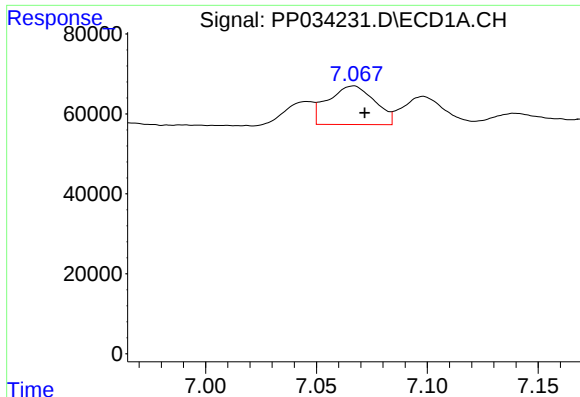


#26 AR-1254-1

R.T.: 7.067 min
Delta R.T.: -0.005 min
Response: 142224
Conc: 51.96 ng/ml m

Instrument :
ECD_P
ClientSampleId :
X127-5B


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:49 PM

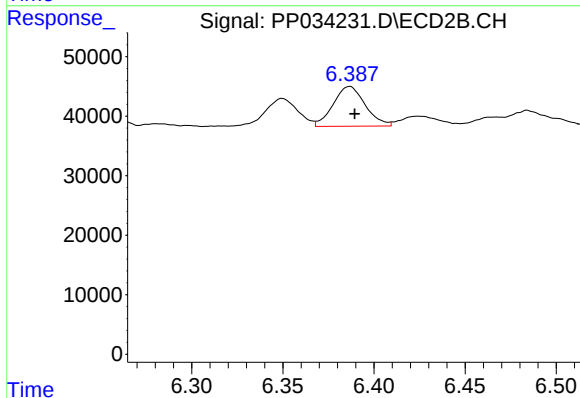


#26 AR-1254-1

R.T.: 6.387 min
Delta R.T.: -0.003 min
Response: 81761
Conc: 48.76 ng/ml

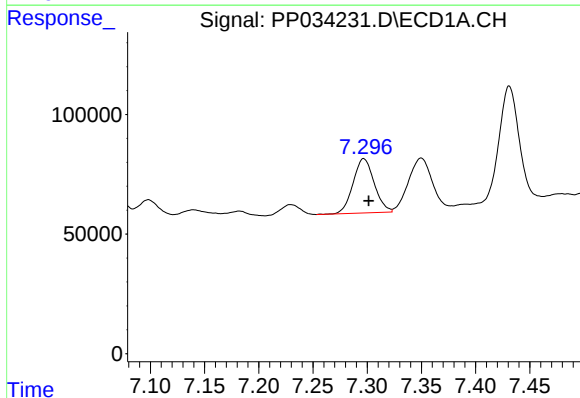


#27 AR-1254-2

R.T.: 7.297 min
Delta R.T.: -0.005 min
Response: 308315
Conc: 74.04 ng/ml

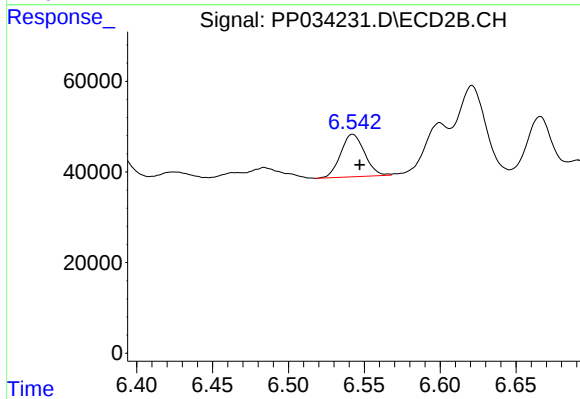

#27 AR-1254-2

R.T.: 6.542 min
Delta R.T.: -0.005 min
Response: 102784
Conc: 70.88 ng/ml

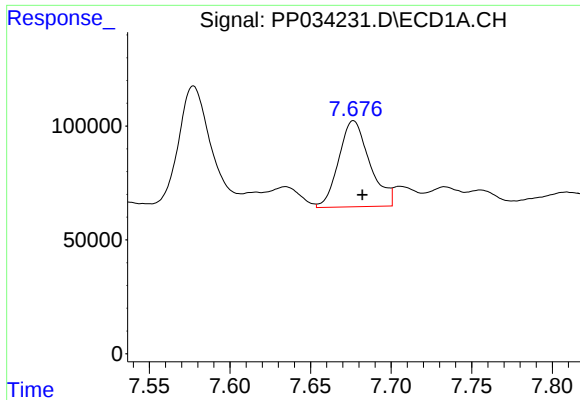


#28 AR-1254-3

R.T.: 7.677 min
Delta R.T.: -0.005 min
Response: 506939
Conc: 116.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-5B


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:49 PM

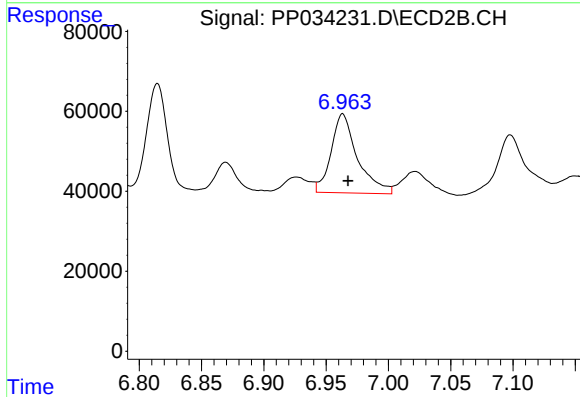


#28 AR-1254-3

R.T.: 6.963 min
Delta R.T.: -0.004 min
Response: 291206
Conc: 127.16 ng/ml

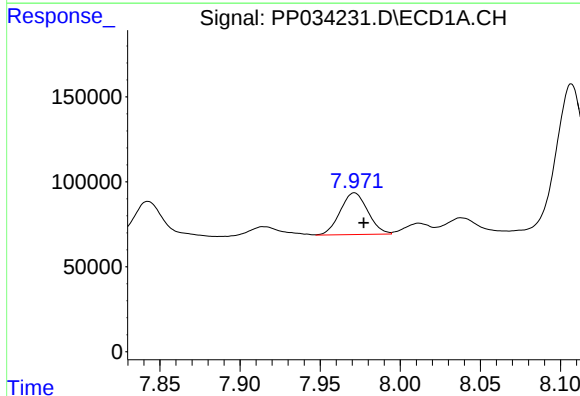


#29 AR-1254-4

R.T.: 7.971 min
Delta R.T.: -0.006 min
Response: 294802
Conc: 101.55 ng/ml

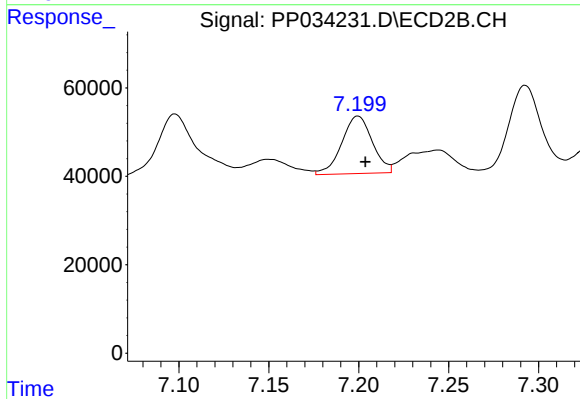

#29 AR-1254-4

R.T.: 7.200 min
Delta R.T.: -0.004 min
Response: 153951
Conc: 128.75 ng/ml

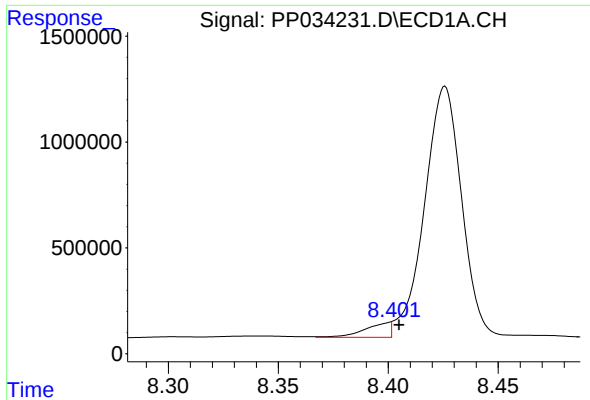


#30 AR-1254-5

R.T.: 8.401 min
Delta R.T.: -0.004 min
Response: 600010
Conc: 179.74 ng/ml m

Instrument :
ECD_P
ClientSampleId :
X127-5B

Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:49 PM

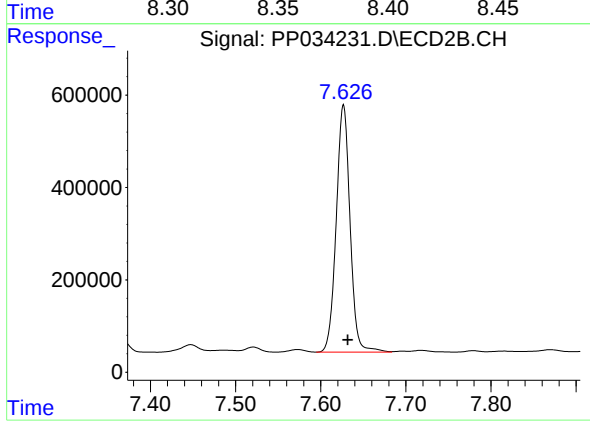

#30 AR-1254-5

R.T.: 7.627 min
Delta R.T.: -0.005 min
Response: 6046568
Conc: 3274.69 ng/ml