

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032221\
 Data File : PP034233.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Mar 2021 20:18
 Operator : DD\AJ
 Sample : M1660-18
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-6B

Manual Integrations
 APPROVED

Ankita
 3/23/2021 1:38:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 02:07:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.848	4.261	1150252	642402	13.692	14.517
2) SA Decachlor...	10.771	9.576	832141	319217	10.604	12.097
Target Compounds						
26) L6 AR-1254-1	7.067	6.387	237424	130819	86.747m	78.013
27) L6 AR-1254-2	7.296	6.543	472848	189289	113.555	130.528
28) L6 AR-1254-3	7.676	6.964	766602	483506	176.506	211.126
29) L6 AR-1254-4	7.972	7.200	494181	243341	170.223	203.504
30) L6 AR-1254-5	8.398	7.627	1427721	992855	427.686	537.708 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032221\
Data File : PP034233.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Mar 2021 20:18
Operator : DD\AJ
Sample : M1660-18
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
X127-6B


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 02:07:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

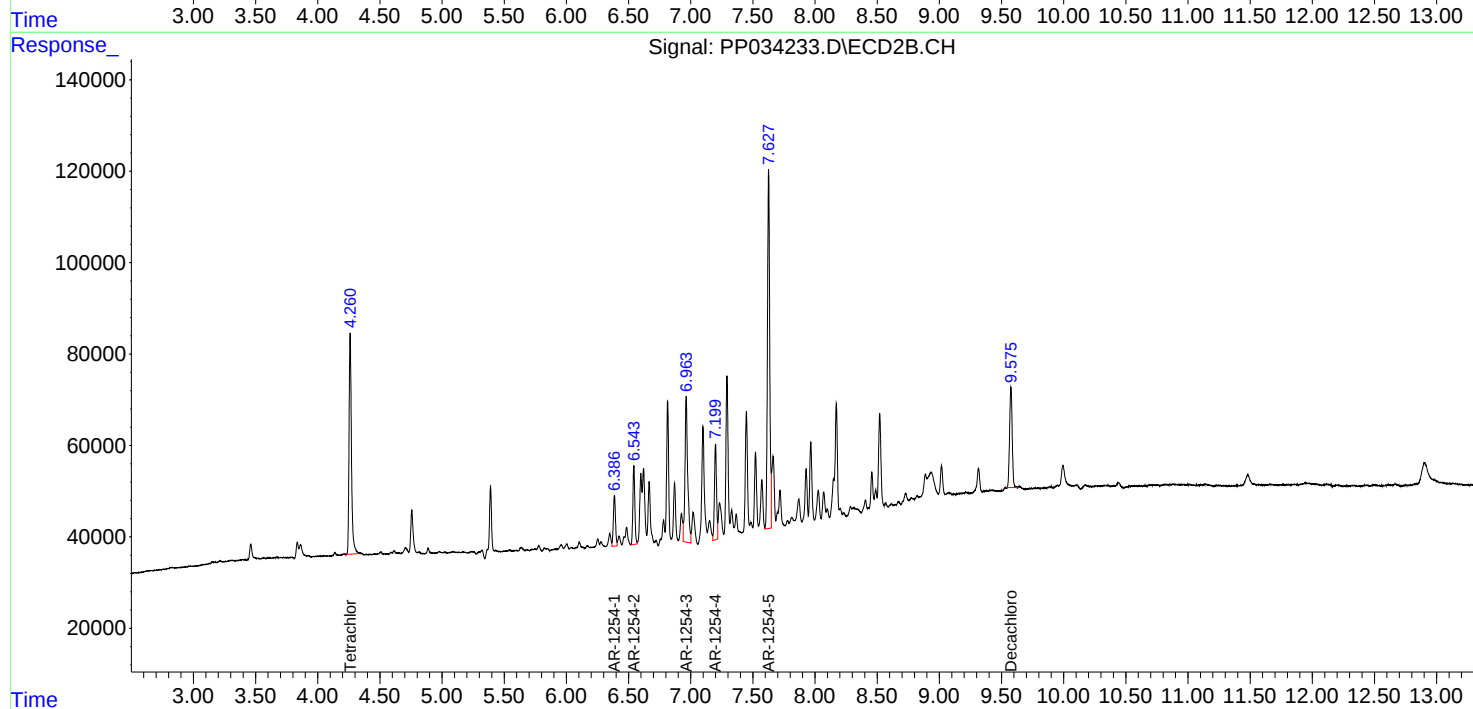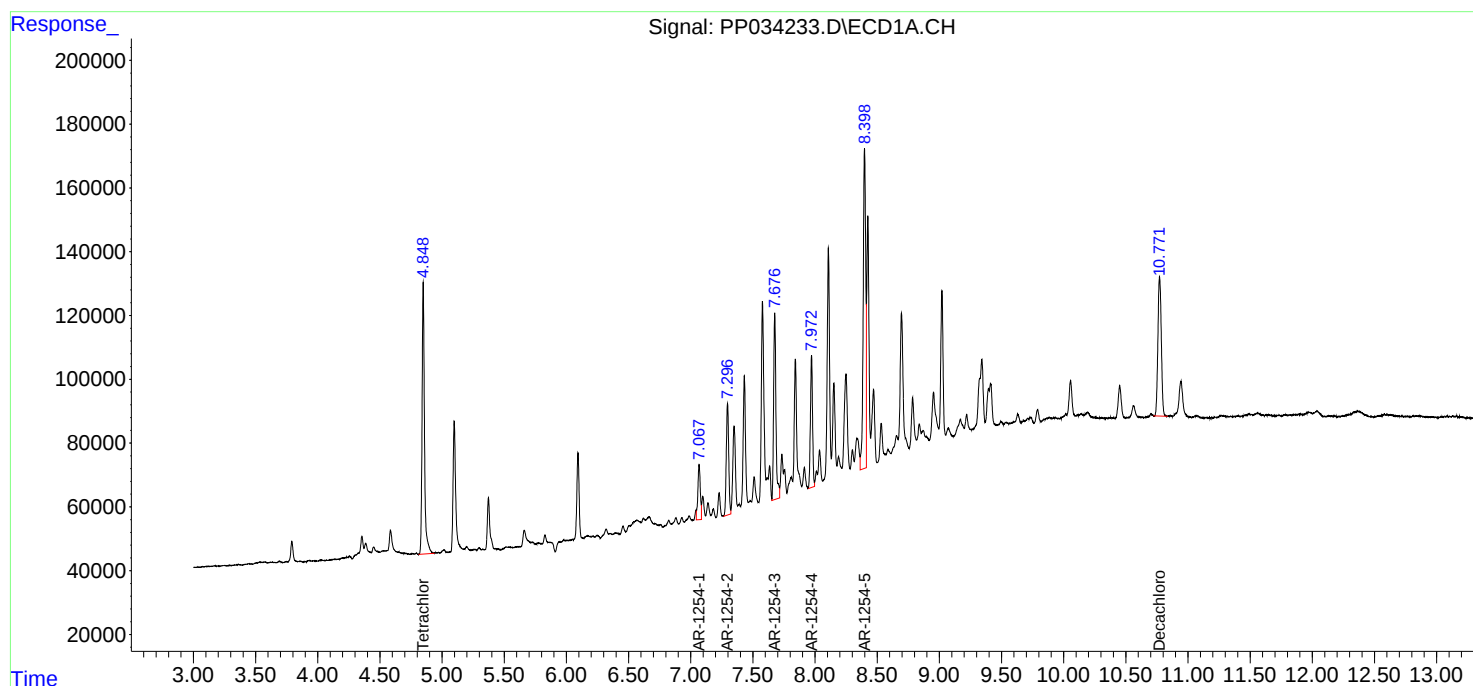

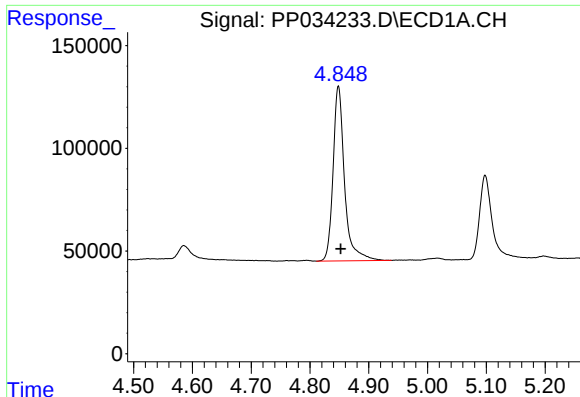


#1 Tetrachloro-m-xylene

R.T.: 4.848 min
Delta R.T.: -0.004 min
Response: 1150252
Conc: 13.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-6B


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:51 PM

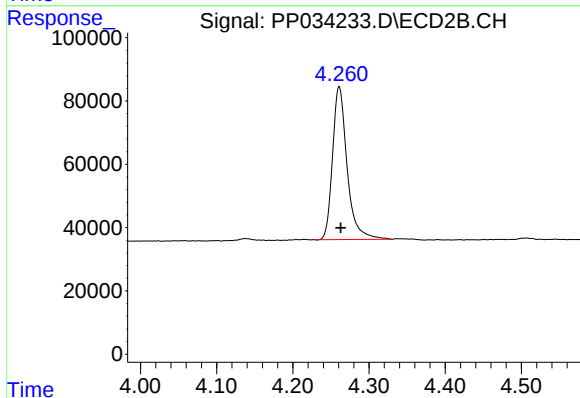


#1 Tetrachloro-m-xylene

R.T.: 4.261 min
Delta R.T.: -0.002 min
Response: 642402
Conc: 14.52 ng/ml

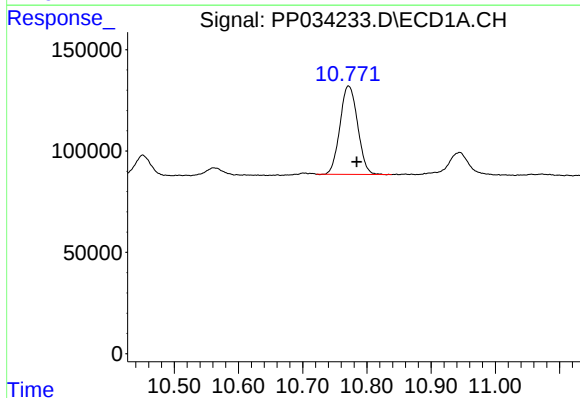


#2 Decachlorobiphenyl

R.T.: 10.771 min
Delta R.T.: -0.013 min
Response: 832141
Conc: 10.60 ng/ml

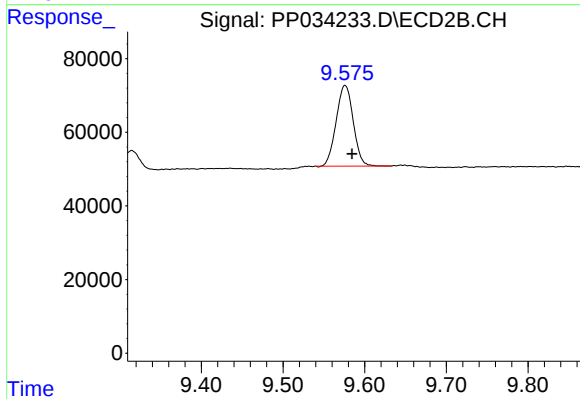

#2 Decachlorobiphenyl

R.T.: 9.576 min
Delta R.T.: -0.009 min
Response: 319217
Conc: 12.10 ng/ml

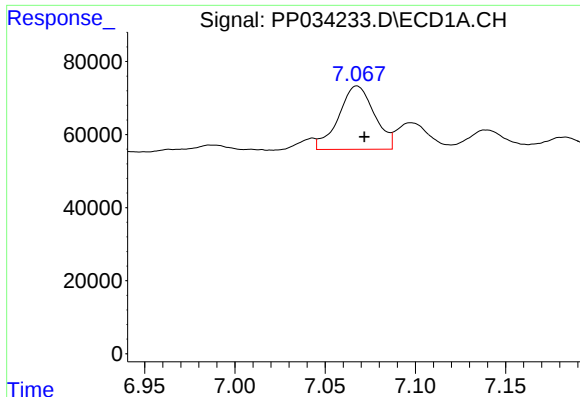


#26 AR-1254-1

R.T.: 7.067 min
Delta R.T.: -0.005 min
Response: 237424
Conc: 86.75 ng/ml m

Instrument :
ECD_P
ClientSampleId :
X127-6B


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:51 PM

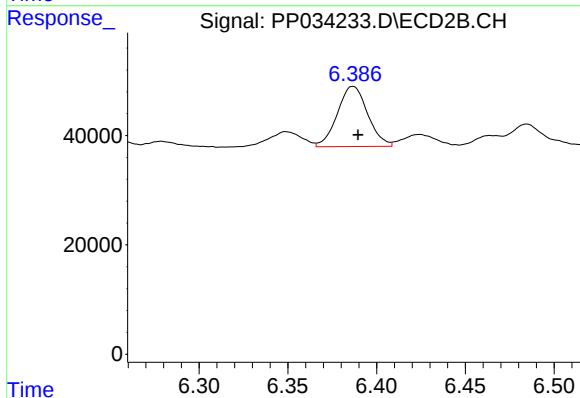


#26 AR-1254-1

R.T.: 6.387 min
Delta R.T.: -0.003 min
Response: 130819
Conc: 78.01 ng/ml

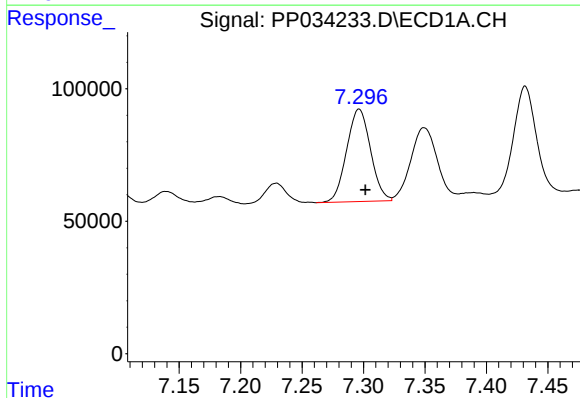


#27 AR-1254-2

R.T.: 7.296 min
Delta R.T.: -0.005 min
Response: 472848
Conc: 113.55 ng/ml

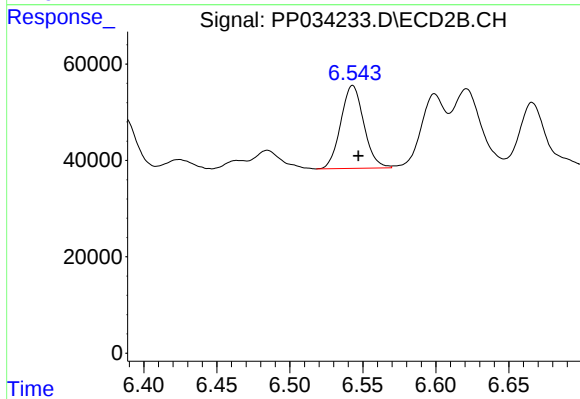

#27 AR-1254-2

R.T.: 6.543 min
Delta R.T.: -0.004 min
Response: 189289
Conc: 130.53 ng/ml

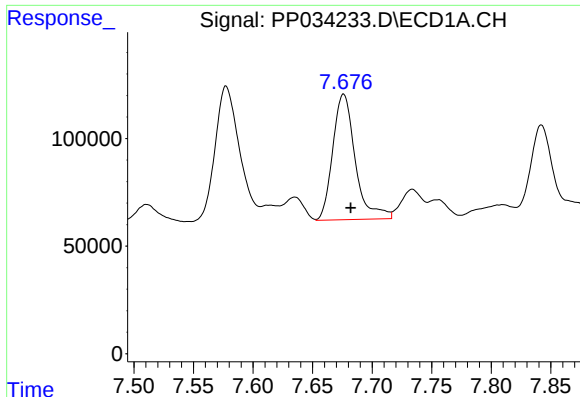


#28 AR-1254-3

R.T.: 7.676 min
Delta R.T.: -0.006 min
Response: 766602
Conc: 176.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-6B


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:51 PM

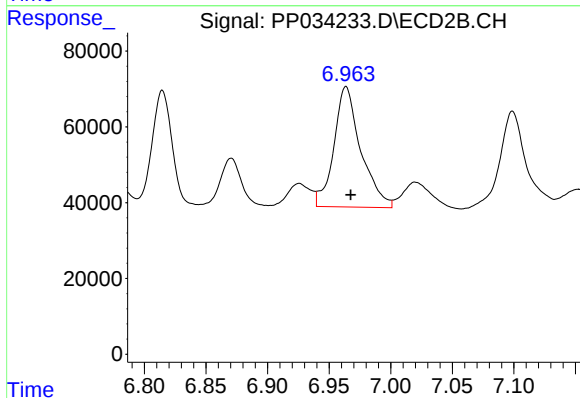


#28 AR-1254-3

R.T.: 6.964 min
Delta R.T.: -0.004 min
Response: 483506
Conc: 211.13 ng/ml

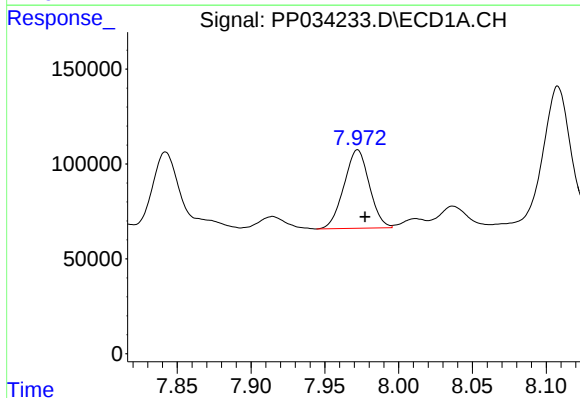


#29 AR-1254-4

R.T.: 7.972 min
Delta R.T.: -0.005 min
Response: 494181
Conc: 170.22 ng/ml

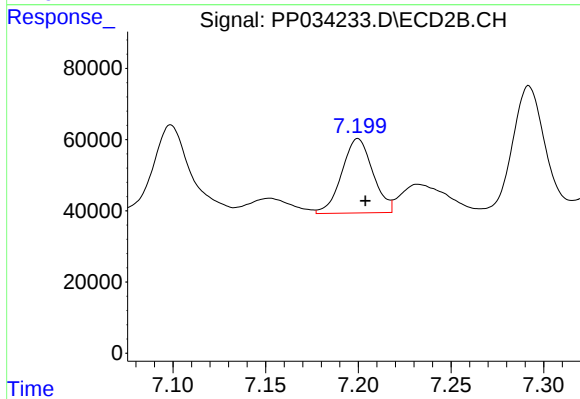

#29 AR-1254-4

R.T.: 7.200 min
Delta R.T.: -0.004 min
Response: 243341
Conc: 203.50 ng/ml

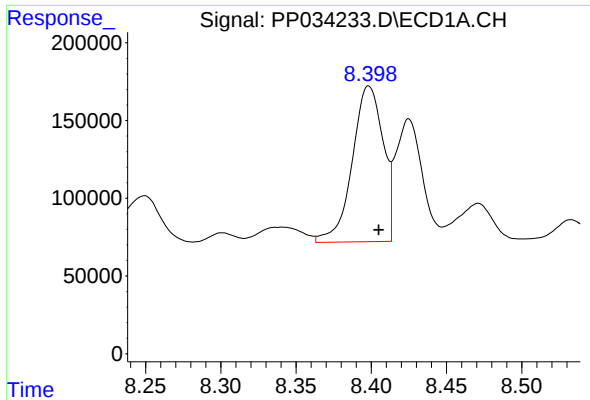


#30 AR-1254-5

R.T.: 8.398 min
Delta R.T.: -0.007 min
Response: 1427721
Conc: 427.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-6B

Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:51 PM

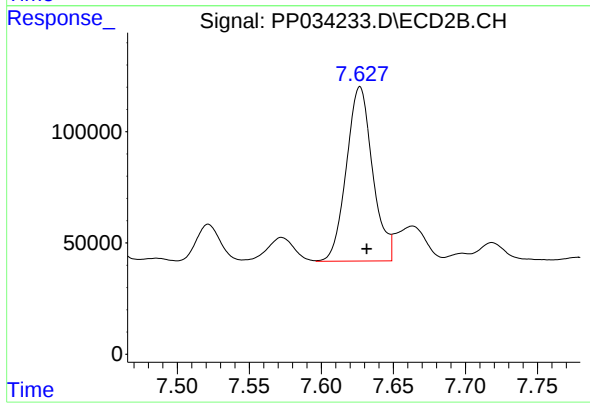

#30 AR-1254-5

R.T.: 7.627 min
Delta R.T.: -0.005 min
Response: 992855
Conc: 537.71 ng/ml