

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032221\
 Data File : PP034234.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Mar 2021 20:35
 Operator : DD\AJ
 Sample : M1660-19
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-6C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 02:07:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.849	4.261	2489897	1376378	29.639	31.103
2)	SA Decachlor...	10.773	9.576	2942872	1063946	37.500	40.318
Target Compounds							
26)	L6 AR-1254-1	7.067	6.386	258902	150457	94.594	89.724
27)	L6 AR-1254-2	7.296	6.543	457628	171655	109.900	118.368
28)	L6 AR-1254-3	7.676	6.963	849047	558115	195.488	243.705
29)	L6 AR-1254-4	7.970	7.199	434078	212447	149.520	177.668
30)	L6 AR-1254-5	8.398	7.626	1606213	1670853	481.154	904.897 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032221\
Data File : PP034234.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Mar 2021 20:35
Operator : DD\AJ
Sample : M1660-19
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
X127-6C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 02:07:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

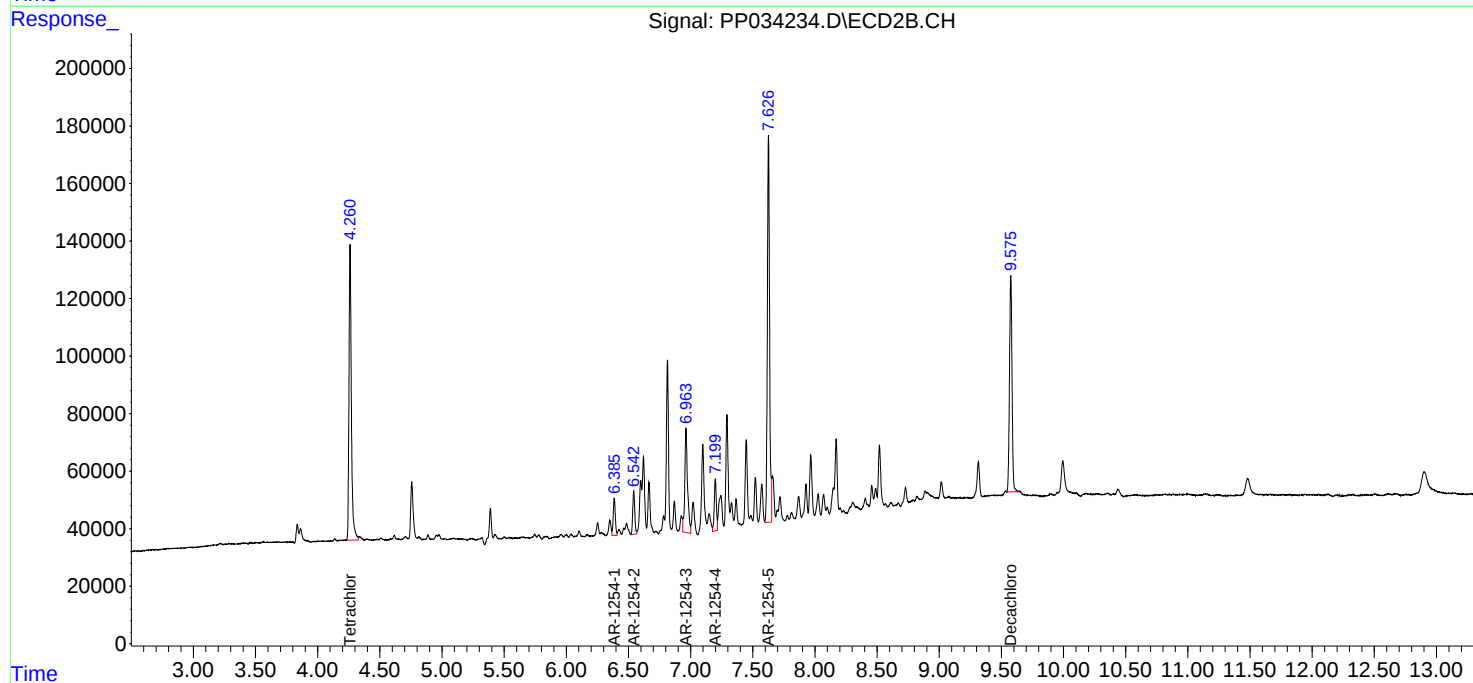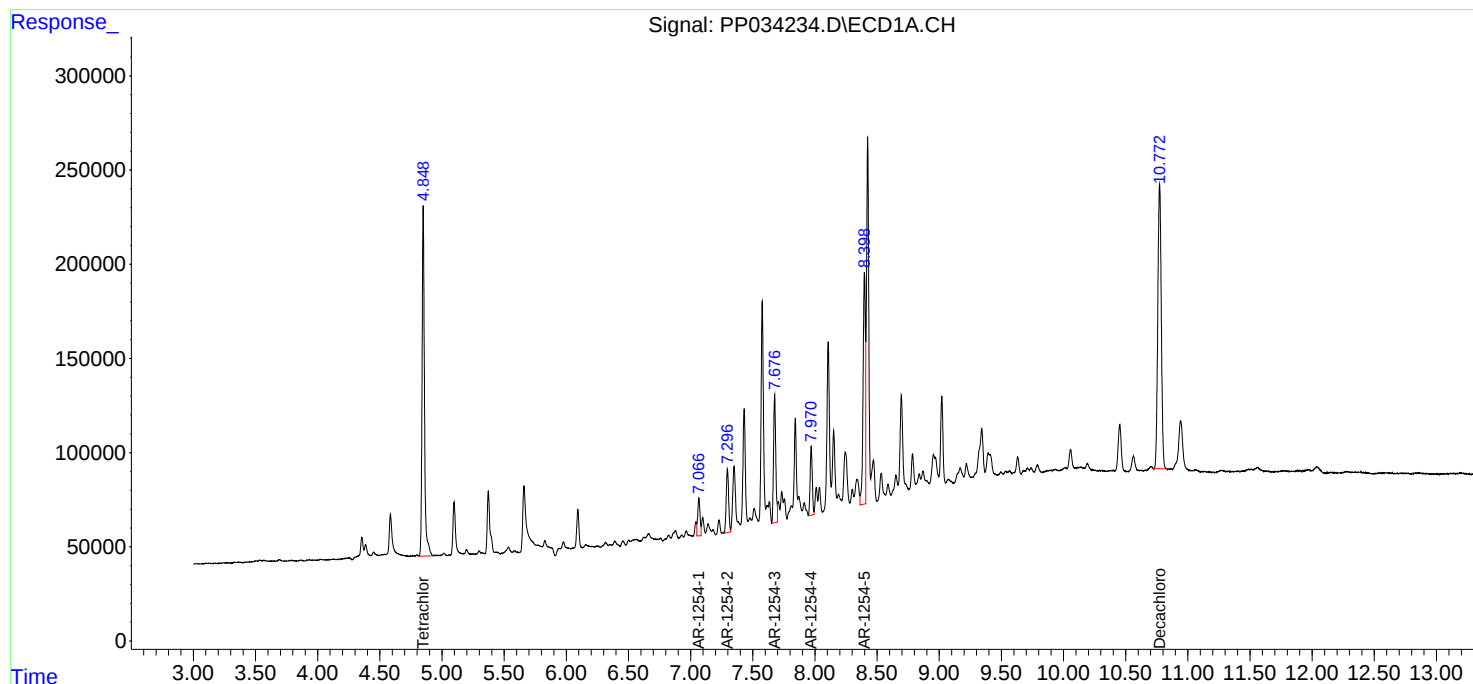


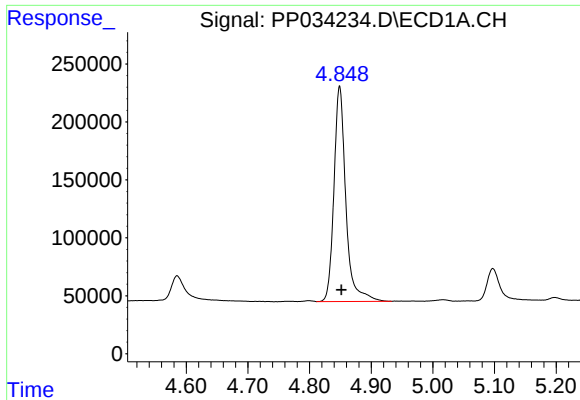

#1 Tetrachloro-m-xylene


R.T.: 4.849 min
Delta R.T.: -0.003 min
Response: 2489897
Conc: 29.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-6C

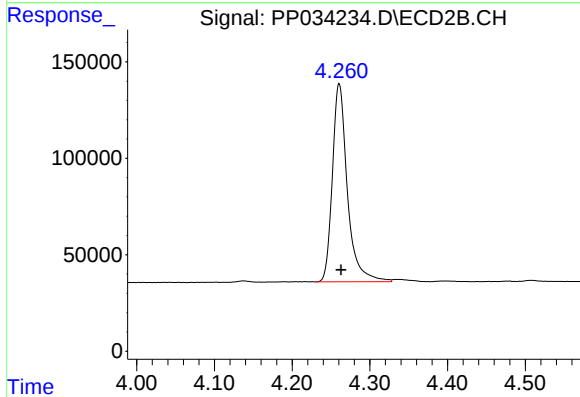


#1 Tetrachloro-m-xylene

R.T.: 4.261 min
Delta R.T.: -0.002 min
Response: 1376378
Conc: 31.10 ng/ml

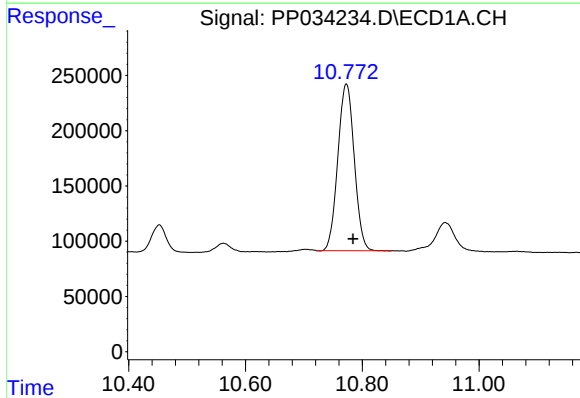


#2 Decachlorobiphenyl

R.T.: 10.773 min
Delta R.T.: -0.011 min
Response: 2942872
Conc: 37.50 ng/ml

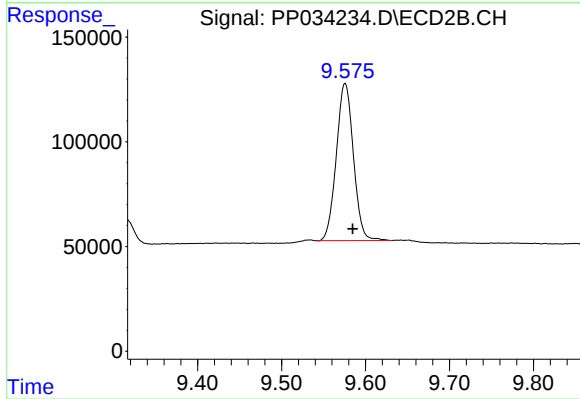

#2 Decachlorobiphenyl


R.T.: 9.576 min
Delta R.T.: -0.009 min
Response: 1063946
Conc: 40.32 ng/ml

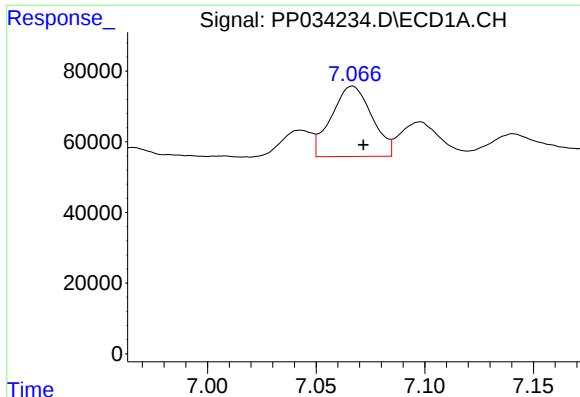

#26 AR-1254-1


R.T.: 7.067 min
Delta R.T.: -0.005 min
Response: 258902
Conc: 94.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-6C

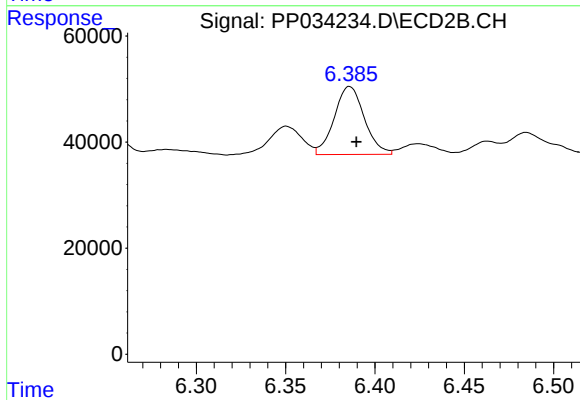


#26 AR-1254-1

R.T.: 6.386 min
Delta R.T.: -0.004 min
Response: 150457
Conc: 89.72 ng/ml

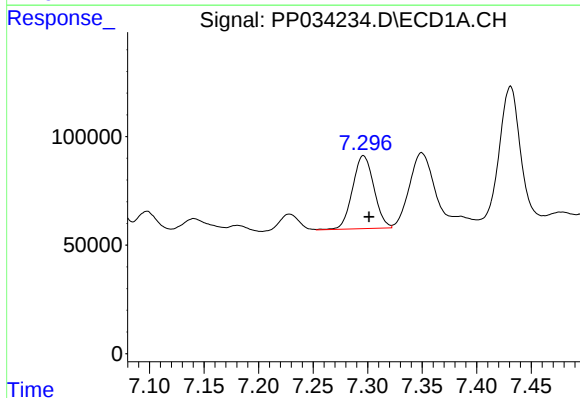


#27 AR-1254-2

R.T.: 7.296 min
Delta R.T.: -0.005 min
Response: 457628
Conc: 109.90 ng/ml

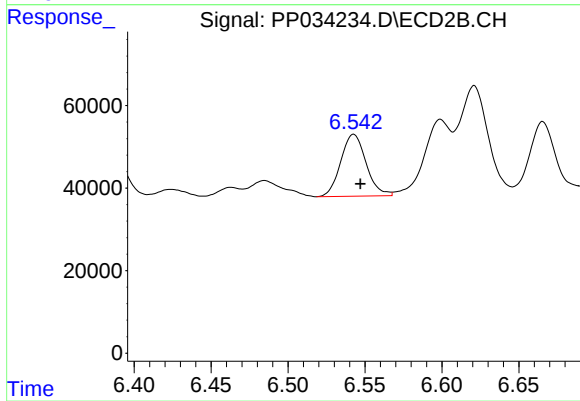

#27 AR-1254-2


R.T.: 6.543 min
Delta R.T.: -0.004 min
Response: 171655
Conc: 118.37 ng/ml

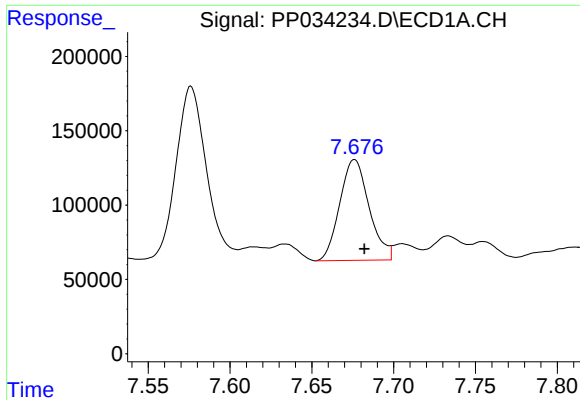

#28 AR-1254-3


R.T.: 7.676 min
Delta R.T.: -0.006 min
Response: 849047
Conc: 195.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-6C

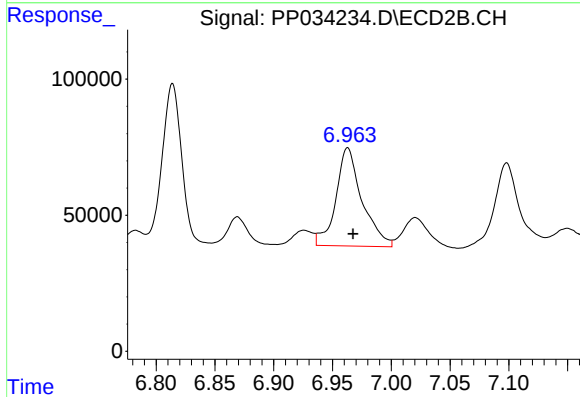


#28 AR-1254-3

R.T.: 6.963 min
Delta R.T.: -0.005 min
Response: 558115
Conc: 243.71 ng/ml

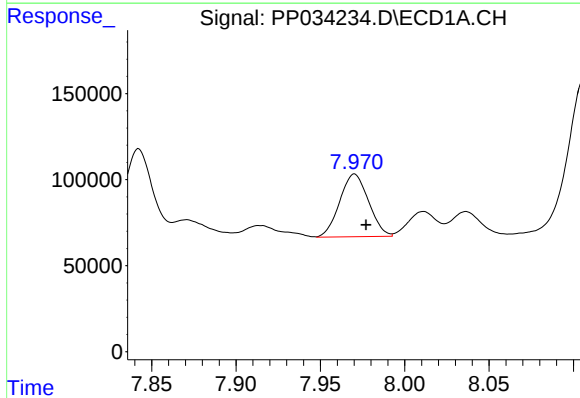


#29 AR-1254-4

R.T.: 7.970 min
Delta R.T.: -0.007 min
Response: 434078
Conc: 149.52 ng/ml

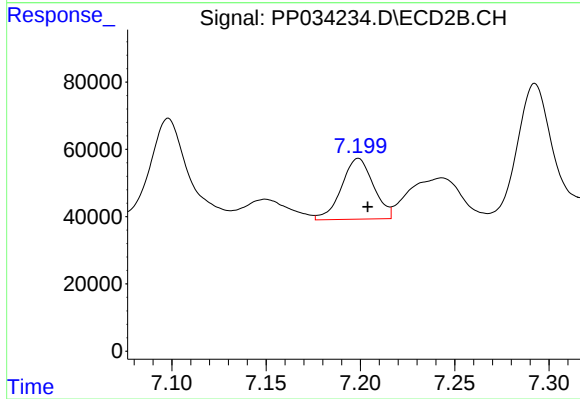

#29 AR-1254-4


R.T.: 7.199 min
Delta R.T.: -0.005 min
Response: 212447
Conc: 177.67 ng/ml

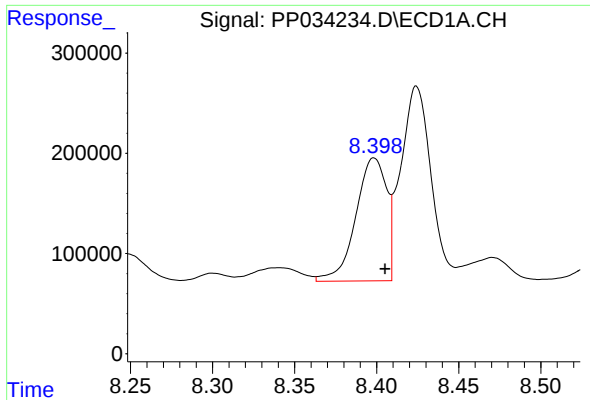

#30 AR-1254-5

R.T.: 8.398 min
Delta R.T.: -0.007 min
Response: 1606213
Conc: 481.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-6C

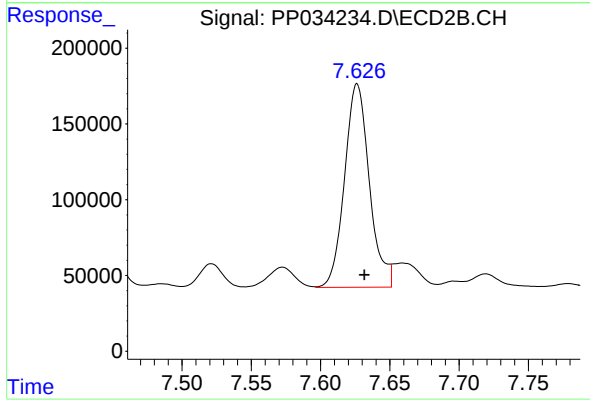

#30 AR-1254-5

R.T.: 7.626 min
Delta R.T.: -0.005 min
Response: 1670853
Conc: 904.90 ng/ml