

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032221\
 Data File : PP034245.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Mar 2021 00:32
 Operator : DD\AJ
 Sample : M1663-11
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-DUP6

Manual Integrations
 APPROVED

Ankita
 3/23/2021 1:38:57 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 02:13:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.848	4.260	1459937	866538	17.379m	19.582m
2) SA Decachlor...	10.772	9.575	1286156	451733	16.389m	17.118m
Target Compounds						
26) L6 AR-1254-1	7.066	6.385	266119	173831	97.231m	103.663
27) L6 AR-1254-2	7.295	6.542	735920	324296	176.732	223.625 #
28) L6 AR-1254-3	7.676	6.963	1226400	768393	282.372	335.525
29) L6 AR-1254-4	7.971	7.198	1055130	510237	363.444	426.708
30) L6 AR-1254-5	8.398	7.625	3045531	2777410	912.314	1504.184 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032221\
Data File : PP034245.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Mar 2021 00:32
Operator : DD\AJ
Sample : M1663-11
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
X127-DUP6


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:57 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 02:13:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

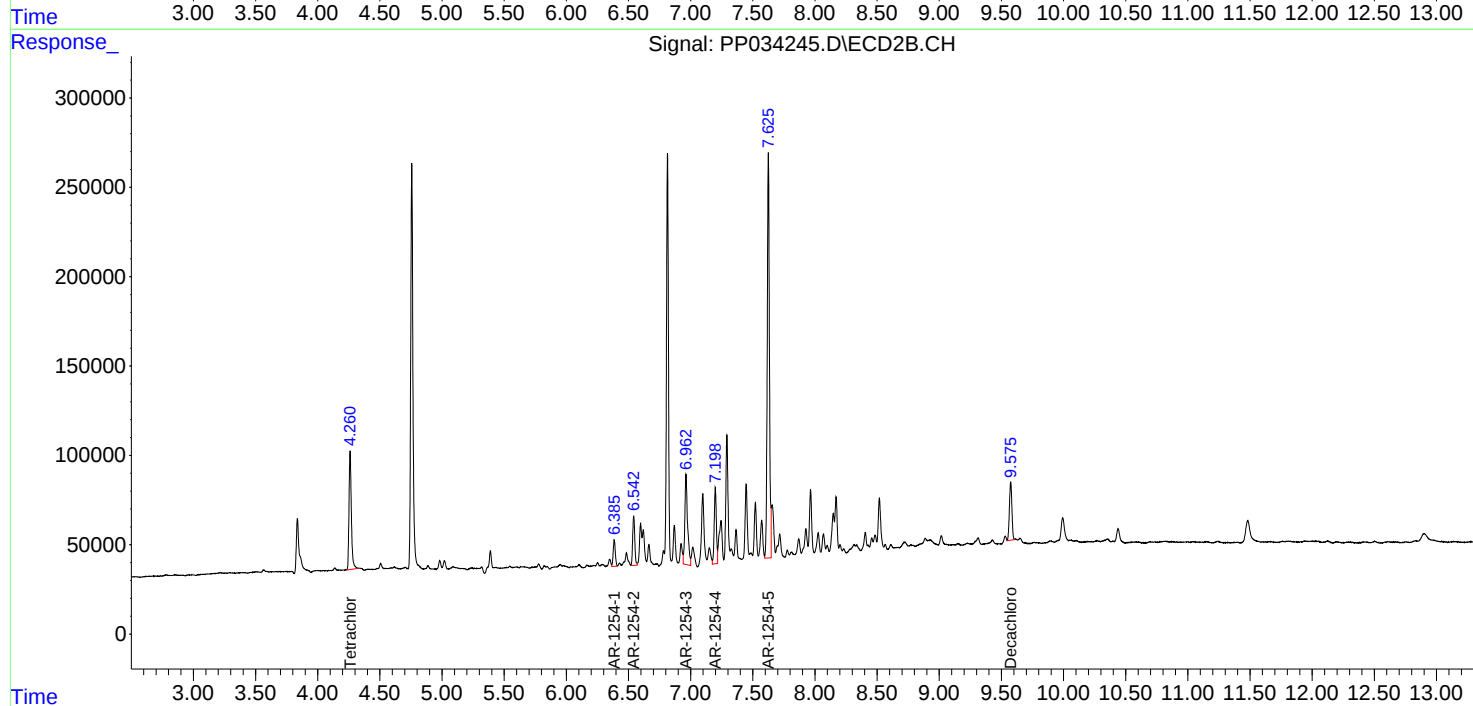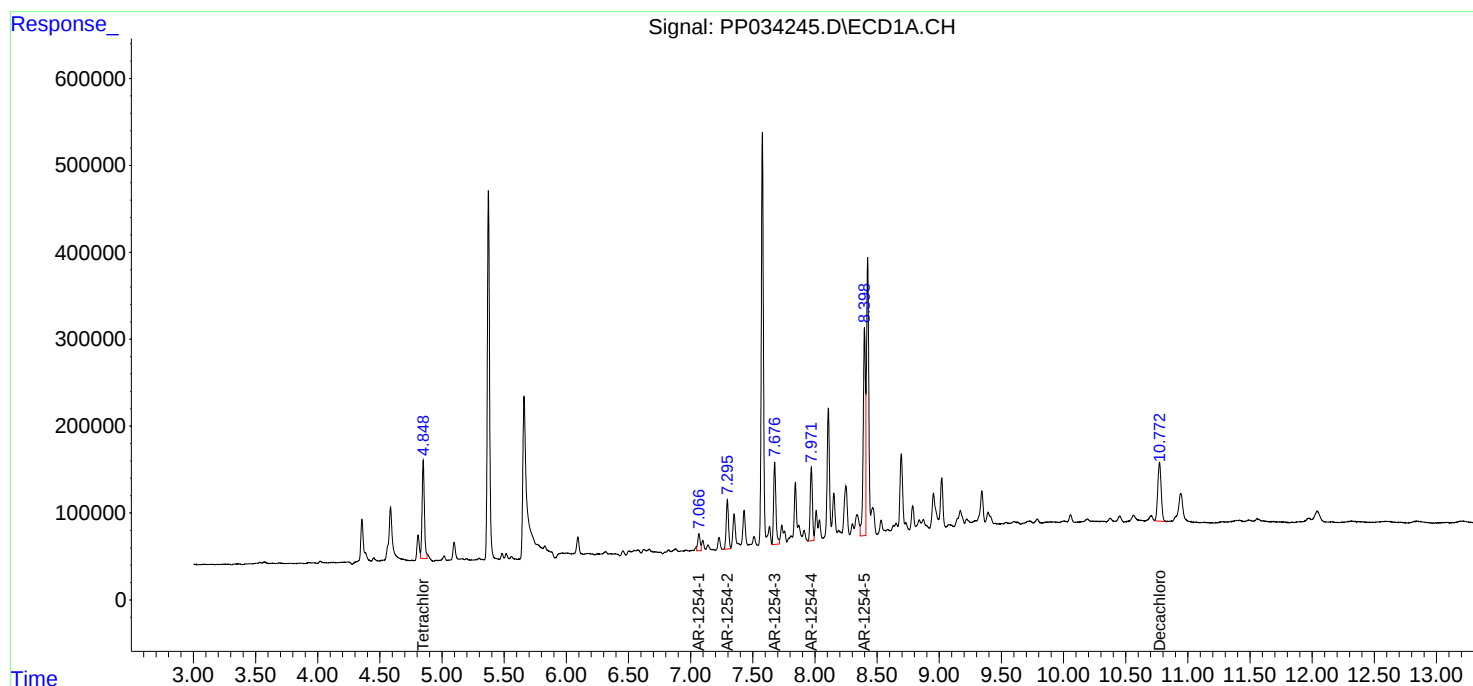

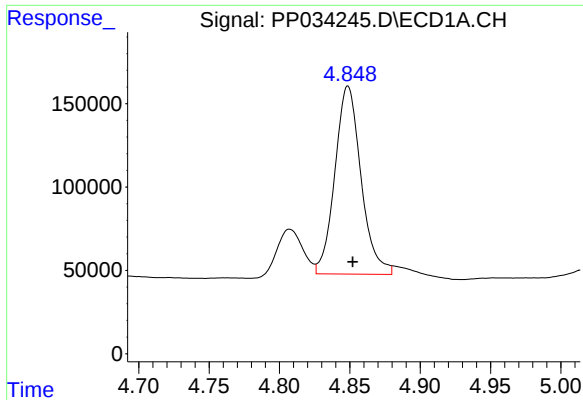


#1 Tetrachloro-m-xylene

R.T.: 4.848 min
Delta R.T.: -0.004 min
Response: 1459937
Conc: 17.38 ng/ml m

Instrument :
ECD_P
ClientSampleId :
X127-DUP6


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:57 PM

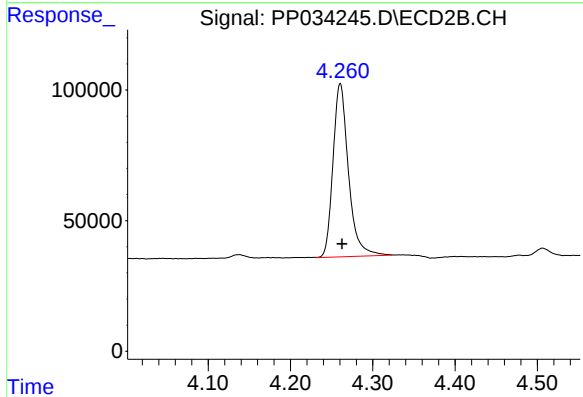


#1 Tetrachloro-m-xylene

R.T.: 4.260 min
Delta R.T.: -0.003 min
Response: 866538
Conc: 19.58 ng/ml m

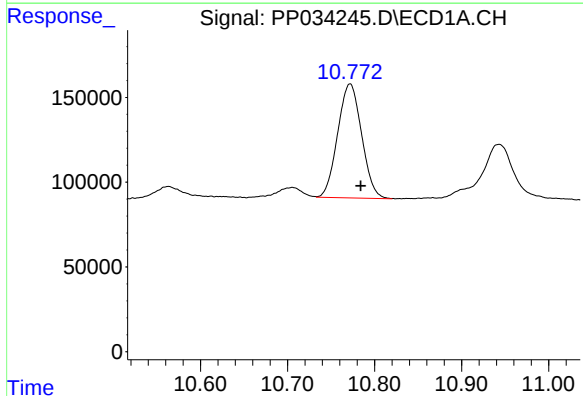


#2 Decachlorobiphenyl

R.T.: 10.772 min
Delta R.T.: -0.012 min
Response: 1286156
Conc: 16.39 ng/ml m

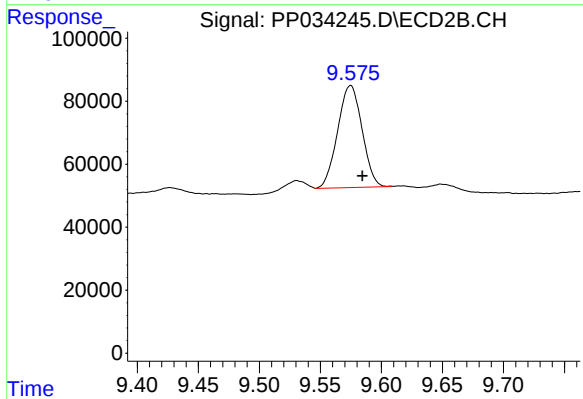

#2 Decachlorobiphenyl

R.T.: 9.575 min
Delta R.T.: -0.010 min
Response: 451733
Conc: 17.12 ng/ml m

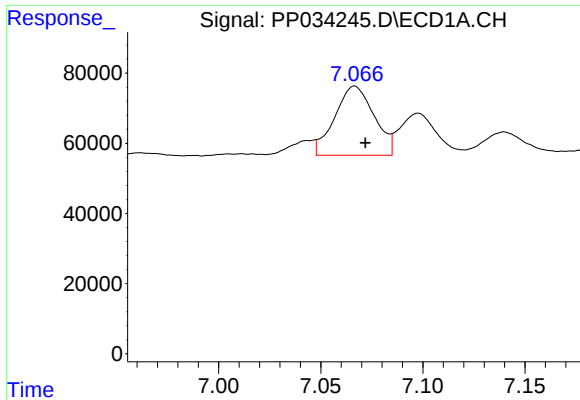


#26 AR-1254-1

R.T.: 7.066 min
Delta R.T.: -0.006 min
Response: 266119
Conc: 97.23 ng/ml m

Instrument :
ECD_P
ClientSampleId :
X127-DUP6


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:57 PM

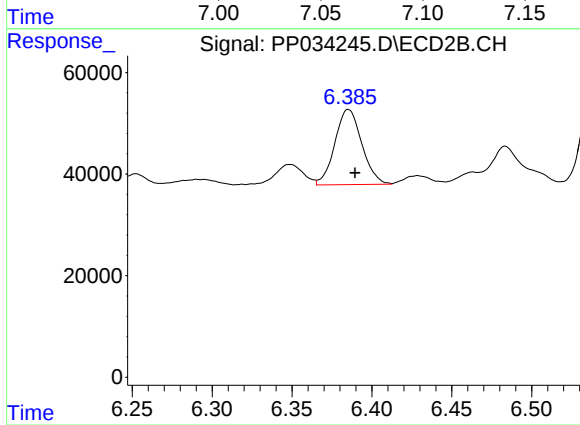


#26 AR-1254-1

R.T.: 6.385 min
Delta R.T.: -0.004 min
Response: 173831
Conc: 103.66 ng/ml

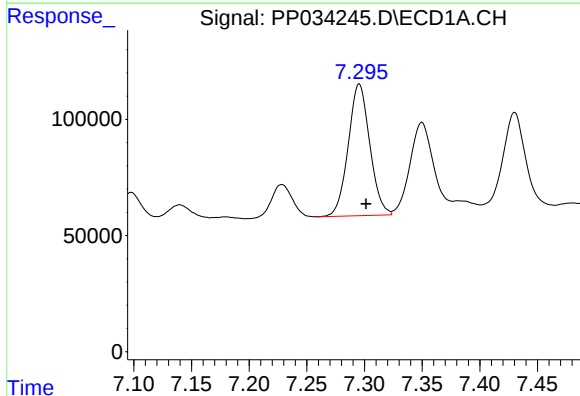


#27 AR-1254-2

R.T.: 7.295 min
Delta R.T.: -0.006 min
Response: 735920
Conc: 176.73 ng/ml

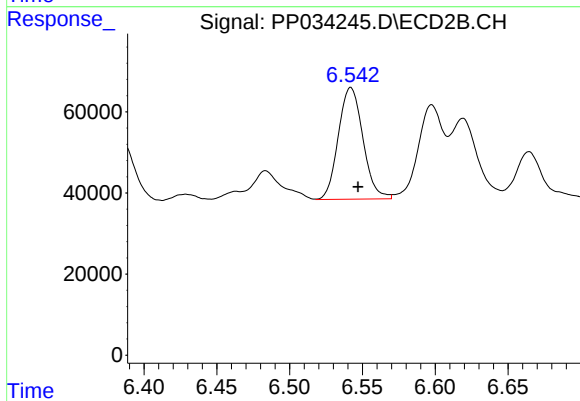

#27 AR-1254-2

R.T.: 6.542 min
Delta R.T.: -0.005 min
Response: 324296
Conc: 223.62 ng/ml

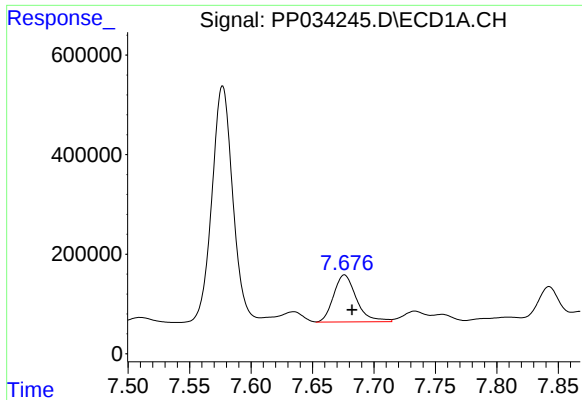


#28 AR-1254-3

R.T.: 7.676 min
Delta R.T.: -0.006 min
Response: 1226400
Conc: 282.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-DUP6


Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:57 PM

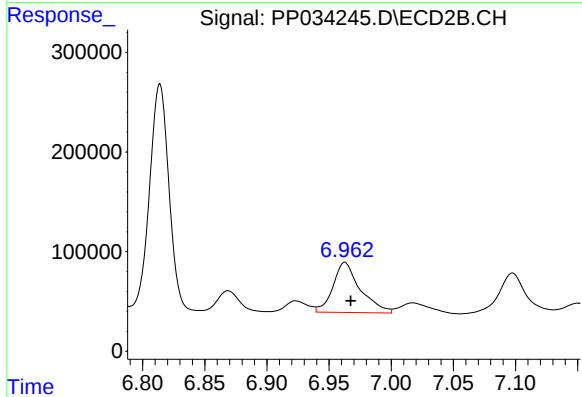


#28 AR-1254-3

R.T.: 6.963 min
Delta R.T.: -0.005 min
Response: 768393
Conc: 335.52 ng/ml

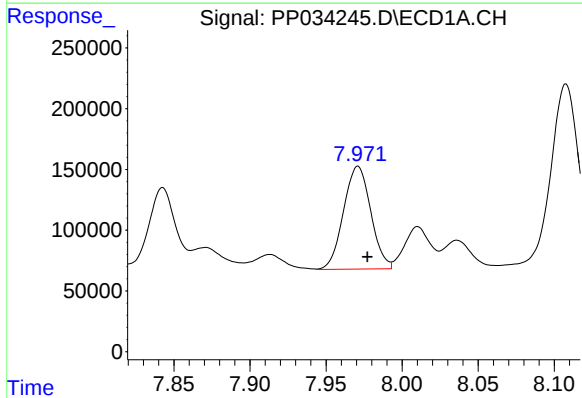


#29 AR-1254-4

R.T.: 7.971 min
Delta R.T.: -0.006 min
Response: 1055130
Conc: 363.44 ng/ml

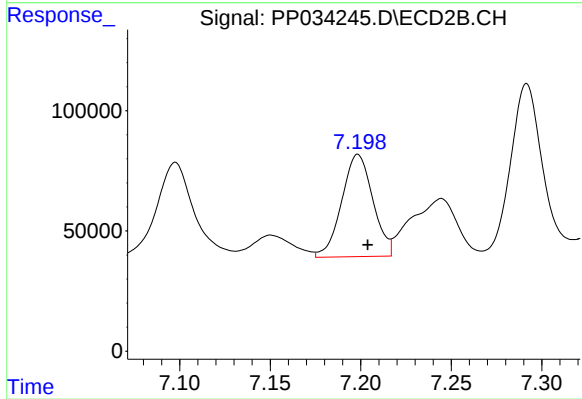

#29 AR-1254-4

R.T.: 7.198 min
Delta R.T.: -0.005 min
Response: 510237
Conc: 426.71 ng/ml

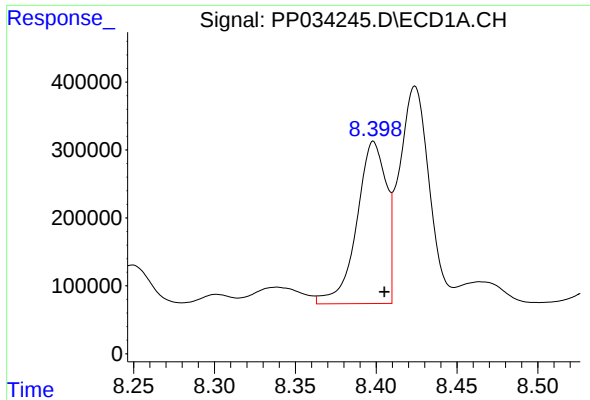


#30 AR-1254-5

R.T.: 8.398 min
Delta R.T.: -0.007 min
Response: 3045531
Conc: 912.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-DUP6

Manual Integrations
APPROVED

Ankita
3/23/2021 1:38:57 PM

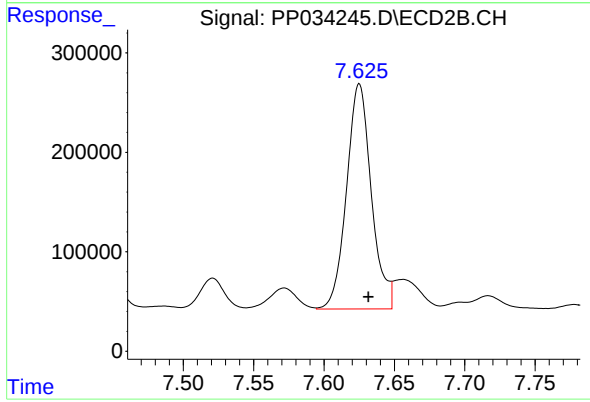

#30 AR-1254-5

R.T.: 7.625 min
Delta R.T.: -0.006 min
Response: 2777410
Conc: 1504.18 ng/ml