

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032221\
 Data File : PP034255.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Mar 2021 4:11
 Operator : DD\AJ
 Sample : M1753-03
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 32539

Manual Integrations
 APPROVED

Ankita
 3/23/2021 1:39:09 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 04:49:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.850	4.264	1755290	746453	20.895	16.868
2) SA Decachlor...	10.786	9.589	1087178	640990	13.853m	24.290 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032221\
Data File : PP034255.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Mar 2021 4:11
Operator : DD\AJ
Sample : M1753-03
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
32539


Manual Integrations
APPROVED

Ankita
3/23/2021 1:39:09 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 04:49:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

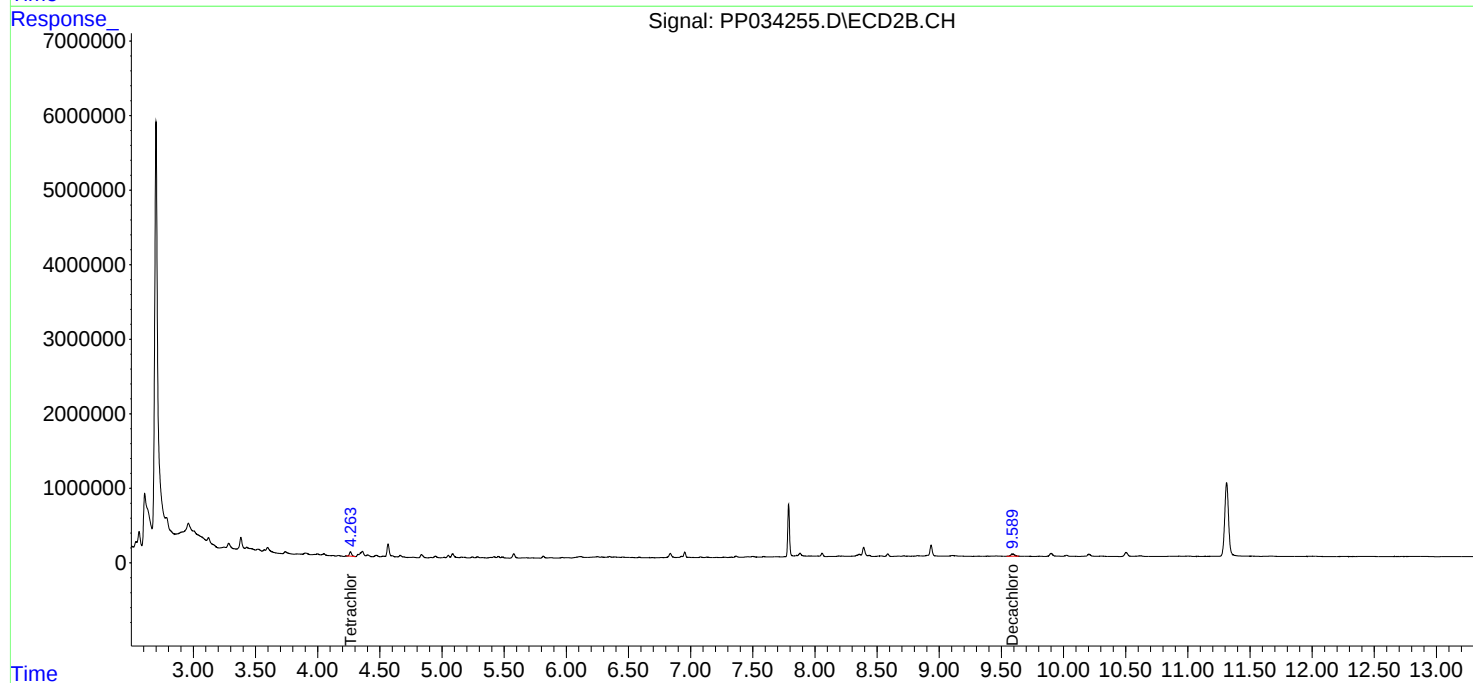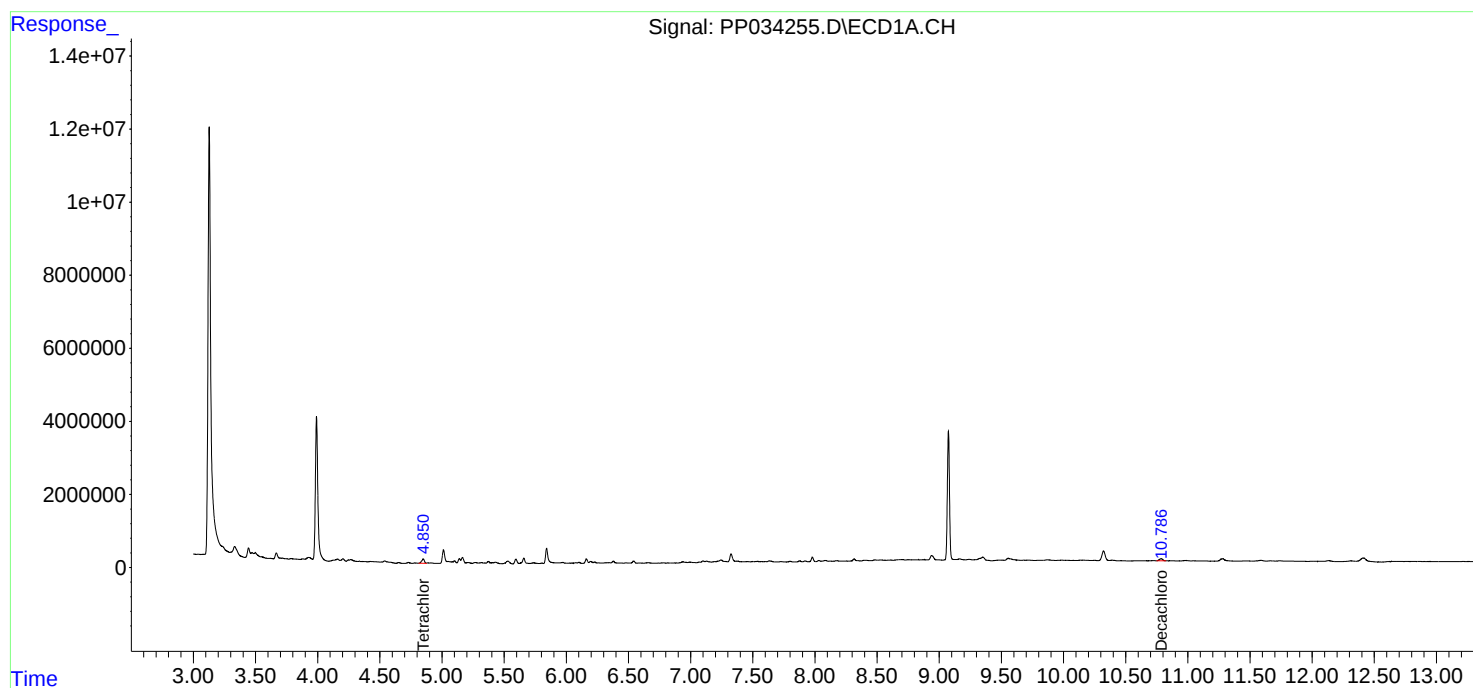

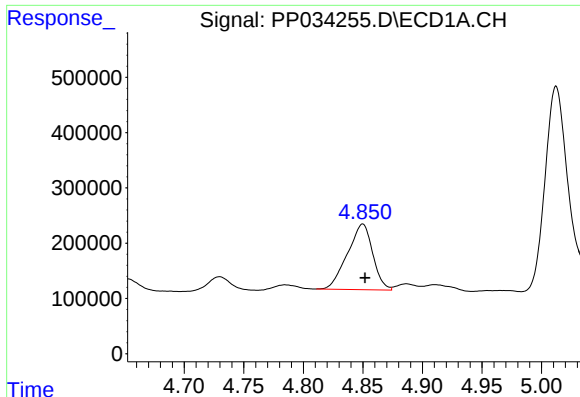


#1 Tetrachloro-m-xylene

R.T.: 4.850 min
Delta R.T.: -0.002 min
Response: 1755290
Conc: 20.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
32539


Manual Integrations
APPROVED

Ankita
3/23/2021 1:39:09 PM

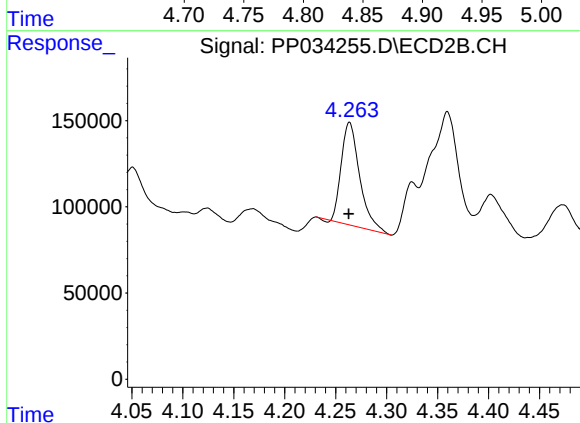


#1 Tetrachloro-m-xylene

R.T.: 4.264 min
Delta R.T.: 0.000 min
Response: 746453
Conc: 16.87 ng/ml

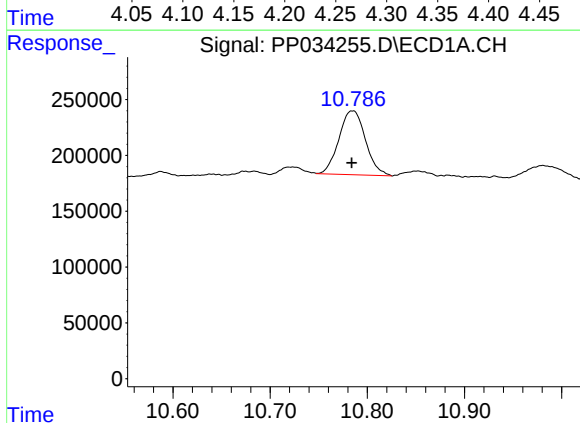

#2 Decachlorobiphenyl

R.T.: 10.786 min
Delta R.T.: 0.002 min
Response: 1087178
Conc: 13.85 ng/ml m

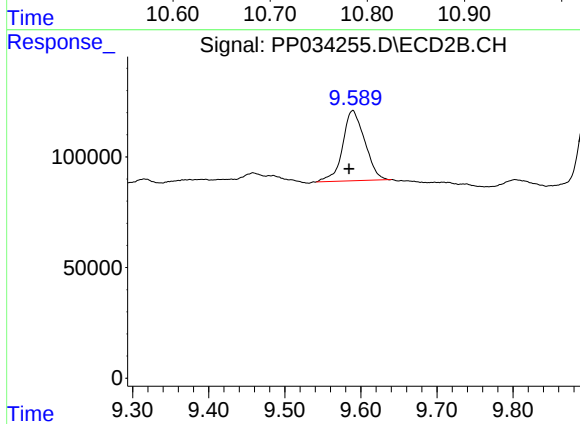

#2 Decachlorobiphenyl

R.T.: 9.589 min
Delta R.T.: 0.005 min
Response: 640990
Conc: 24.29 ng/ml