

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032224\
 Data File : PP063691.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Mar 2024 18:25
 Operator : YP\AJ
 Sample : P1820-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WASTE-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 21 23:16:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 19 06:23:02 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.489	3.640	39324719	43304056	16.480	18.138
2)	SA Decachlor...	10.357	8.675	40745747	36018226	16.048	13.328
Target Compounds							
3)	L1 AR-1016-1	0.000	4.716f	0	251656	N.D.	3.046 #
8)	L2 AR-1221-1	4.676f	3.866	2936334	910047	107.868	36.601 #
9)	L2 AR-1221-2	0.000	3.935	0	1753388	N.D.	85.556 #
16)	L4 AR-1242-1	0.000	4.716f	0	251656	N.D.	4.269 #
21)	L5 AR-1248-1	0.000	4.716f	0	251656	N.D.	5.650 #
24)	L5 AR-1248-4	6.572	0.000	1916344	0	23.434	N.D. #
25)	L5 AR-1248-5	6.572f	0.000	1916344	0	23.497	N.D. #
29)	L6 AR-1254-4	7.428	0.000	1585844	0	17.406	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032224\
Data File : PP063691.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Mar 2024 18:25
Operator : YP\AJ
Sample : P1820-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
WASTE-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 21 23:16:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 19 06:23:02 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

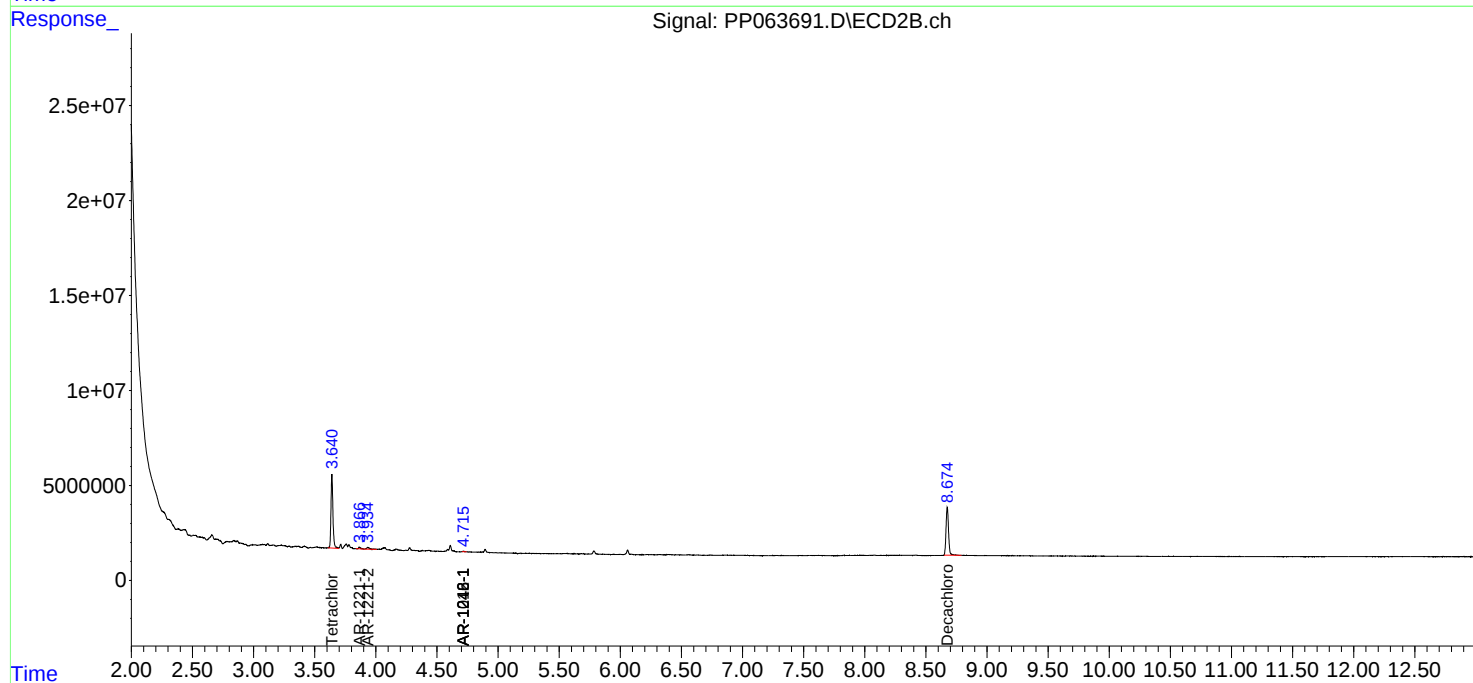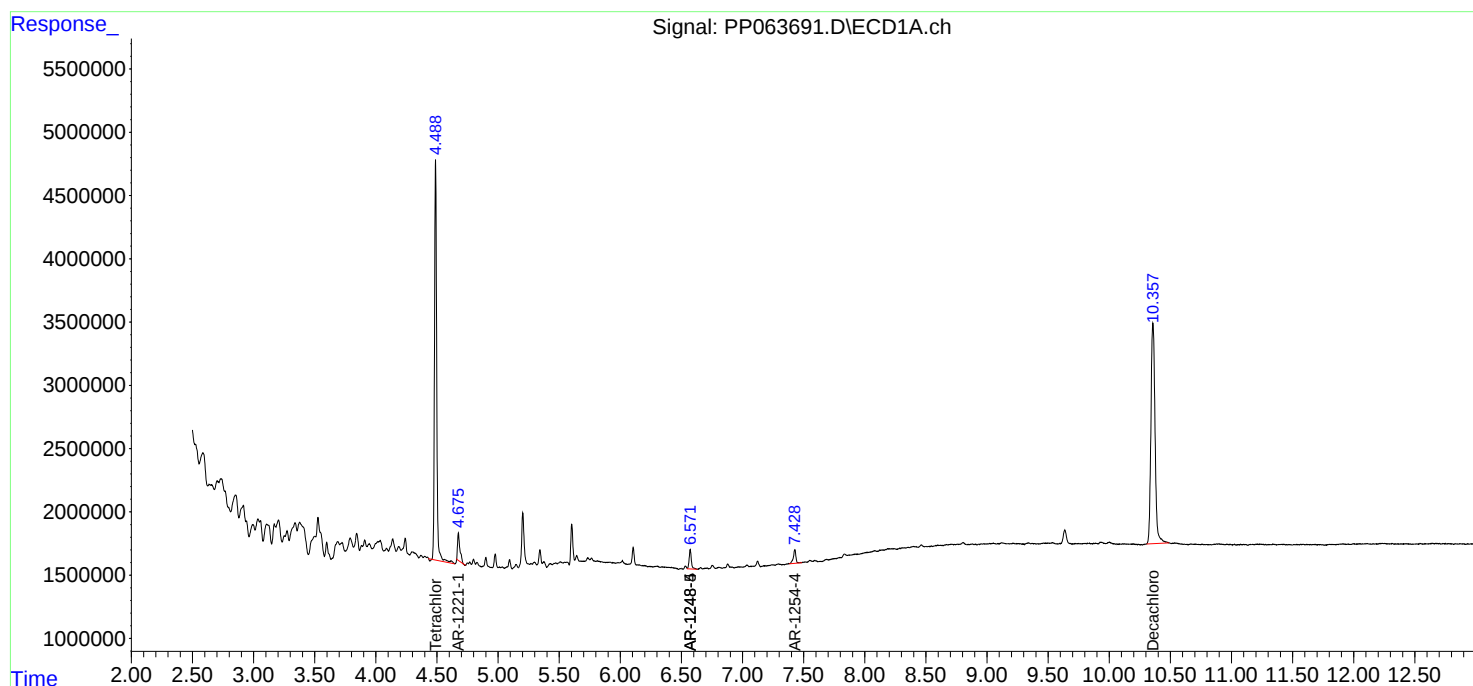


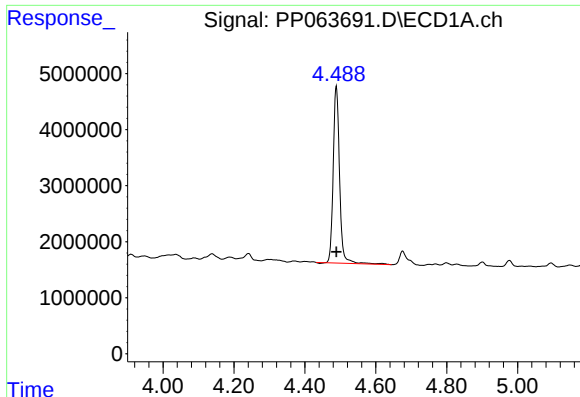

#1 Tetrachloro-m-xylene


R.T.: 4.489 min
Delta R.T.: 0.000 min
Response: 39324719
Conc: 16.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
WASTE-WATER

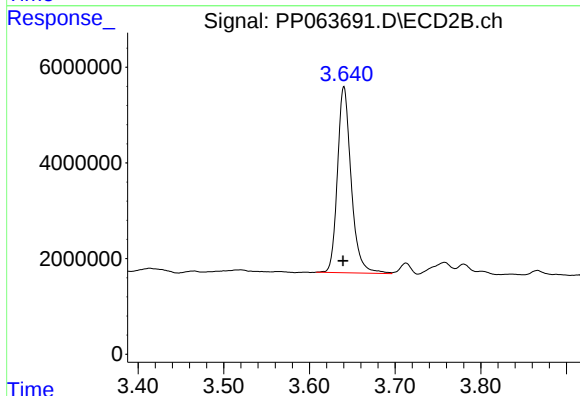


#1 Tetrachloro-m-xylene

R.T.: 3.640 min
Delta R.T.: 0.001 min
Response: 43304056
Conc: 18.14 ng/ml

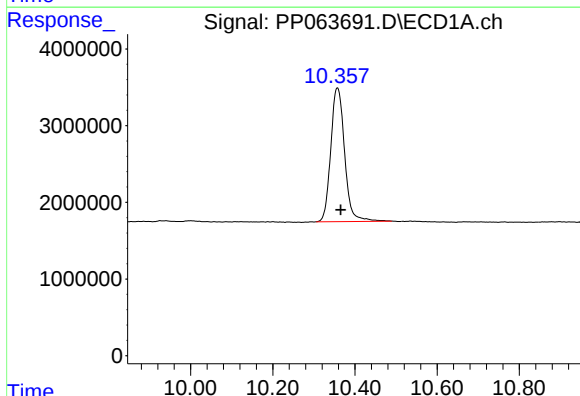


#2 Decachlorobiphenyl

R.T.: 10.357 min
Delta R.T.: -0.008 min
Response: 40745747
Conc: 16.05 ng/ml

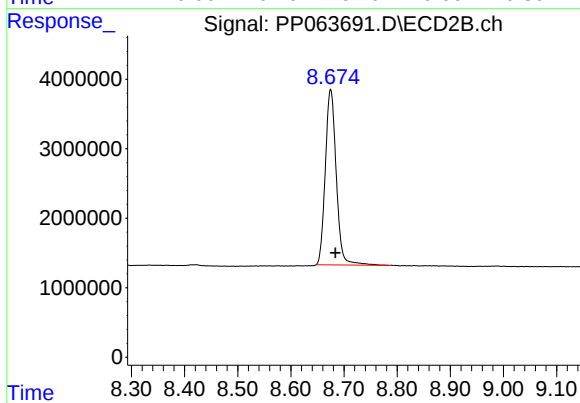

#2 Decachlorobiphenyl


R.T.: 8.675 min
Delta R.T.: -0.009 min
Response: 36018226
Conc: 13.33 ng/ml

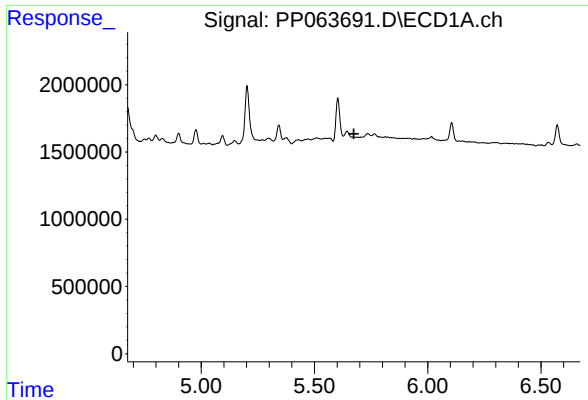

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.673 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
WASTE-WATER

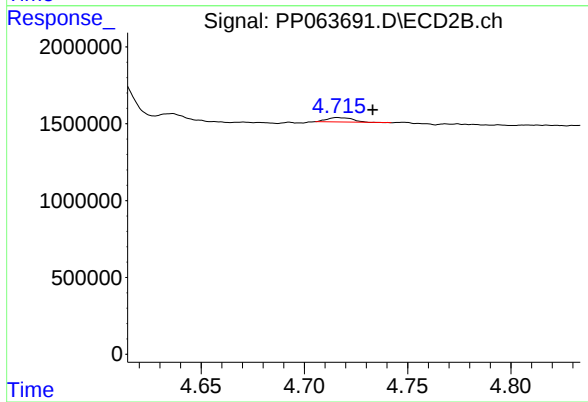


#3 AR-1016-1

R.T.: 4.716 min
Delta R.T.: -0.017 min
Response: 251656
Conc: 3.05 ng/ml

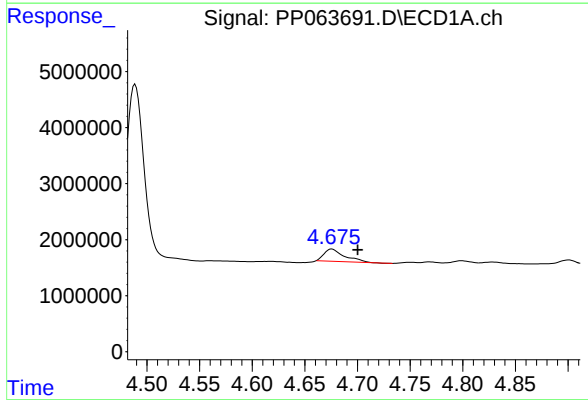


#8 AR-1221-1

R.T.: 4.676 min
Delta R.T.: -0.024 min
Response: 2936334
Conc: 107.87 ng/ml

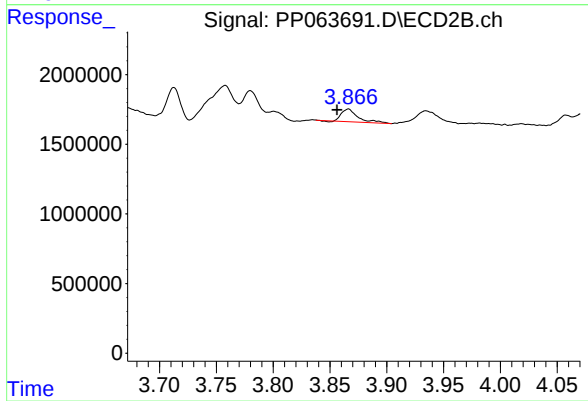

#8 AR-1221-1


R.T.: 3.866 min
Delta R.T.: 0.010 min
Response: 910047
Conc: 36.60 ng/ml

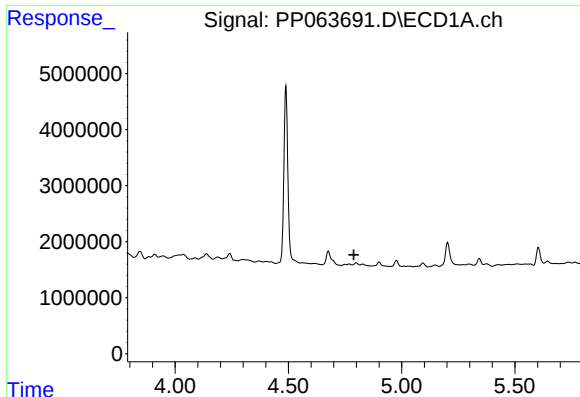

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.789 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
WASTE-WATER

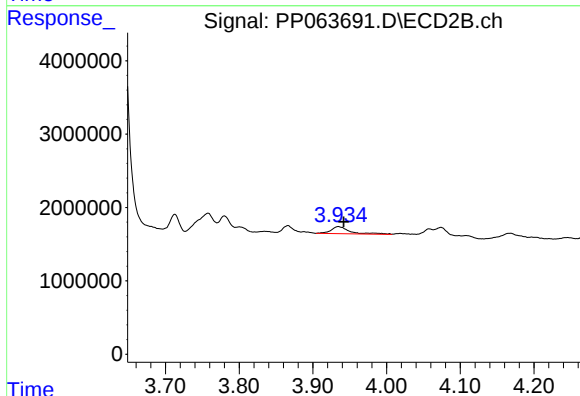


#9 AR-1221-2

R.T.: 3.935 min
Delta R.T.: -0.007 min
Response: 1753388
Conc: 85.56 ng/ml

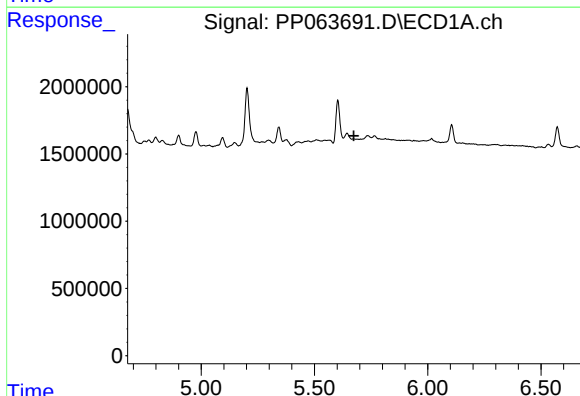


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T.: 5.674 min
Response: 0
Conc: N.D.

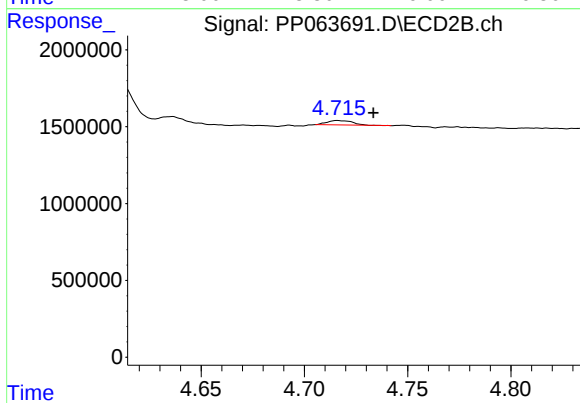

#16 AR-1242-1


R.T.: 4.716 min
Delta R.T.: -0.017 min
Response: 251656
Conc: 4.27 ng/ml

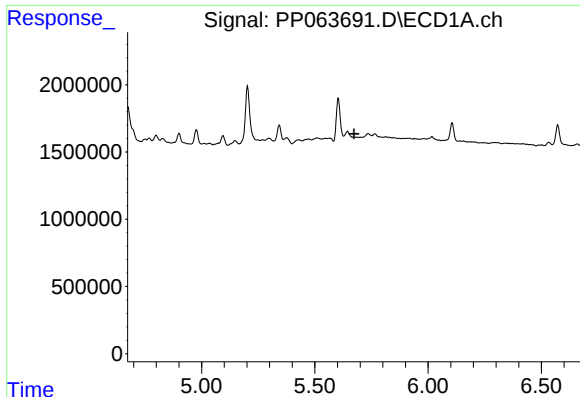

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 5.673 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
WASTE-WATER

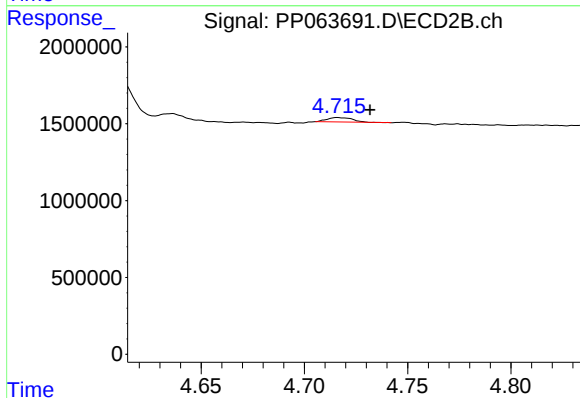


#21 AR-1248-1

R.T.: 4.716 min
Delta R.T.: -0.016 min
Response: 251656
Conc: 5.65 ng/ml

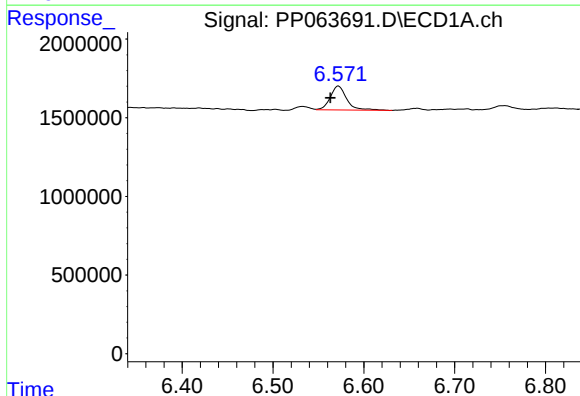


#24 AR-1248-4

R.T.: 6.572 min
Delta R.T.: 0.009 min
Response: 1916344
Conc: 23.43 ng/ml

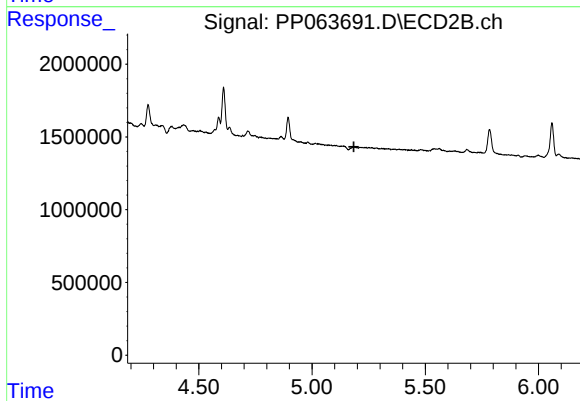

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.185 min
Response: 0
Conc: N.D.

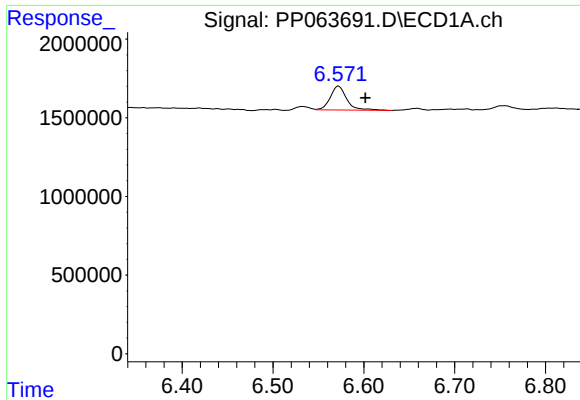

#25 AR-1248-5


R.T.: 6.572 min
Delta R.T.: -0.030 min
Response: 1916344
Conc: 23.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
WASTE-WATER

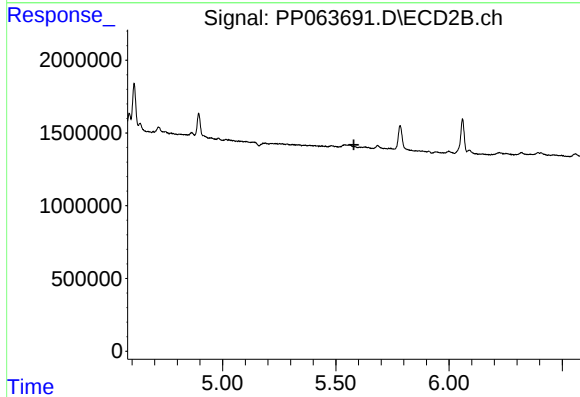


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.580 min
Response: 0
Conc: N.D.

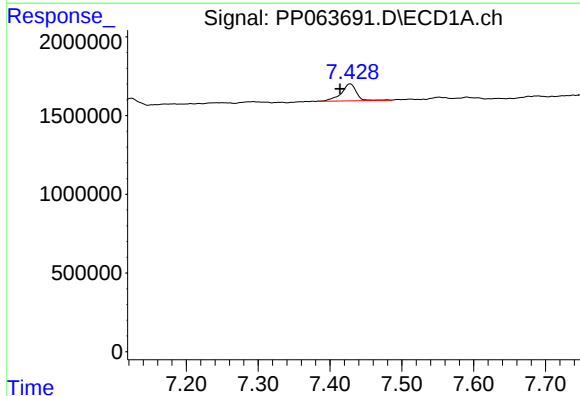

#29 AR-1254-4

R.T.: 7.428 min
Delta R.T.: 0.014 min
Response: 1585844
Conc: 17.41 ng/ml

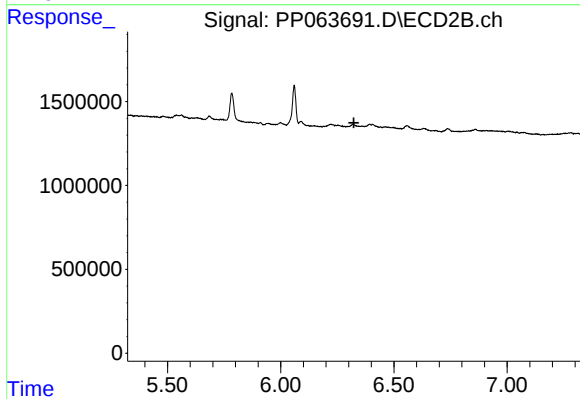

#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.323 min
Response: 0
Conc: N.D.