

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032224\
 Data File : PP063692.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Mar 2024 18:41
 Operator : YP\AJ
 Sample : P1821-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEATER-1-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 21 23:18:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 19 06:23:02 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.488	3.639	41880444	43136104	17.551	18.067
2) SA Decachlor...	10.355	8.675	27887186	24759246	10.984	9.162
Target Compounds						
9) L2 AR-1221-2	0.000	3.939	0	611965	N.D.	29.861 #
33) L7 AR-1260-3	0.000	6.576	0	431656	N.D.	2.686 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032224\
Data File : PP063692.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Mar 2024 18:41
Operator : YP\AJ
Sample : P1821-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HEATER-1-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 21 23:18:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 19 06:23:02 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

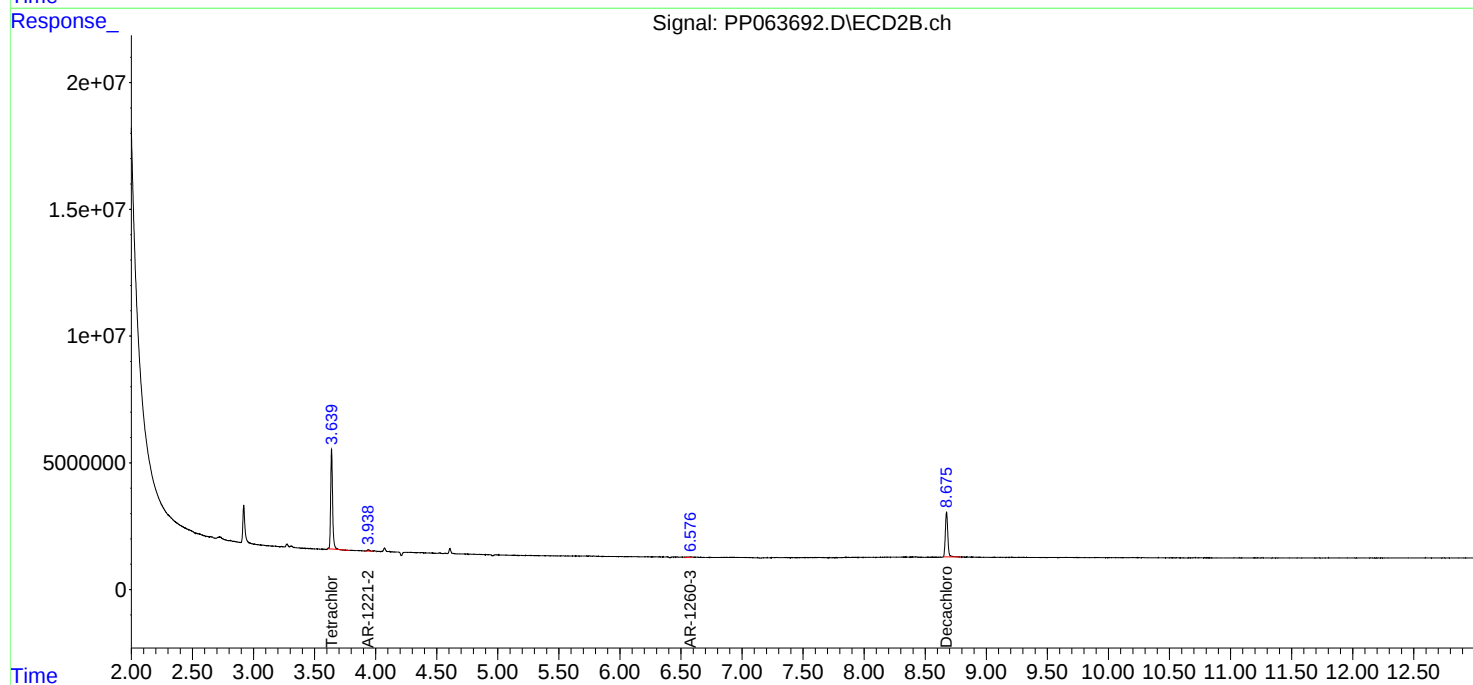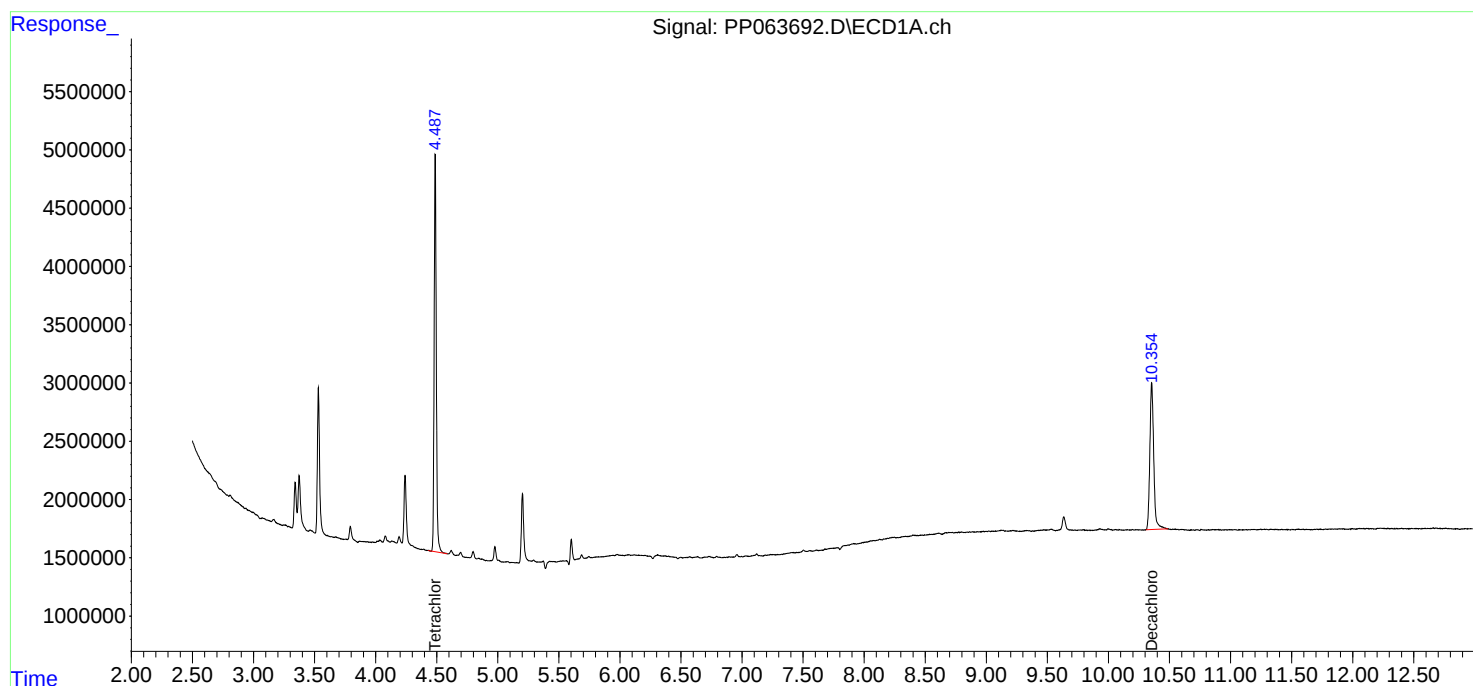


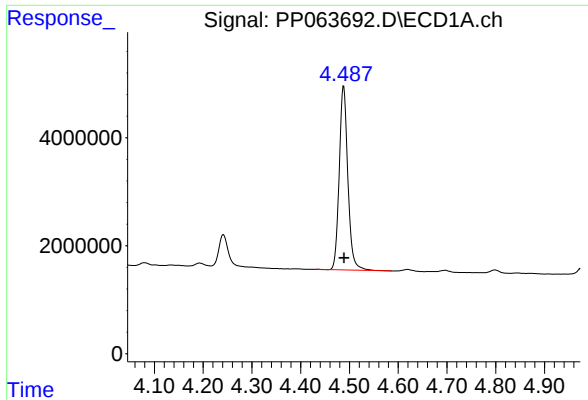

#1 Tetrachloro-m-xylene


R.T.: 4.488 min
Delta R.T.: 0.000 min
Response: 41880444
Conc: 17.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEATER-1-2

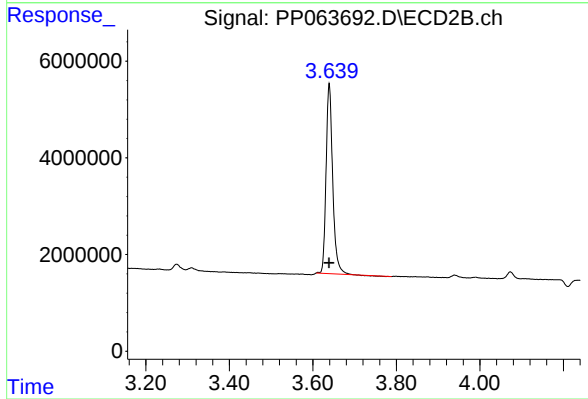


#1 Tetrachloro-m-xylene

R.T.: 3.639 min
Delta R.T.: 0.000 min
Response: 43136104
Conc: 18.07 ng/ml

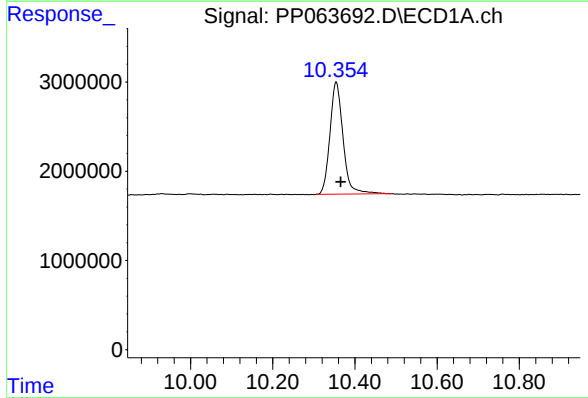


#2 Decachlorobiphenyl

R.T.: 10.355 min
Delta R.T.: -0.011 min
Response: 27887186
Conc: 10.98 ng/ml

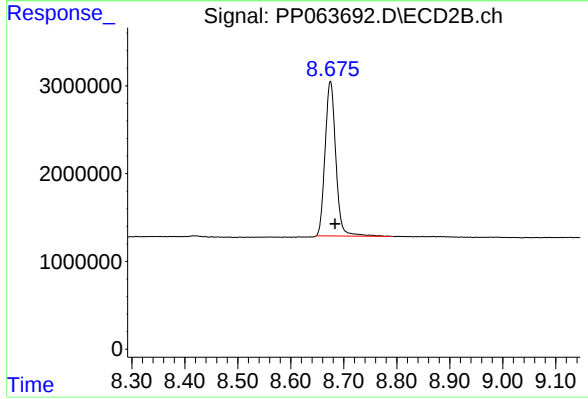

#2 Decachlorobiphenyl


R.T.: 8.675 min
Delta R.T.: -0.009 min
Response: 24759246
Conc: 9.16 ng/ml

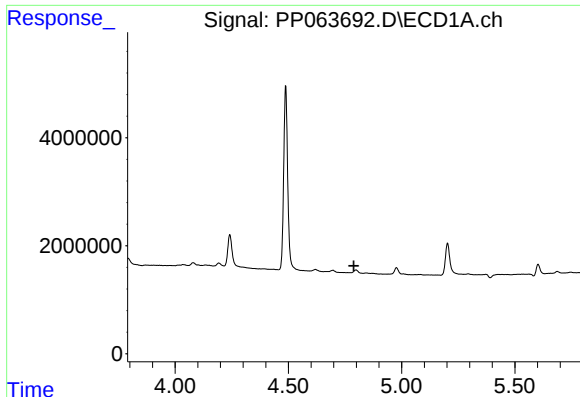

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.789 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEATER-1-2

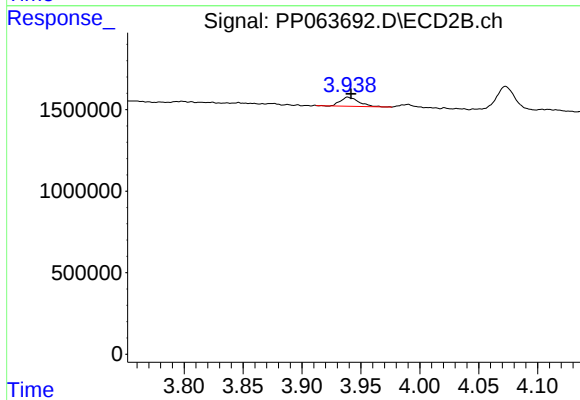


#9 AR-1221-2

R.T.: 3.939 min
Delta R.T.: -0.003 min
Response: 611965
Conc: 29.86 ng/ml

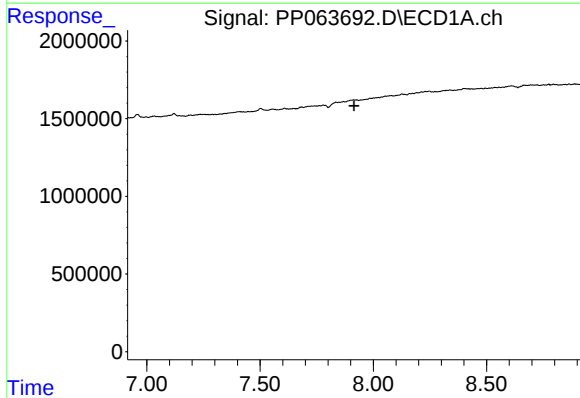

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.915 min
Response: 0
Conc: N.D.

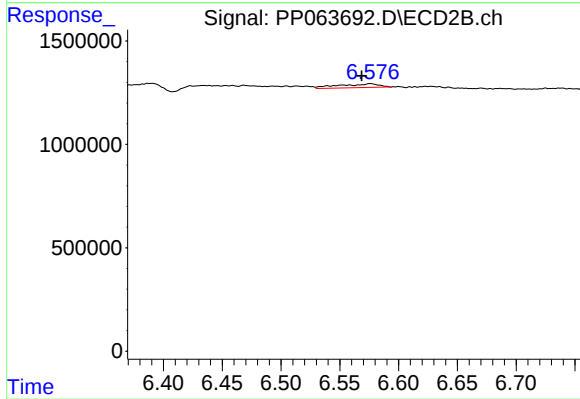

#33 AR-1260-3

R.T.: 6.576 min
Delta R.T.: 0.007 min
Response: 431656
Conc: 2.69 ng/ml