

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032224\
 Data File : PP063673.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Mar 2024 12:33
 Operator : YP\AJ
 Sample : P1808-01 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC274686-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/22/2024
 Supervised By :Ankita Jodhani 03/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 21 13:02:22 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 19 06:23:02 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.486	3.637	2980389	2919432	1.249m	1.223
2) SA Decachlor...	10.363	8.681	3120444	3079860	1.229	1.140

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032224\
Data File : PP063673.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Mar 2024 12:33
Operator : YP\AJ
Sample : P1808-01 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC274686-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/22/2024
Supervised By :Ankita Jodhani 03/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 21 13:02:22 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 19 06:23:02 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

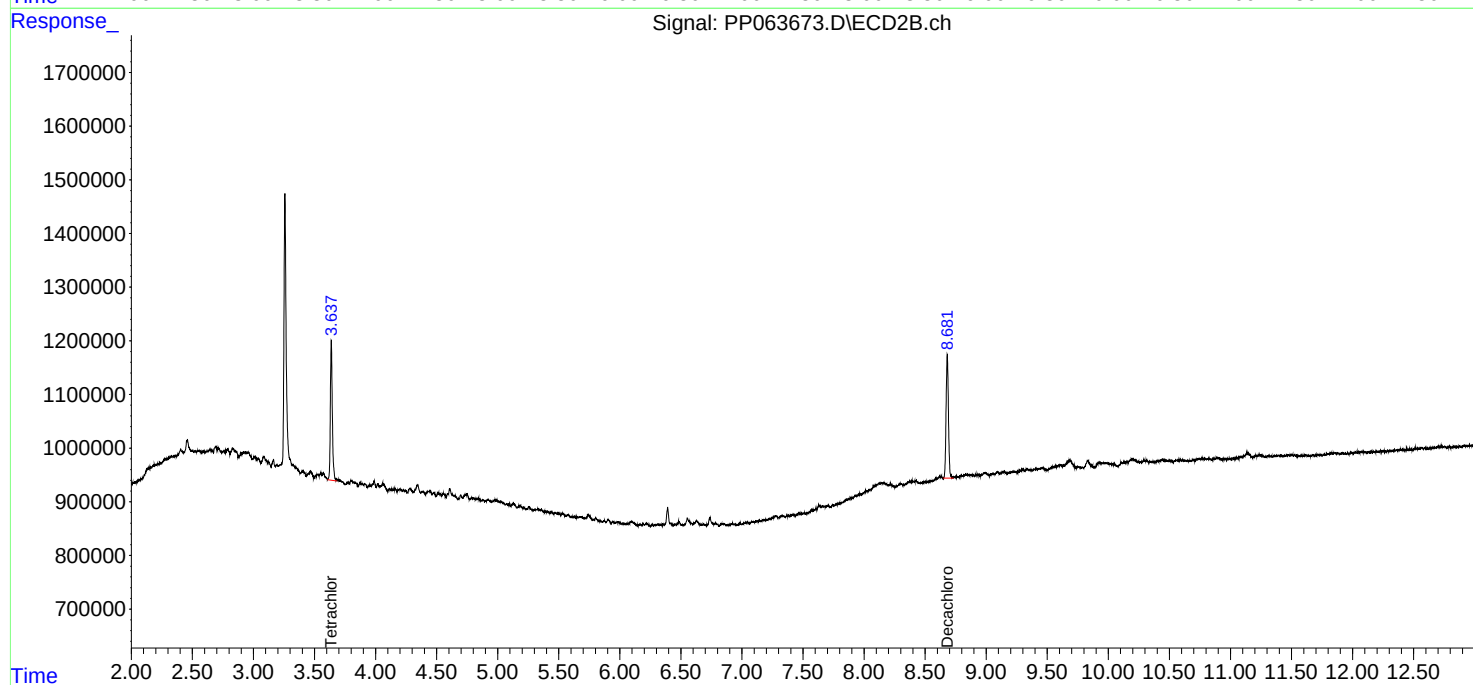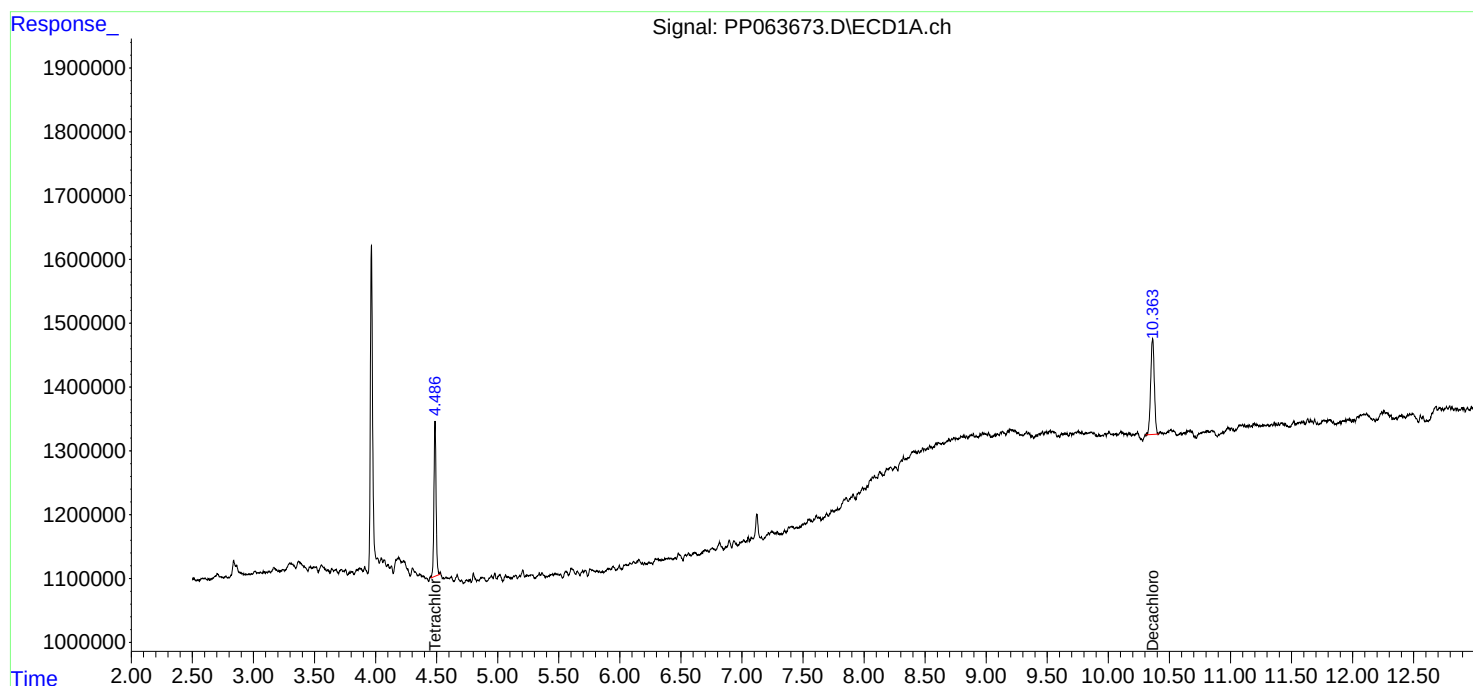

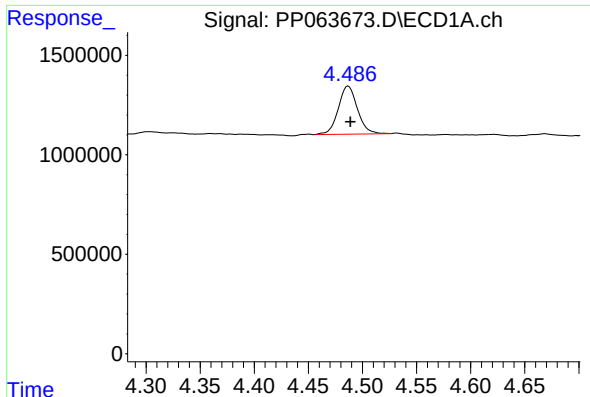


#1 Tetrachloro-m-xylene

R.T.: 4.486 min
Delta R.T.: -0.003 min
Response: 2980389
Conc: 1.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC274686-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/22/2024
Supervised By :Ankita Jodhani 03/22/2024

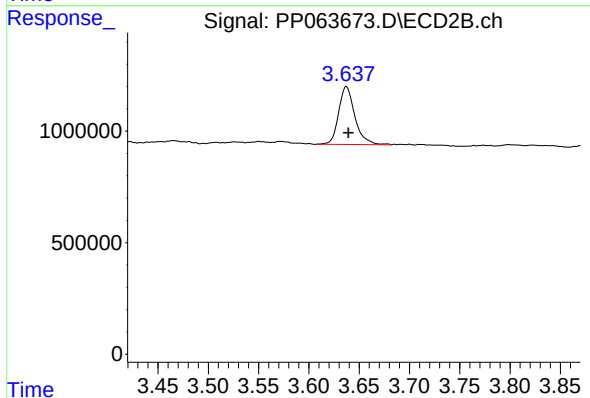


#1 Tetrachloro-m-xylene

R.T.: 3.637 min
Delta R.T.: -0.002 min
Response: 2919432
Conc: 1.22 ng/ml

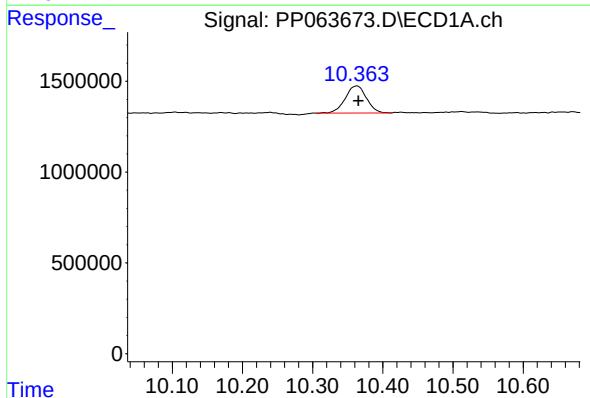

#2 Decachlorobiphenyl

R.T.: 10.363 min
Delta R.T.: -0.003 min
Response: 3120444
Conc: 1.23 ng/ml

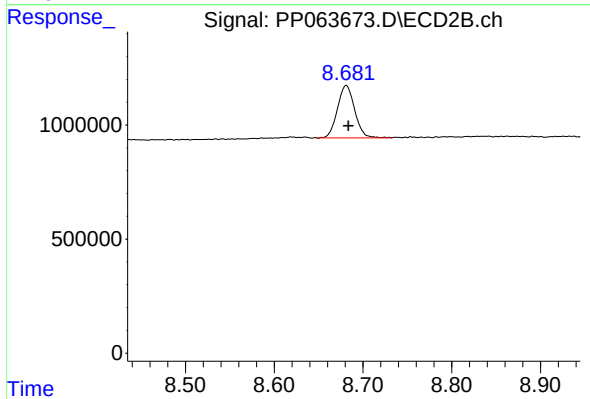

#2 Decachlorobiphenyl

R.T.: 8.681 min
Delta R.T.: -0.003 min
Response: 3079860
Conc: 1.14 ng/ml