

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032321\
 Data File : PP034264.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Mar 2021 10:08
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 02:53:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.851	4.260	1908402	1083300	22.717	24.480
2)	SA Decachlor...	10.773	9.575	1985196	709732	25.297	26.895
Target Compounds							
9)	L2 AR-1221-2	5.199	4.615	26298	15872	38.211	44.756
28)	L6 AR-1254-3	7.695	0.000	1523521	0	350.782	N.D. #
35)	L7 AR-1260-5	0.000	8.170	0	32046	N.D.	10.320 #
37)	L8 AR-1262-2	0.000	8.170	0	32046	N.D.	9.928 #
40)	L8 AR-1262-5	10.065	0.000	32780	0	11.542	N.D. #
43)	L9 AR-1268-3	9.641	0.000	73812	0	8.300	N.D. #
44)	L9 AR-1268-4	10.065	0.000	32780	0	10.530	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032321\
Data File : PP034264.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Mar 2021 10:08
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 02:53:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

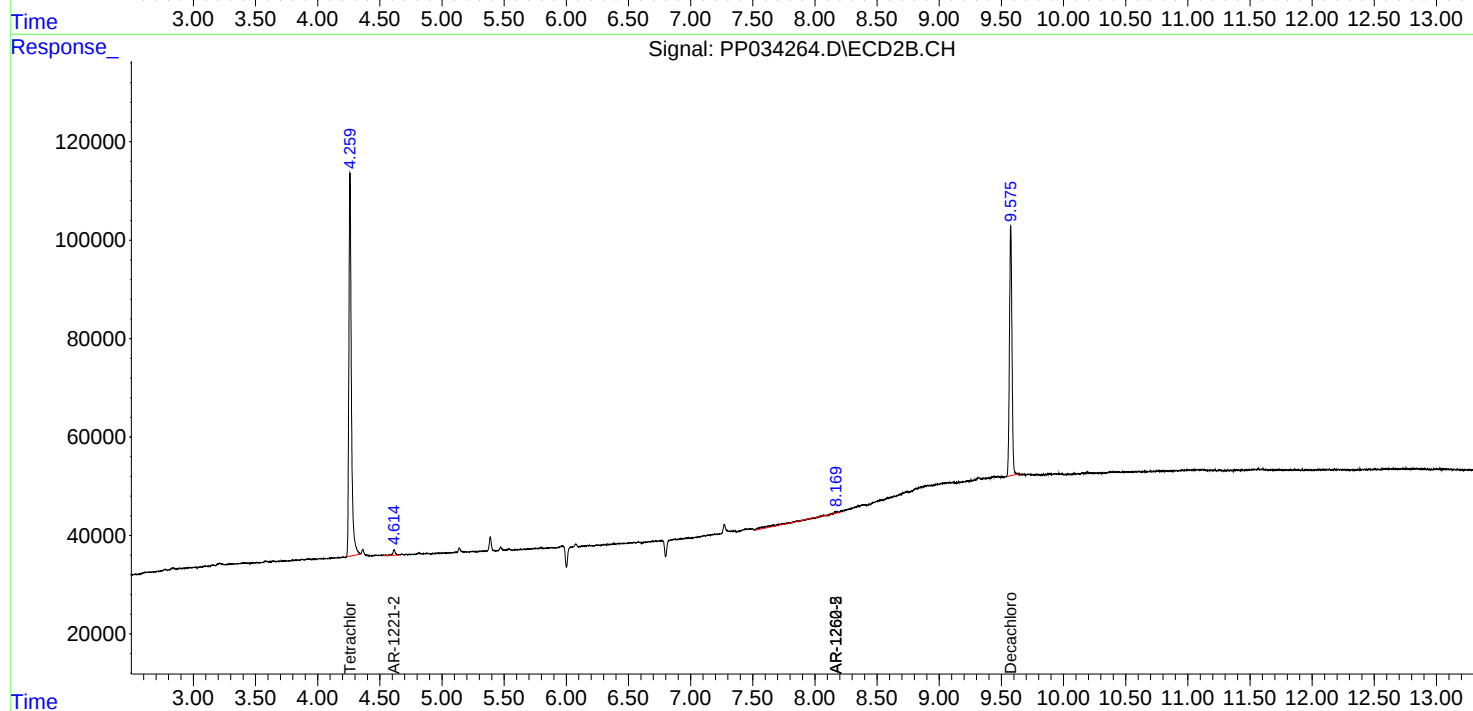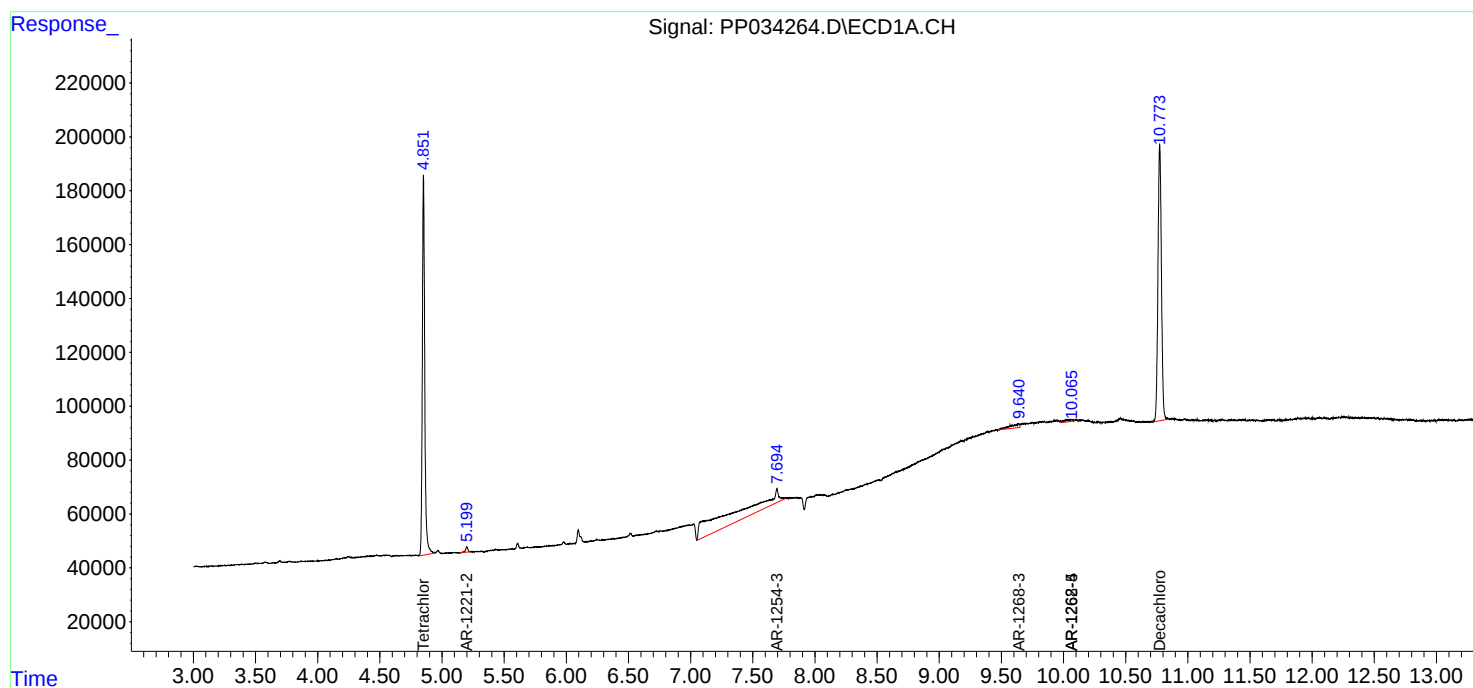


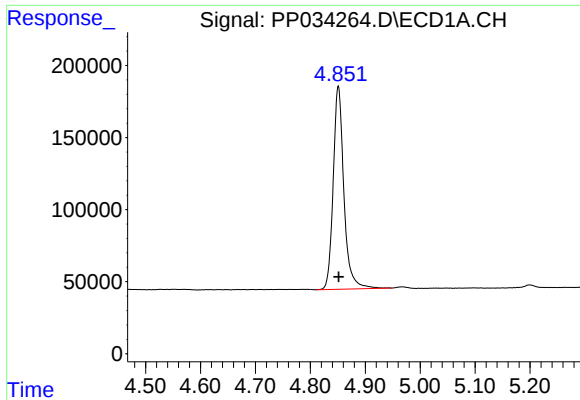

#1 Tetrachloro-m-xylene


R.T.: 4.851 min
Delta R.T.: -0.001 min
Response: 1908402
Conc: 22.72 ng/ml

Instrument :
ECD_P
ClientSampleId :

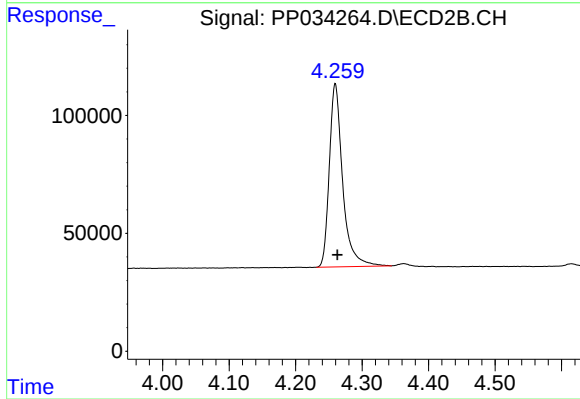


#1 Tetrachloro-m-xylene

R.T.: 4.260 min
Delta R.T.: -0.003 min
Response: 1083300
Conc: 24.48 ng/ml

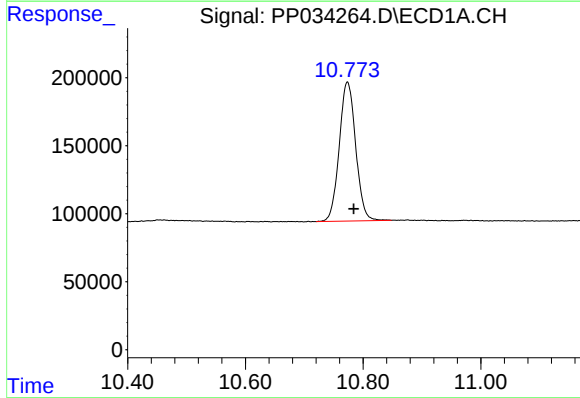


#2 Decachlorobiphenyl

R.T.: 10.773 min
Delta R.T.: -0.011 min
Response: 1985196
Conc: 25.30 ng/ml

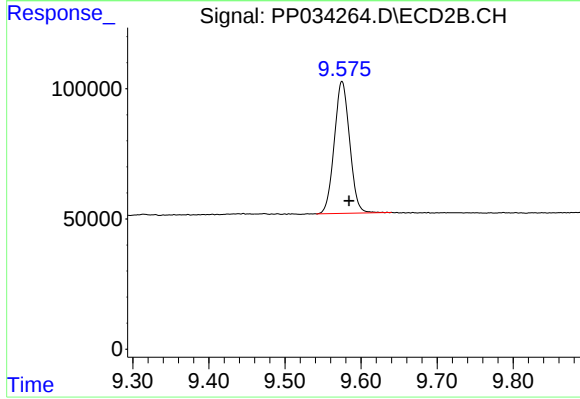

#2 Decachlorobiphenyl


R.T.: 9.575 min
Delta R.T.: -0.009 min
Response: 709732
Conc: 26.89 ng/ml

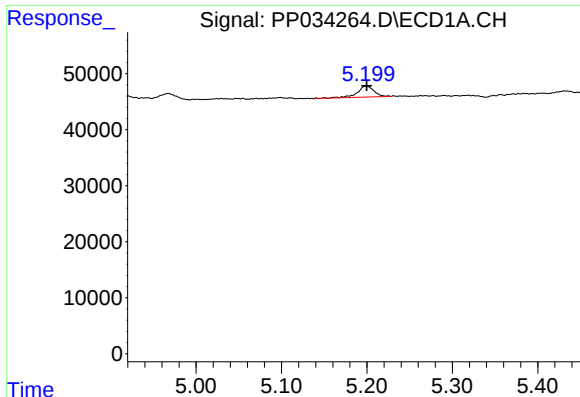

#9 AR-1221-2


R.T.: 5.199 min
Delta R.T.: 0.000 min
Response: 26298
Conc: 38.21 ng/ml

Instrument :
ECD_P
ClientSampleId :

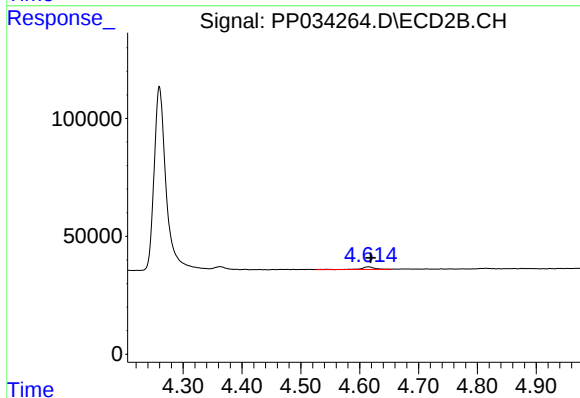


#9 AR-1221-2

R.T.: 4.615 min
Delta R.T.: -0.004 min
Response: 15872
Conc: 44.76 ng/ml

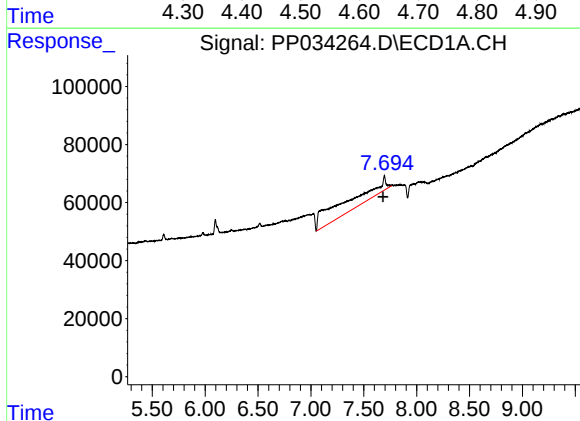


#28 AR-1254-3

R.T.: 7.695 min
Delta R.T.: 0.013 min
Response: 1523521
Conc: 350.78 ng/ml

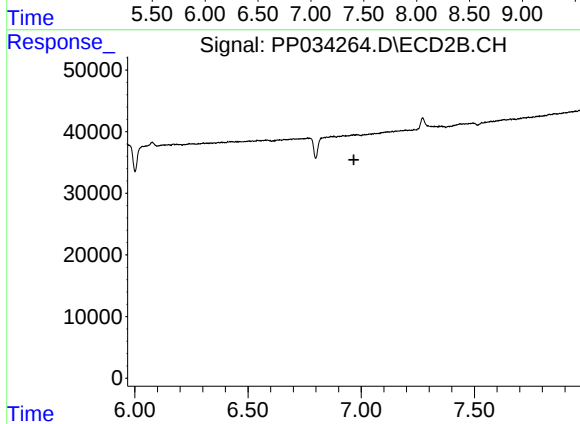

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 6.968 min
Response: 0
Conc: N.D.

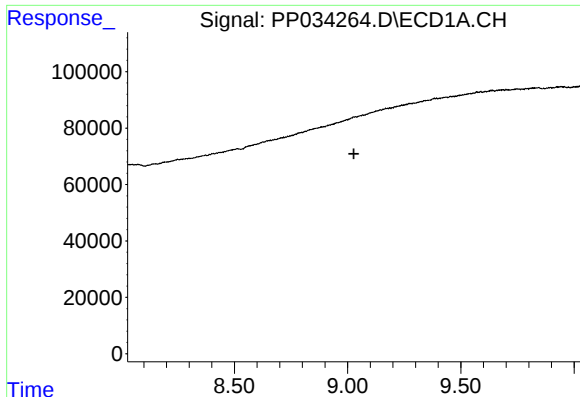

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 9.028 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

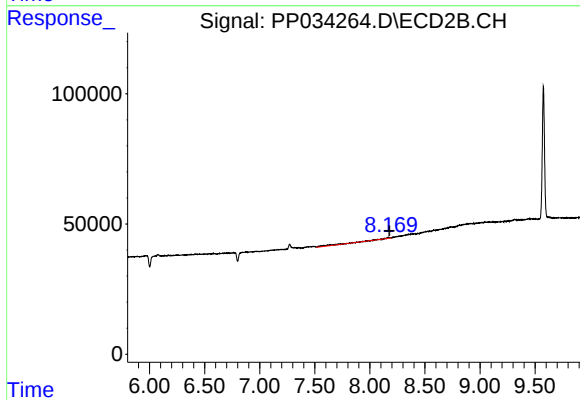


#35 AR-1260-5

R.T.: 8.170 min
Delta R.T.: -0.007 min
Response: 32046
Conc: 10.32 ng/ml

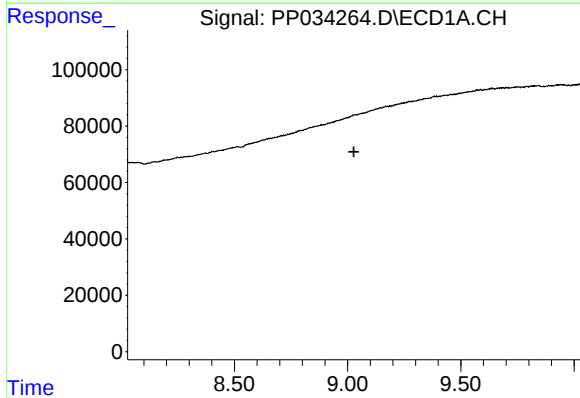


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 9.028 min
Response: 0
Conc: N.D.

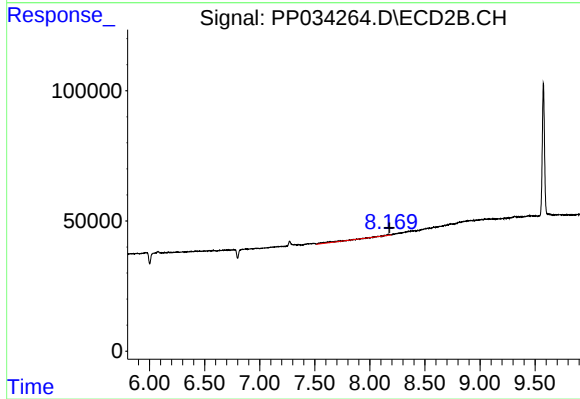

#37 AR-1262-2


R.T.: 8.170 min
Delta R.T.: -0.007 min
Response: 32046
Conc: 9.93 ng/ml

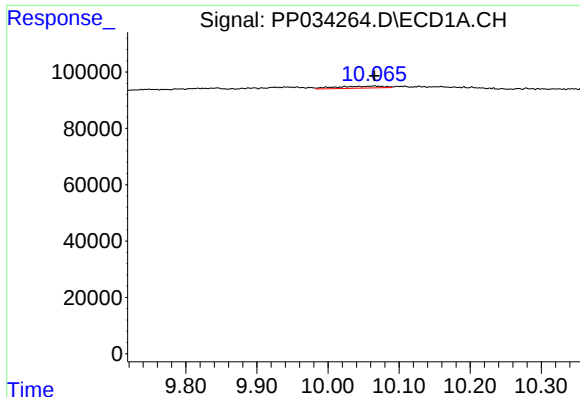

#40 AR-1262-5


R.T.: 10.065 min
Delta R.T.: 0.000 min
Response: 32780
Conc: 11.54 ng/ml

Instrument :
ECD_P
ClientSampleId :

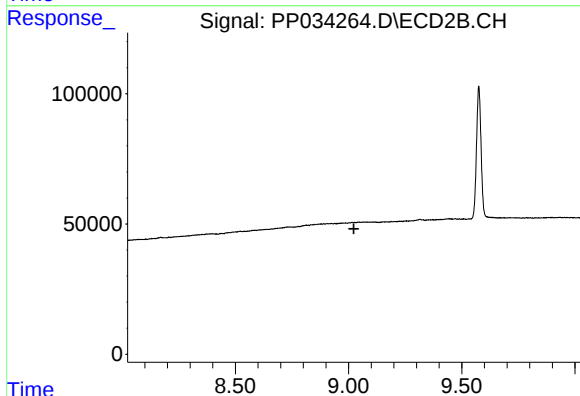


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 9.024 min
Response: 0
Conc: N.D.

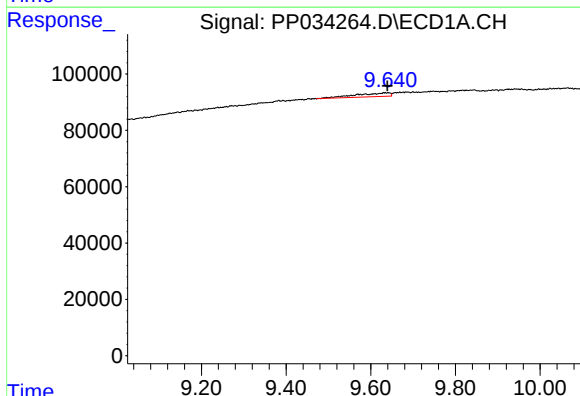


#43 AR-1268-3

R.T.: 9.641 min
Delta R.T.: 0.001 min
Response: 73812
Conc: 8.30 ng/ml

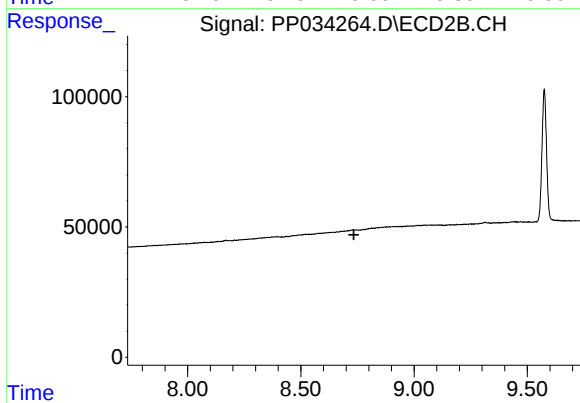

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T. : 8.734 min
Response: 0
Conc: N.D.

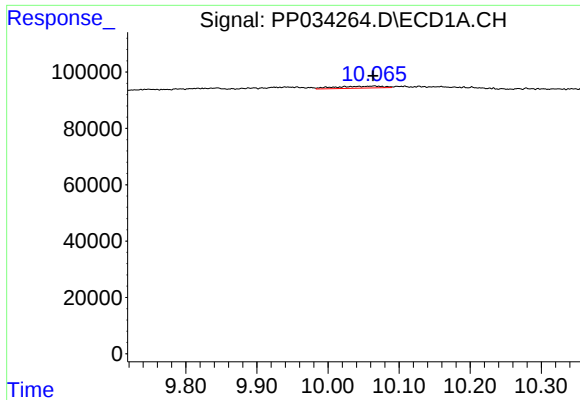

#44 AR-1268-4

R.T.: 10.065 min
Delta R.T.: 0.001 min
Response: 32780
Conc: 10.53 ng/ml

Instrument :
ECD_P
ClientSampleId :

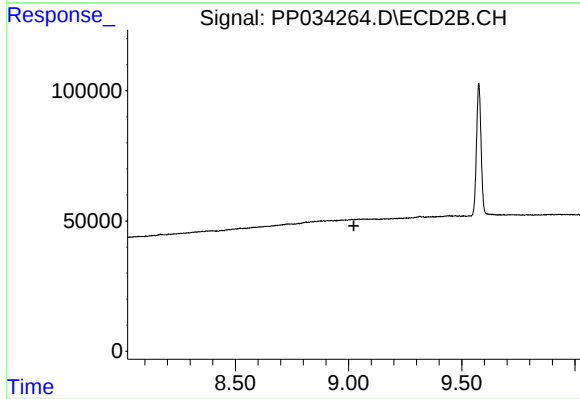

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 9.024 min
Response: 0
Conc: N.D.