

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032321\
 Data File : PP034291.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Mar 2021 17:42
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 03:03:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.848	4.260	1877749	1079967	22.352	24.405
2)	SA Decachlor...	10.771	9.574	1977463	736666	25.198	27.916
Target Compounds							
9)	L2 AR-1221-2	5.197	4.616	26120	15809	37.953	44.580
20)	L4 AR-1242-5	7.138	0.000	411042	0	269.617	N.D. #
25)	L5 AR-1248-5	7.138	0.000	411042	0	158.393	N.D. #
28)	L6 AR-1254-3	7.692	0.000	446952	0	102.908	N.D. #
30)	L6 AR-1254-5	8.380f	0.000	105683	0	31.658	N.D. #
31)	L7 AR-1260-1	7.848	0.000	151242	0	47.451	N.D. #
32)	L7 AR-1260-2	0.000	7.271f	0	39642	N.D.	22.155 #
34)	L7 AR-1260-4	8.715	0.000	34503	0	9.910	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032321\
Data File : PP034291.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Mar 2021 17:42
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 03:03:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

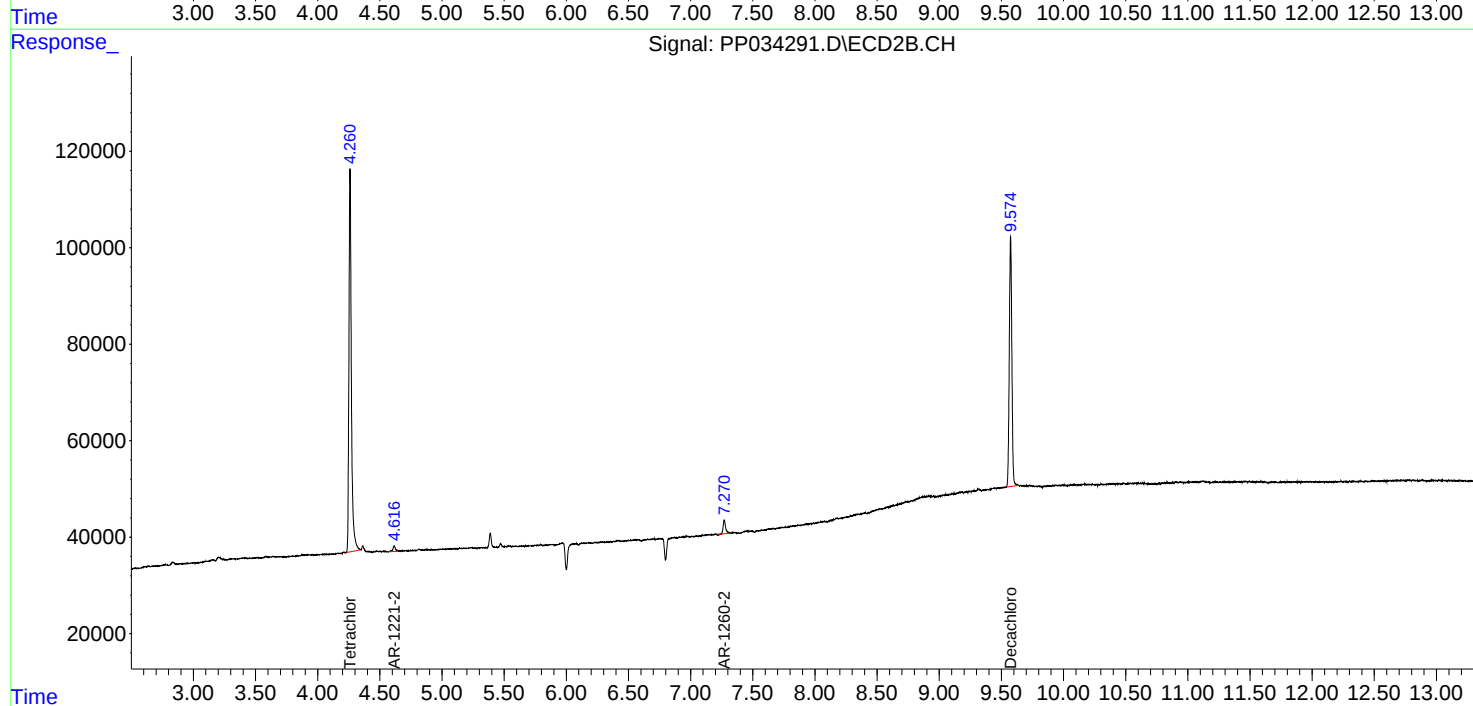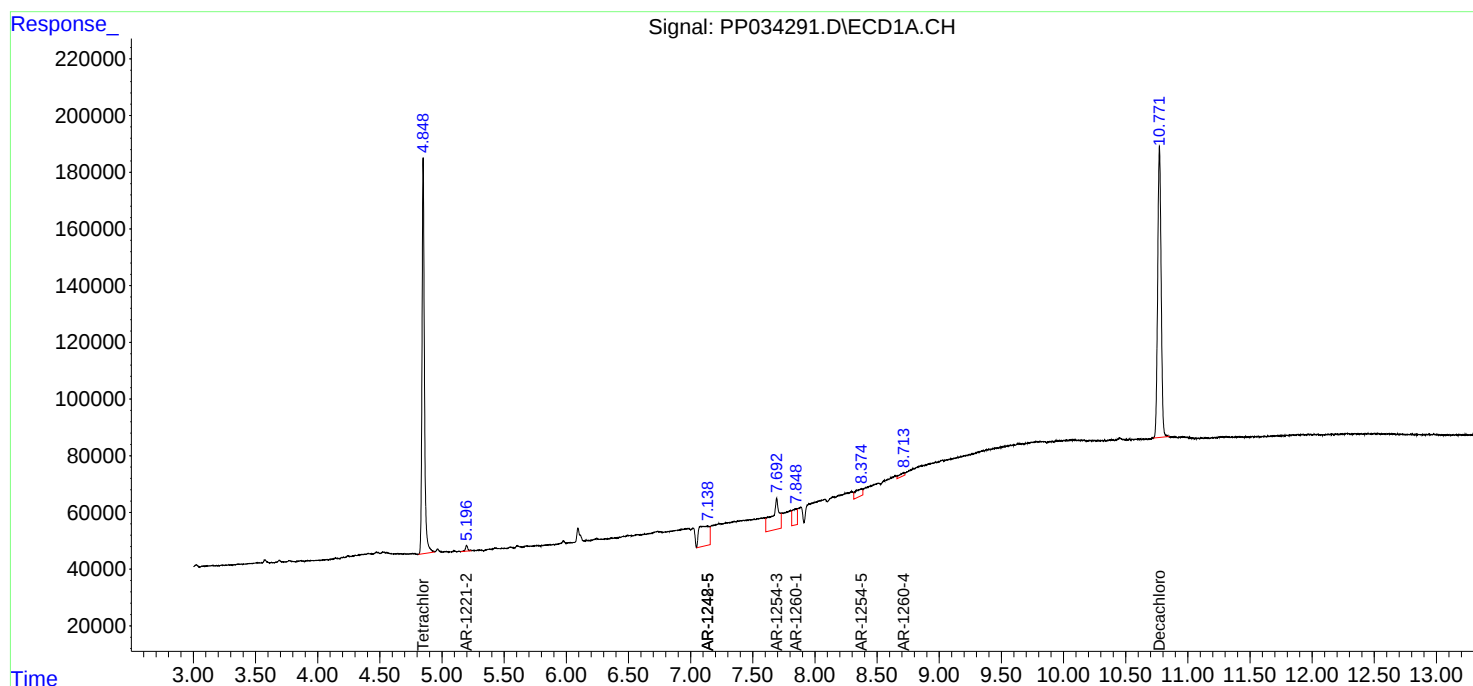


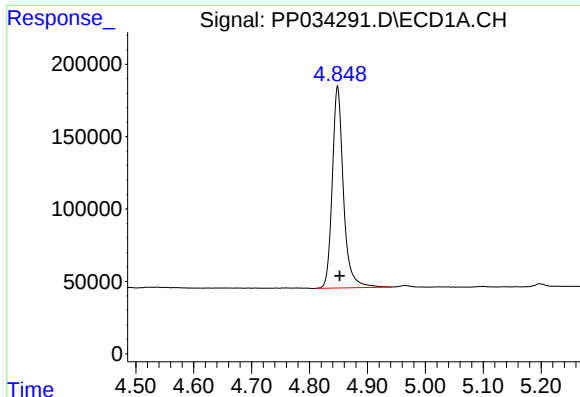

#1 Tetrachloro-m-xylene


R.T.: 4.848 min
Delta R.T.: -0.004 min
Response: 1877749
Conc: 22.35 ng/ml

Instrument :
ECD_P
ClientSampleId :

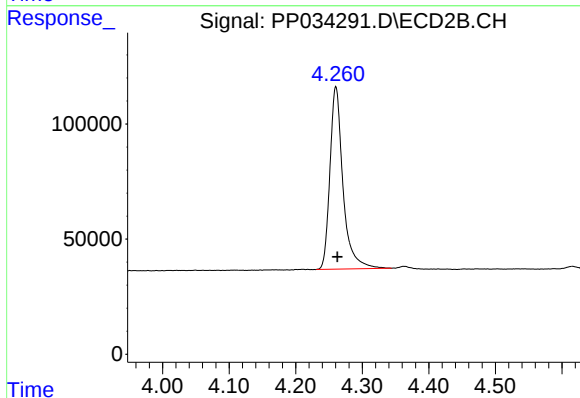


#1 Tetrachloro-m-xylene

R.T.: 4.260 min
Delta R.T.: -0.002 min
Response: 1079967
Conc: 24.40 ng/ml

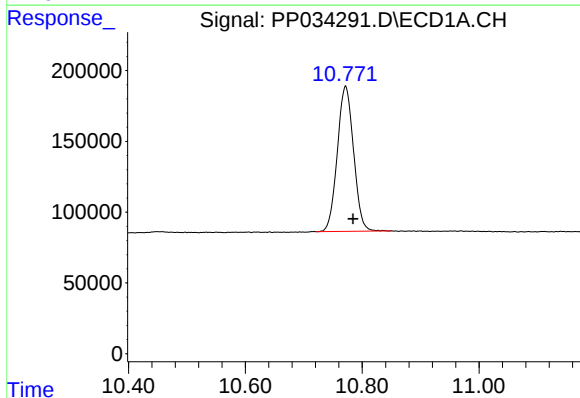


#2 Decachlorobiphenyl

R.T.: 10.771 min
Delta R.T.: -0.013 min
Response: 1977463
Conc: 25.20 ng/ml

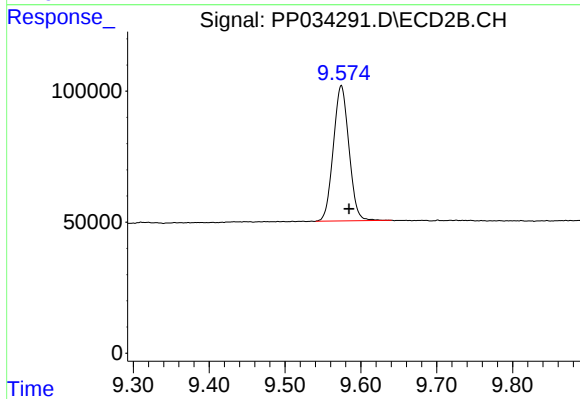

#2 Decachlorobiphenyl


R.T.: 9.574 min
Delta R.T.: -0.010 min
Response: 736666
Conc: 27.92 ng/ml

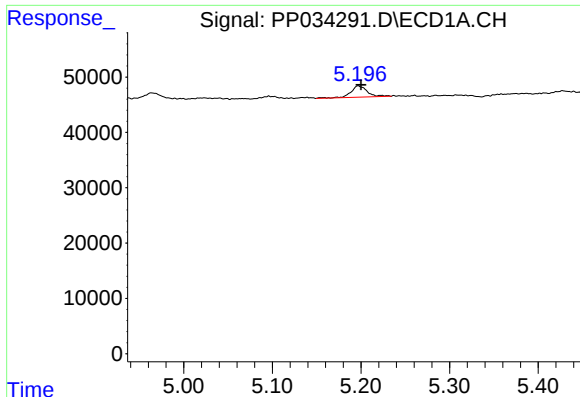

#9 AR-1221-2


R.T.: 5.197 min
Delta R.T.: -0.003 min
Response: 26120
Conc: 37.95 ng/ml

Instrument :
ECD_P
ClientSampleId :

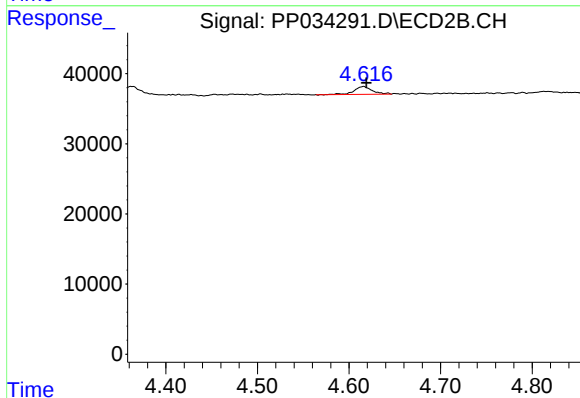


#9 AR-1221-2

R.T.: 4.616 min
Delta R.T.: -0.003 min
Response: 15809
Conc: 44.58 ng/ml

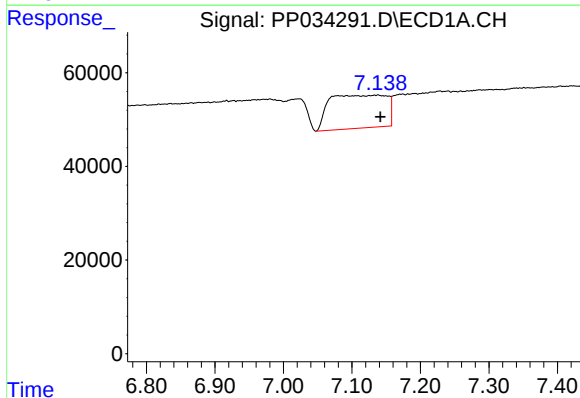


#20 AR-1242-5

R.T.: 7.138 min
Delta R.T.: -0.003 min
Response: 411042
Conc: 269.62 ng/ml

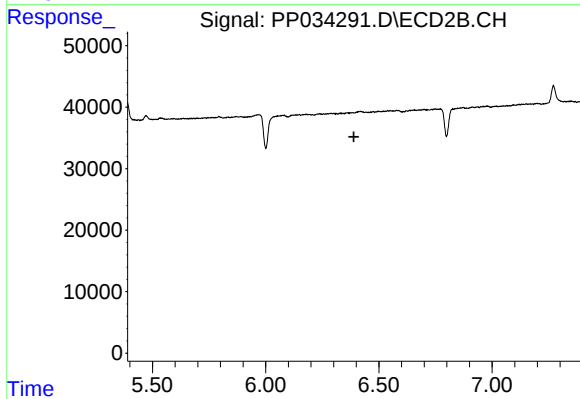

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.389 min
Response: 0
Conc: N.D.

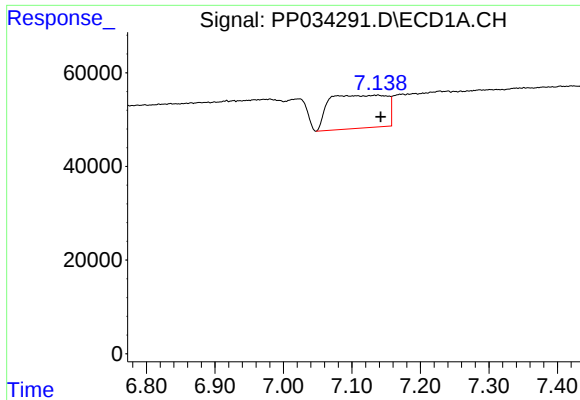

#25 AR-1248-5


R.T.: 7.138 min
Delta R.T.: -0.004 min
Response: 411042
Conc: 158.39 ng/ml

Instrument :
ECD_P
ClientSampleId :

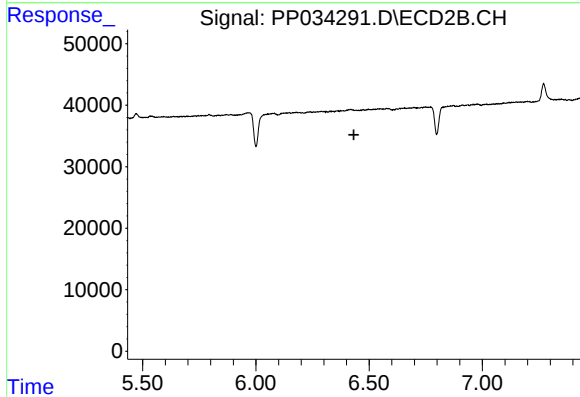


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 6.433 min
Response: 0
Conc: N.D.

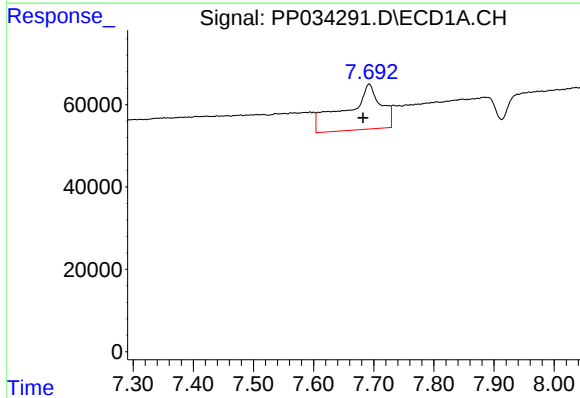


#28 AR-1254-3

R.T.: 7.692 min
Delta R.T.: 0.010 min
Response: 446952
Conc: 102.91 ng/ml

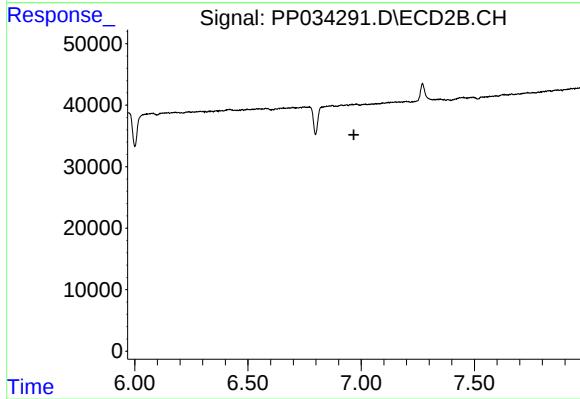

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.968 min
Response: 0
Conc: N.D.

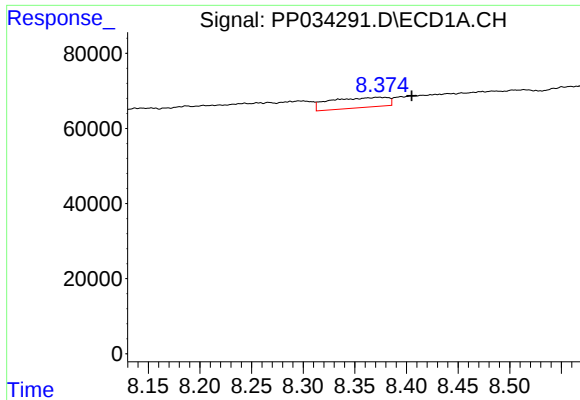

#30 AR-1254-5


R.T.: 8.380 min
Delta R.T.: -0.025 min
Response: 105683
Conc: 31.66 ng/ml

Instrument :
ECD_P
ClientSampleId :

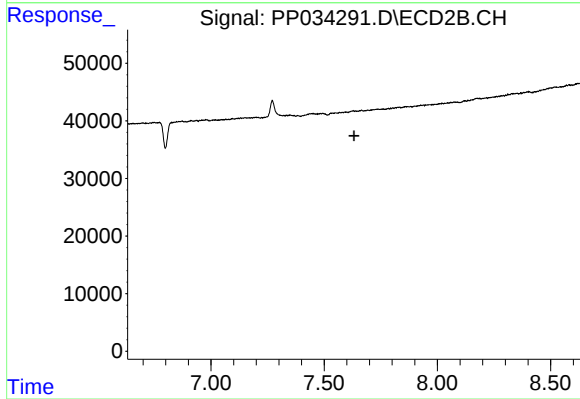


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.632 min
Response: 0
Conc: N.D.

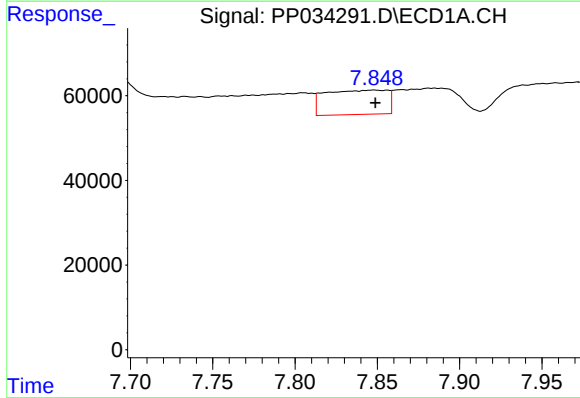


#31 AR-1260-1

R.T.: 7.848 min
Delta R.T.: 0.000 min
Response: 151242
Conc: 47.45 ng/ml

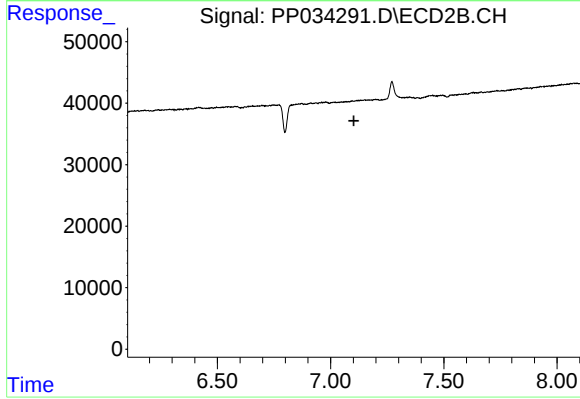

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 7.103 min
Response: 0
Conc: N.D.

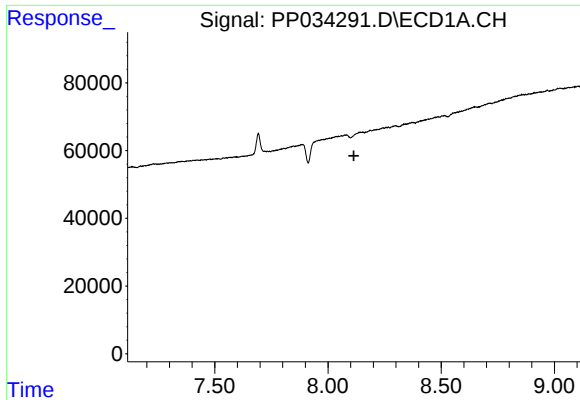

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 8.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

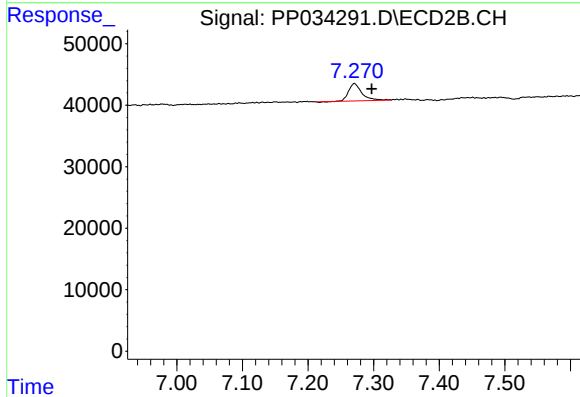


#32 AR-1260-2

R.T.: 7.271 min
Delta R.T.: -0.026 min
Response: 39642
Conc: 22.15 ng/ml

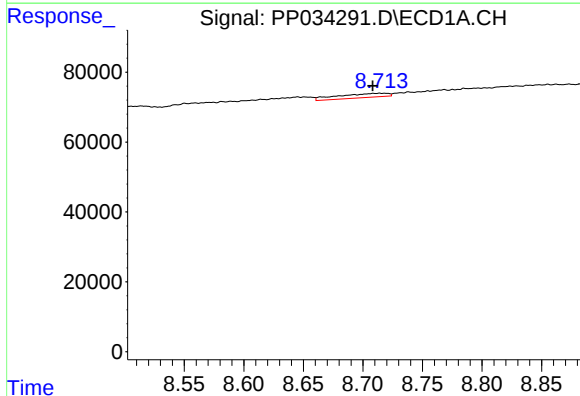

#34 AR-1260-4

R.T.: 8.715 min
Delta R.T.: 0.007 min
Response: 34503
Conc: 9.91 ng/ml

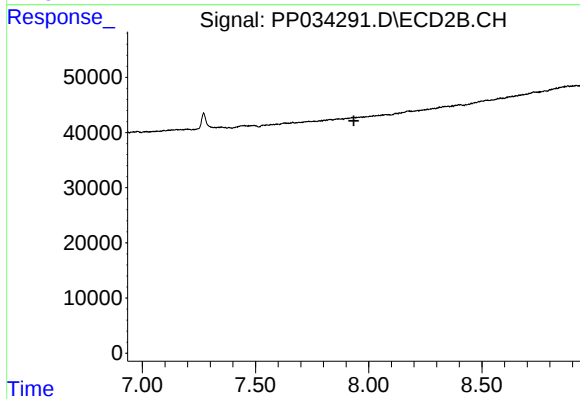

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.934 min
Response: 0
Conc: N.D.